

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112019\
 Data File : PS007754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2019 16:57
 Operator : SM\AJ
 Sample : PB124979BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 02:39:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.442	5.161	824.9E6	393.3E6	598.965	559.836
Target Compounds							
1) T	Dalapon	2.003	1.706	122.7E6	418.9E6	67.847	352.829 #
2) T	3,5-DICHL...	0.000	4.496	0	62182406	N.D.	68.829
5) T	DICAMBA	5.534	5.326	47020823	45519853	9.243	17.201 #
6) T	MCP	0.000	5.326	0	45519853	N.D.	23.431
7) T	MCPA	0.000	5.530	0	9998721	N.D.	3.327
9) T	2,4-D	6.393	6.063	367.5E6	5639225	262.050	6.993 #
10) T	Pentachlo...	0.000	6.372	0	20403151	N.D.	2.084
11) T	2,4,5-TP ...	0.000	6.766	0	21392270	N.D.	5.463



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112019\
Data File : PS007754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2019 16:57
Operator : SM\AJ
Sample : PB124979BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 02:39:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

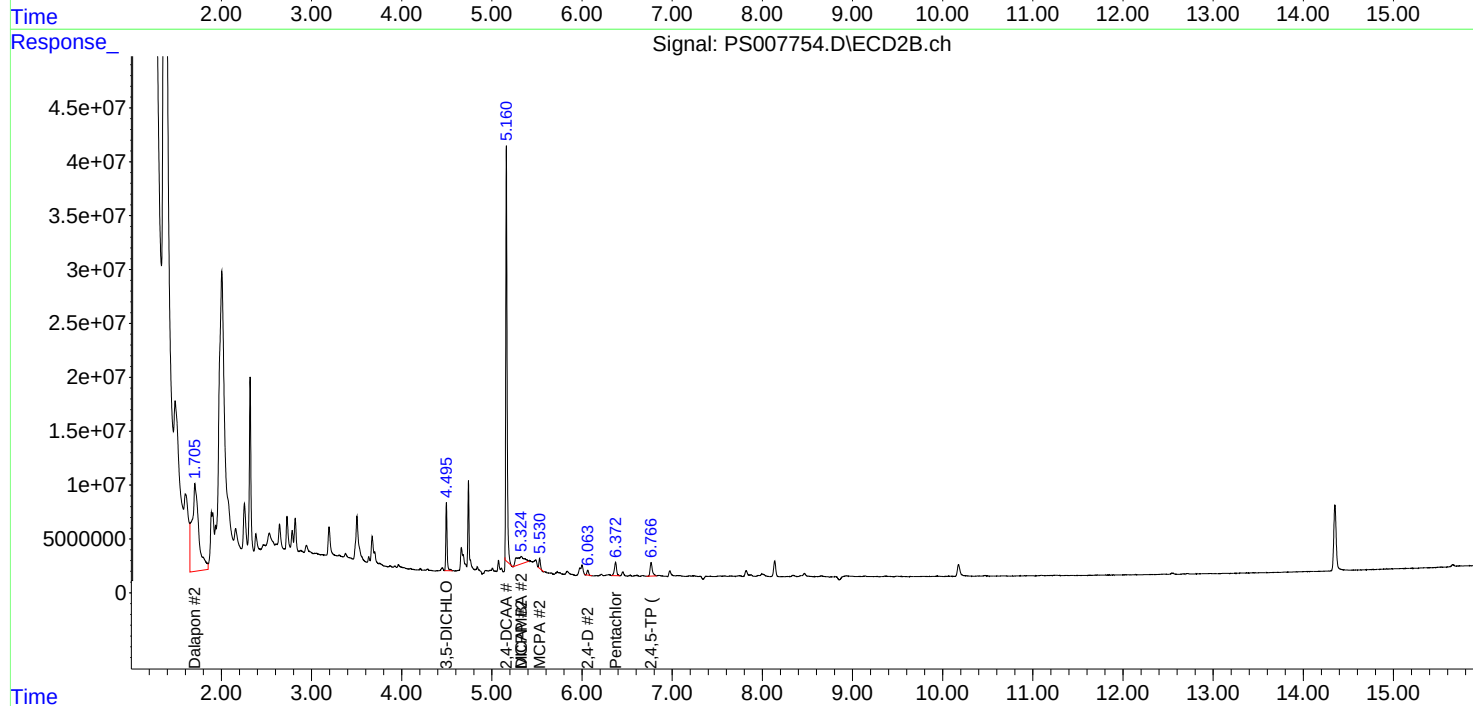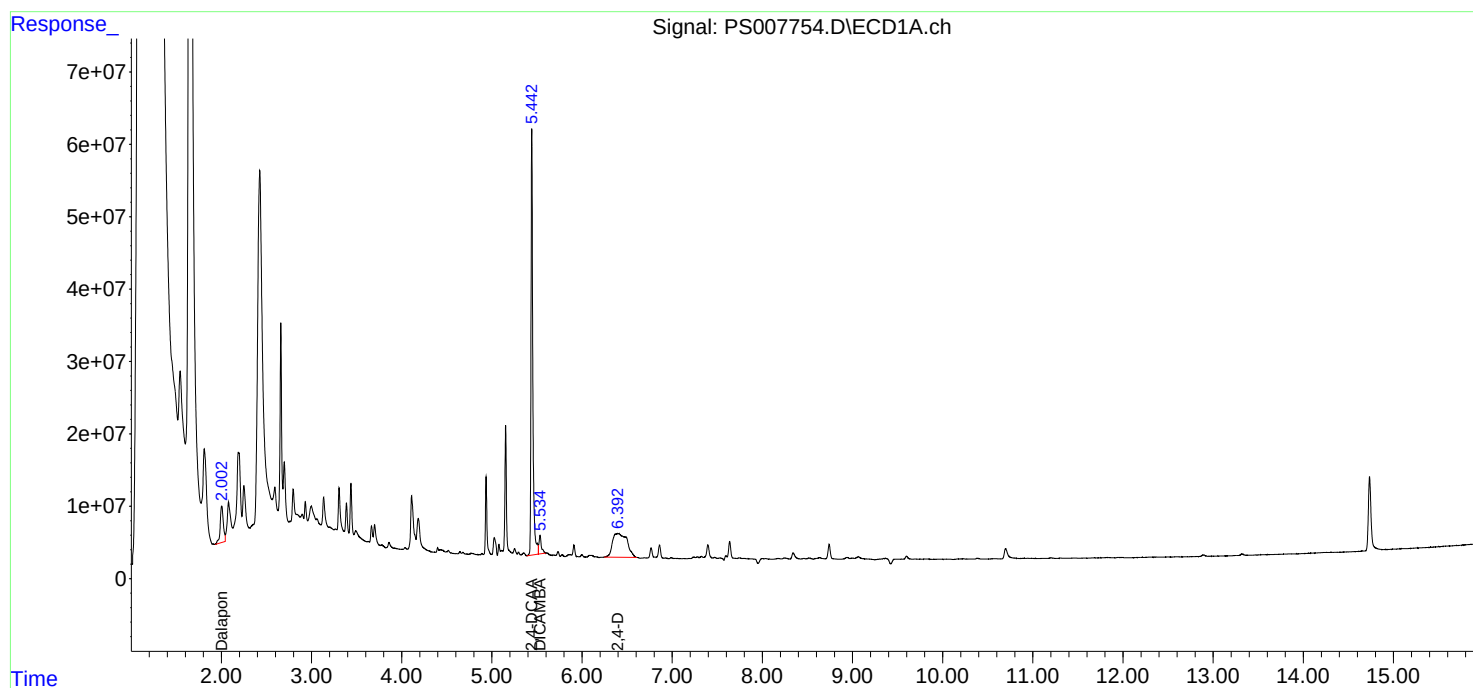


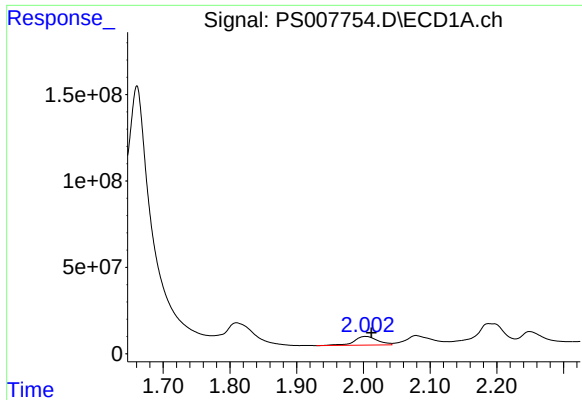

#1 Dalapon


R.T.: 2.003 min
Delta R.T.: -0.009 min
Response: 122748288
Conc: 67.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

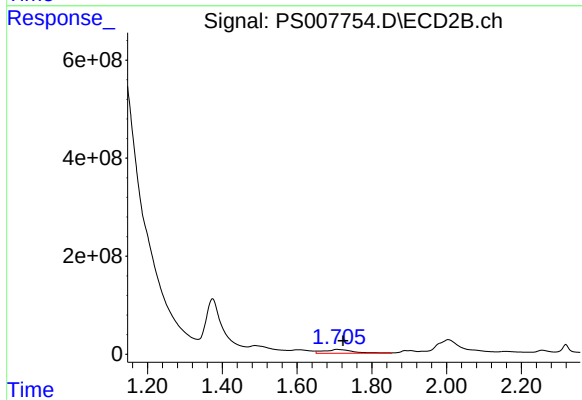


#1 Dalapon

R.T.: 1.706 min
Delta R.T.: -0.017 min
Response: 418949534
Conc: 352.83 ng/ml

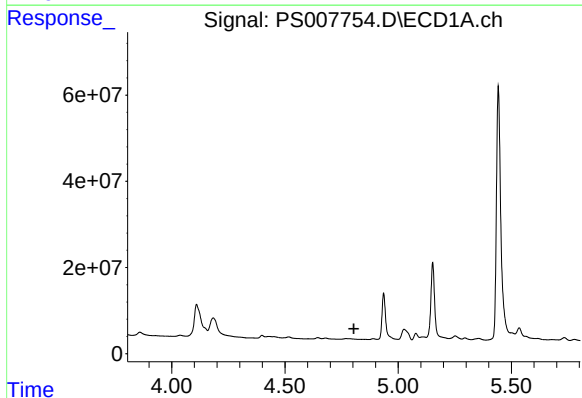


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

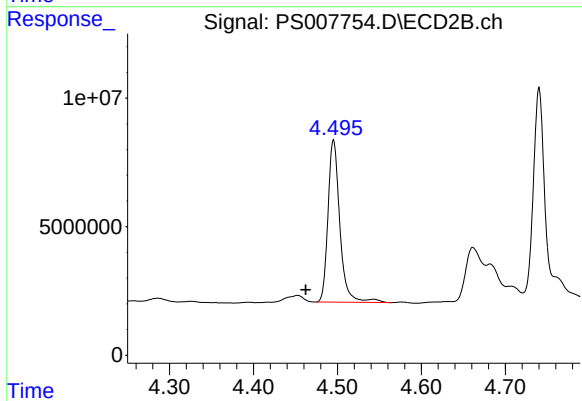

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.496 min
Delta R.T.: 0.033 min
Response: 62182406
Conc: 68.83 ng/ml

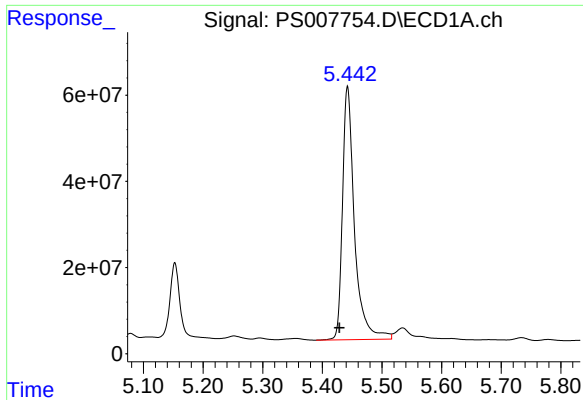

#4 2,4-DCAA


R.T.: 5.442 min
Delta R.T.: 0.014 min
Response: 824885427
Conc: 598.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

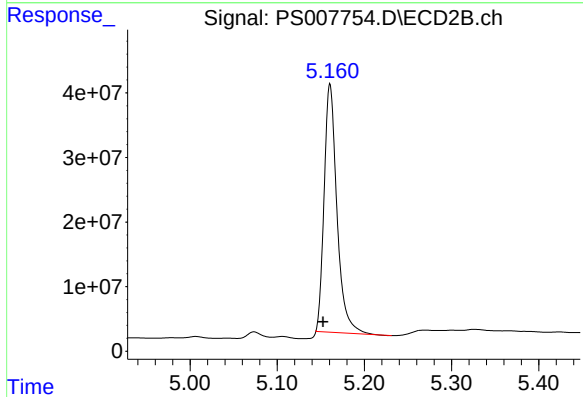


#4 2,4-DCAA

R.T.: 5.161 min
Delta R.T.: 0.008 min
Response: 393320492
Conc: 559.84 ng/ml

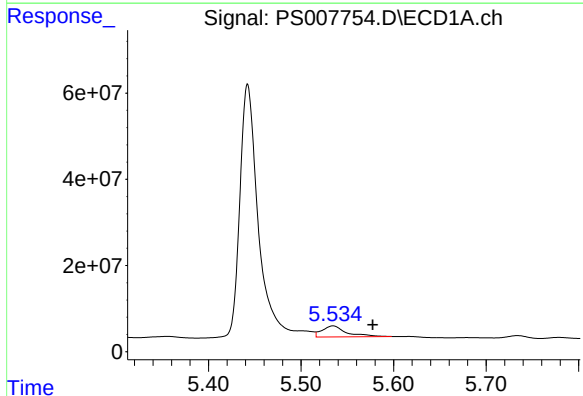


#5 DICAMBA

R.T.: 5.534 min
Delta R.T.: -0.043 min
Response: 47020823
Conc: 9.24 ng/ml

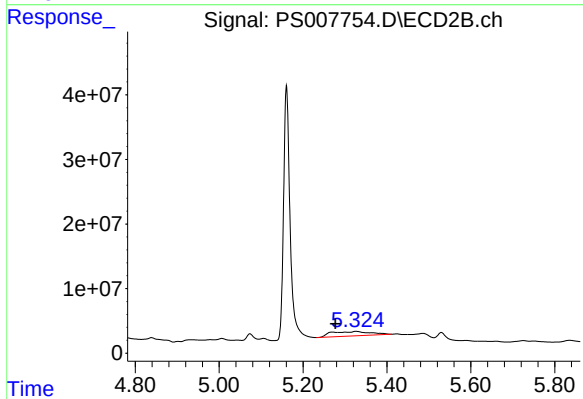

#5 DICAMBA


R.T.: 5.326 min
Delta R.T.: 0.049 min
Response: 45519853
Conc: 17.20 ng/ml

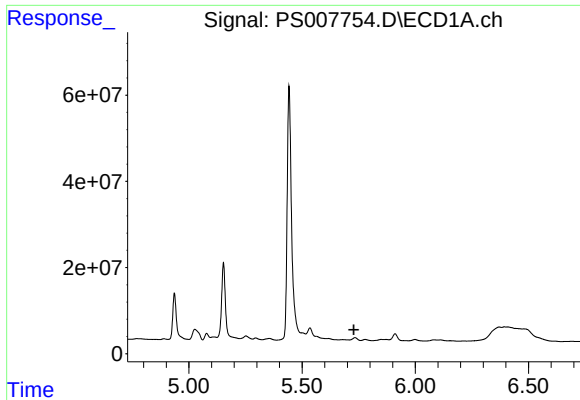

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

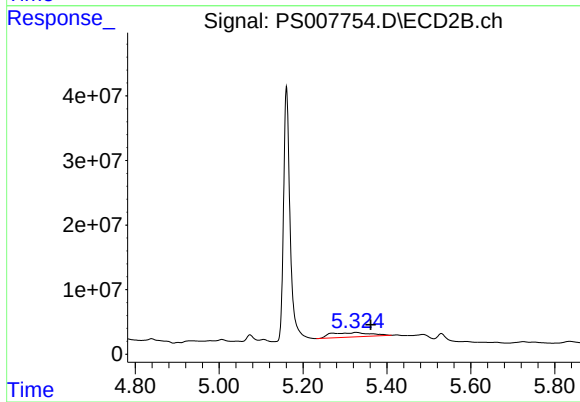


#6 MCP

R.T.: 5.326 min
Delta R.T.: -0.035 min
Response: 45519853
Conc: 23.43 ug/ml

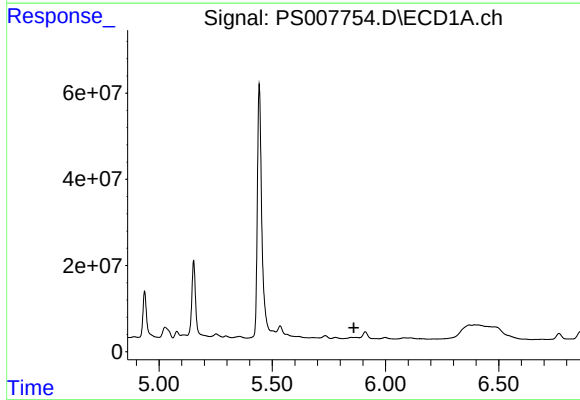


#7 MCP

R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

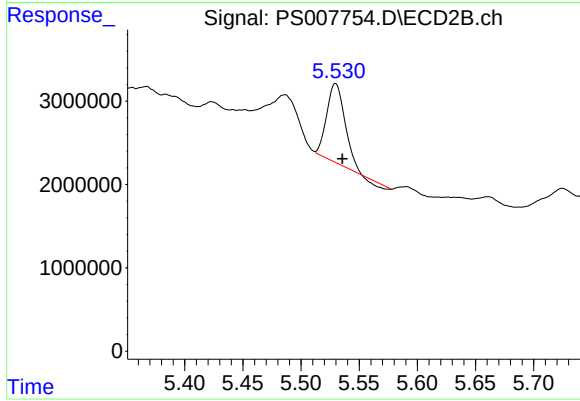

#7 MCP


R.T.: 5.530 min
Delta R.T.: -0.006 min
Response: 9998721
Conc: 3.33 ug/ml

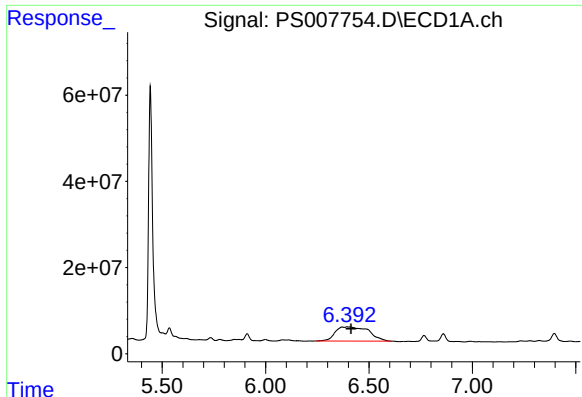

#9 2,4-D


R.T.: 6.393 min
Delta R.T.: -0.021 min
Response: 367537499
Conc: 262.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

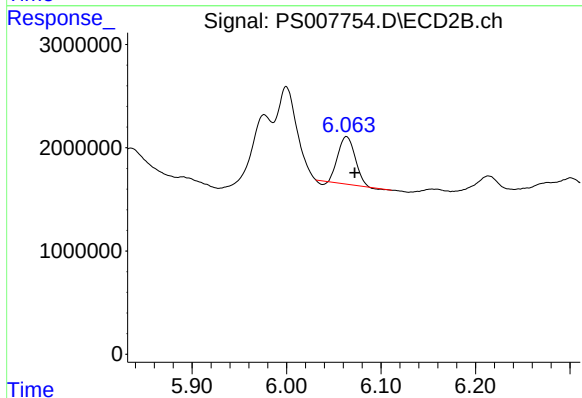


#9 2,4-D

R.T.: 6.063 min
Delta R.T.: -0.009 min
Response: 5639225
Conc: 6.99 ng/ml

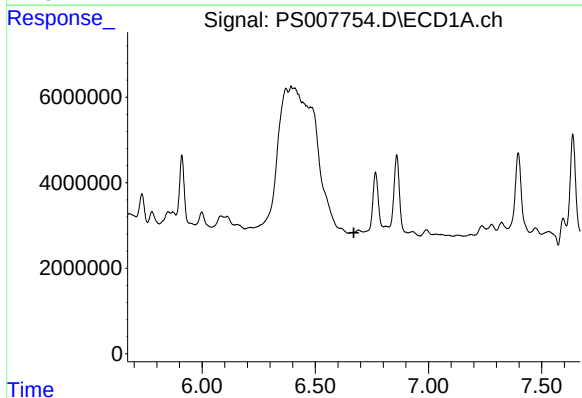


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.671 min
Response: 0
Conc: N.D.

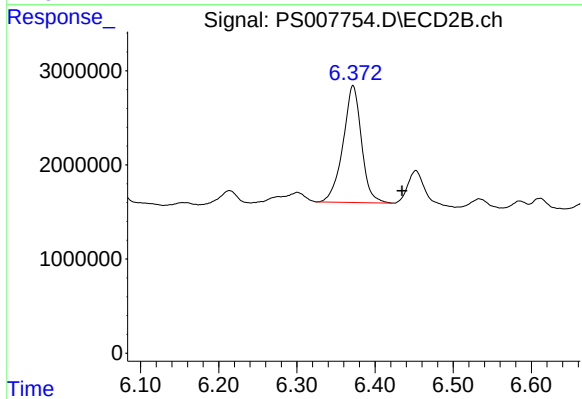

#10 Pentachlorophenol


R.T.: 6.372 min
Delta R.T.: -0.063 min
Response: 20403151
Conc: 2.08 ng/ml

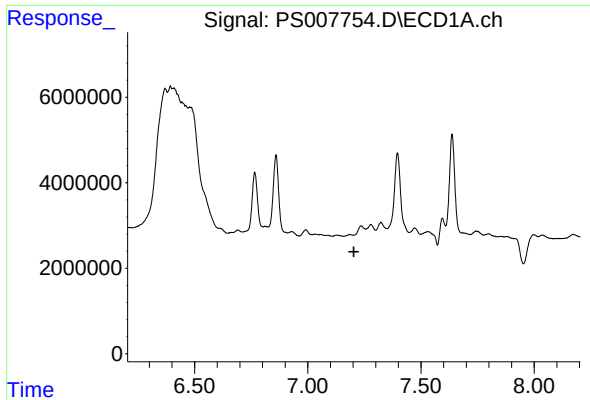

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

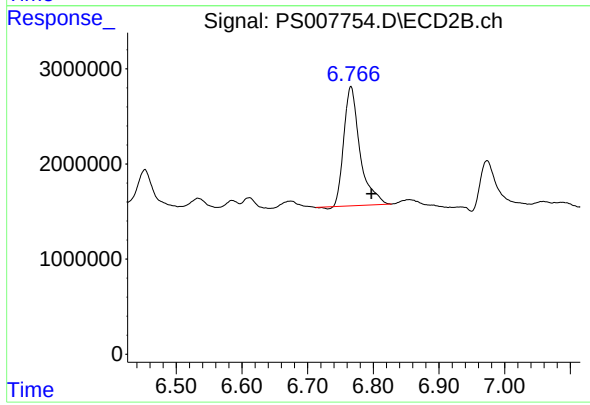

#11 2,4,5-TP (SILVEX)

R.T.: 6.766 min
Delta R.T.: -0.031 min
Response: 21392270
Conc: 5.46 ng/ml