

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112019\  
 Data File : PS007766.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Nov 2019 21:21  
 Operator : SM\AJ  
 Sample : K5938-02  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 21 02:43:54 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110619.M  
 Quant Title : 8080.M  
 QLast Update : Wed Nov 06 02:45:11 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------------|-------|-------|----------|----------|---------|-----------|
| -----                       |              |       |       |          |          |         |           |
| System Monitoring Compounds |              |       |       |          |          |         |           |
| 4) S                        | 2,4-DCAA     | 5.434 | 5.156 | 222.5E6  | 60057167 | 161.537 | 85.483 #  |
| Target Compounds            |              |       |       |          |          |         |           |
| 1) T                        | Dalapon      | 1.993 | 1.701 | 98409355 | 268.7E6  | 54.394  | 226.259 # |
| 2) T                        | 3,5-DICHL... | 0.000 | 4.447 | 0        | 7019289  | N.D.    | 7.770     |
| 7) T                        | MCPA         | 0.000 | 5.529 | 0        | 15249241 | N.D.    | 5.073     |
| 10) T                       | Pentachlo... | 0.000 | 6.441 | 0        | 13062951 | N.D.    | 1.334     |
| 11) T                       | 2,4,5-TP ... | 0.000 | 6.757 | 0        | 14952400 | N.D.    | 3.818     |
| 15) T                       | Picloram     | 0.000 | 8.907 | 0        | 8547972  | N.D.    | 1.459     |
| 16) T                       | DCPA         | 0.000 | 8.907 | 0        | 8547972  | N.D.    | 1.636     |
| -----                       |              |       |       |          |          |         |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112019\  
Data File : PS007766.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Nov 2019 21:21  
Operator : SM\AJ  
Sample : K5938-02  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 21 02:43:54 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110619.M  
Quant Title : 8080.M  
QLast Update : Wed Nov 06 02:45:11 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

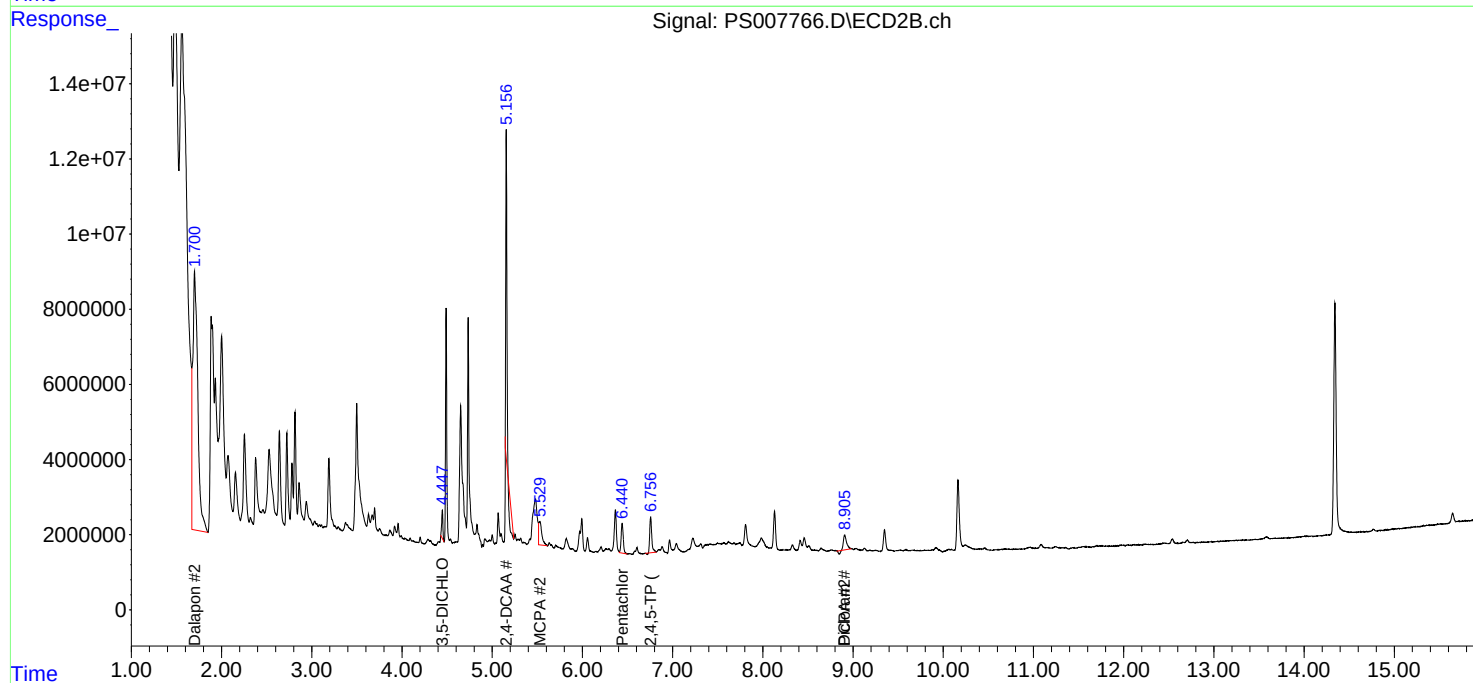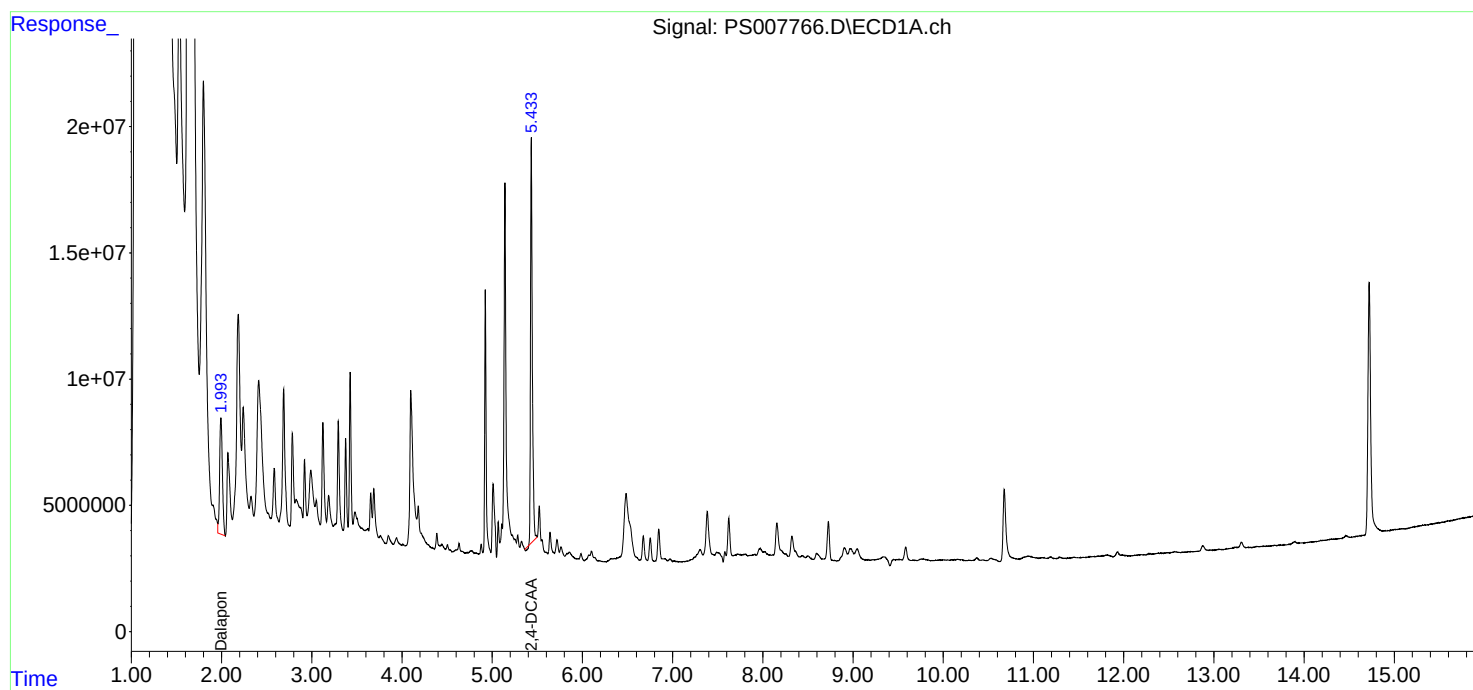


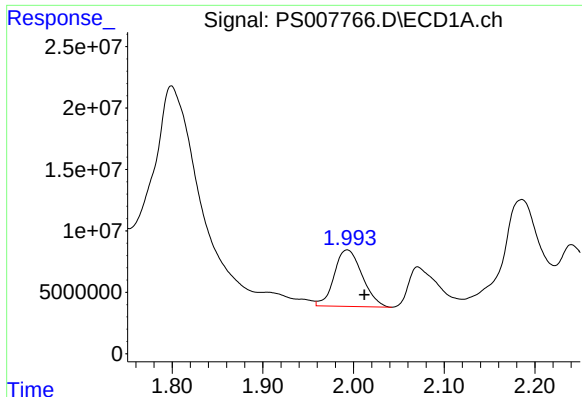

#1 Dalapon


R.T.: 1.993 min  
Delta R.T.: -0.019 min  
Response: 98409355  
Conc: 54.39 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

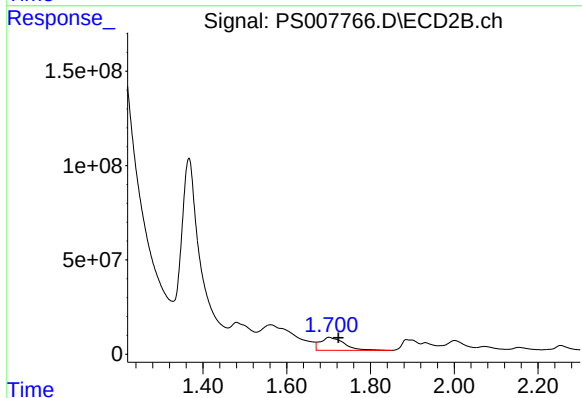


#1 Dalapon

R.T.: 1.701 min  
Delta R.T.: -0.022 min  
Response: 268660998  
Conc: 226.26 ng/ml

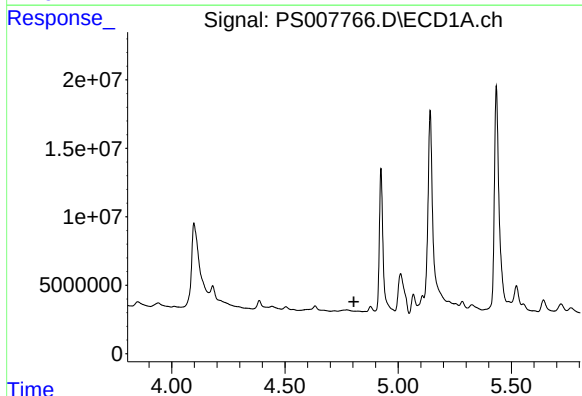


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 4.804 min  
Response: 0  
Conc: N.D.

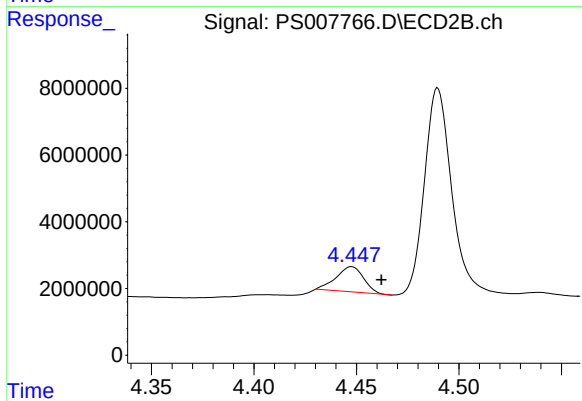

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min  
Delta R.T.: -0.015 min  
Response: 7019289  
Conc: 7.77 ng/ml

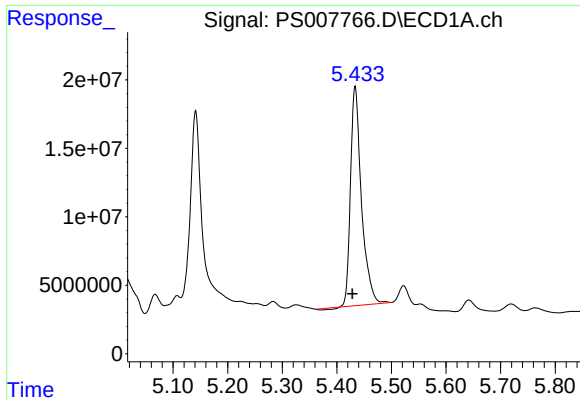

#4 2,4-DCAA


R.T.: 5.434 min  
Delta R.T.: 0.005 min  
Response: 222465719  
Conc: 161.54 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

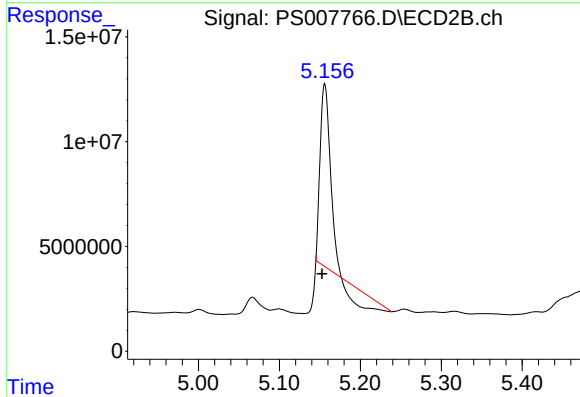


#4 2,4-DCAA

R.T.: 5.156 min  
Delta R.T.: 0.004 min  
Response: 60057167  
Conc: 85.48 ng/ml

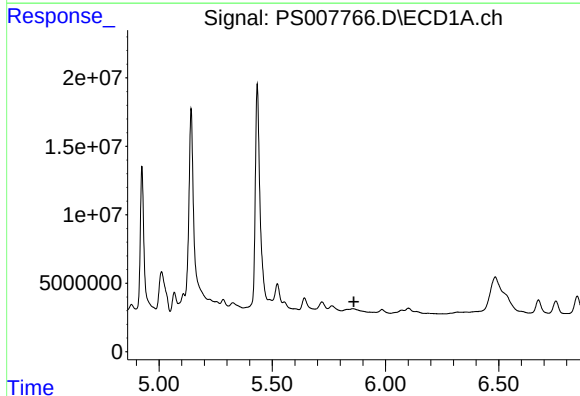


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 5.860 min  
Response: 0  
Conc: N.D.

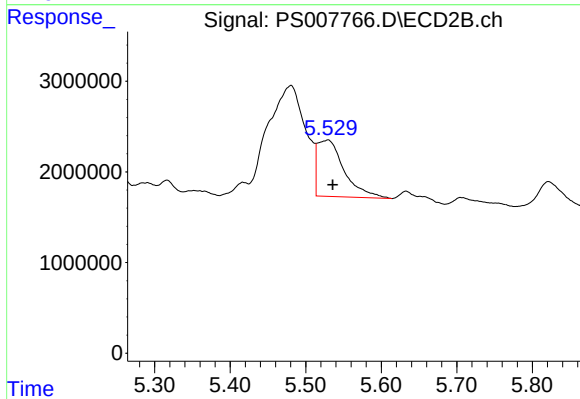

#7 MCPA


R.T.: 5.529 min  
Delta R.T.: -0.007 min  
Response: 15249241  
Conc: 5.07 ug/ml

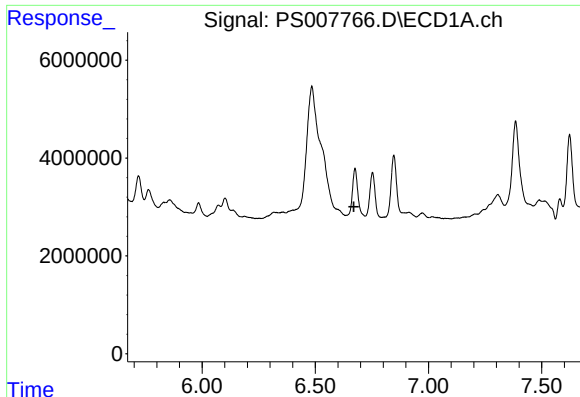

#10 Pentachlorophenol


R.T.: 0.000 min  
Exp R.T.: 6.671 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

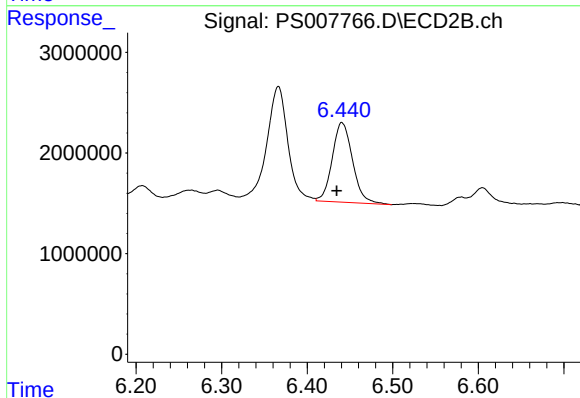


#10 Pentachlorophenol

R.T.: 6.441 min  
Delta R.T.: 0.006 min  
Response: 13062951  
Conc: 1.33 ng/ml

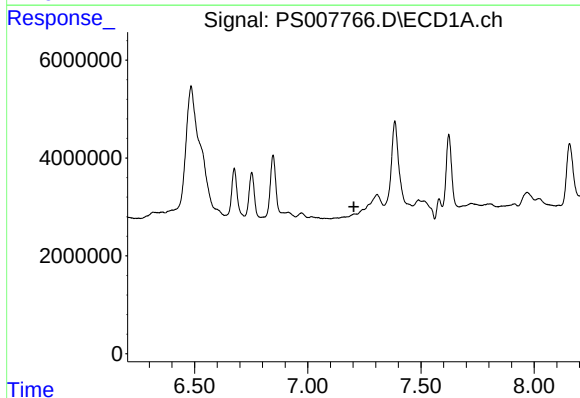


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min  
Exp R.T.: 7.203 min  
Response: 0  
Conc: N.D.

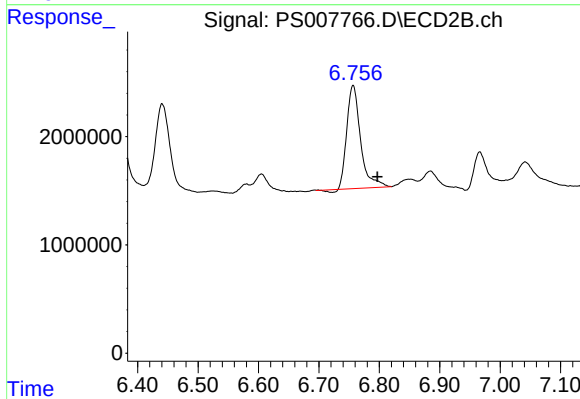

#11 2,4,5-TP (SILVEX)


R.T.: 6.757 min  
Delta R.T.: -0.040 min  
Response: 14952400  
Conc: 3.82 ng/ml

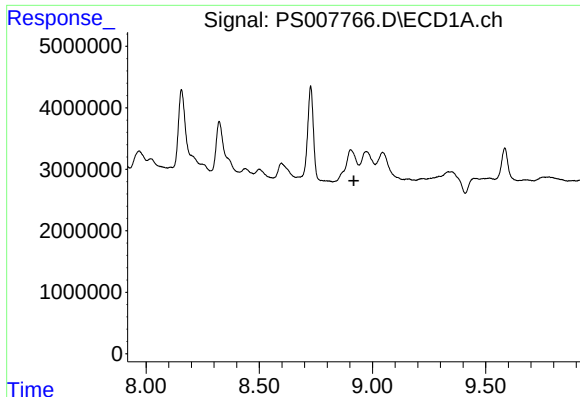

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 8.918 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

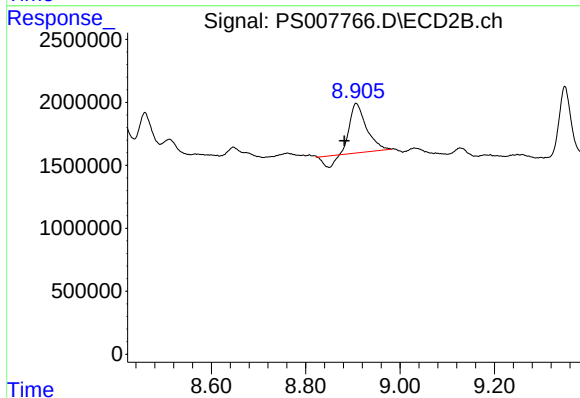


#15 Picloram

R.T.: 8.907 min  
Delta R.T.: 0.025 min  
Response: 8547972  
Conc: 1.46 ng/ml

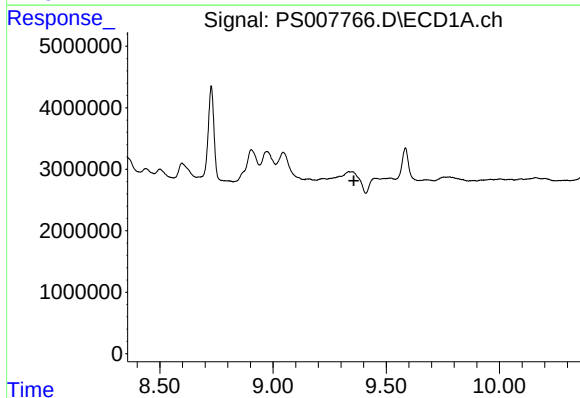

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 9.357 min  
Response: 0  
Conc: N.D.

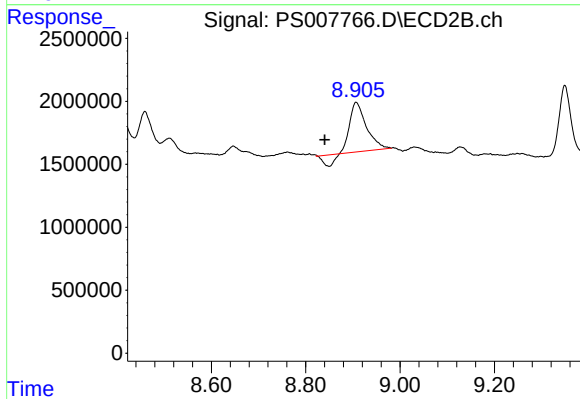

#16 DCPA

R.T.: 8.907 min  
Delta R.T.: 0.067 min  
Response: 8547972  
Conc: 1.64 ng/ml