

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
 Data File : PS024862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 08:19
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 11:47:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.764	0	831527	N.D.	1.233
Target Compounds							
1) T	Dalapon	2.511	2.559	7691905	5855002	3.193	5.557 #
2) T	3,5-DICHL...	5.697	5.915f	797765	228835	<MDL	<MDL #
3) T	4-Nitroph...	6.193	6.368	11850041	196757	9.142	<MDL #
5) T	DICAMBA	0.000	6.973	0	7107177	N.D.	2.446
6) T	MCP	6.675	7.052	9311977	308421	1.495	<MDL #
7) T	MCPA	0.000	7.182f	0	3622494	N.D.	1.175
8) T	DICHLORPROP	0.000	7.556	0	3378842	N.D.	4.625
9) T	2,4-D	7.247	7.770f	42113536	723792	15.321	<MDL #
10) T	Pentachlo...	0.000	8.259	0	567395	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.610	0	511584	N.D.	<MDL
12) T	2,4,5-T	0.000	8.987	0	679863	N.D.	<MDL
13) T	2,4-DB	0.000	9.521	0	295399	N.D.	<MDL
14) T	DINOSEB	0.000	9.806	0	469128	N.D.	<MDL
15) T	Picloram	9.679	10.762	34984884	32060954	1.967	5.277 #
16) T	DCPA	0.000	10.762	0	32060954	N.D.	6.379



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
Data File : PS024862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 08:19
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 11:47:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

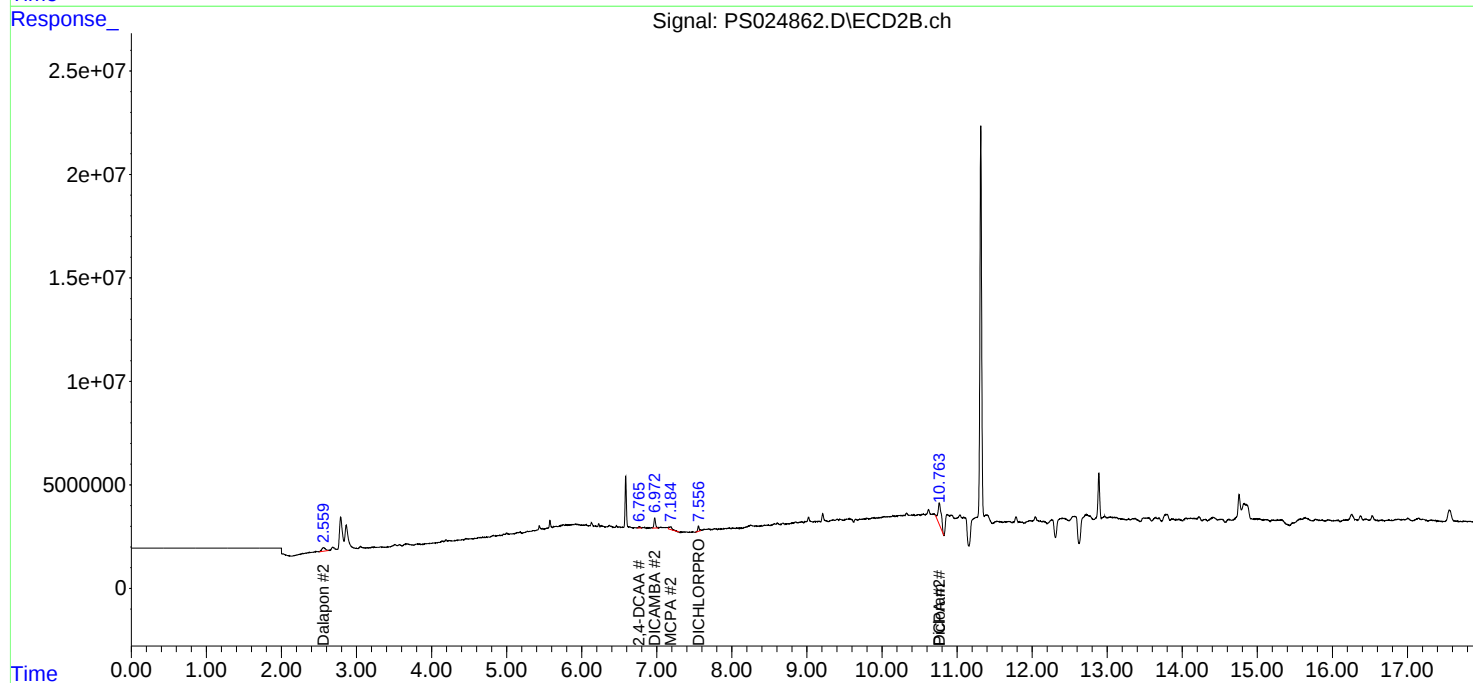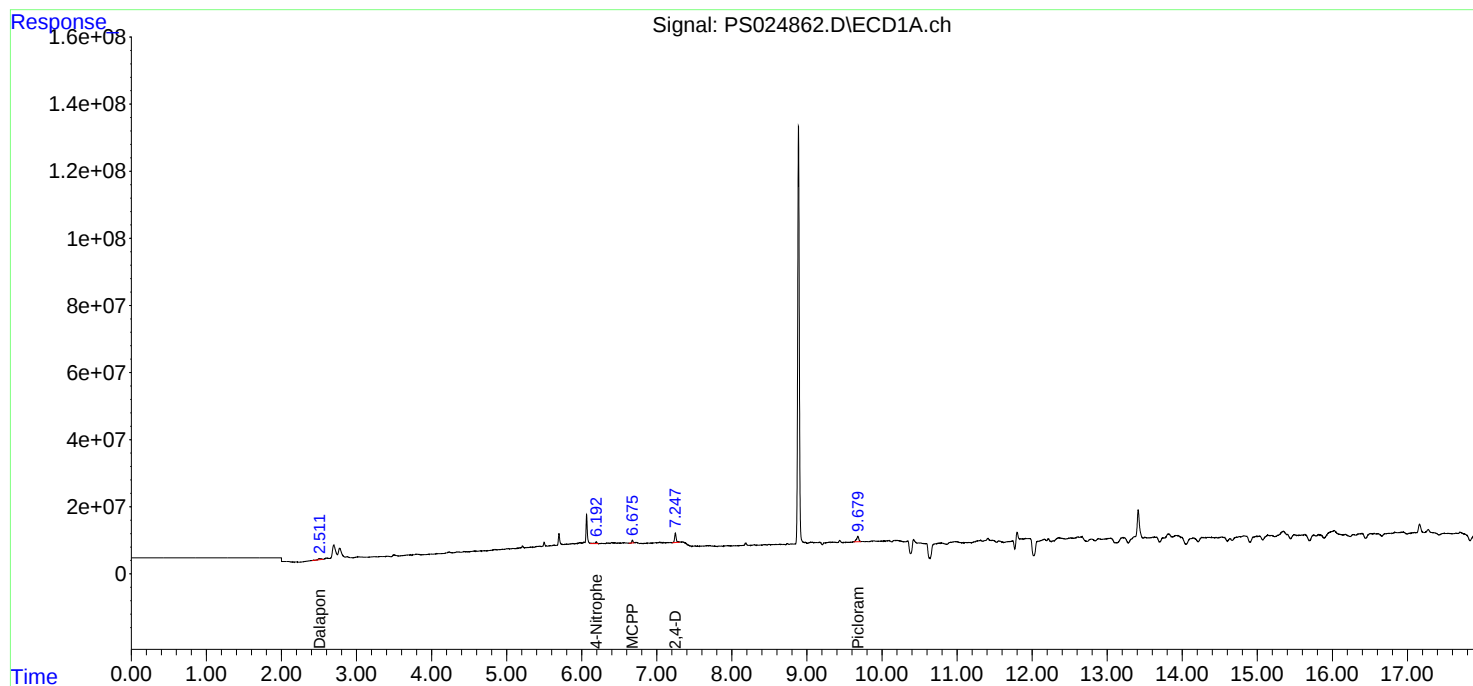


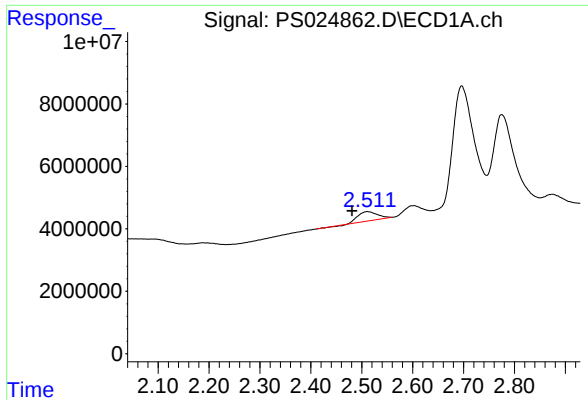

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.030 min
Response: 7691905
Conc: 3.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

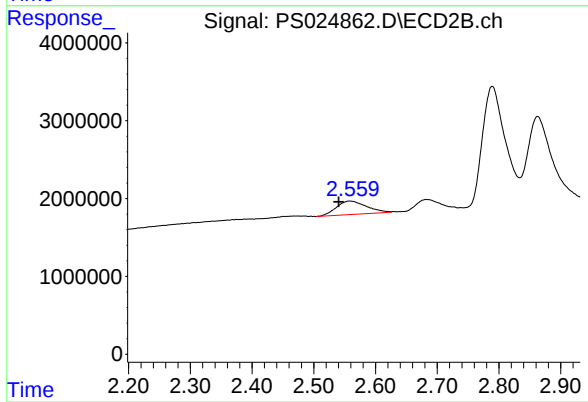


#1 Dalapon

R.T.: 2.559 min
Delta R.T.: 0.018 min
Response: 5855002
Conc: 5.56 ng/ml

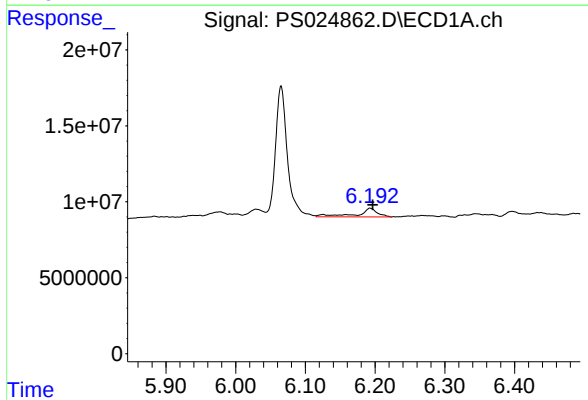


#3 4-Nitrophenol

R.T.: 6.193 min
Delta R.T.: -0.003 min
Response: 11850041
Conc: 9.14 ng/ml

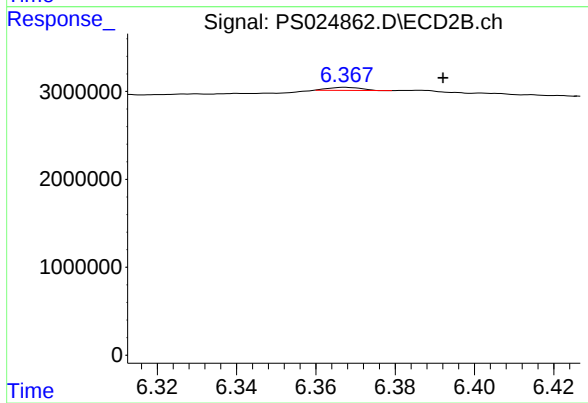

#3 4-Nitrophenol


R.T.: 6.368 min
Delta R.T.: -0.024 min
Response: 196757
Conc: N.D.

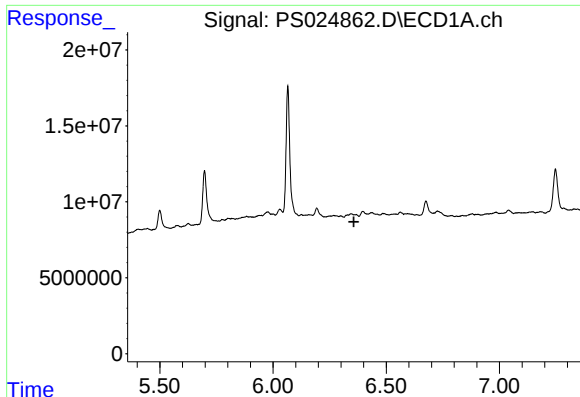

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

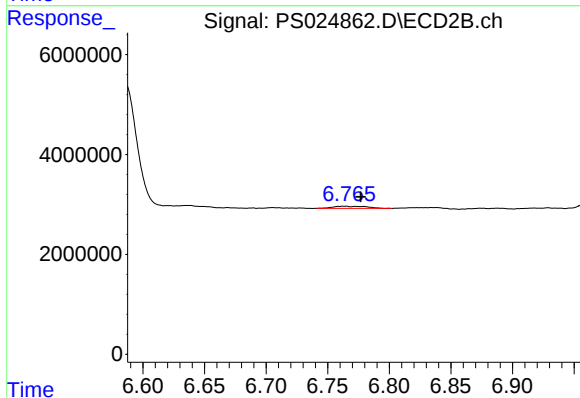


#4 2,4-DCAA

R.T.: 6.764 min
Delta R.T.: -0.012 min
Response: 831527
Conc: 1.23 ng/ml

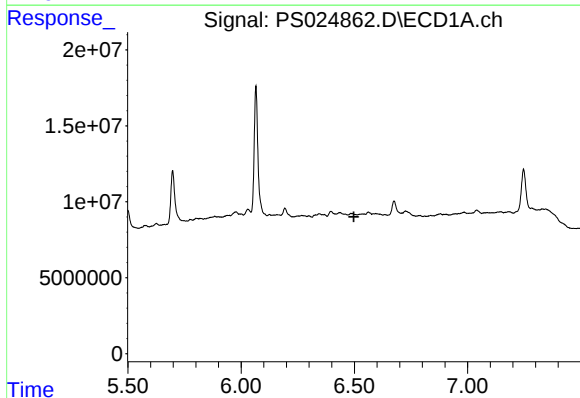


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 6.498 min
Response: 0
Conc: N.D.

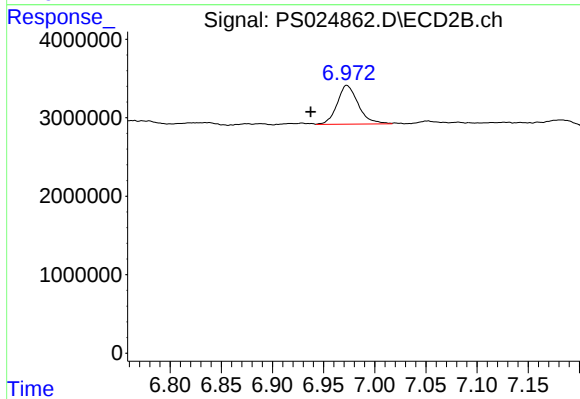

#5 DICAMBA


R.T.: 6.973 min
Delta R.T.: 0.035 min
Response: 7107177
Conc: 2.45 ng/ml

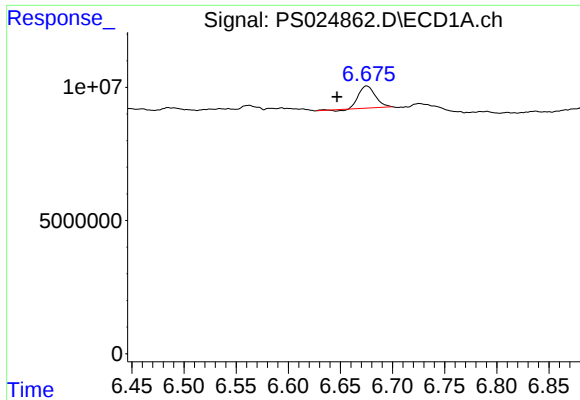

#6 MCPP


R.T.: 6.675 min
Delta R.T.: 0.029 min
Response: 9311977
Conc: 1.49 ug/ml

Instrument :
ECD_S
ClientSampleId :

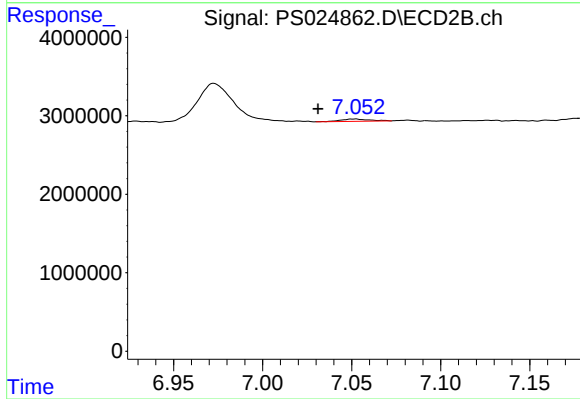


#6 MCPP

R.T.: 7.052 min
Delta R.T.: 0.021 min
Response: 308421
Conc: N.D.

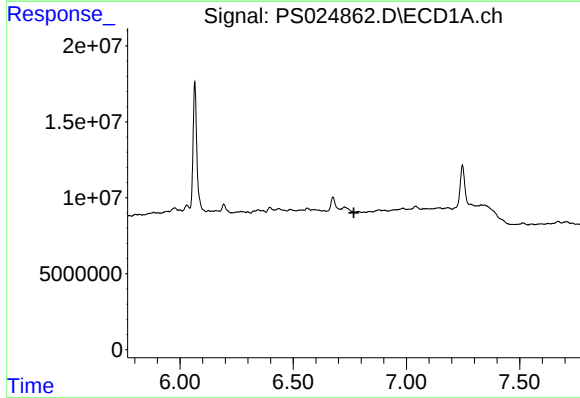


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

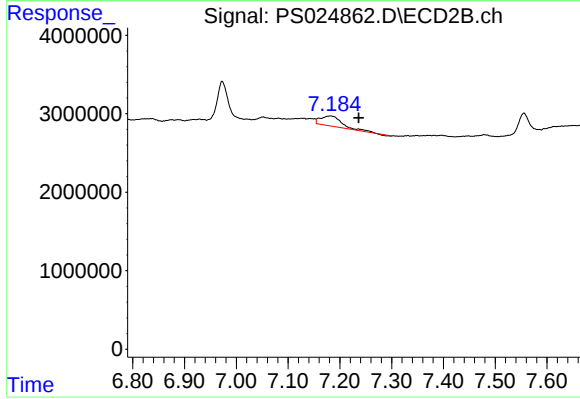

#7 MCPA


R.T.: 7.182 min
Delta R.T.: -0.055 min
Response: 3622494
Conc: 1.18 ug/ml

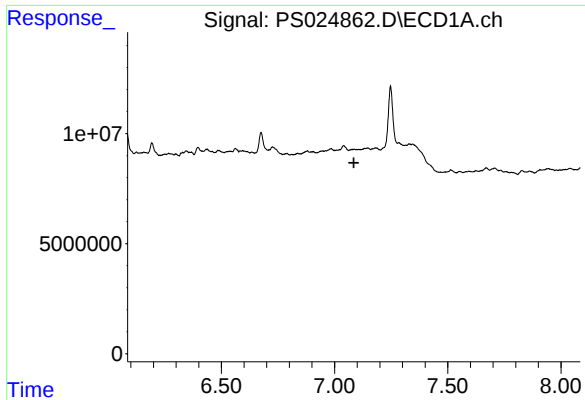

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

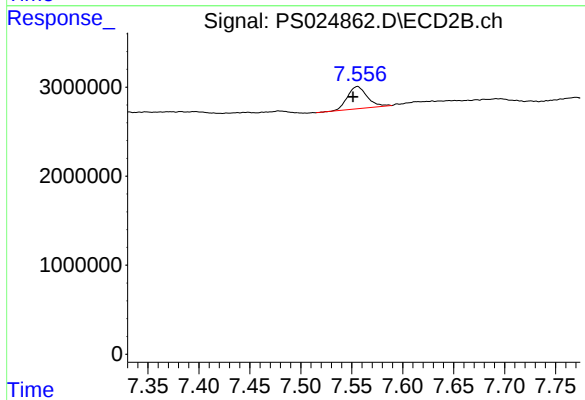


#8 DICHLORPROP

R.T.: 7.556 min
Delta R.T.: 0.004 min
Response: 3378842
Conc: 4.63 ng/ml

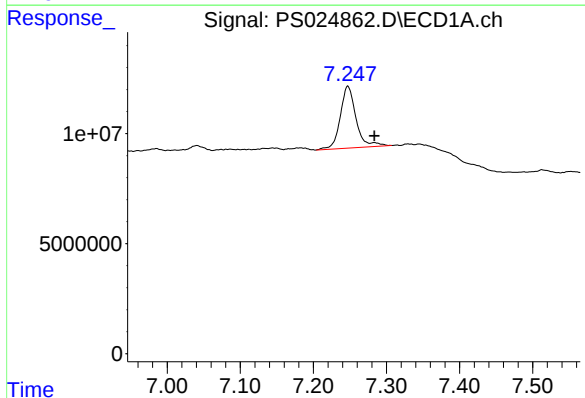


#9 2,4-D

R.T.: 7.247 min
Delta R.T.: -0.036 min
Response: 42113536
Conc: 15.32 ng/ml

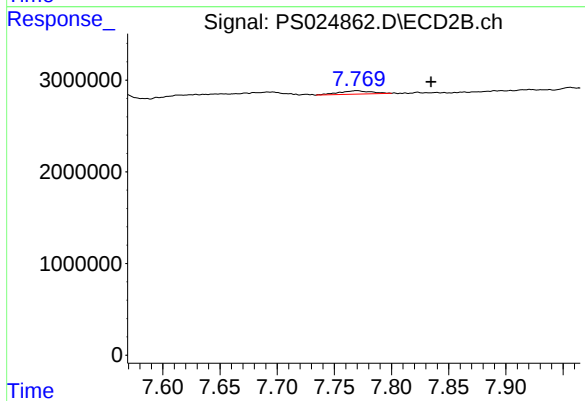

#9 2,4-D


R.T.: 7.770 min
Delta R.T.: -0.065 min
Response: 723792
Conc: N.D.

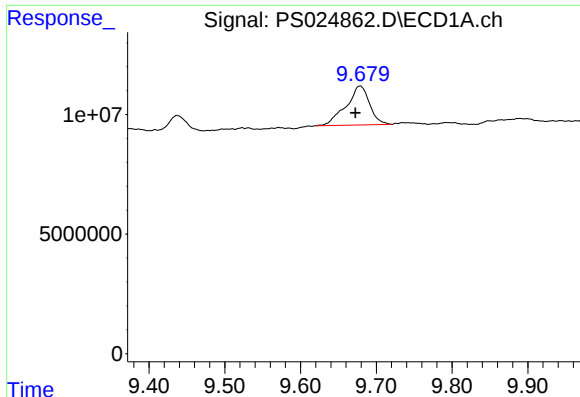

#15 Picloram


R.T.: 9.679 min
Delta R.T.: 0.006 min
Response: 34984884
Conc: 1.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

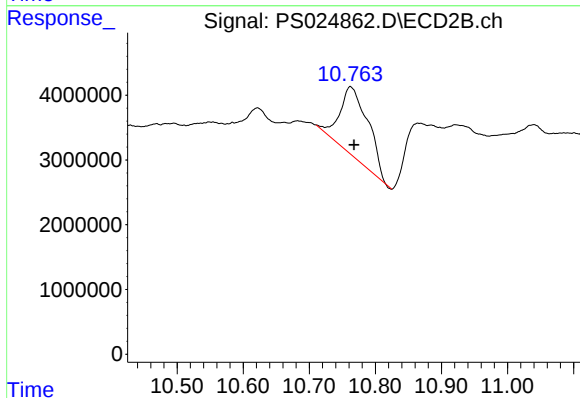


#15 Picloram

R.T.: 10.762 min
Delta R.T.: -0.005 min
Response: 32060954
Conc: 5.28 ng/ml

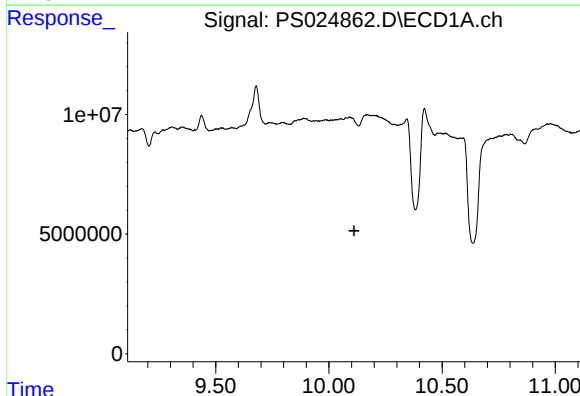

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.111 min
Response: 0
Conc: N.D.

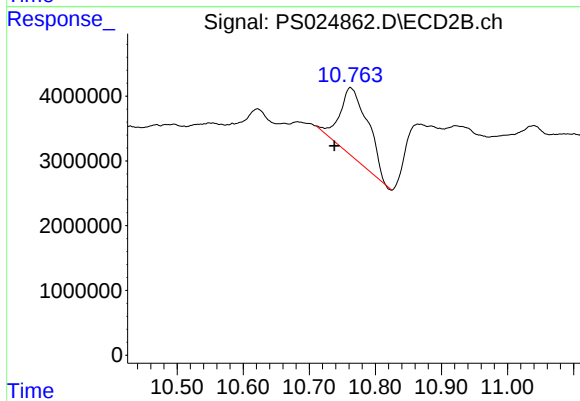

#16 DCPA

R.T.: 10.762 min
Delta R.T.: 0.024 min
Response: 32060954
Conc: 6.38 ng/ml