

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
 Data File : PS024874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 14:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 15:36:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.356	6.773	1136.6E6	372.1E6	556.735	551.571
Target Compounds							
1) T	Dalapon	0.000	2.564	0	3388883	N.D.	3.217
3) T	4-Nitroph...	6.198	6.370	7553460	784606	5.827	1.787 #
6) T	MCP	6.682	7.084f	1504601	225447	<MDL	<MDL #
7) T	MCPA	0.000	7.169f	0	25735383	N.D.	8.348
8) T	DICHLORPROP	0.000	7.563	0	3840624	N.D.	5.258
9) T	2,4-D	0.000	7.774f	0	1191605	N.D.	1.331
11) T	2,4,5-TP ...	0.000	8.613	0	72630	N.D.	<MDL
12) T	2,4,5-T	0.000	8.984	0	458017	N.D.	<MDL
13) T	2,4-DB	0.000	9.489	0	828212	N.D.	1.699
15) T	Picloram	9.683	10.767	11527045	3857255	<MDL	<MDL #
16) T	DCPA	0.000	10.767	0	3857255	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
Data File : PS024874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 14:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 15:36:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

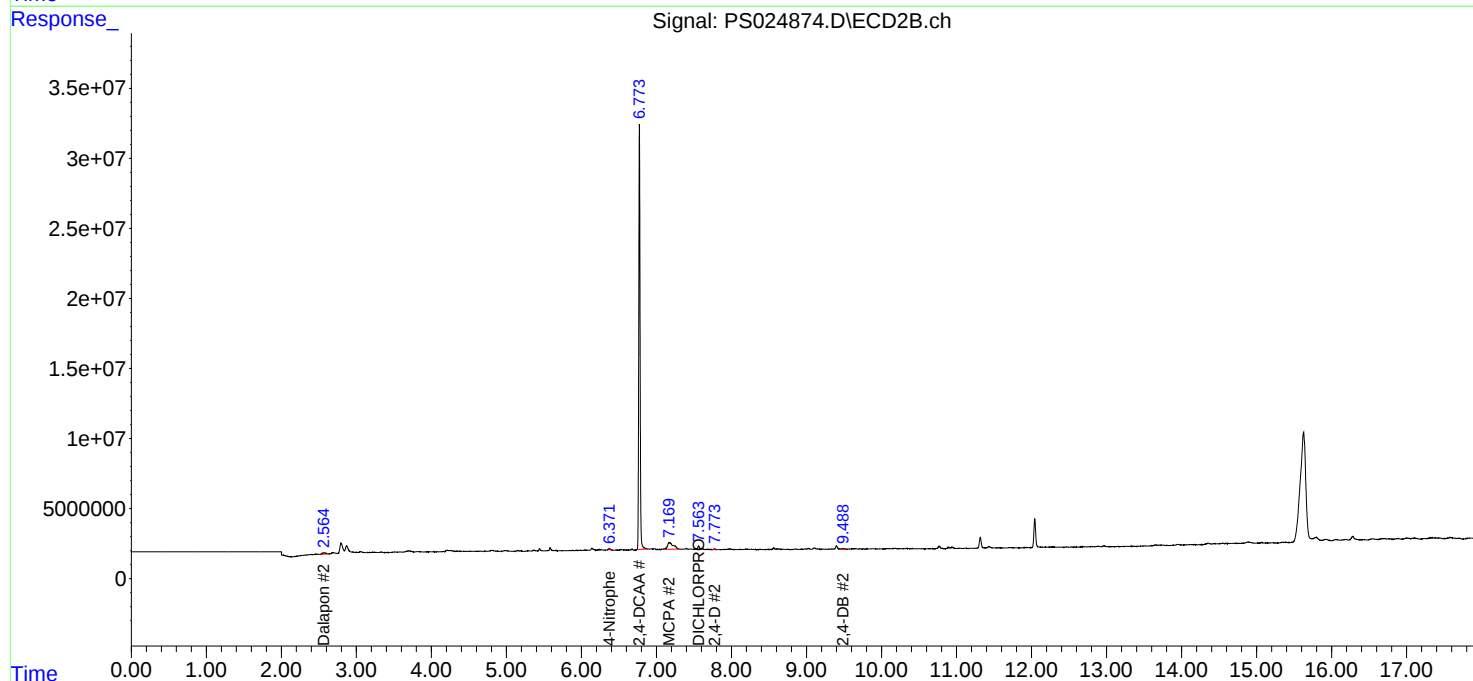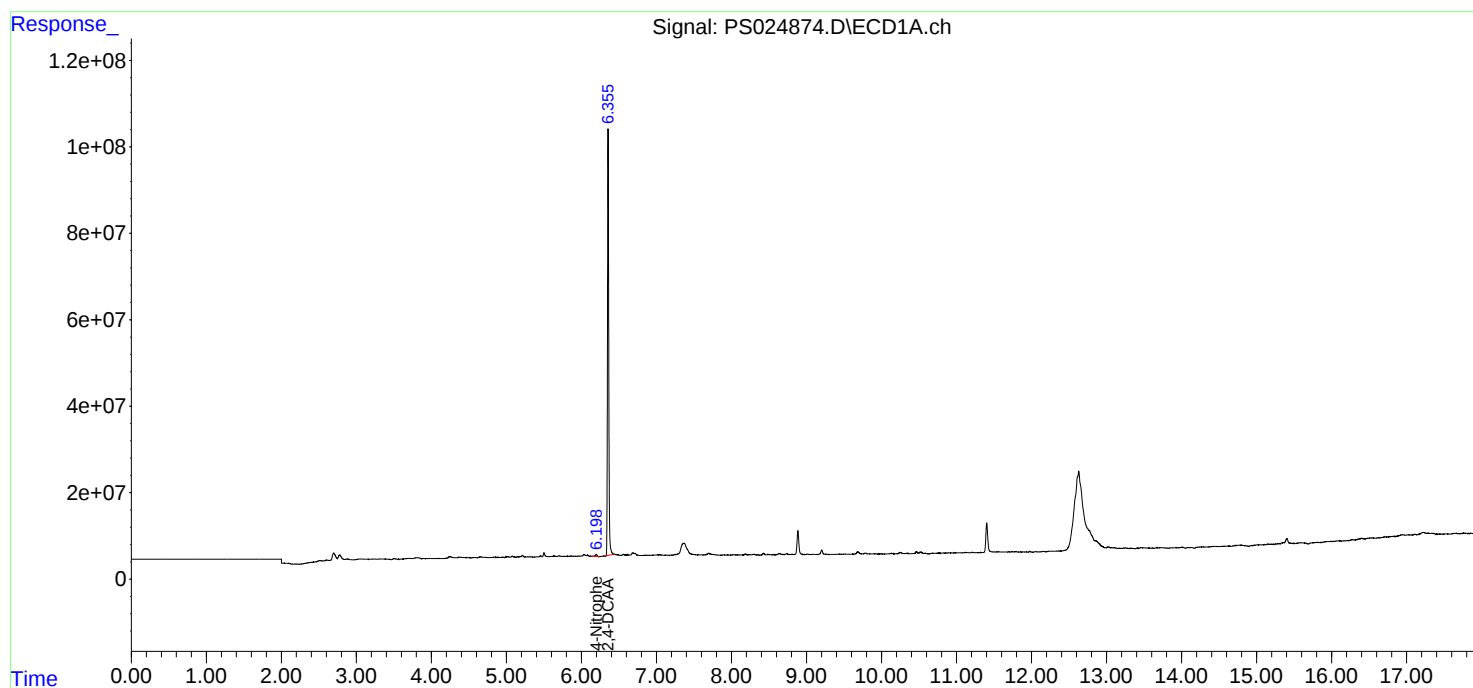


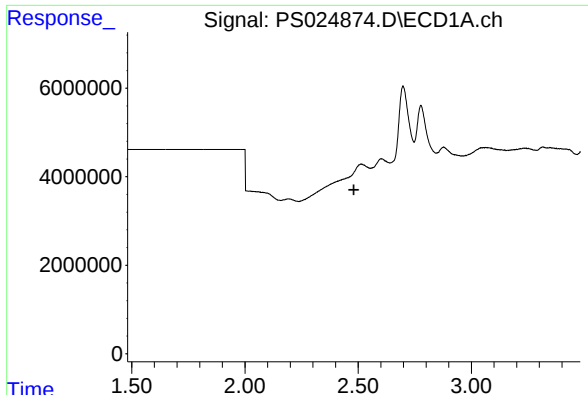

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

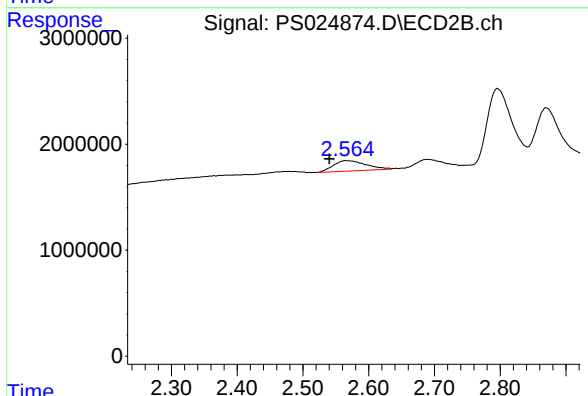


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.024 min
Response: 3388883
Conc: 3.22 ng/ml

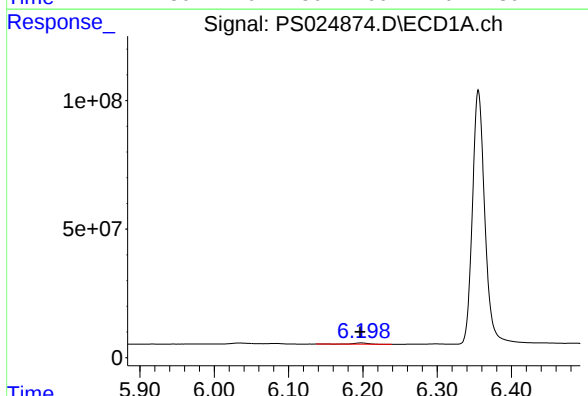


#3 4-Nitrophenol

R.T.: 6.198 min
Delta R.T.: 0.001 min
Response: 7553460
Conc: 5.83 ng/ml

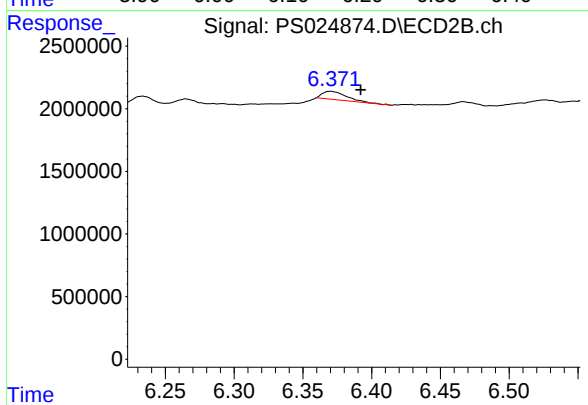

#3 4-Nitrophenol


R.T.: 6.370 min
Delta R.T.: -0.022 min
Response: 784606
Conc: 1.79 ng/ml

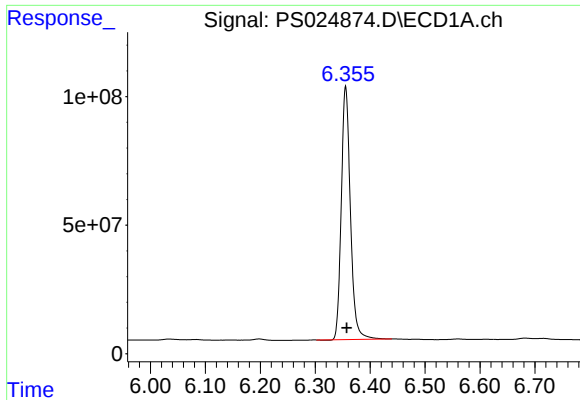

#4 2,4-DCAA


R.T.: 6.356 min
Delta R.T.: -0.002 min
Response: 1136575099
Conc: 556.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

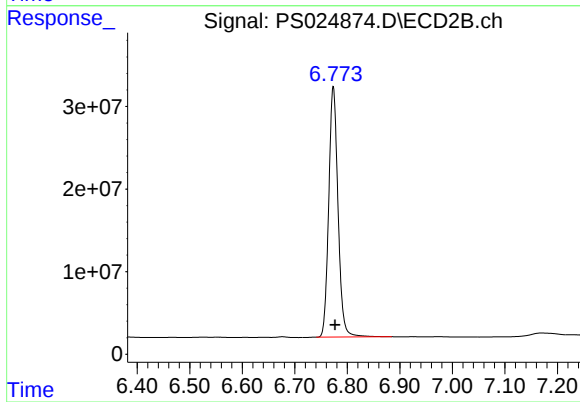


#4 2,4-DCAA

R.T.: 6.773 min
Delta R.T.: -0.003 min
Response: 372089517
Conc: 551.57 ng/ml

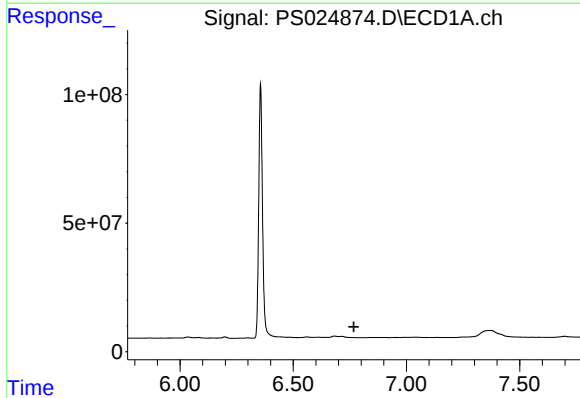


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

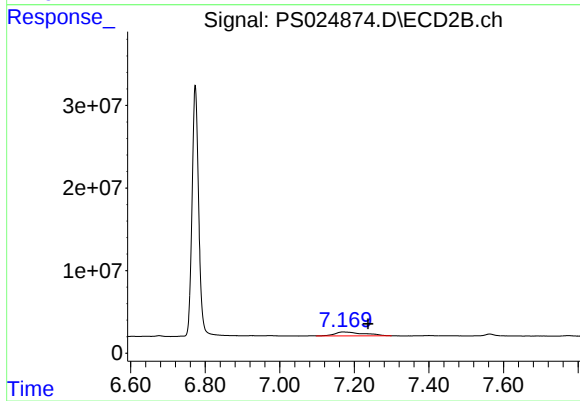

#7 MCPA


R.T.: 7.169 min
Delta R.T.: -0.067 min
Response: 25735383
Conc: 8.35 ug/ml

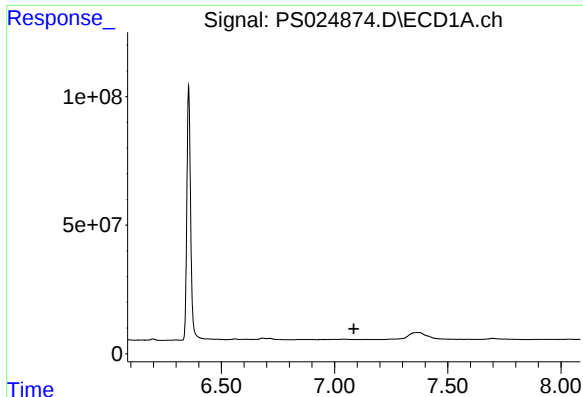

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

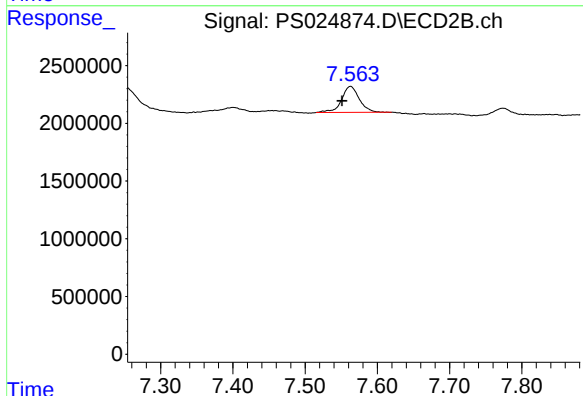


#8 DICHLORPROP

R.T.: 7.563 min
Delta R.T.: 0.012 min
Response: 3840624
Conc: 5.26 ng/ml

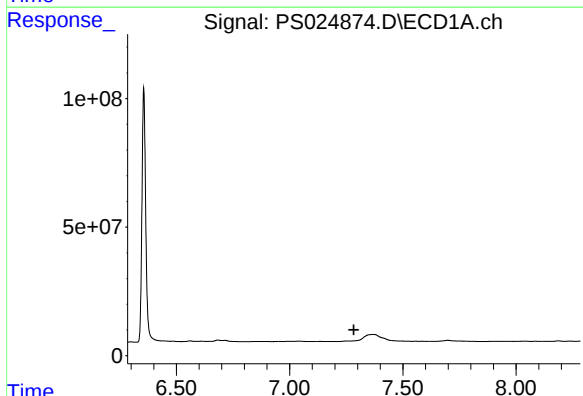


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

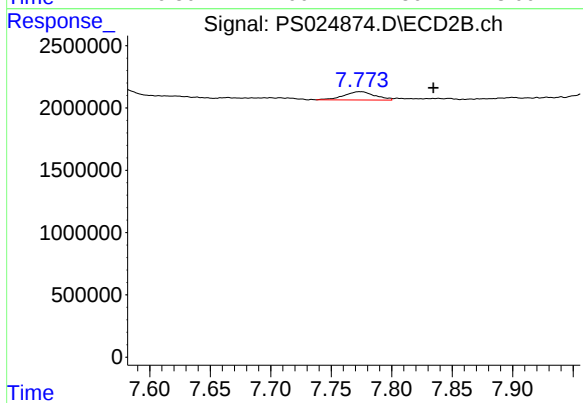

#9 2,4-D


R.T.: 7.774 min
Delta R.T.: -0.061 min
Response: 1191605
Conc: 1.33 ng/ml

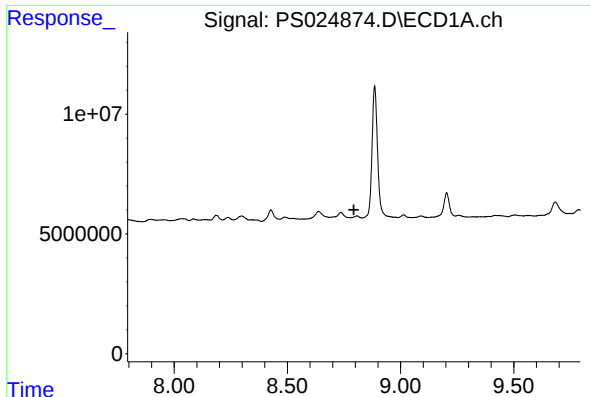

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

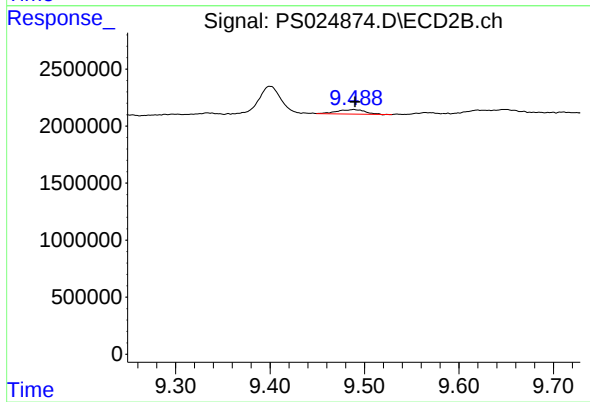

#13 2,4-DB

R.T.: 9.489 min
Delta R.T.: -0.001 min
Response: 828212
Conc: 1.70 ng/ml