

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
 Data File : PS024884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2023 18:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:16:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.356	6.773	1133.2E6	373.2E6	555.095	553.249
Target Compounds						
1) T Dalapon	0.000	2.567	0	3085849	N.D.	2.929
5) T DICAMBA	0.000	6.976	0	783762	N.D.	<MDL
6) T MCPP	6.680	7.083f	5209898	431530	<MDL	<MDL #
8) T DICHLORPROP	0.000	7.561	0	4973931	N.D.	6.809
9) T 2,4-D	0.000	7.770f	0	632963	N.D.	<MDL
11) T 2,4,5-TP ...	0.000	8.609	0	36991	N.D.	<MDL
12) T 2,4,5-T	0.000	8.984	0	608564	N.D.	<MDL
13) T 2,4-DB	0.000	9.482	0	871126	N.D.	1.787
15) T Picloram	0.000	10.766	0	2871821	N.D.	<MDL
16) T DCPA	0.000	10.734	0	449515	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
Data File : PS024884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2023 18:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:16:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

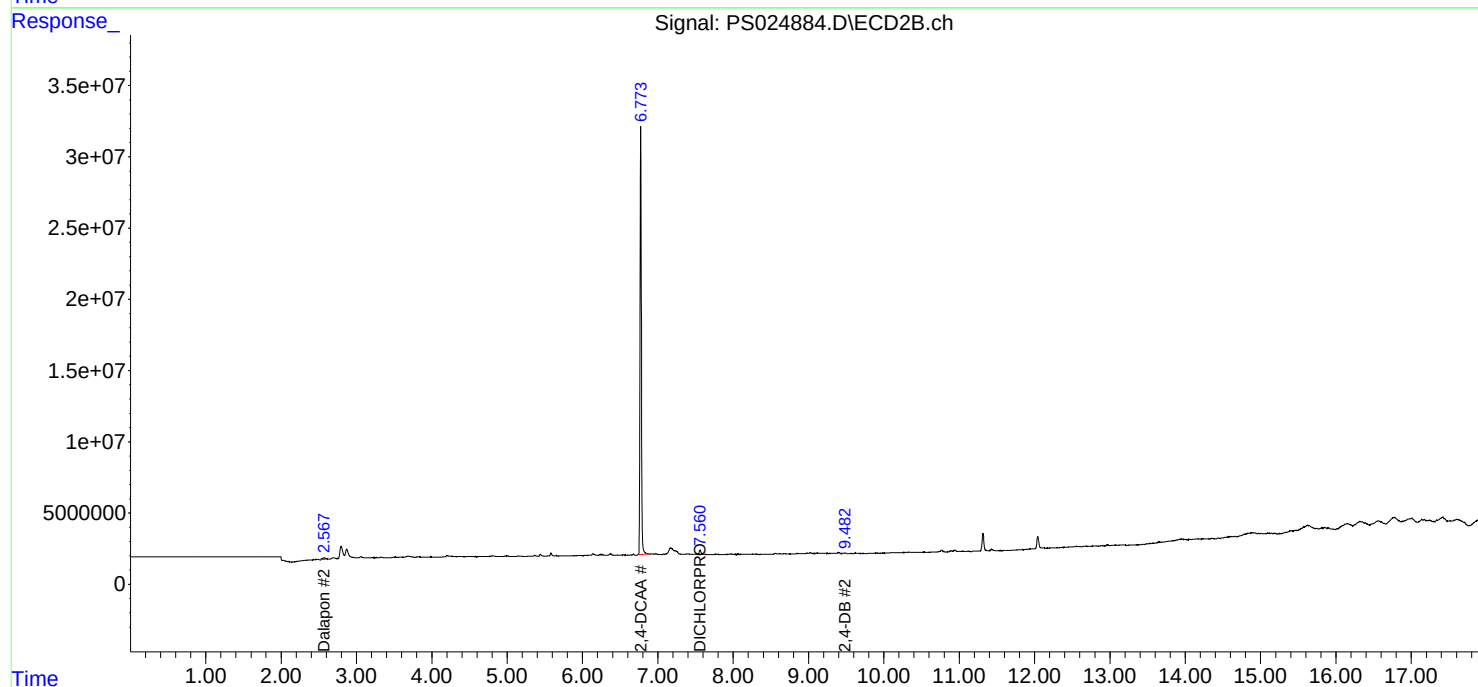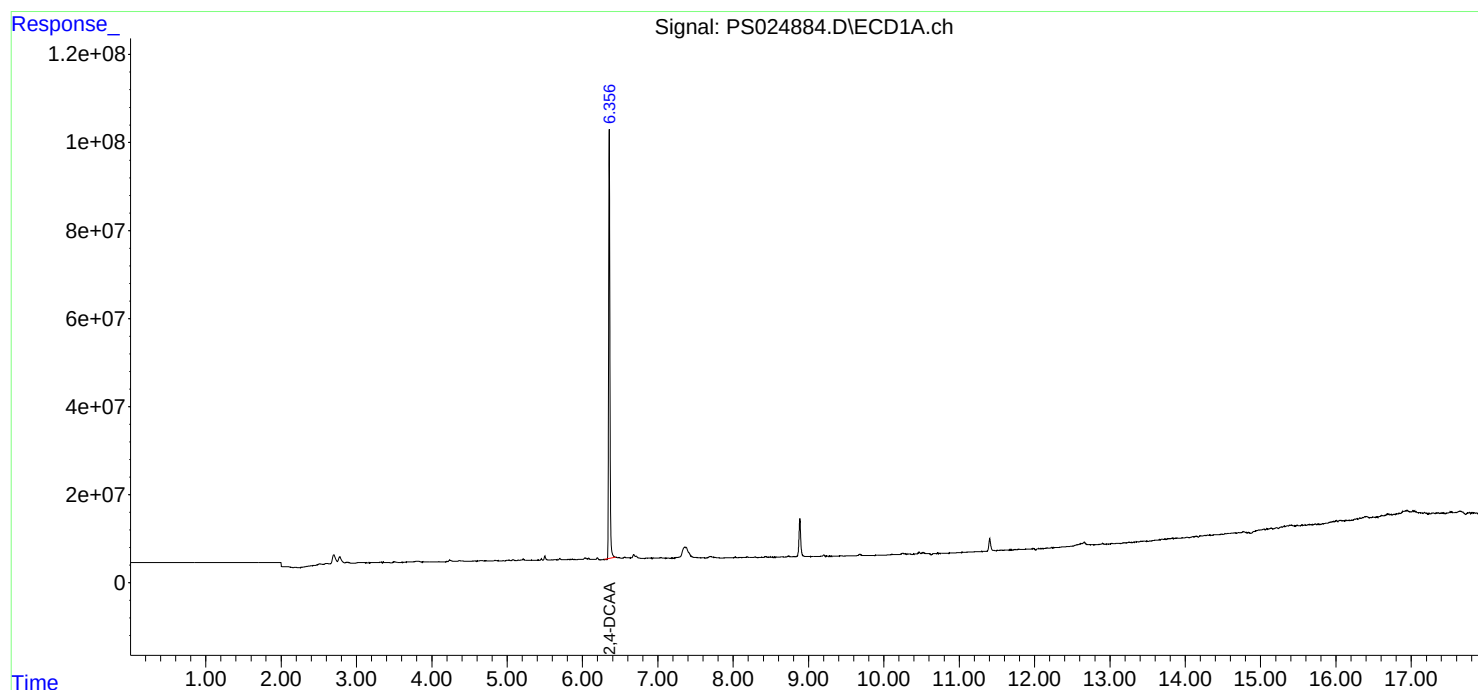


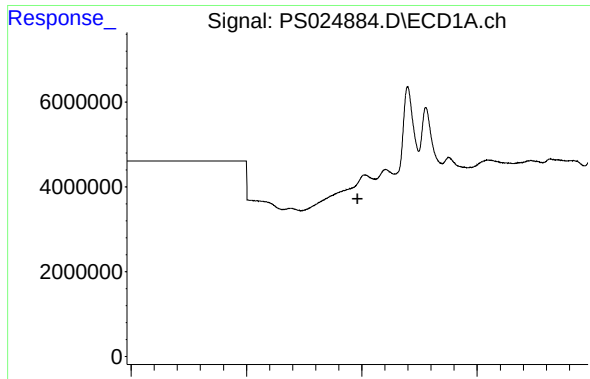

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

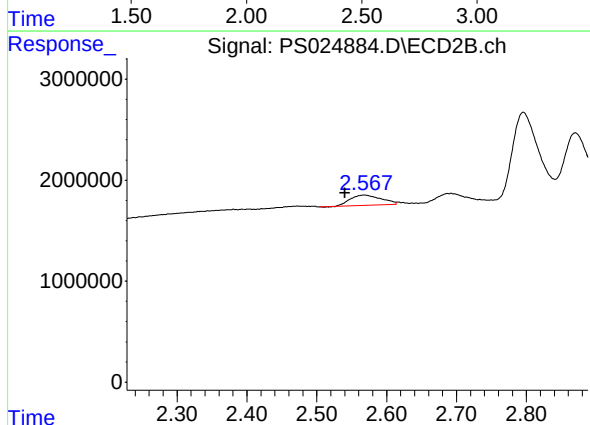


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.026 min
Response: 3085849
Conc: 2.93 ng/ml

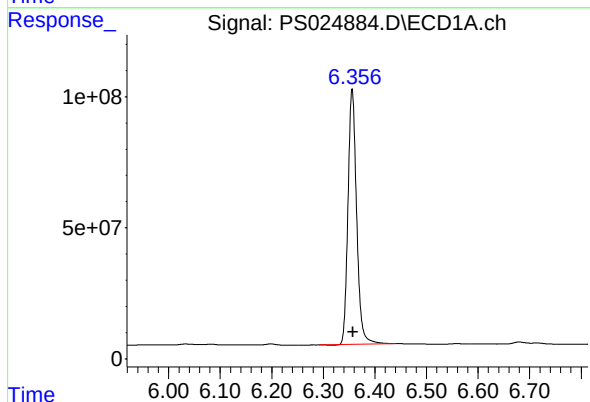


#4 2,4-DCAA

R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 1133228846
Conc: 555.10 ng/ml

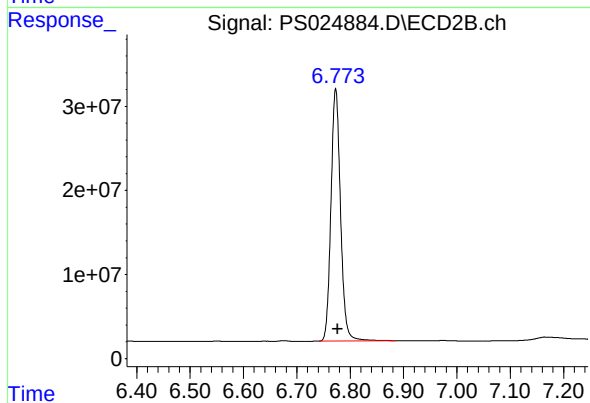

#4 2,4-DCAA


R.T.: 6.773 min
Delta R.T.: -0.004 min
Response: 373220899
Conc: 553.25 ng/ml

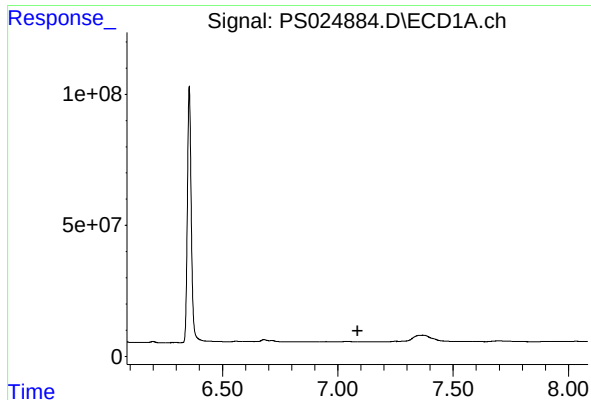

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

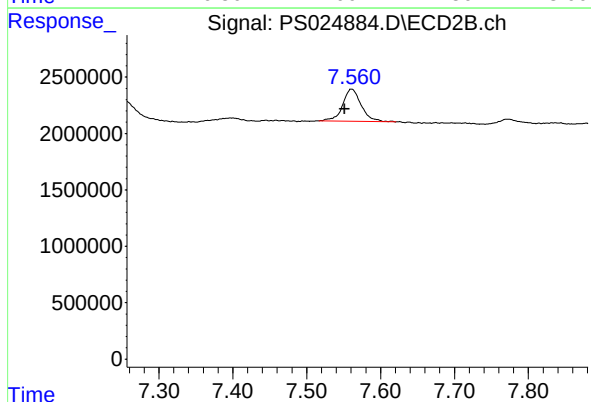


#8 DICHLORPROP

R.T.: 7.561 min
Delta R.T.: 0.009 min
Response: 4973931
Conc: 6.81 ng/ml

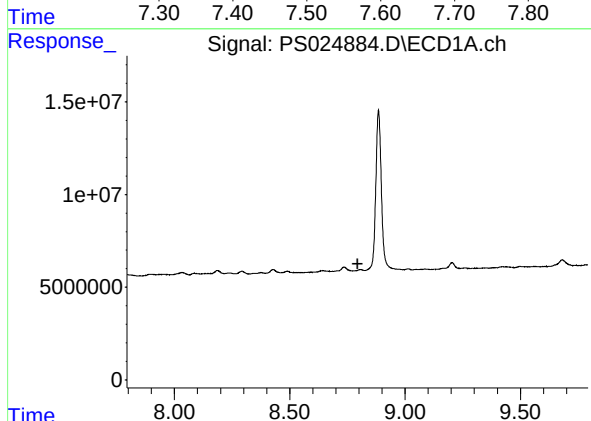

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

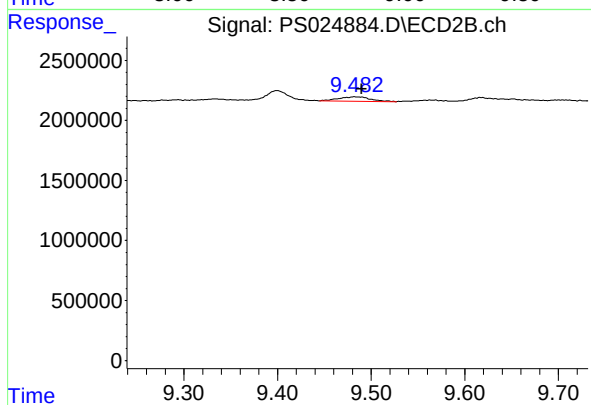

#13 2,4-DB

R.T.: 9.482 min
Delta R.T.: -0.008 min
Response: 871126
Conc: 1.79 ng/ml