

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
 Data File : PS024897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 00:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 04:15:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.355	6.773	1152.1E6	374.4E6	564.343	554.964
Target Compounds						
1) T Dalapon	0.000	2.566	0	3989870	N.D.	3.787
3) T 4-Nitroph...	0.000	6.369	0	606440	N.D.	1.381
6) T MCPP	6.677	7.081f	5174165	566018	<MDL	<MDL #
8) T DICHLORPROP	0.000	7.560	0	5595660	N.D.	7.660
9) T 2,4-D	0.000	7.770f	0	418654	N.D.	<MDL
12) T 2,4,5-T	0.000	8.985	0	328930	N.D.	<MDL
13) T 2,4-DB	0.000	9.489	0	649764	N.D.	1.333
14) T DINOSEB	9.784f	9.884f	8274469	512994	<MDL	<MDL #
15) T Picloram	9.677	10.764	24707667	5966123	1.389	<MDL #
16) T DCPA	0.000	10.764	0	5966123	N.D.	1.187



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112023\
Data File : PS024897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 00:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 04:15:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

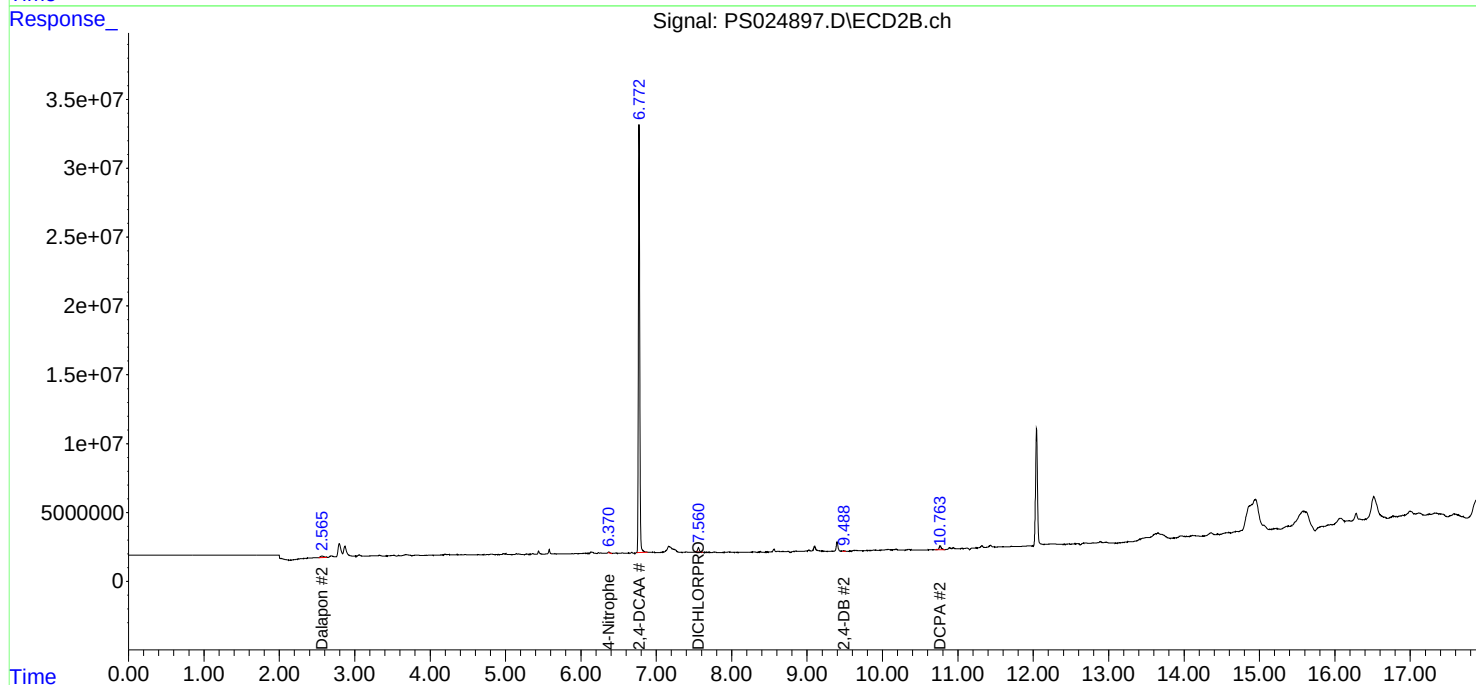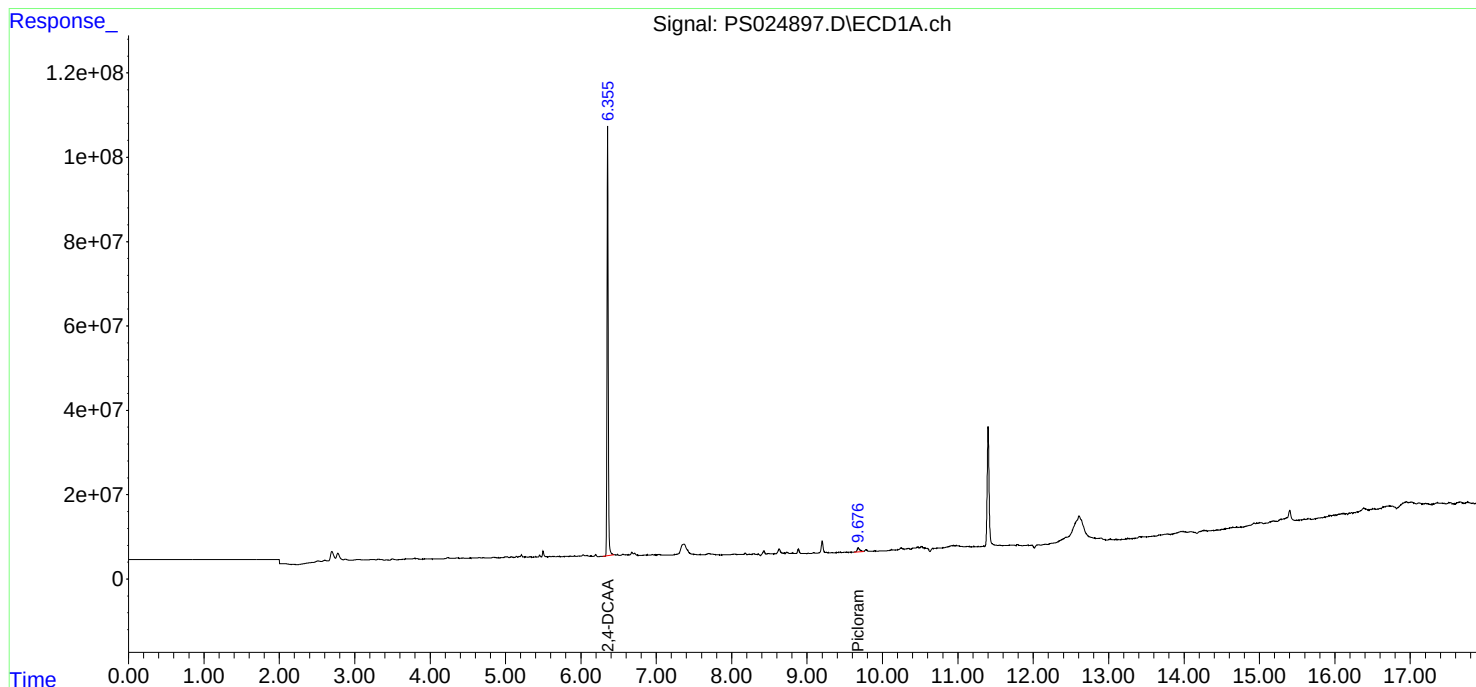


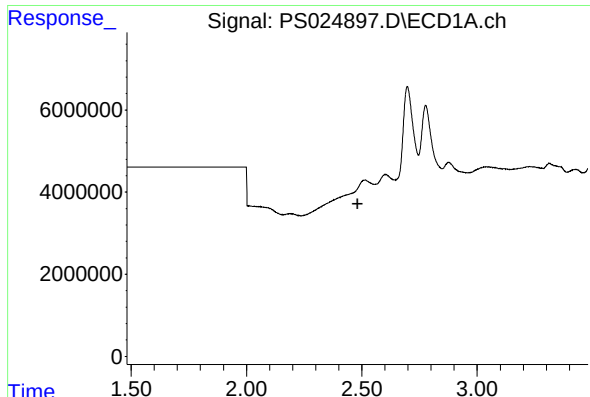

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

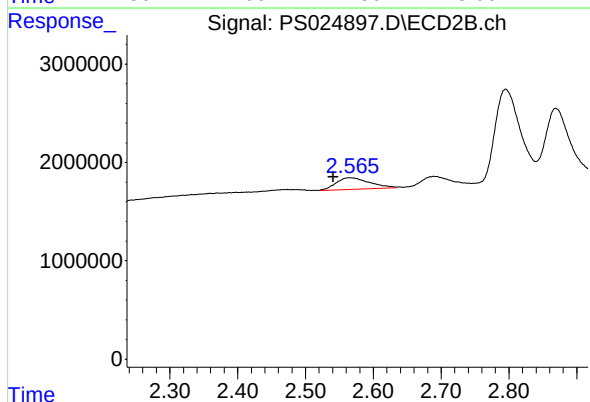


#1 Dalapon

R.T.: 2.566 min
Delta R.T.: 0.025 min
Response: 3989870
Conc: 3.79 ng/ml

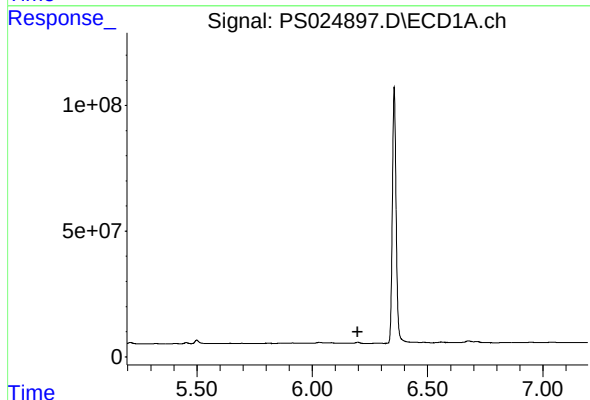


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

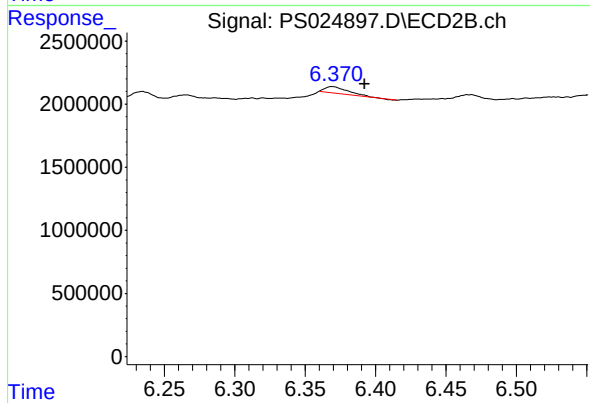

#3 4-Nitrophenol


R.T.: 6.369 min
Delta R.T.: -0.023 min
Response: 606440
Conc: 1.38 ng/ml

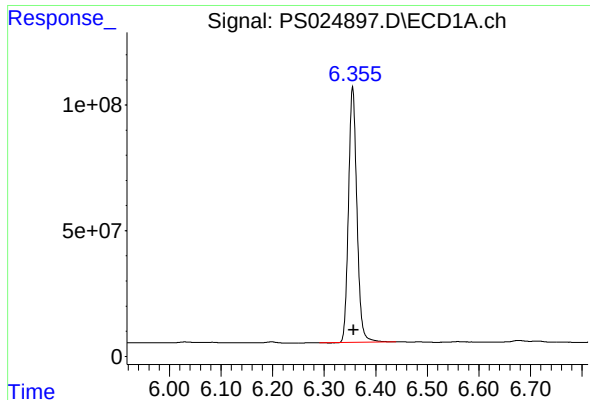

#4 2,4-DCAA


R.T.: 6.355 min
Delta R.T.: -0.002 min
Response: 1152108381
Conc: 564.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

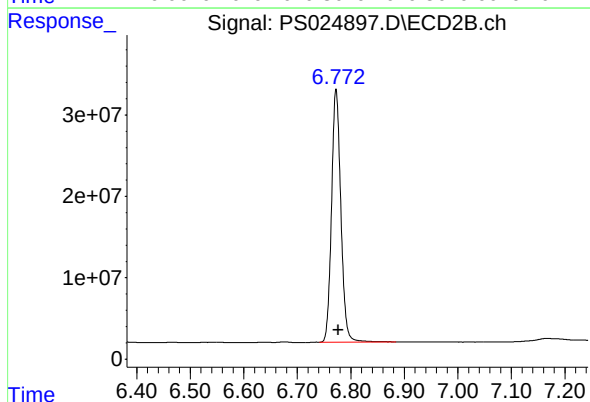


#4 2,4-DCAA

R.T.: 6.773 min
Delta R.T.: -0.004 min
Response: 374378255
Conc: 554.96 ng/ml

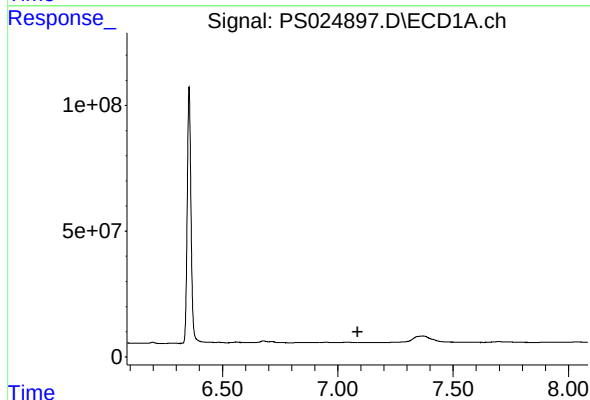


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

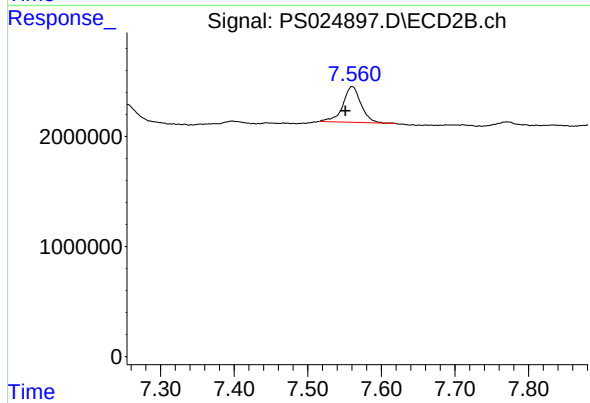

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.009 min
Response: 5595660
Conc: 7.66 ng/ml

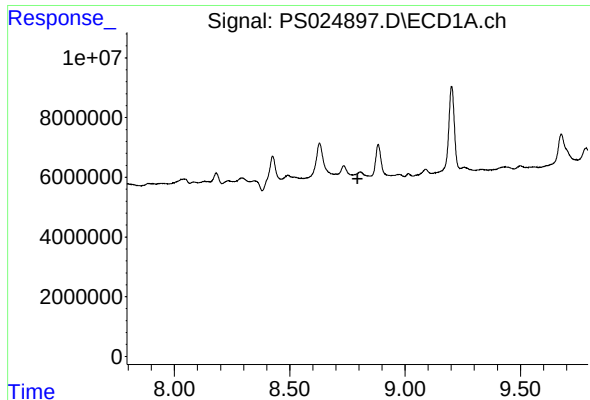

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

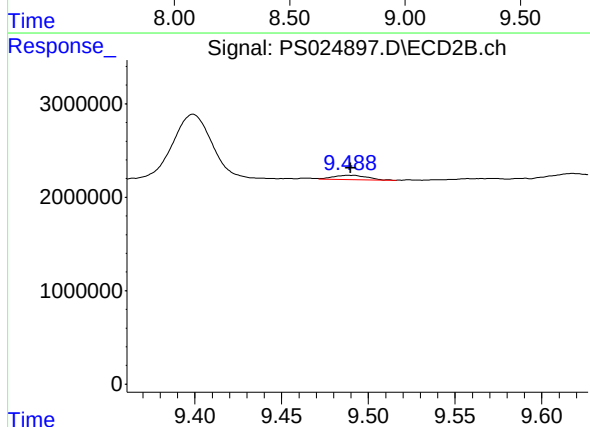


#13 2,4-DB

R.T.: 9.489 min
Delta R.T.: 0.000 min
Response: 649764
Conc: 1.33 ng/ml

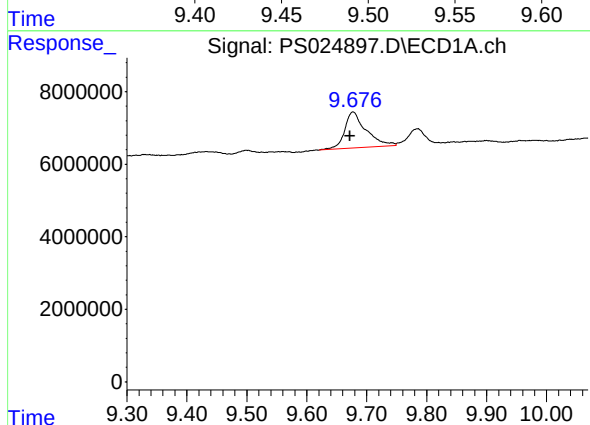


#15 Picloram

R.T.: 9.677 min
Delta R.T.: 0.005 min
Response: 24707667
Conc: 1.39 ng/ml

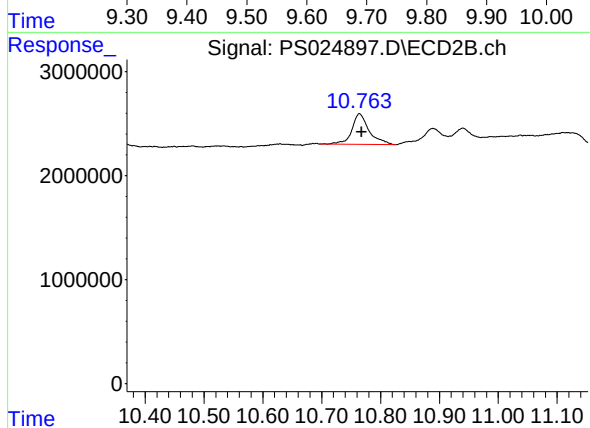

#15 Picloram


R.T.: 10.764 min
Delta R.T.: -0.003 min
Response: 5966123
Conc: N.D.

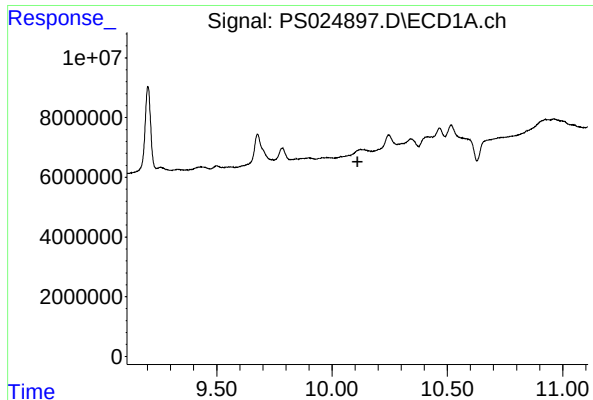

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

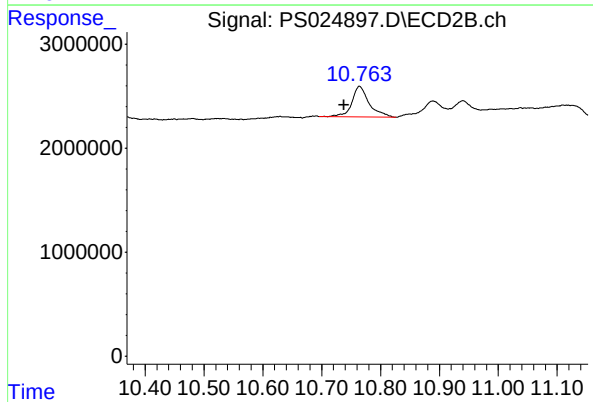

#16 DCPA

R.T.: 10.764 min
Delta R.T.: 0.026 min
Response: 5966123
Conc: 1.19 ng/ml