

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 13:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 23:56:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.733	1443.2E6	645.3E6	564.672	499.308
Target Compounds							
3) T	4-Nitroph...	7.028	0.000	4727032	0	2.783	N.D. #
7) T	MCPA	7.782	8.259f	215482	6801941	<MDL	1.098 #
8) T	DICHLORPROP	8.098f	8.700f	304896	2782120	<MDL	1.905 #
14) T	DINOSEB	11.311	0.000	830796	0	<MDL	N.D. #
15) T	Picloram	11.131	12.349	22441213	15342927	<MDL	1.355 #
16) T	DCPA	11.602	12.349f	1216333	15342927	<MDL	1.582 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 13:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 23:56:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

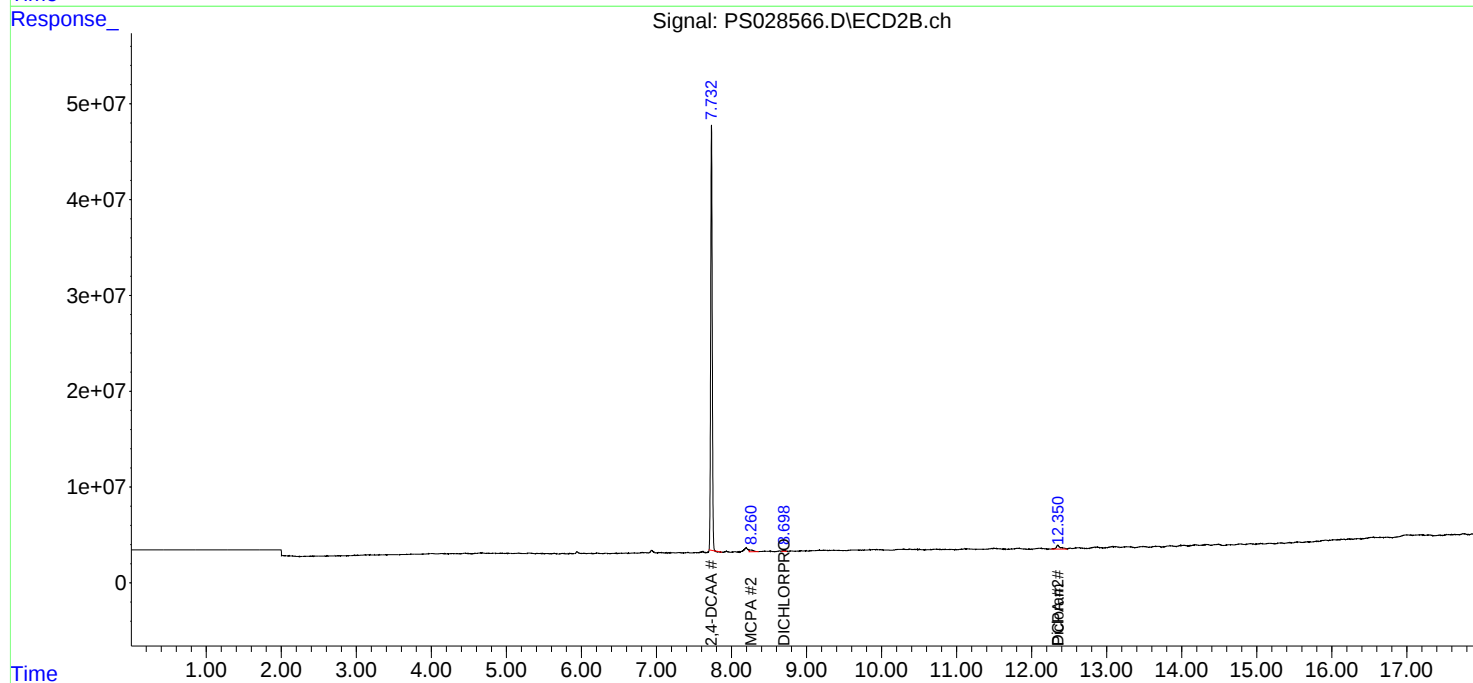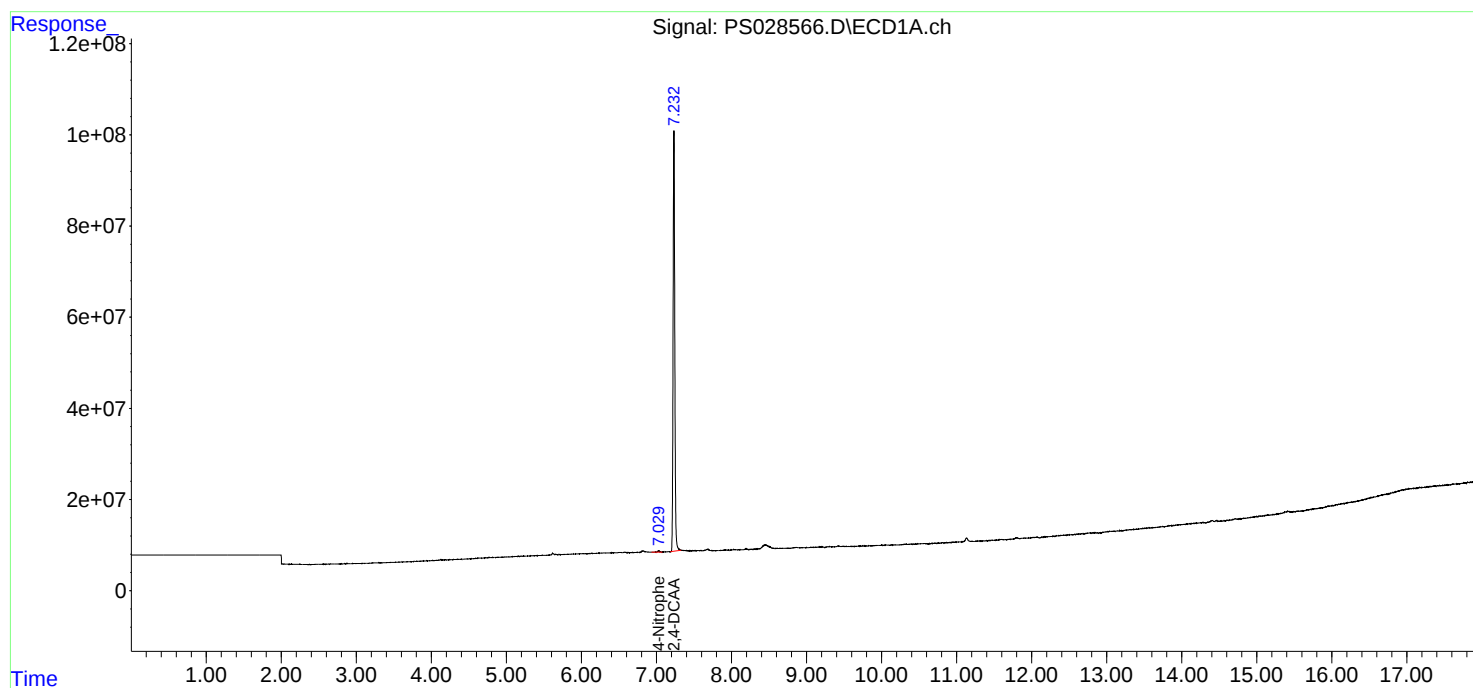


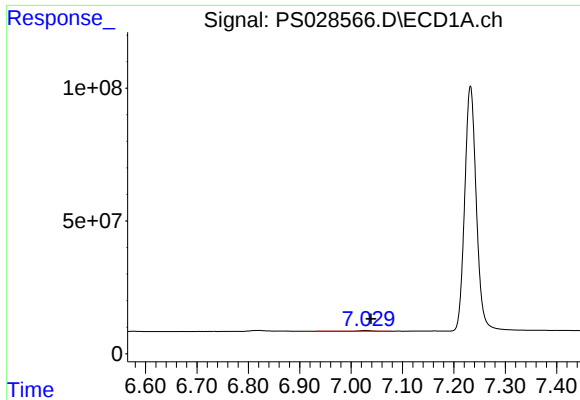

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.011 min
Response: 4727032
Conc: 2.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

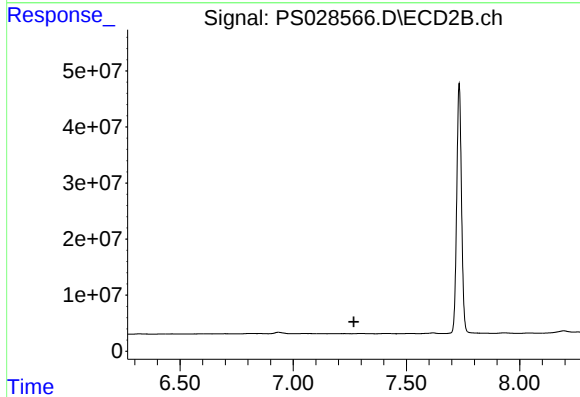


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

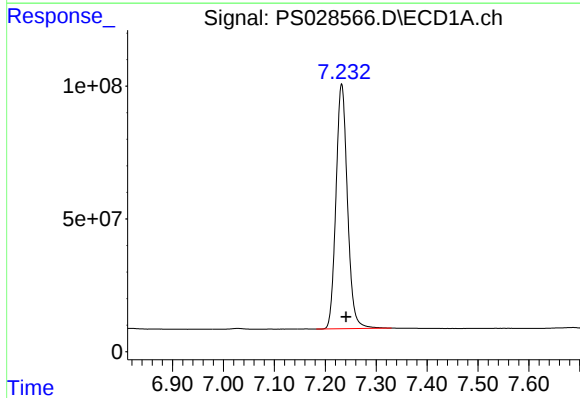


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.009 min
Response: 1443235514
Conc: 564.67 ng/ml

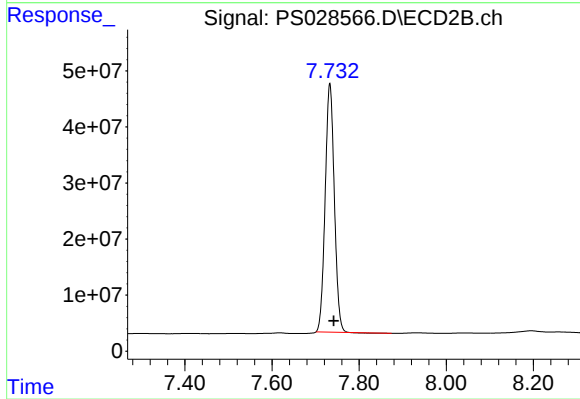

#4 2,4-DCAA


R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 645258131
Conc: 499.31 ng/ml

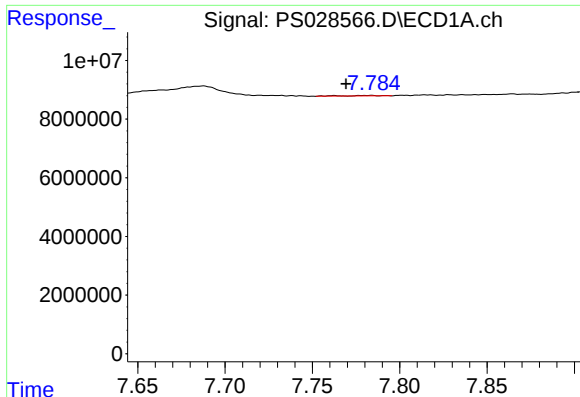

#7 MCPA


R.T.: 7.782 min
Delta R.T.: 0.012 min
Response: 215482
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

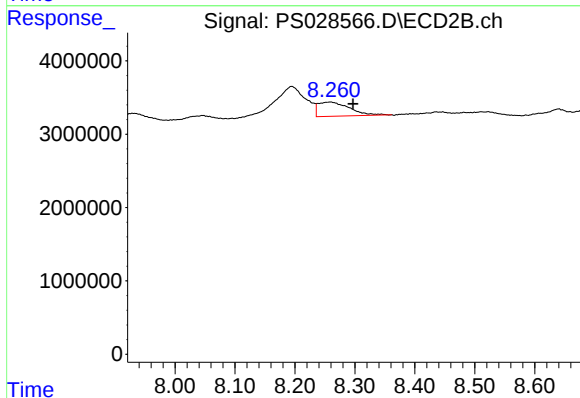


#7 MCPA

R.T.: 8.259 min
Delta R.T.: -0.038 min
Response: 6801941
Conc: 1.10 ug/ml

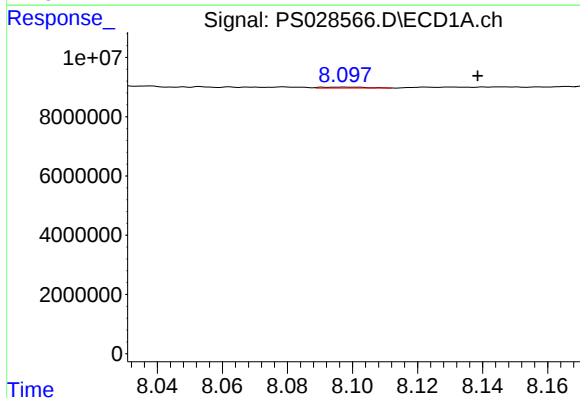


#8 DICHLORPROP

R.T.: 8.098 min
Delta R.T.: -0.041 min
Response: 304896
Conc: N.D.

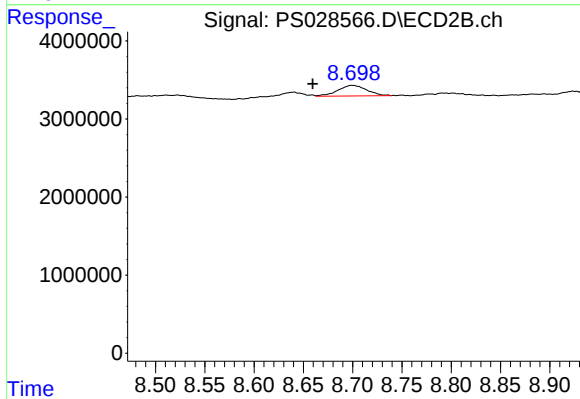

#8 DICHLORPROP


R.T.: 8.700 min
Delta R.T.: 0.040 min
Response: 2782120
Conc: 1.90 ng/ml

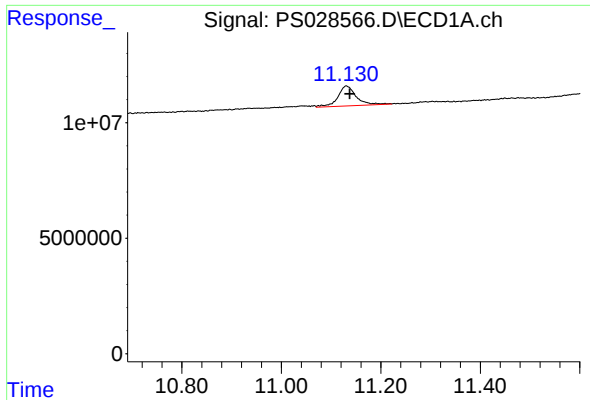

#15 Picloram


R.T.: 11.131 min
Delta R.T.: -0.007 min
Response: 22441213
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

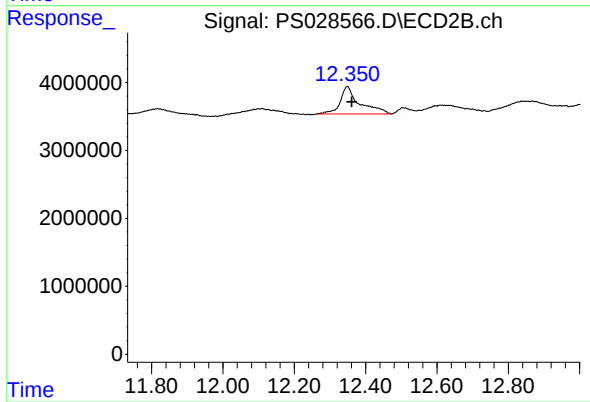


#15 Picloram

R.T.: 12.349 min
Delta R.T.: -0.012 min
Response: 15342927
Conc: 1.36 ng/ml

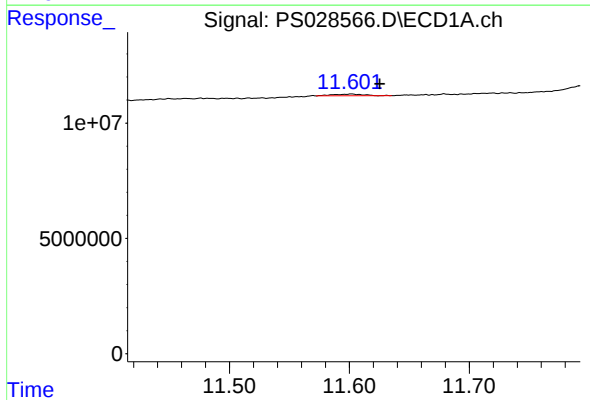

#16 DCPA

R.T.: 11.602 min
Delta R.T.: -0.024 min
Response: 1216333
Conc: N.D.

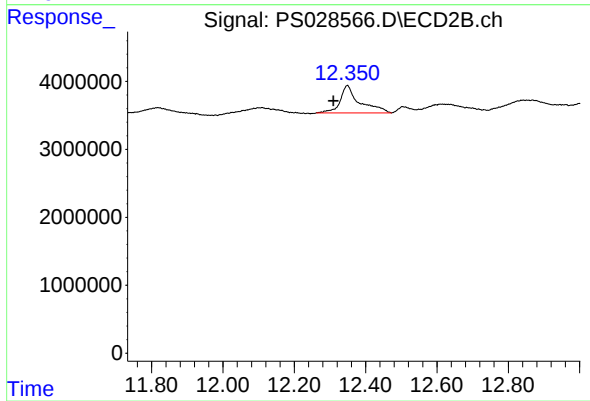

#16 DCPA

R.T.: 12.349 min
Delta R.T.: 0.040 min
Response: 15342927
Conc: 1.58 ng/ml