

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 16:52
 Operator : AR\AJ
 Sample : PB165132BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 23:57:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	7.733	1534.3E6	677.0E6	600.283	523.875
Target Compounds							
1) T	Dalapon	2.609f	2.690	70625658	147.1E6	21.023	60.769 #
2) T	3,5-DICHL...	6.458f	6.716	1389120	15639345	<MDL	8.093 #
3) T	4-Nitroph...	7.024	7.261	10019177	1439591	5.899	1.667 #
5) T	DICAMBA	0.000	7.925	0	12556441	N.D.	2.201
6) T	MCP	7.655f	8.027	201.7E6	3840658	28.669	<MDL #
7) T	MCPA	7.748	8.256f	5311686	16495273	<MDL	2.663 #
8) T	DICHLORPROP	8.155	8.697f	853942	98758807	<MDL	67.617 #
9) T	2,4-D	8.379	0.000	6446716	0	2.017	N.D. #
10) T	Pentachlo...	8.659	9.507	9767586	4213301	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.937f	0	4161528	N.D.	<MDL
12) T	2,4,5-T	9.535	10.280f	32470414	43279986	1.827	5.163 #
13) T	2,4-DB	10.108	0.000	18348021	0	6.732	N.D. #
14) T	DINOSEB	11.381f	11.254	12267983	21784398	<MDL	3.940 #
15) T	Picloram	11.126	12.346	134.1E6	36270051	4.763	3.204 #
16) T	DCPA	0.000	12.346f	0	36270051	N.D.	3.740



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 16:52
Operator : AR\AJ
Sample : PB165132BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 23:57:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

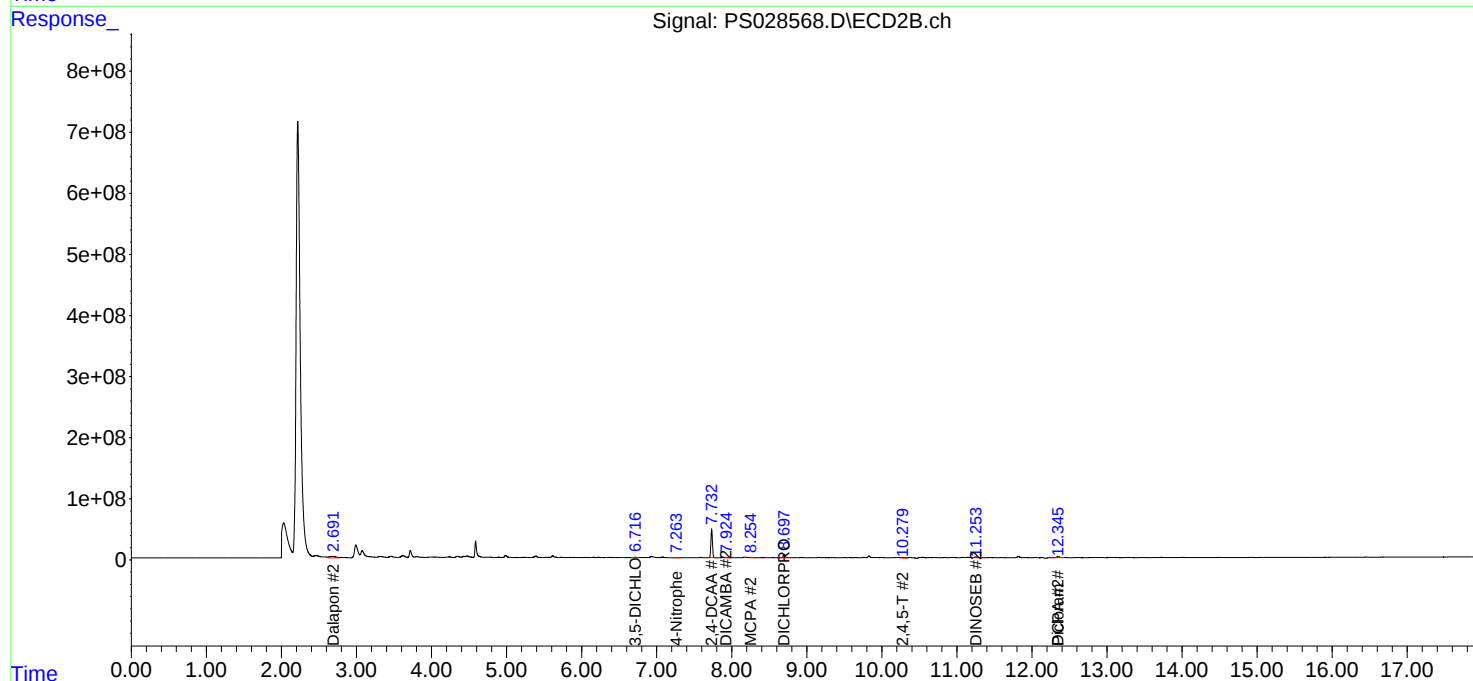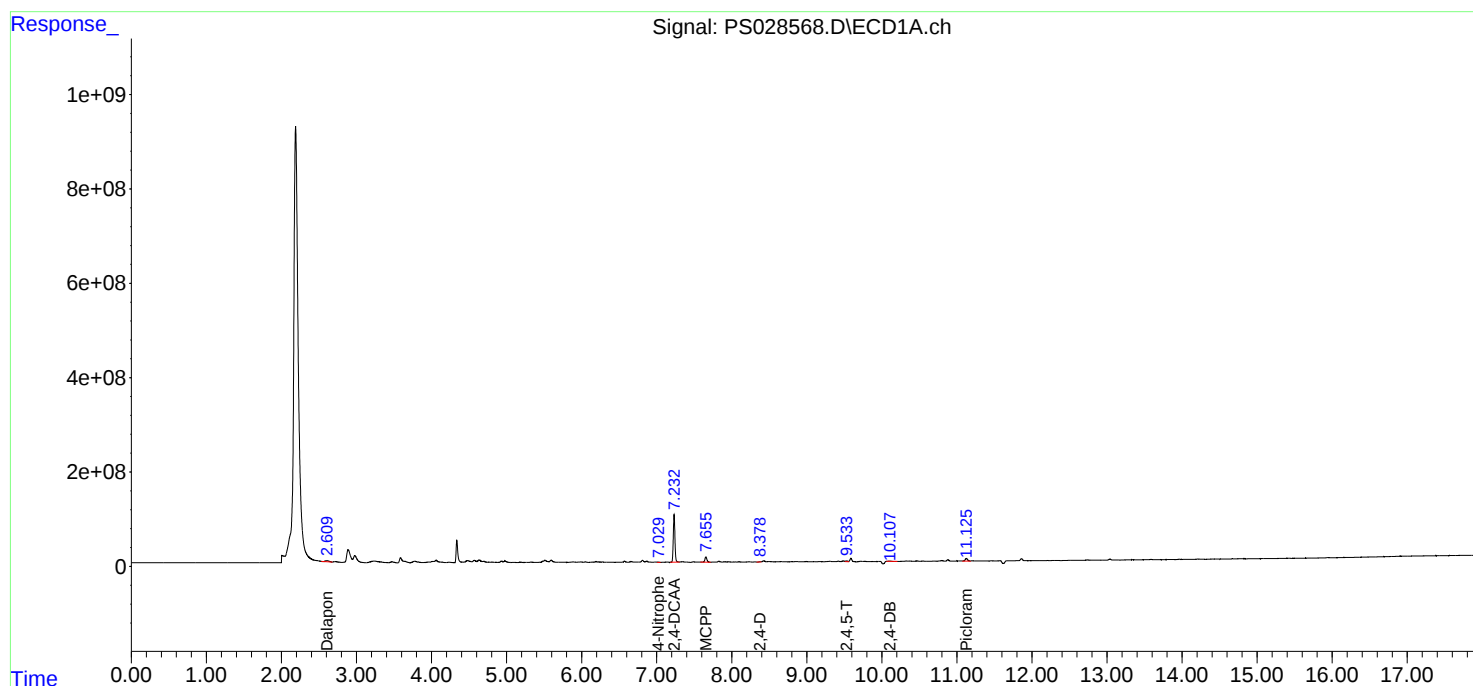


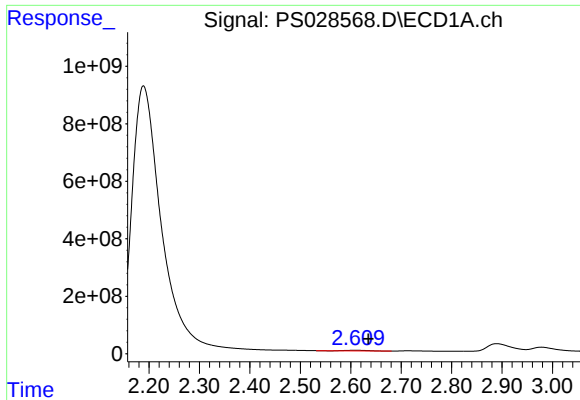

#1 Dalapon


R.T.: 2.609 min
Delta R.T.: -0.026 min
Response: 70625658
Conc: 21.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

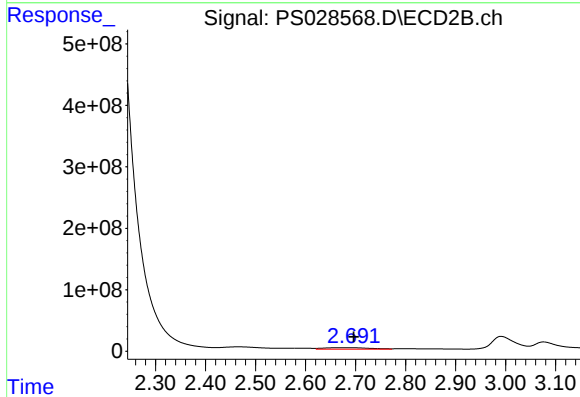


#1 Dalapon

R.T.: 2.690 min
Delta R.T.: -0.006 min
Response: 147055200
Conc: 60.77 ng/ml

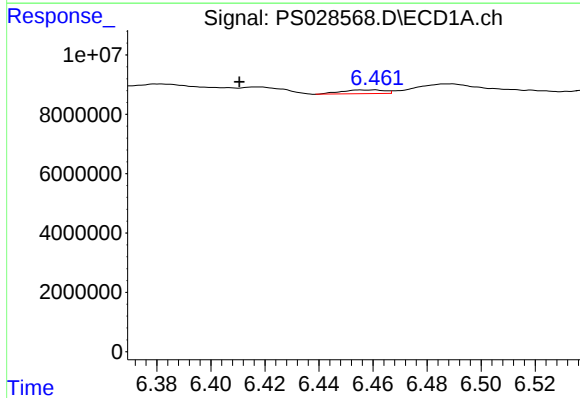


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.458 min
Delta R.T.: 0.048 min
Response: 1389120
Conc: N.D.

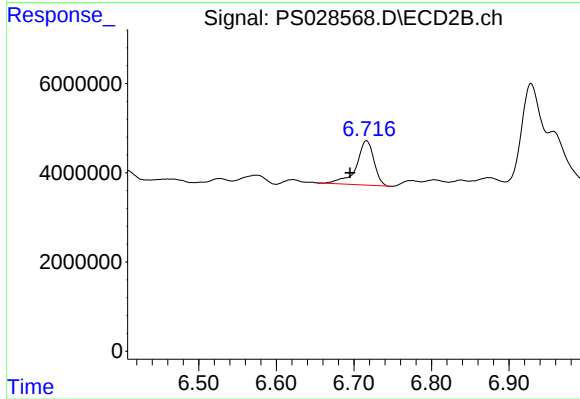

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.716 min
Delta R.T.: 0.021 min
Response: 15639345
Conc: 8.09 ng/ml

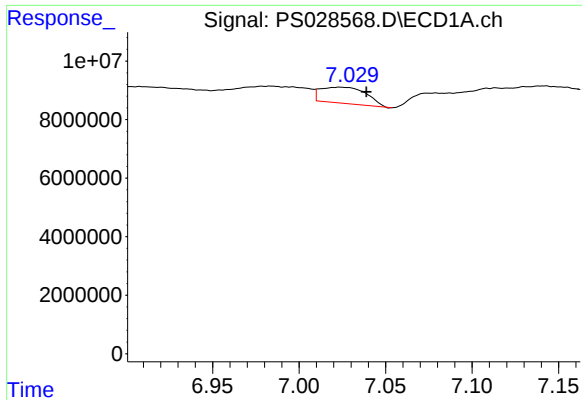

#3 4-Nitrophenol


R.T.: 7.024 min
Delta R.T.: -0.015 min
Response: 10019177
Conc: 5.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

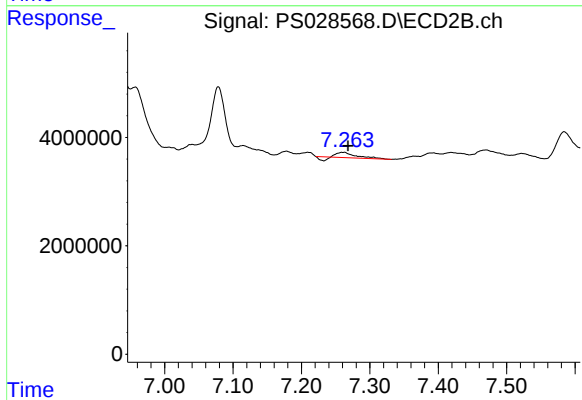


#3 4-Nitrophenol

R.T.: 7.261 min
Delta R.T.: -0.007 min
Response: 1439591
Conc: 1.67 ng/ml

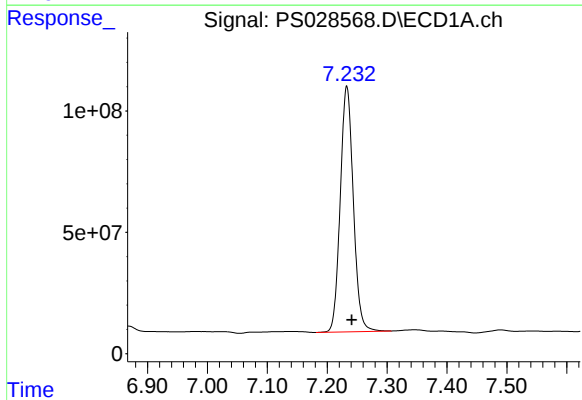


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.008 min
Response: 1534253464
Conc: 600.28 ng/ml

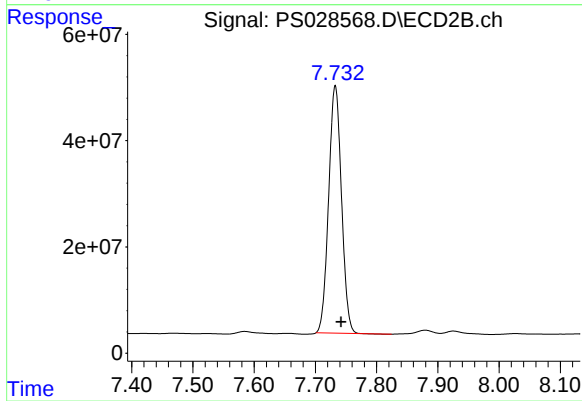

#4 2,4-DCAA


R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 677005667
Conc: 523.87 ng/ml

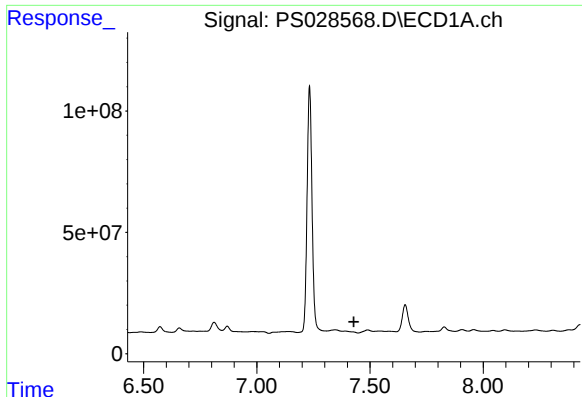

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

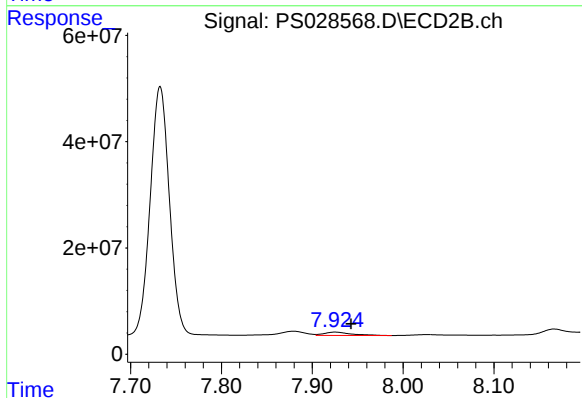


#5 DICAMBA

R.T.: 7.925 min
Delta R.T.: -0.017 min
Response: 12556441
Conc: 2.20 ng/ml

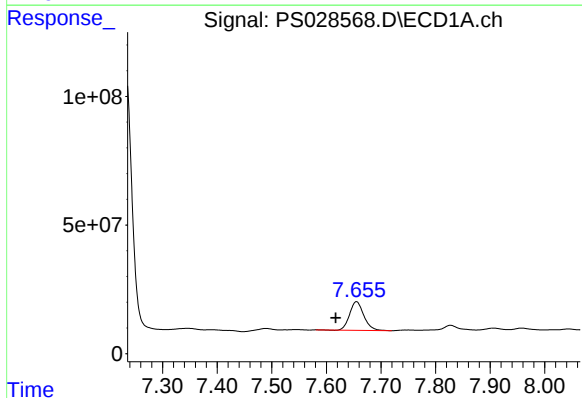


#6 MCP

R.T.: 7.655 min
Delta R.T.: 0.038 min
Response: 201676271
Conc: 28.67 ug/ml

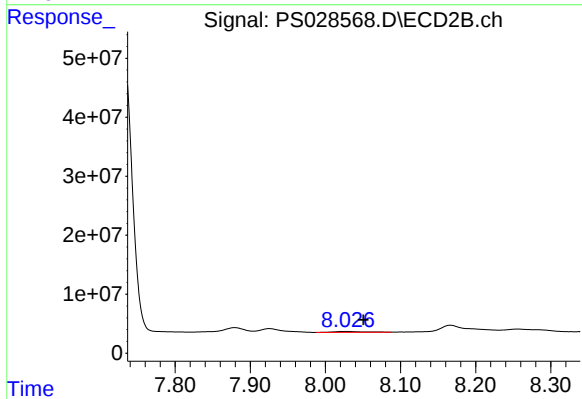

#6 MCP


R.T.: 8.027 min
Delta R.T.: -0.024 min
Response: 3840658
Conc: N.D.

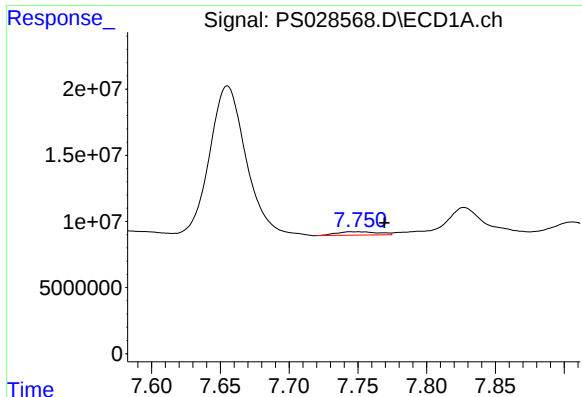

#7 MCPA


R.T.: 7.748 min
Delta R.T.: -0.021 min
Response: 5311686
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

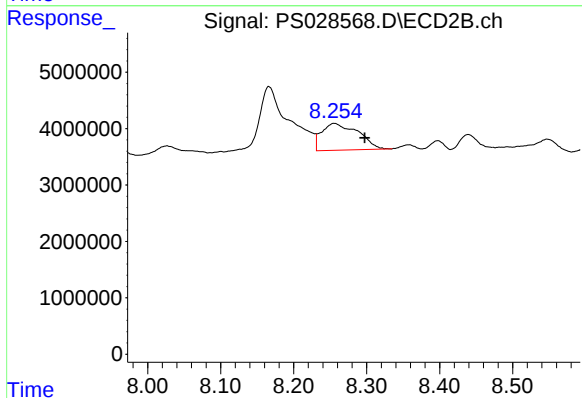


#7 MCPA

R.T.: 8.256 min
Delta R.T.: -0.042 min
Response: 16495273
Conc: 2.66 ug/ml

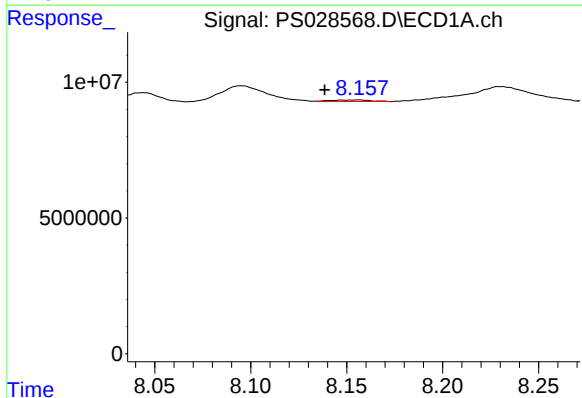


#8 DICHLORPROP

R.T.: 8.155 min
Delta R.T.: 0.016 min
Response: 853942
Conc: N.D.

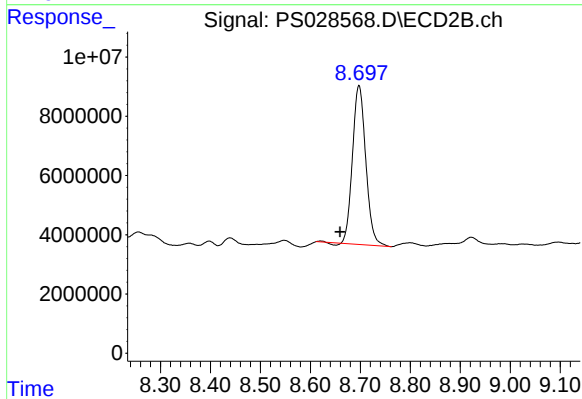

#8 DICHLORPROP


R.T.: 8.697 min
Delta R.T.: 0.038 min
Response: 98758807
Conc: 67.62 ng/ml

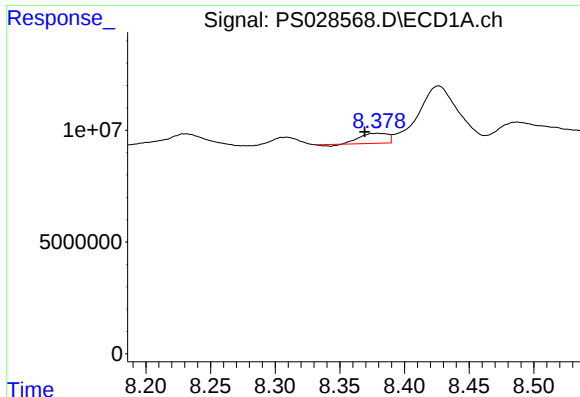

#9 2,4-D


R.T.: 8.379 min
Delta R.T.: 0.010 min
Response: 6446716
Conc: 2.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

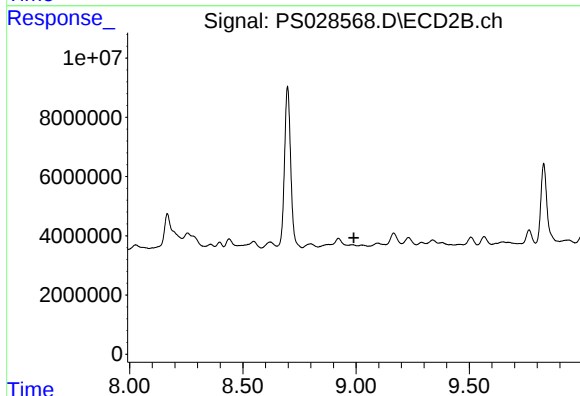


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.990 min
Response: 0
Conc: N.D.

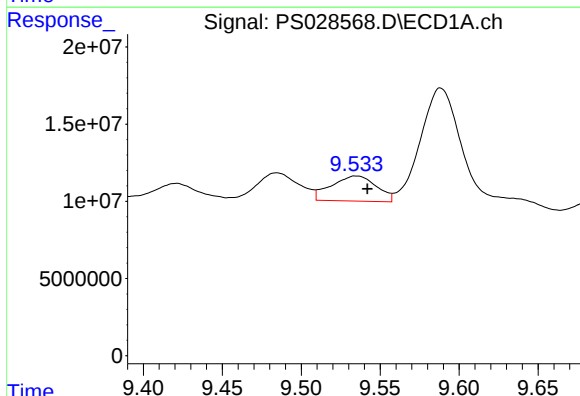


#12 2,4,5-T

R.T.: 9.535 min
Delta R.T.: -0.007 min
Response: 32470414
Conc: 1.83 ng/ml

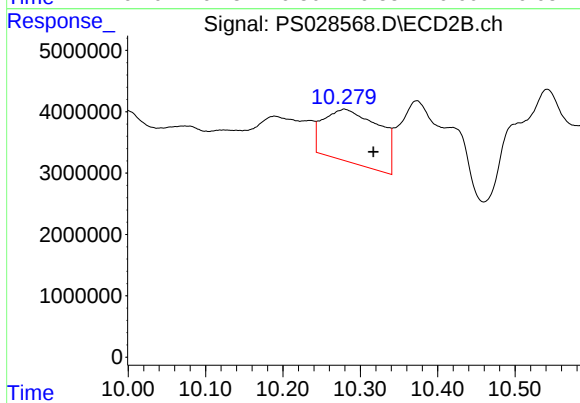

#12 2,4,5-T


R.T.: 10.280 min
Delta R.T.: -0.037 min
Response: 43279986
Conc: 5.16 ng/ml

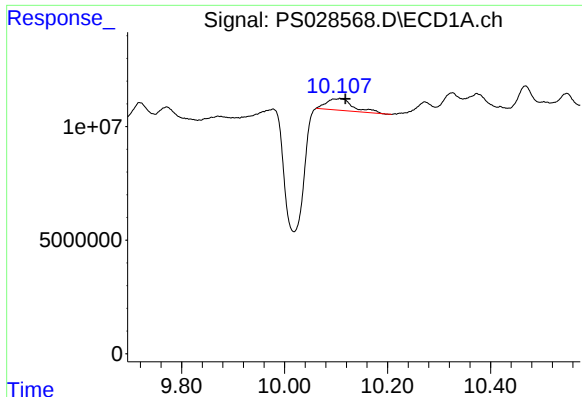

#13 2,4-DB


R.T.: 10.108 min
Delta R.T.: -0.010 min
Response: 18348021
Conc: 6.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

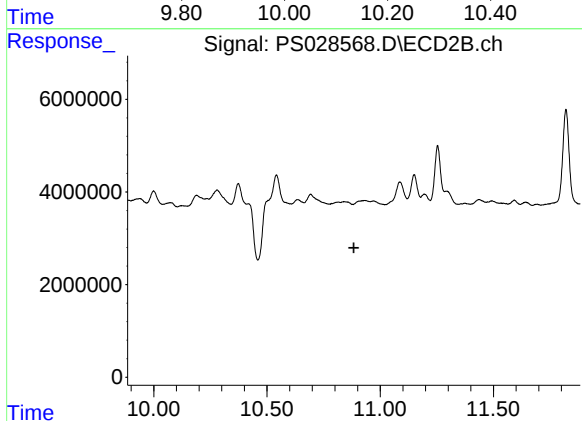


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.884 min
Response: 0
Conc: N.D.

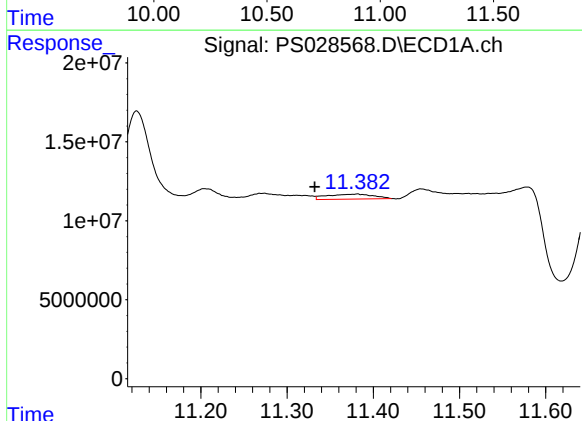


#14 DINOSEB

R.T.: 11.381 min
Delta R.T.: 0.049 min
Response: 12267983
Conc: N.D.

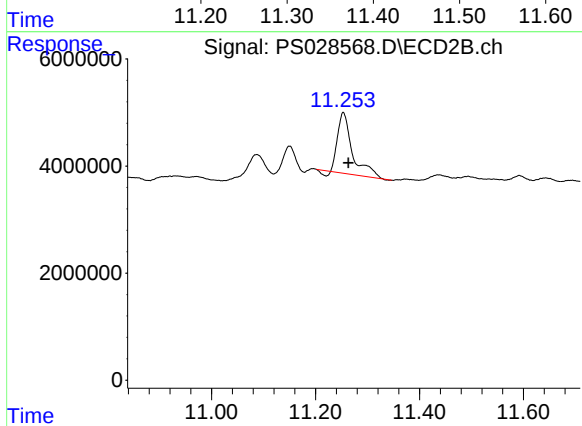

#14 DINOSEB


R.T.: 11.254 min
Delta R.T.: -0.010 min
Response: 21784398
Conc: 3.94 ng/ml

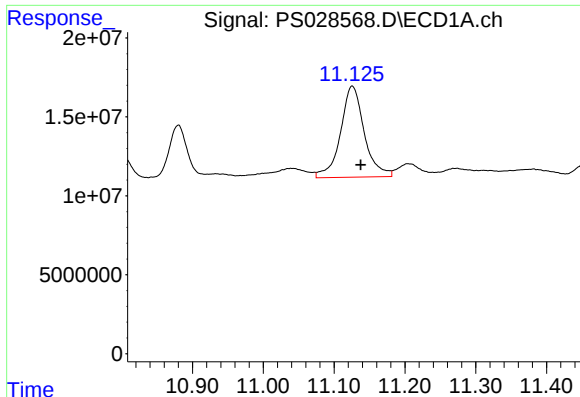

#15 Picloram


R.T.: 11.126 min
Delta R.T.: -0.012 min
Response: 134119593
Conc: 4.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

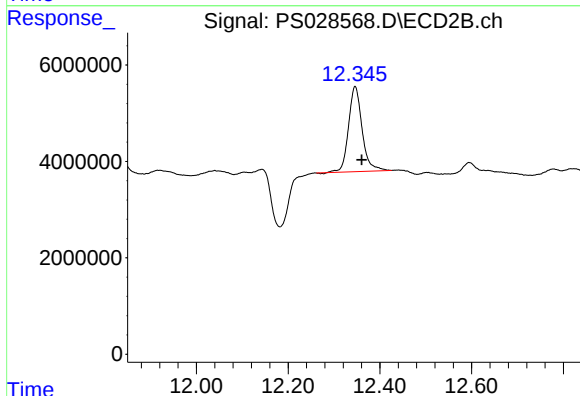


#15 Picloram

R.T.: 12.346 min
Delta R.T.: -0.015 min
Response: 36270051
Conc: 3.20 ng/ml

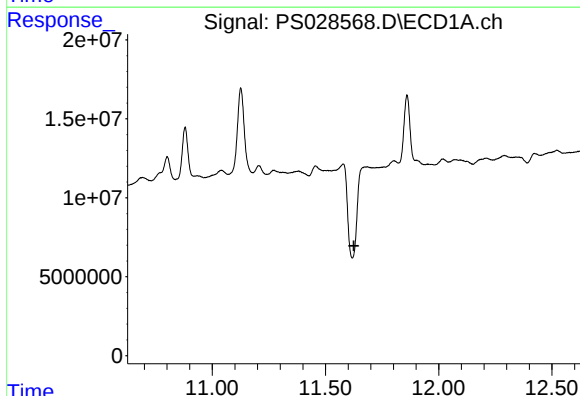

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.625 min
Response: 0
Conc: N.D.

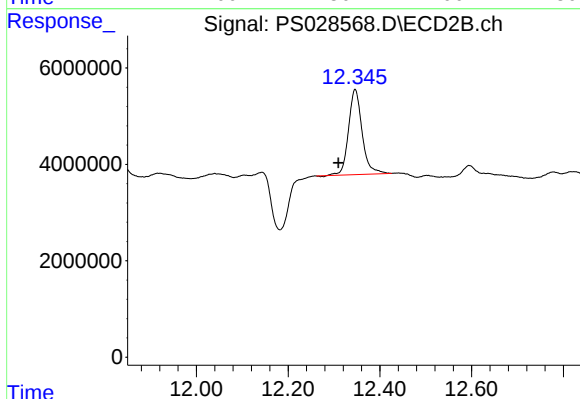

#16 DCPA

R.T.: 12.346 min
Delta R.T.: 0.037 min
Response: 36270051
Conc: 3.74 ng/ml