

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 17:40
 Operator : AR\AJ
 Sample : P4893-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 23:59:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.733	753.3E6	302.5E6	294.741	234.105
Target Compounds							
1) T	Dalapon	0.000	2.706	0	133.7E6	N.D.	55.237
2) T	3,5-DICHL...	6.399	0.000	1949518	0	<MDL	N.D. #
3) T	4-Nitroph...	7.025	7.293	8148654	1703077	4.798	1.973 #
5) T	DICAMBA	7.434	7.924	8861216	12441591	<MDL	2.181 #
6) T	MCPD	7.654f	8.070	173.2E6	1636607	24.625	<MDL #
7) T	MCPA	7.779	8.289	29367634	13594519	2.878	2.195
8) T	DICHLORPROP	8.171f	8.697f	4442904	76263872	1.505	52.215 #
9) T	2,4-D	0.000	8.981	0	2206575	N.D.	1.409
10) T	Pentachlo...	8.656	9.507	15303790	9300958	<MDL	<MDL #
11) T	2,4,5-TP ...	9.251	9.940f	-20264488	13717185	N.D.	1.626
12) T	2,4,5-T	9.532	10.301	20787751	66073042	1.170	7.882 #
13) T	2,4-DB	10.137	10.839f	24319547	2923220	8.923	2.790 #
14) T	DINOSEB	11.349	11.253	25017197	6333728	1.755	1.146 #
15) T	Picloram	11.125	12.346	111.0E6	24953082	3.942	2.205 #
16) T	DCPA	0.000	12.297	0	2155755	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 17:40
Operator : AR\AJ
Sample : P4893-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 23:59:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

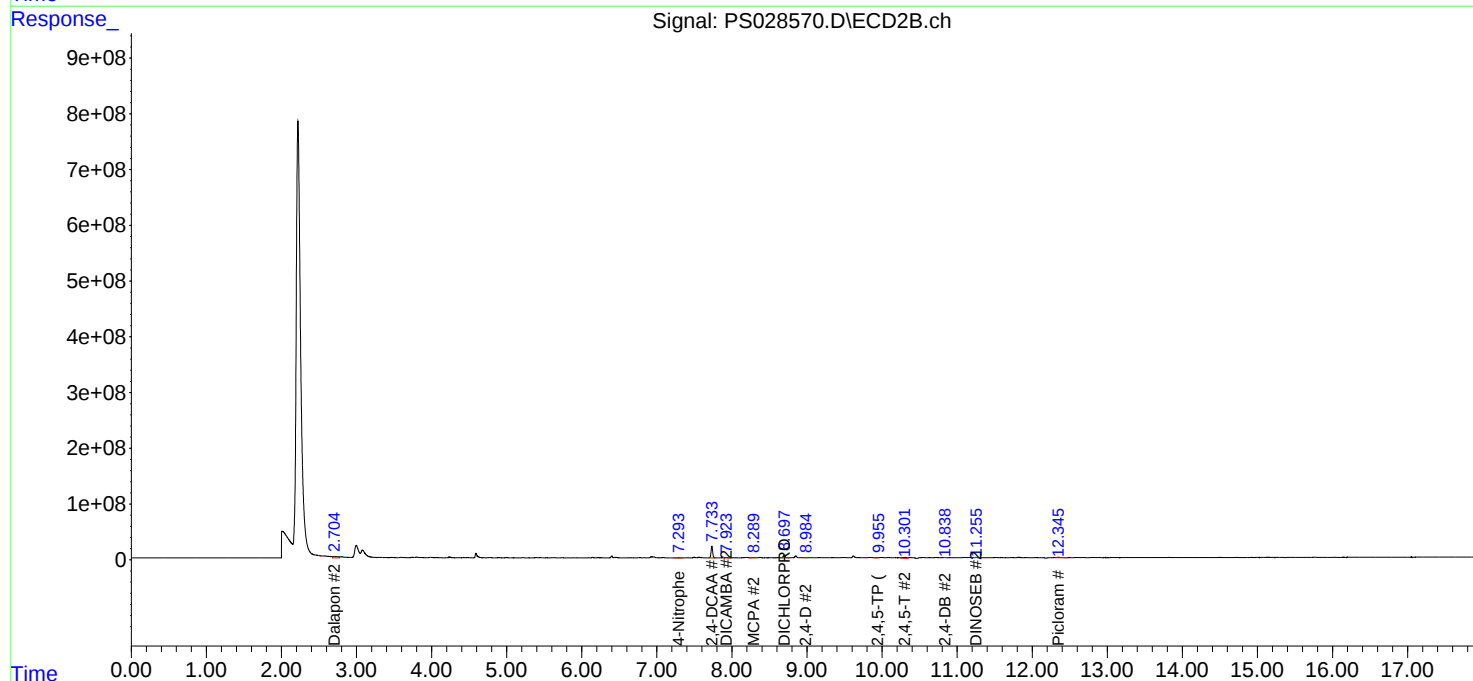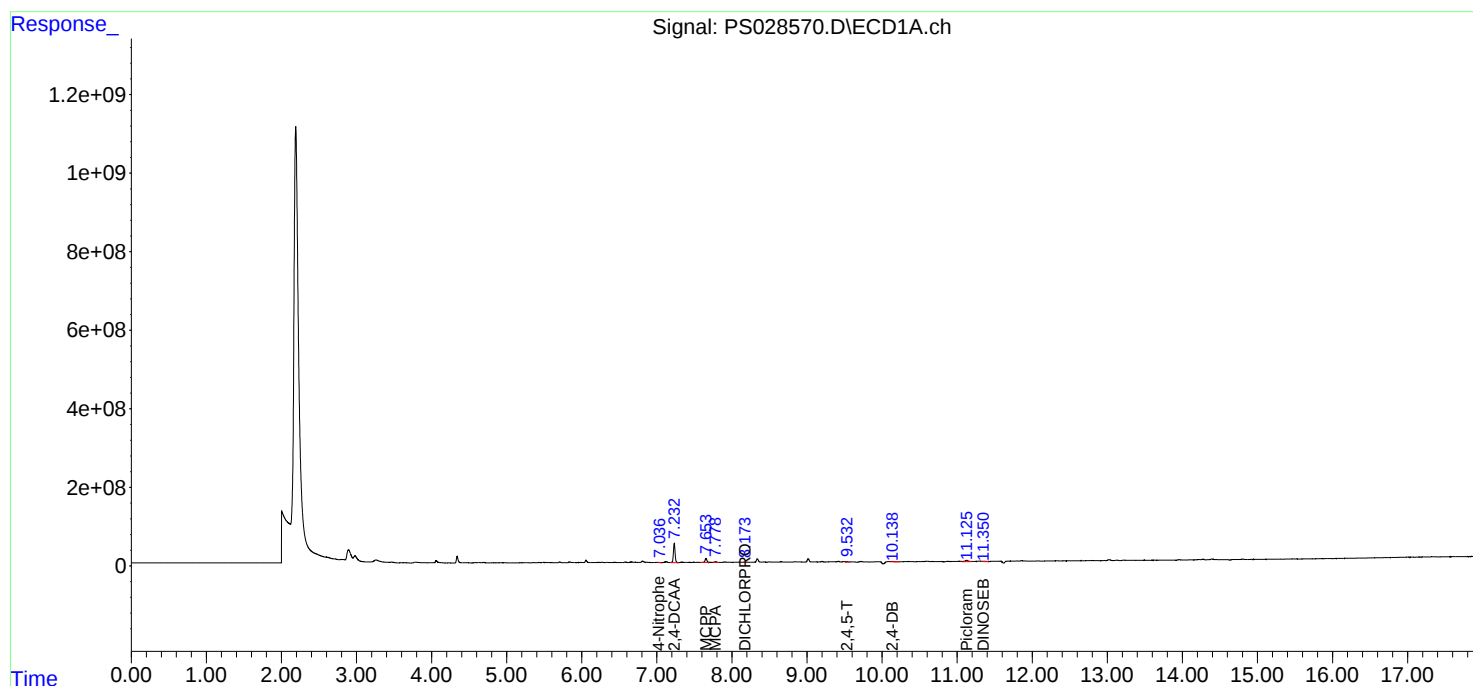


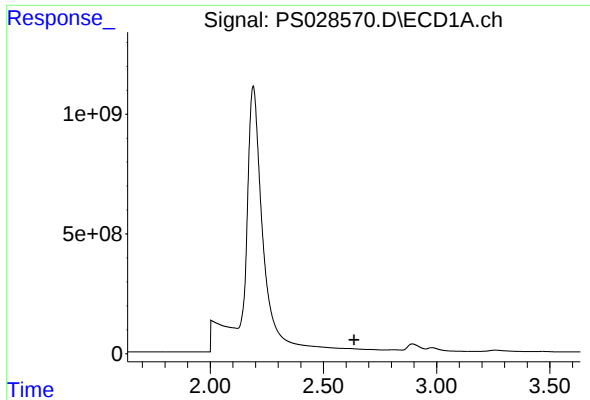

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.635 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

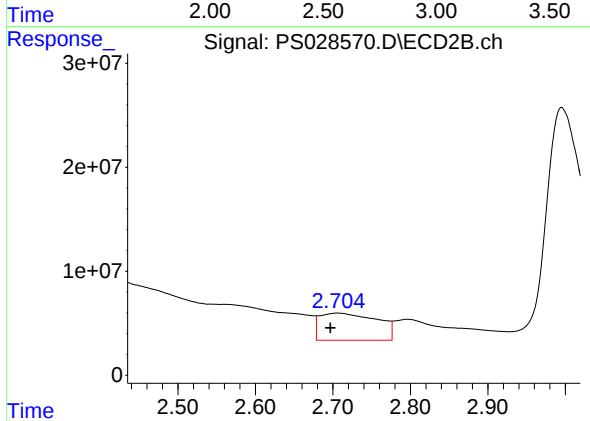


#1 Dalapon

R.T.: 2.706 min
Delta R.T.: 0.009 min
Response: 133668732
Conc: 55.24 ng/ml

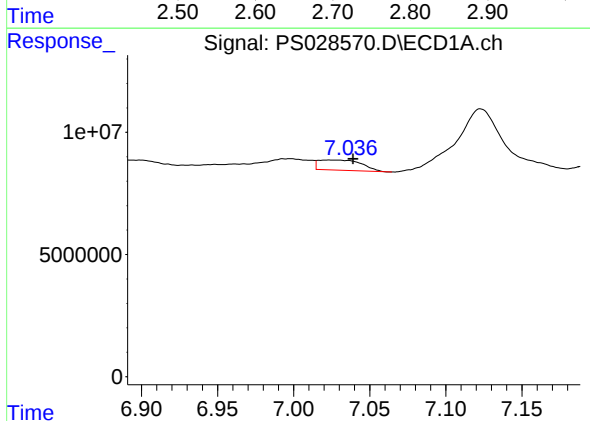


#3 4-Nitrophenol

R.T.: 7.025 min
Delta R.T.: -0.014 min
Response: 8148654
Conc: 4.80 ng/ml

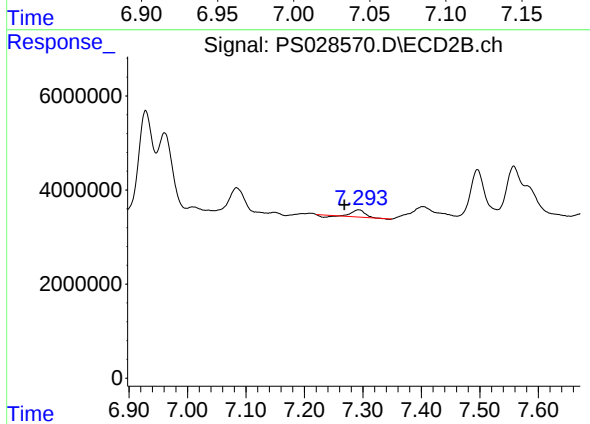

#3 4-Nitrophenol


R.T.: 7.293 min
Delta R.T.: 0.025 min
Response: 1703077
Conc: 1.97 ng/ml

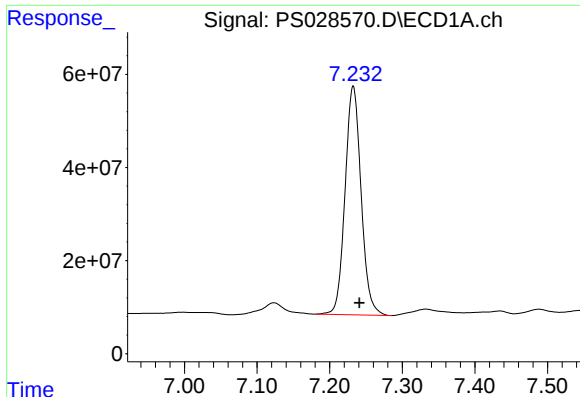

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.009 min
Response: 753322113
Conc: 294.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

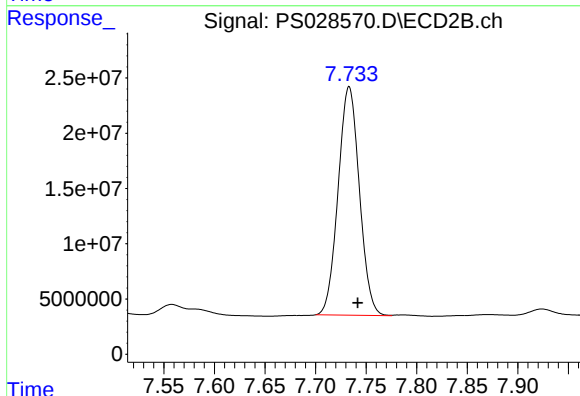


#4 2,4-DCAA

R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 302534631
Conc: 234.10 ng/ml

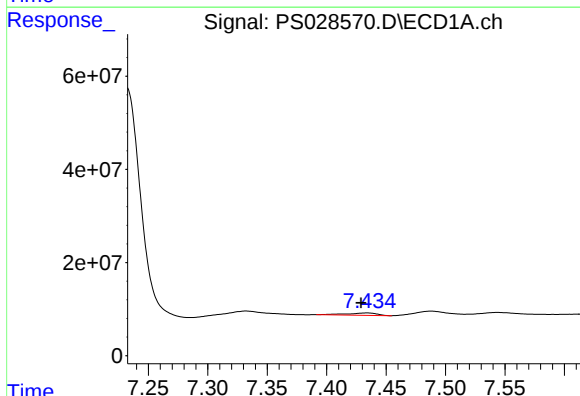


#5 DICAMBA

R.T.: 7.434 min
Delta R.T.: 0.005 min
Response: 8861216
Conc: N.D.

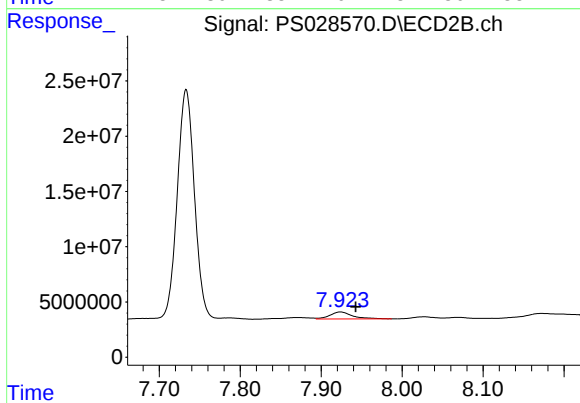

#5 DICAMBA


R.T.: 7.924 min
Delta R.T.: -0.019 min
Response: 12441591
Conc: 2.18 ng/ml

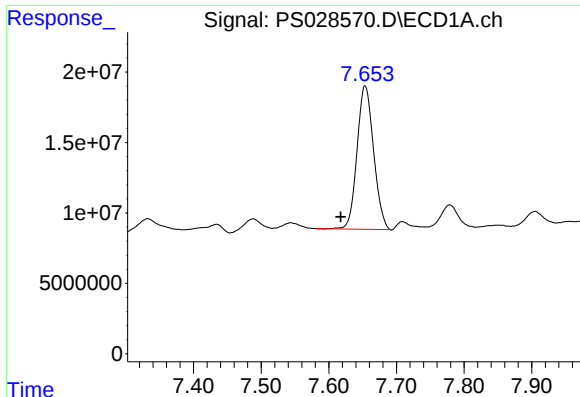

#6 MCP


R.T.: 7.654 min
Delta R.T.: 0.036 min
Response: 173226441
Conc: 24.62 ug/ml

Instrument :
ECD_S
ClientSampleId :

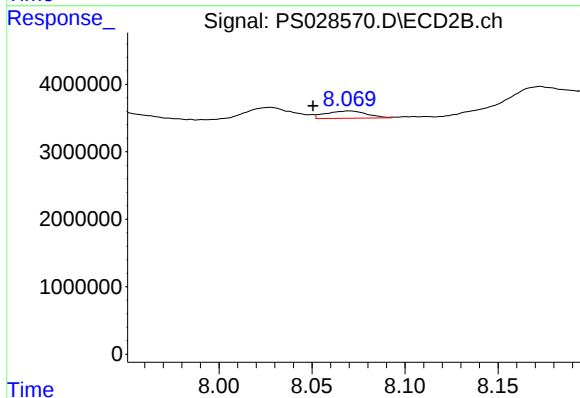


#6 MCP

R.T.: 8.070 min
Delta R.T.: 0.019 min
Response: 1636607
Conc: N.D.

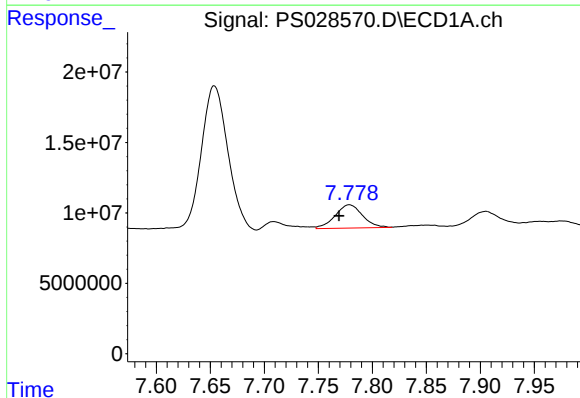


#7 MCP

R.T.: 7.779 min
Delta R.T.: 0.010 min
Response: 29367634
Conc: 2.88 ug/ml

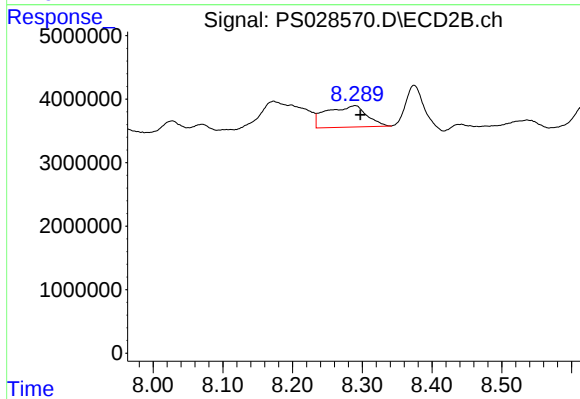

#7 MCP


R.T.: 8.289 min
Delta R.T.: -0.008 min
Response: 13594519
Conc: 2.19 ug/ml

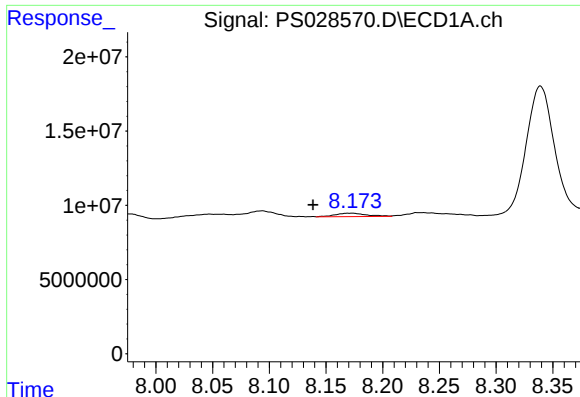

#8 DICHLORPROP


R.T.: 8.171 min
Delta R.T.: 0.033 min
Response: 4442904
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

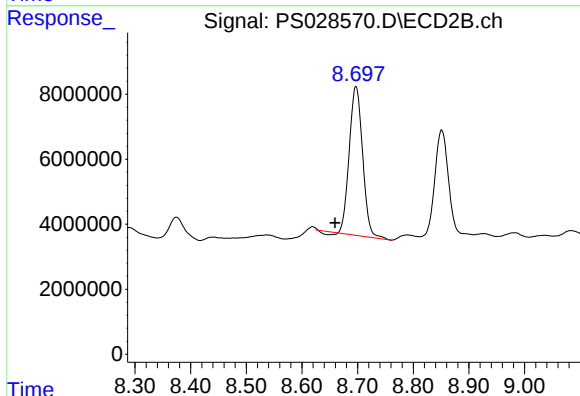


#8 DICHLORPROP

R.T.: 8.697 min
Delta R.T.: 0.037 min
Response: 76263872
Conc: 52.22 ng/ml

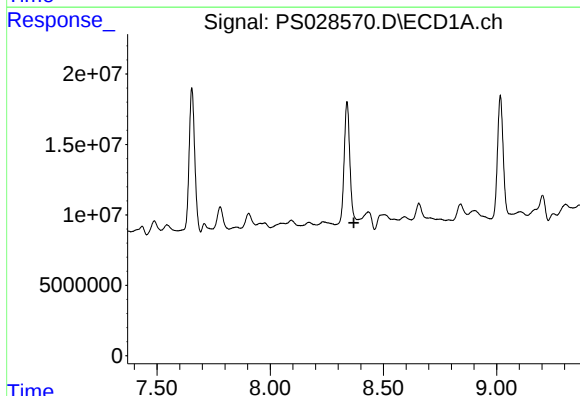


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.369 min
Response: 0
Conc: N.D.

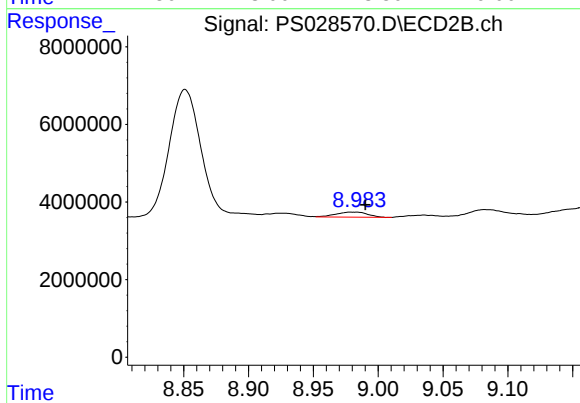

#9 2,4-D


R.T.: 8.981 min
Delta R.T.: -0.009 min
Response: 2206575
Conc: 1.41 ng/ml

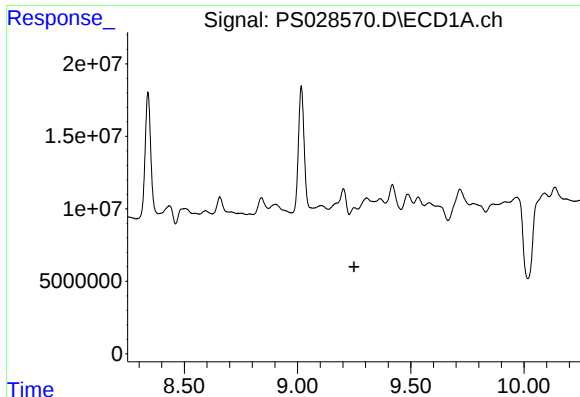

#11 2,4,5-TP (SILVEX)


R.T.: 9.251 min
Delta R.T.: 0.002 min
Response: -20264488
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

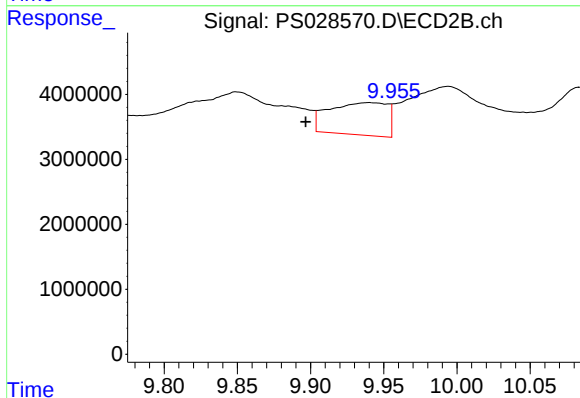


#11 2,4,5-TP (SILVEX)

R.T.: 9.940 min
Delta R.T.: 0.044 min
Response: 13717185
Conc: 1.63 ng/ml

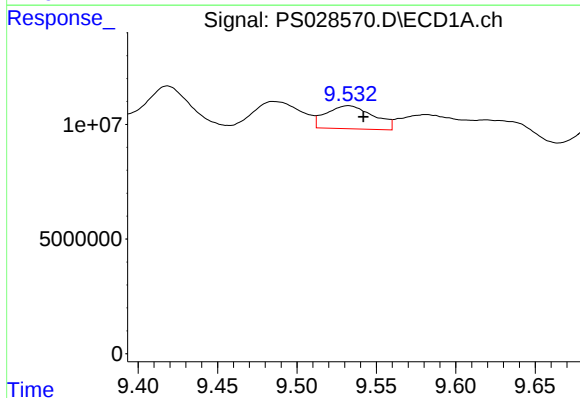


#12 2,4,5-T

R.T.: 9.532 min
Delta R.T.: -0.010 min
Response: 20787751
Conc: 1.17 ng/ml

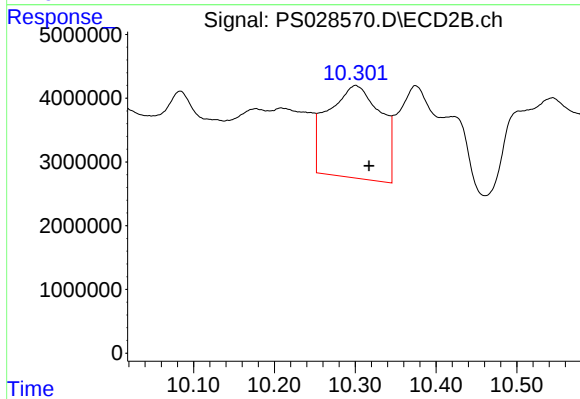

#12 2,4,5-T


R.T.: 10.301 min
Delta R.T.: -0.016 min
Response: 66073042
Conc: 7.88 ng/ml

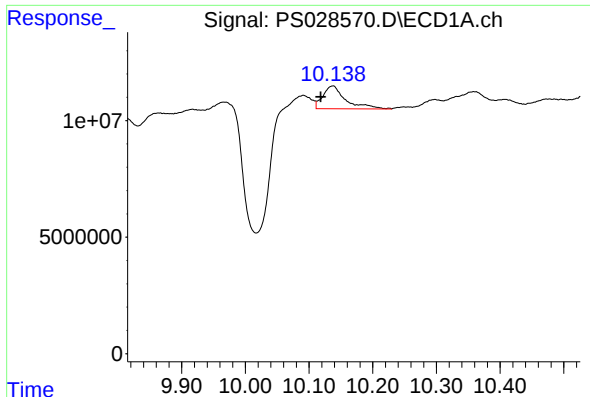

#13 2,4-DB


R.T.: 10.137 min
Delta R.T.: 0.018 min
Response: 24319547
Conc: 8.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

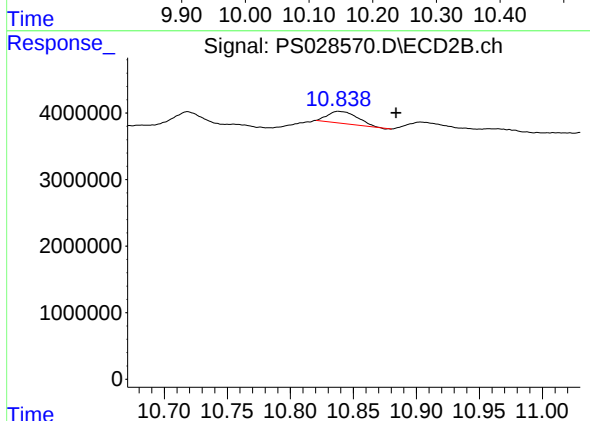


#13 2,4-DB

R.T.: 10.839 min
Delta R.T.: -0.045 min
Response: 2923220
Conc: 2.79 ng/ml

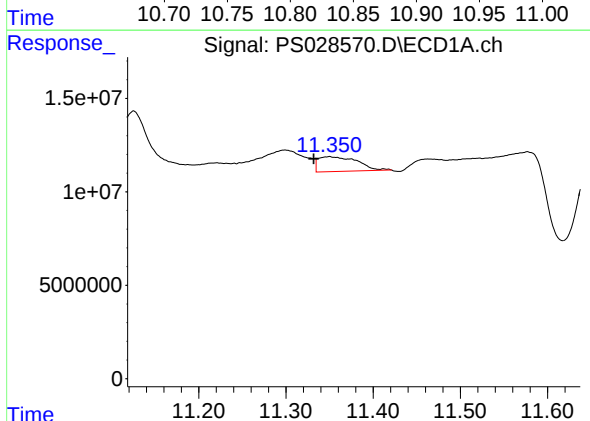


#14 DINOSEB

R.T.: 11.349 min
Delta R.T.: 0.017 min
Response: 25017197
Conc: 1.75 ng/ml

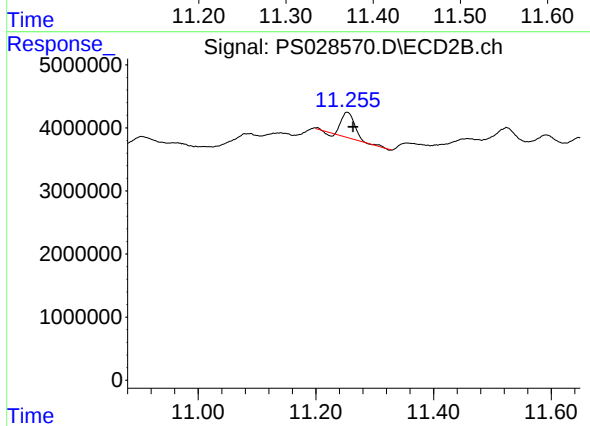

#14 DINOSEB


R.T.: 11.253 min
Delta R.T.: -0.010 min
Response: 6333728
Conc: 1.15 ng/ml

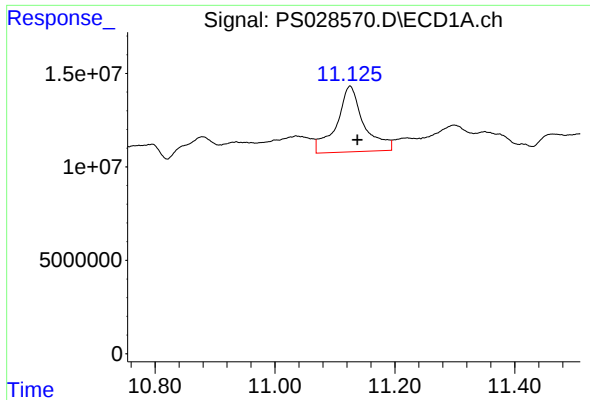

#15 Picloram

R.T.: 11.125 min
Delta R.T.: -0.012 min
Response: 111003636
Conc: 3.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

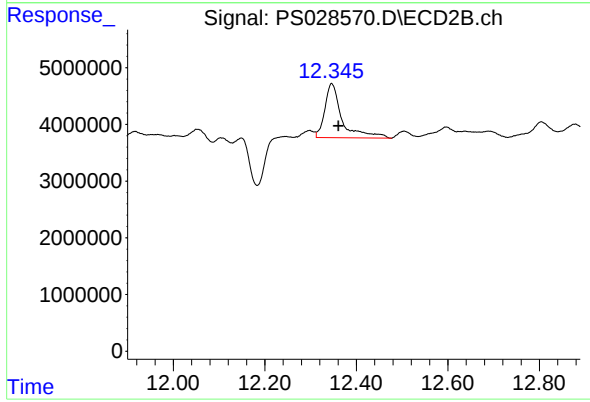

#15 Picloram

R.T.: 12.346 min
Delta R.T.: -0.015 min
Response: 24953082
Conc: 2.20 ng/ml