

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 18:04
 Operator : AR\AJ
 Sample : P4893-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:00:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.733	860.0E6	352.1E6	336.466	272.453
Target Compounds							
1) T	Dalapon	0.000	2.699	0	148.9E6	N.D.	61.526
2) T	3,5-DICHL...	6.394	6.697	6150241	7798516	1.648	4.036 #
3) T	4-Nitroph...	7.014f	7.288	19796150	5018686	11.655	5.813 #
5) T	DICAMBA	7.436	7.925	6368506	11089205	<MDL	1.944 #
6) T	MCPD	7.600	8.025f	2222410	15927162	<MDL	3.703 #
7) T	MCPA	7.762	8.256f	2422681	21892195	<MDL	3.535 #
8) T	DICHLORPROP	8.171f	8.696f	32248013	82517580	10.926	56.497 #
9) T	2,4-D	8.372	8.970	15970672	4436086	4.996	2.834 #
10) T	Pentachlo...	8.655	9.507	363235	9668505	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.849f	0	49523414	N.D.	5.869
12) T	2,4,5-T	9.532	10.302	17279544	65750024	<MDL	7.844 #
13) T	2,4-DB	10.138	0.000	23261385	0	8.534	N.D. #
14) T	DINOSEB	11.361f	11.263	27142445	47231354	1.904	8.543 #
15) T	Picloram	11.160	12.346	217.2E6	4808130	7.713	<MDL #
16) T	DCPA	0.000	12.298	0	4117807	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 18:04
Operator : AR\AJ
Sample : P4893-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:00:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

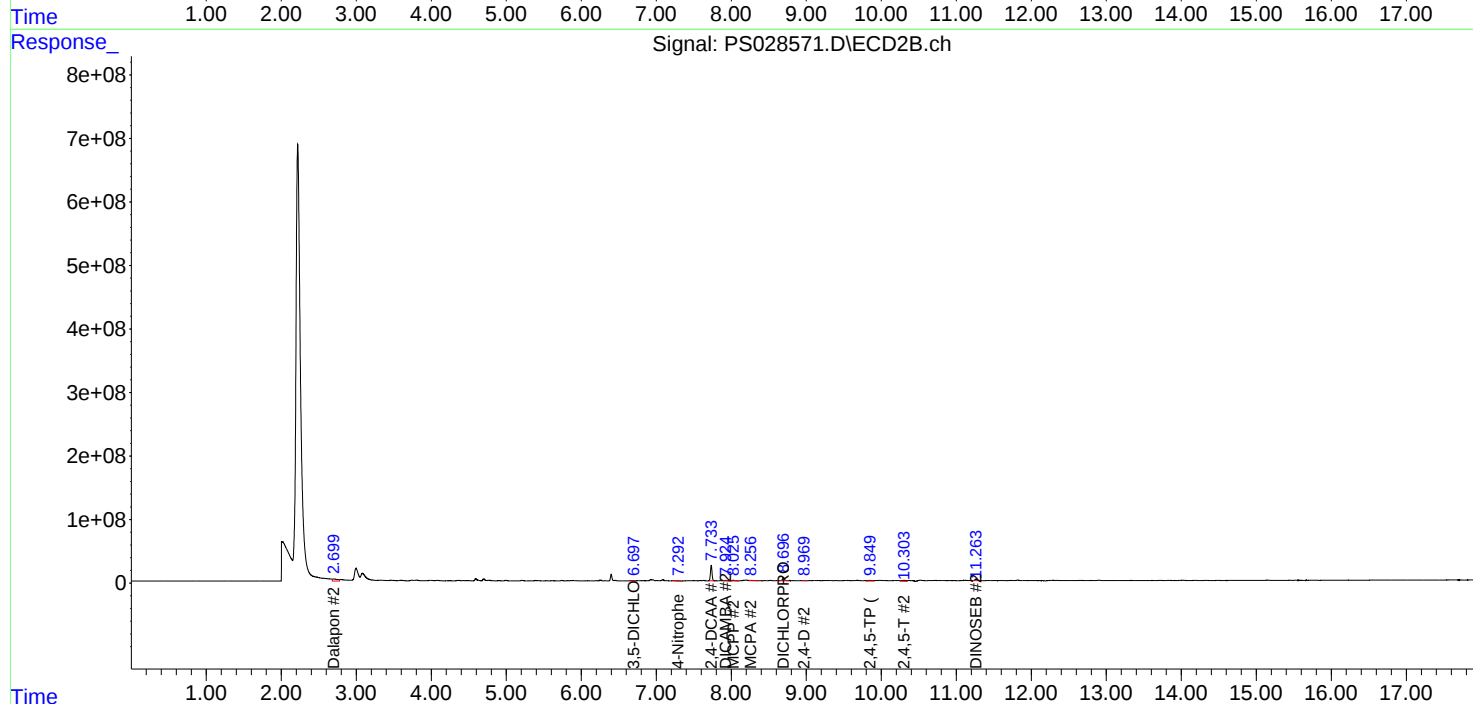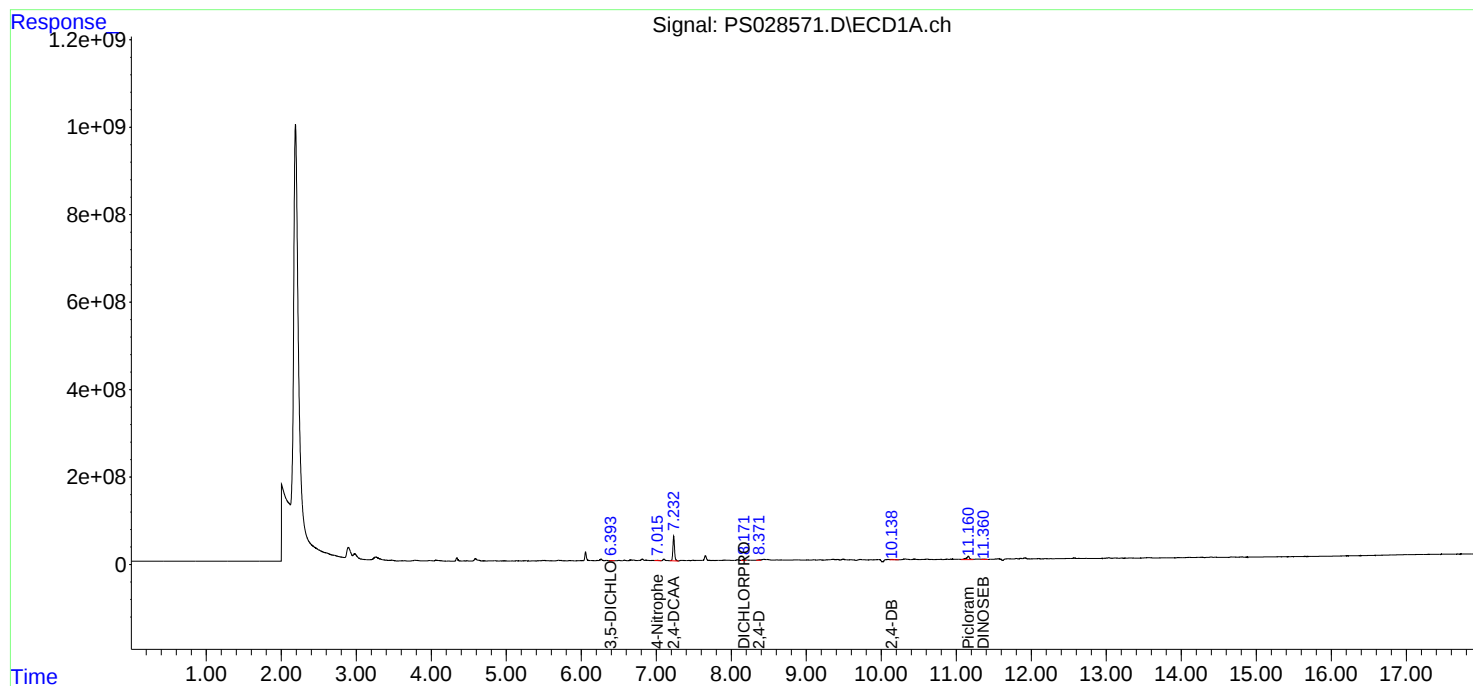


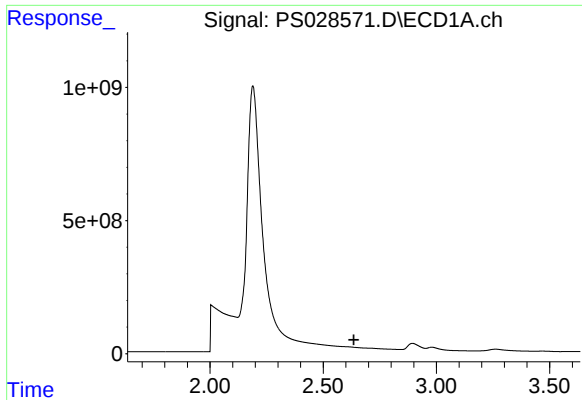

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.635 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

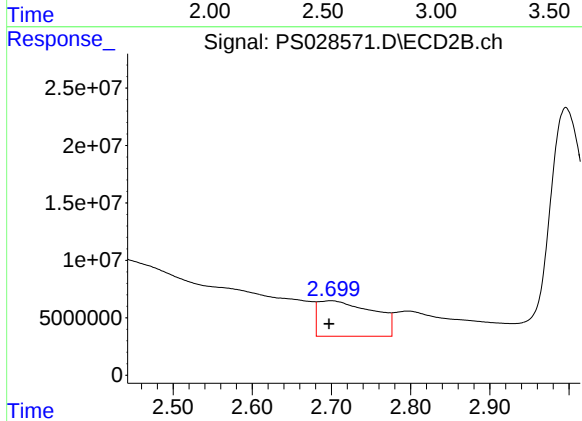


#1 Dalapon

R.T.: 2.699 min
Delta R.T.: 0.003 min
Response: 148888931
Conc: 61.53 ng/ml

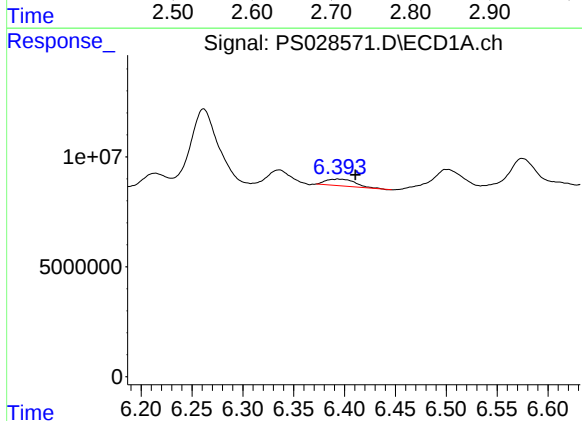


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.394 min
Delta R.T.: -0.017 min
Response: 6150241
Conc: 1.65 ng/ml

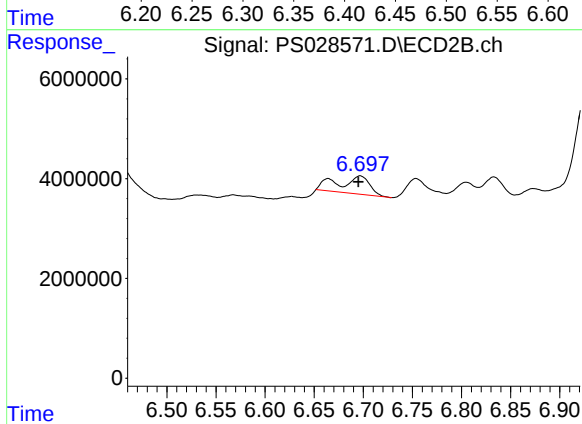

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.697 min
Delta R.T.: 0.002 min
Response: 7798516
Conc: 4.04 ng/ml

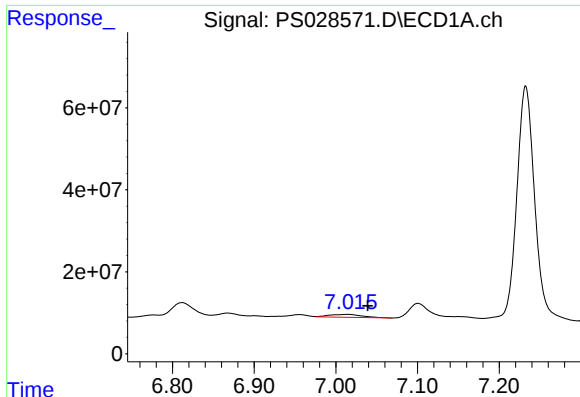

#3 4-Nitrophenol


R.T.: 7.014 min
Delta R.T.: -0.025 min
Response: 19796150
Conc: 11.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

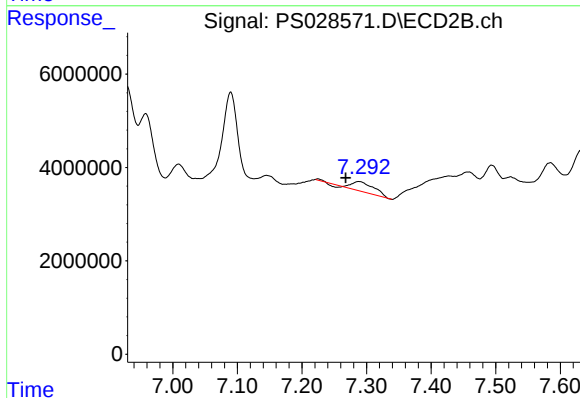


#3 4-Nitrophenol

R.T.: 7.288 min
Delta R.T.: 0.020 min
Response: 5018686
Conc: 5.81 ng/ml

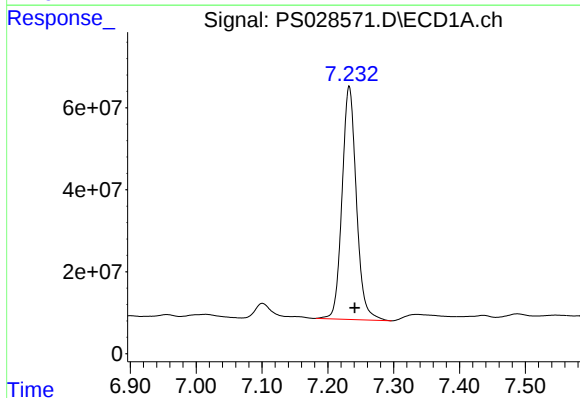


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.008 min
Response: 859968471
Conc: 336.47 ng/ml

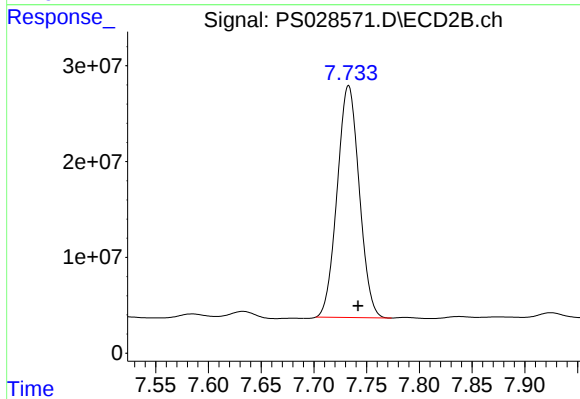

#4 2,4-DCAA


R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 352092475
Conc: 272.45 ng/ml

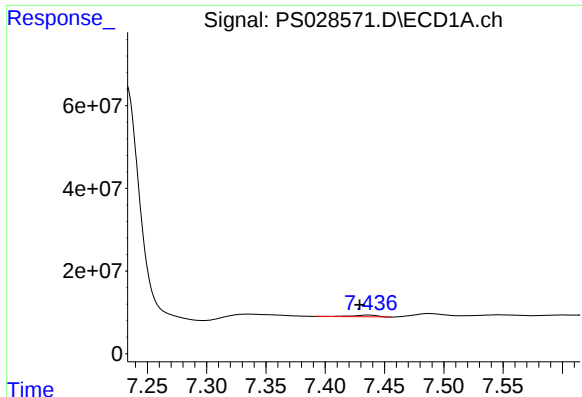

#5 DICAMBA


R.T.: 7.436 min
Delta R.T.: 0.007 min
Response: 6368506
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

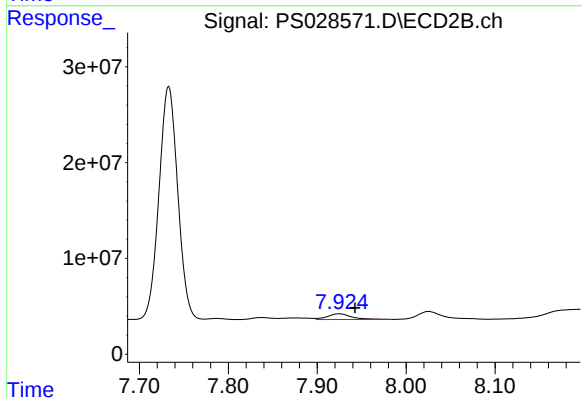


#5 DICAMBA

R.T.: 7.925 min
Delta R.T.: -0.018 min
Response: 11089205
Conc: 1.94 ng/ml

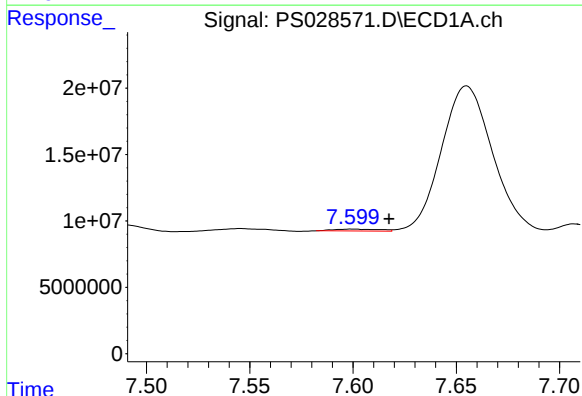


#6 MCP

R.T.: 7.600 min
Delta R.T.: -0.018 min
Response: 2222410
Conc: N.D.

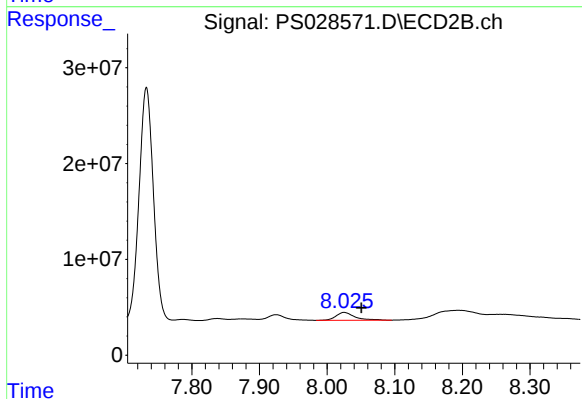

#6 MCP


R.T.: 8.025 min
Delta R.T.: -0.025 min
Response: 15927162
Conc: 3.70 ug/ml

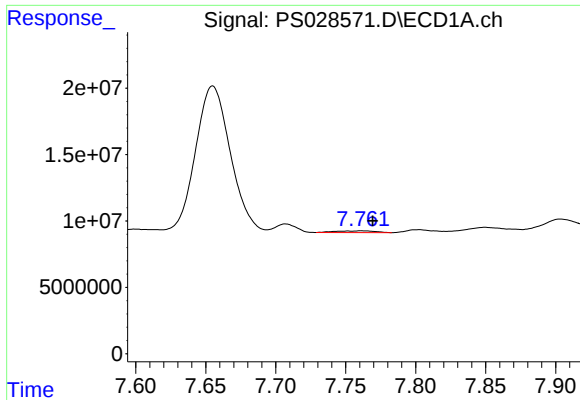

#7 MCPA


R.T.: 7.762 min
Delta R.T.: -0.007 min
Response: 2422681
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

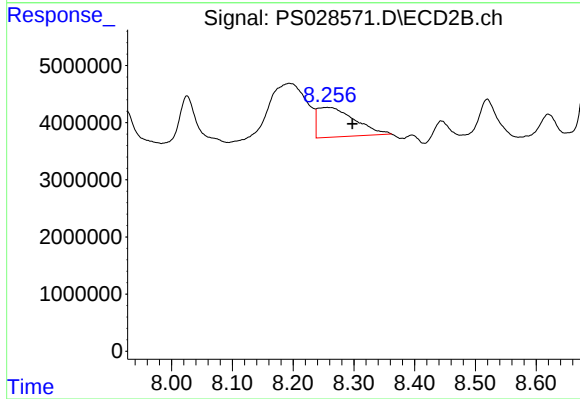


#7 MCPA

R.T.: 8.256 min
Delta R.T.: -0.041 min
Response: 21892195
Conc: 3.53 ug/ml

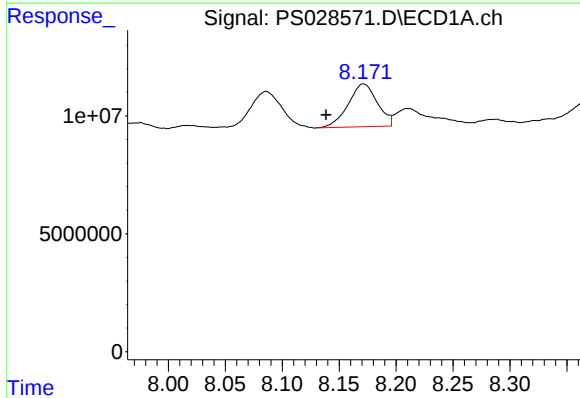


#8 DICHLORPROP

R.T.: 8.171 min
Delta R.T.: 0.033 min
Response: 32248013
Conc: 10.93 ng/ml

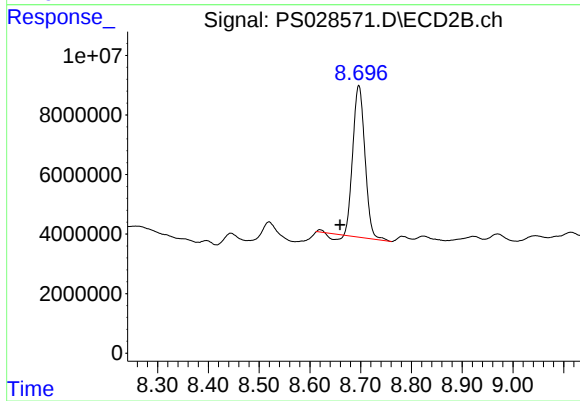

#8 DICHLORPROP


R.T.: 8.696 min
Delta R.T.: 0.037 min
Response: 82517580
Conc: 56.50 ng/ml

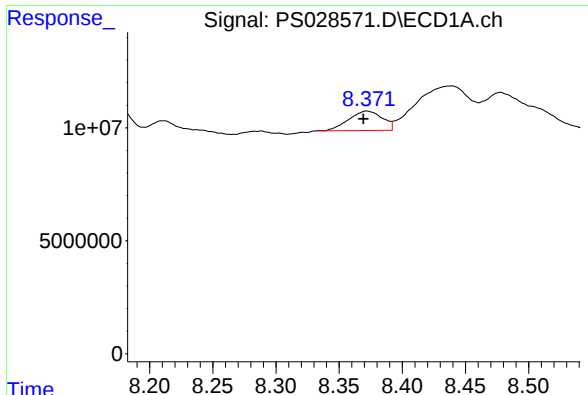

#9 2,4-D


R.T.: 8.372 min
Delta R.T.: 0.003 min
Response: 15970672
Conc: 5.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

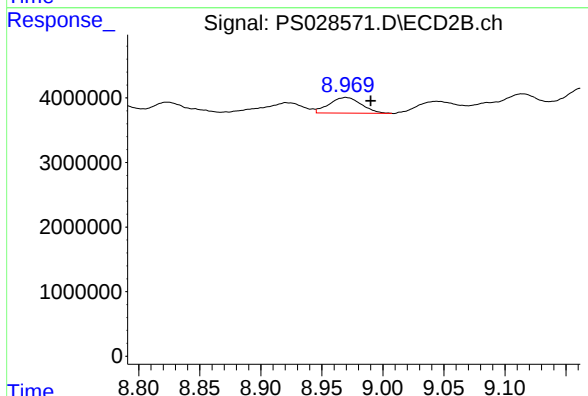


#9 2,4-D

R.T.: 8.970 min
Delta R.T.: -0.021 min
Response: 4436086
Conc: 2.83 ng/ml

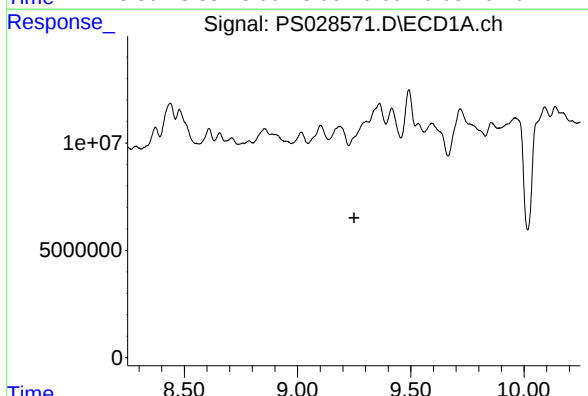


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.249 min
Response: 0
Conc: N.D.

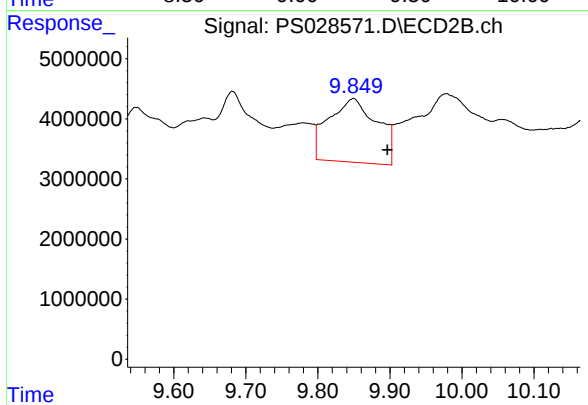

#11 2,4,5-TP (SILVEX)


R.T.: 9.849 min
Delta R.T.: -0.048 min
Response: 49523414
Conc: 5.87 ng/ml

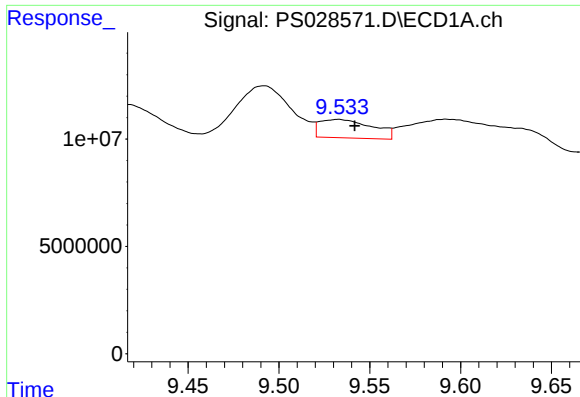

#12 2,4,5-T


R.T.: 9.532 min
Delta R.T.: -0.009 min
Response: 17279544
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

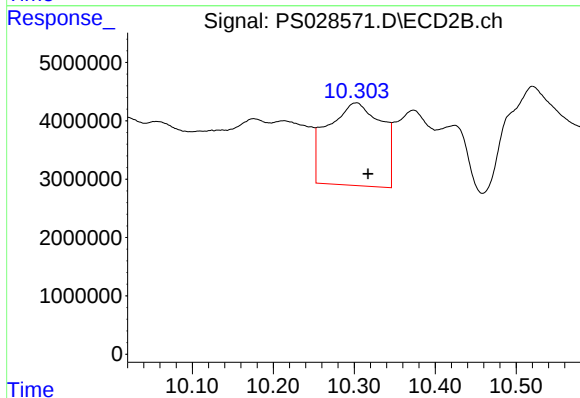


#12 2,4,5-T

R.T.: 10.302 min
Delta R.T.: -0.015 min
Response: 65750024
Conc: 7.84 ng/ml

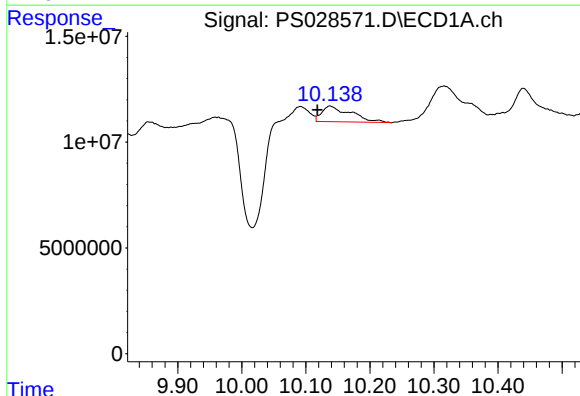


#13 2,4-DB

R.T.: 10.138 min
Delta R.T.: 0.020 min
Response: 23261385
Conc: 8.53 ng/ml

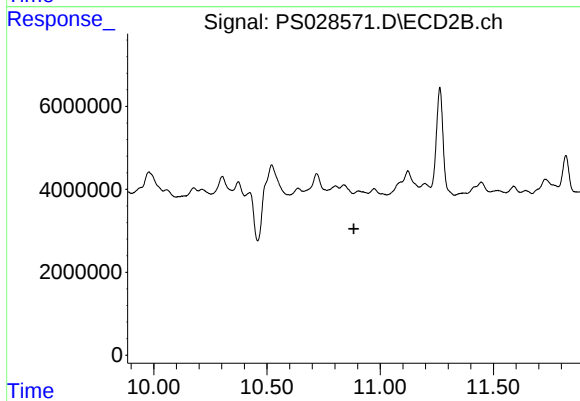

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.884 min
Response: 0
Conc: N.D.

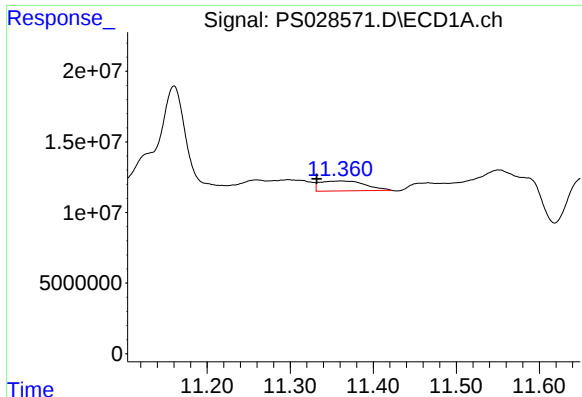

#14 DINOSEB


R.T.: 11.361 min
Delta R.T.: 0.030 min
Response: 27142445
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

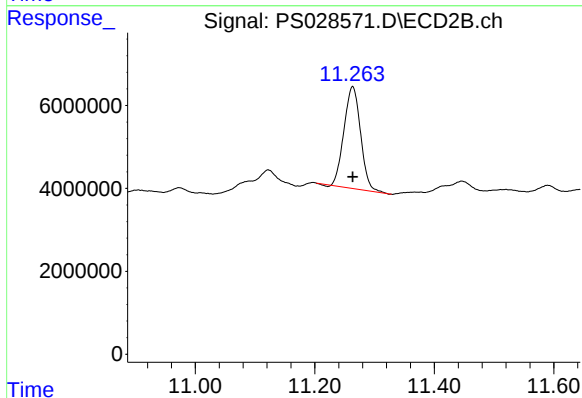


#14 DINOSEB

R.T.: 11.263 min
Delta R.T.: 0.000 min
Response: 47231354
Conc: 8.54 ng/ml

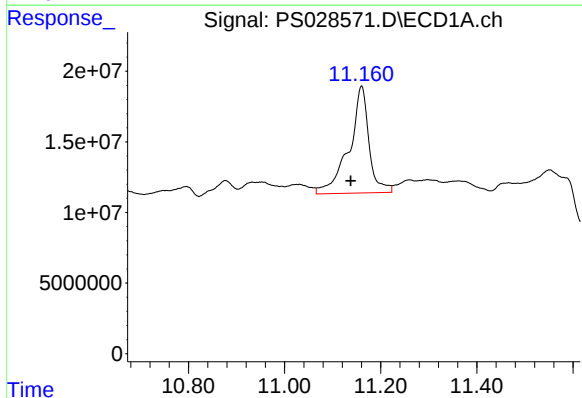

#15 Picloram

R.T.: 11.160 min
Delta R.T.: 0.022 min
Response: 217209353
Conc: 7.71 ng/ml

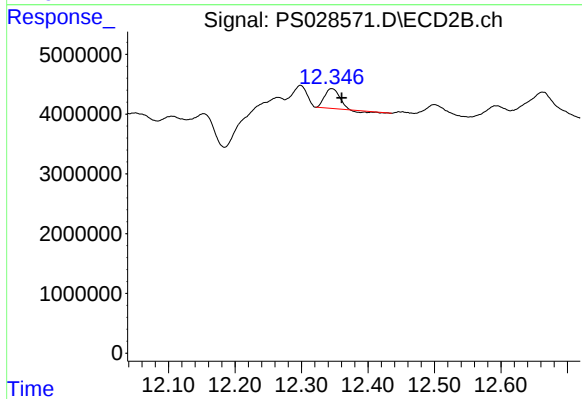

#15 Picloram

R.T.: 12.346 min
Delta R.T.: -0.015 min
Response: 4808130
Conc: N.D.