

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 19:40
 Operator : AR\AJ
 Sample : P4910-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:04:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.259	0.000	579087	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.443f	0.000	171845	0	<MDL	N.D. #
5) T	DICAMBA	0.000	7.931	0	3273177	N.D.	<MDL
6) T	MCP	7.664f	0.000	4832738	0	<MDL	N.D. #
7) T	MCPA	7.777	8.263f	298709	19744714	<MDL	3.188 #
8) T	DICHLORPROP	8.130	8.703f	109196	3160995	<MDL	2.164 #
10) T	Pentachlo...	8.642f	0.000	3741481	0	<MDL	N.D. #
12) T	2,4,5-T	9.522	0.000	895616	0	<MDL	N.D. #
13) T	2,4-DB	10.168f	0.000	5328062	0	1.955	N.D. #
15) T	Picloram	11.146	12.353	3682468	3320138	<MDL	<MDL #
16) T	DCPA	11.651f	12.353f	1539534	3320138	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 19:40
Operator : AR\AJ
Sample : P4910-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:04:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

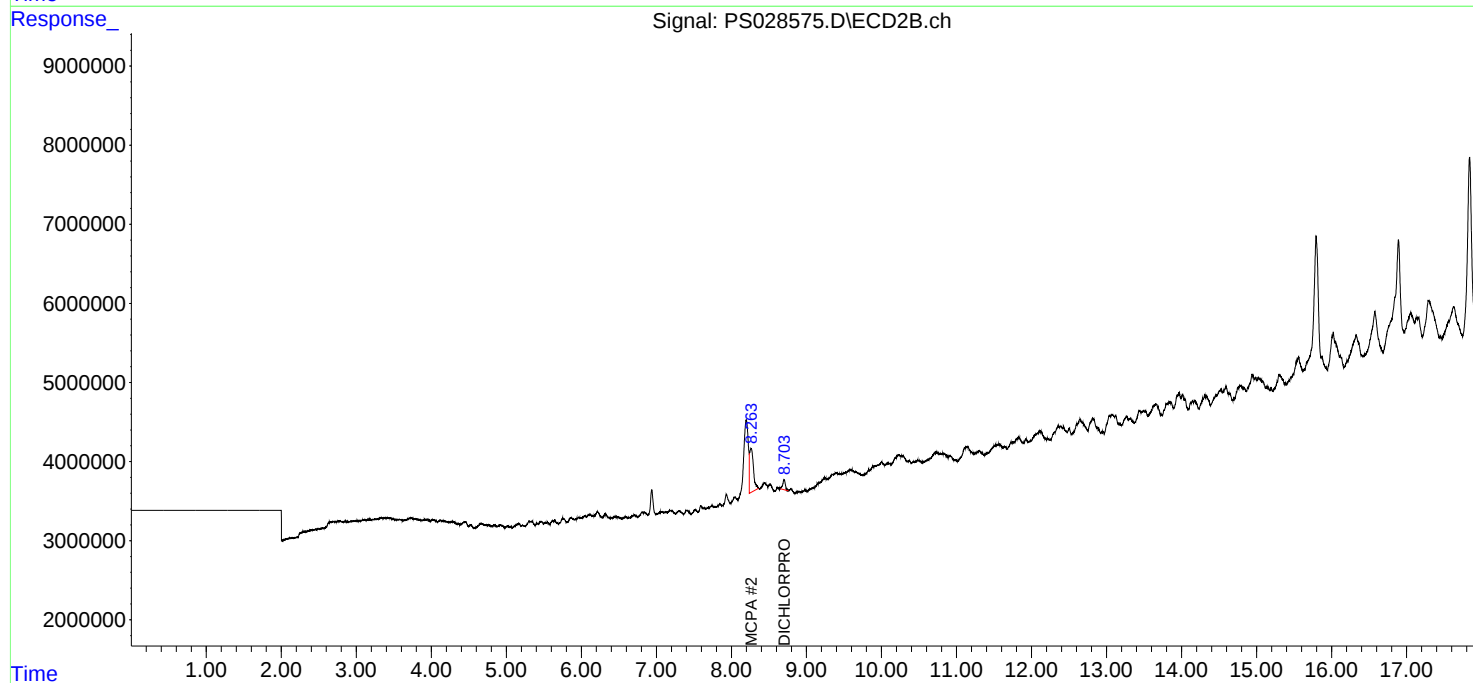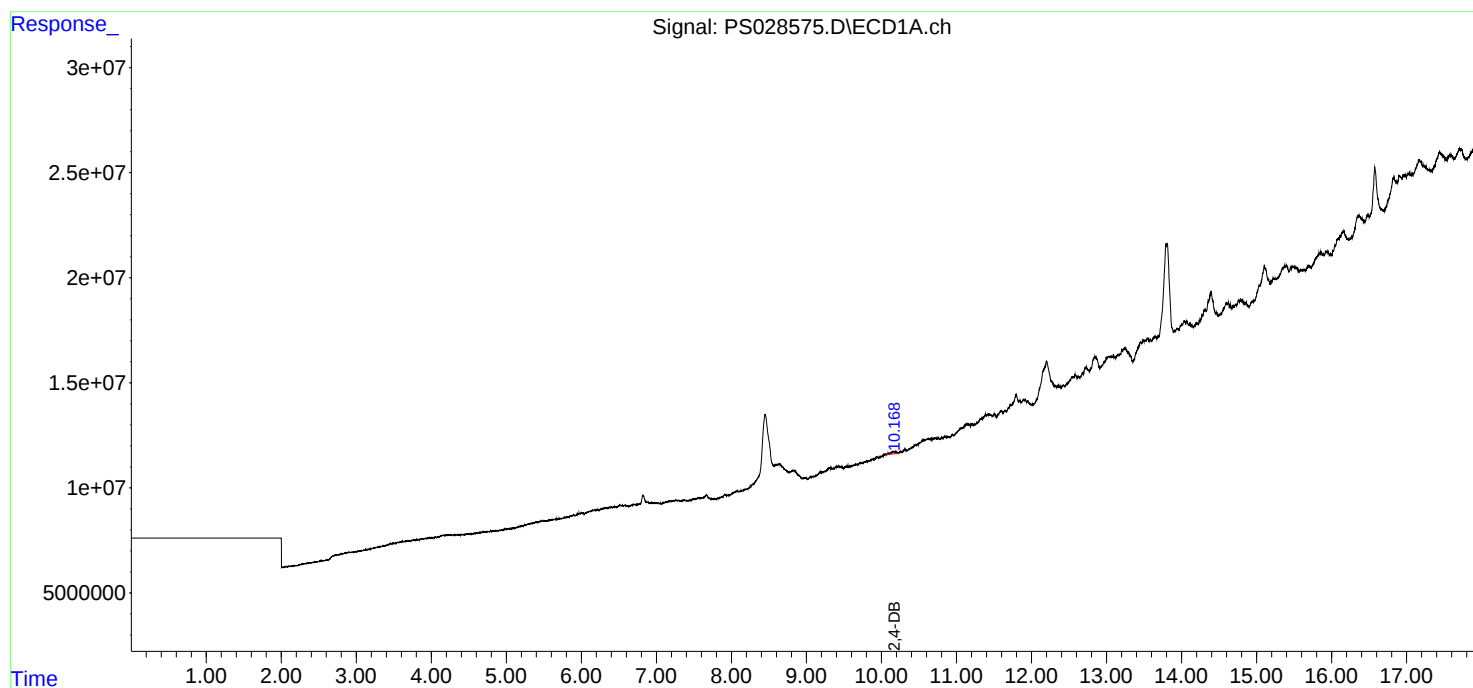


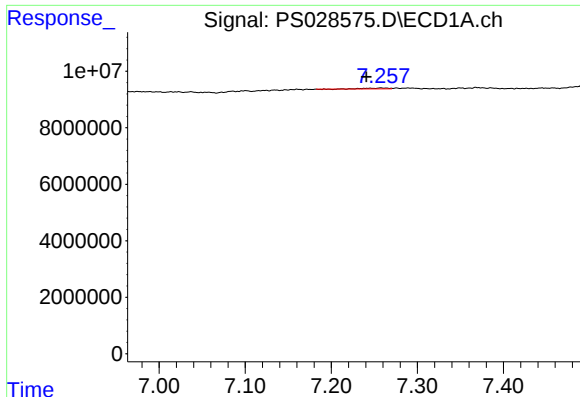

#4 2,4-DCAA


R.T.: 7.259 min
Delta R.T.: 0.018 min
Response: 579087
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

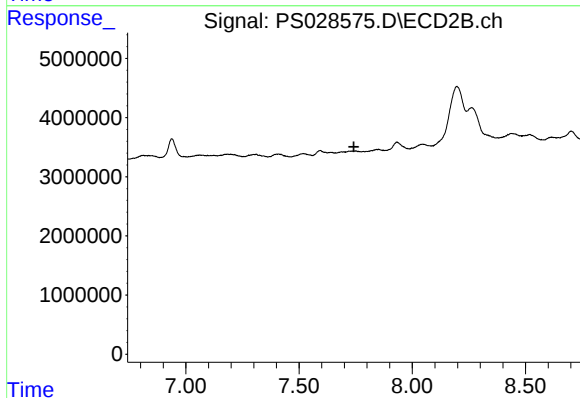


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.742 min
Response: 0
Conc: N.D.

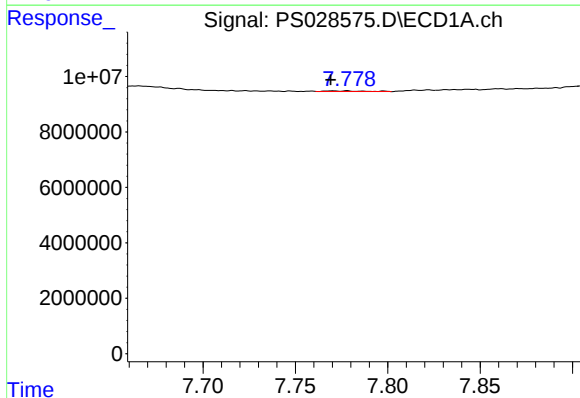


#7 MCPA

R.T.: 7.777 min
Delta R.T.: 0.008 min
Response: 298709
Conc: N.D.

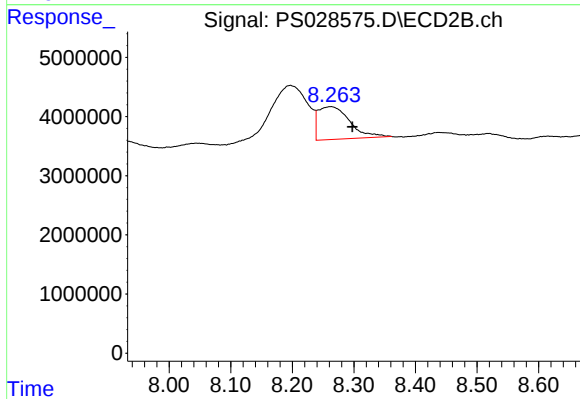

#7 MCPA


R.T.: 8.263 min
Delta R.T.: -0.035 min
Response: 19744714
Conc: 3.19 ug/ml

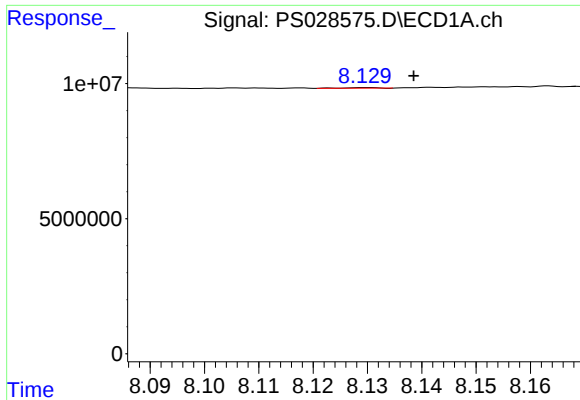

#8 DICHLORPROP


R.T.: 8.130 min
Delta R.T.: -0.009 min
Response: 109196
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

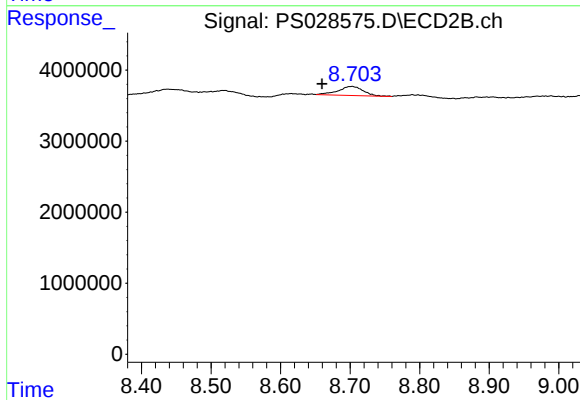


#8 DICHLORPROP

R.T.: 8.703 min
Delta R.T.: 0.043 min
Response: 3160995
Conc: 2.16 ng/ml

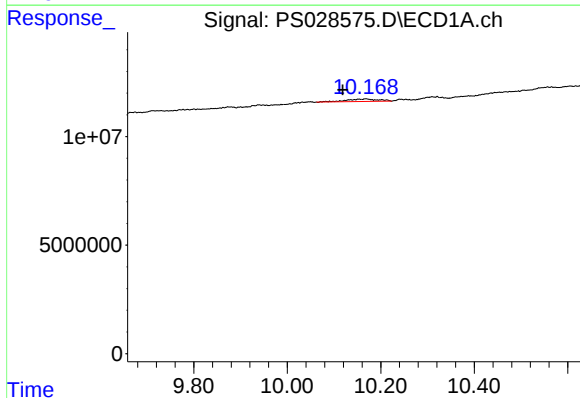

#13 2,4-DB

R.T.: 10.168 min
Delta R.T.: 0.050 min
Response: 5328062
Conc: 1.95 ng/ml

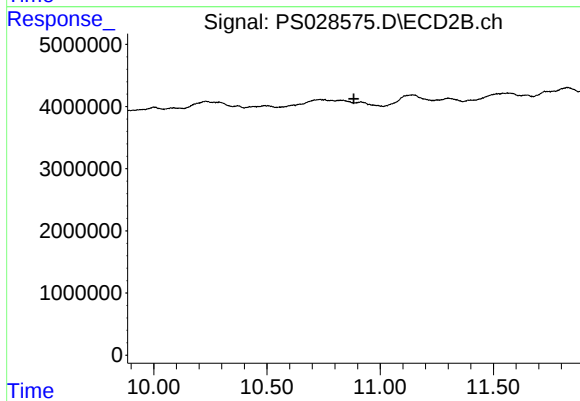

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.884 min
Response: 0
Conc: N.D.