

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 20:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:07:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.733	1438.1E6	656.7E6	562.649	508.168
Target Compounds							
1) T	Dalapon	2.671f	0.000	1336101	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.439f	0.000	34835	0	<MDL	N.D. #
3) T	4-Nitroph...	7.025	0.000	6670882	0	3.928	N.D. #
5) T	DICAMBA	0.000	7.928	0	3245133	N.D.	<MDL
6) T	MCPD	7.659f	0.000	21234446	0	3.019	N.D. #
7) T	MCPA	0.000	8.265f	0	11231783	N.D.	1.813
8) T	DICHLORPROP	8.089f	8.700f	800164	8437156	<MDL	5.777 #
10) T	Pentachlo...	8.695	0.000	541933	0	<MDL	N.D. #
12) T	2,4,5-T	9.547	0.000	599807	0	<MDL	N.D. #
14) T	DINOSEB	11.303f	0.000	3593151	0	<MDL	N.D. #
15) T	Picloram	11.127	12.348	10617163	11806561	<MDL	1.043 #
16) T	DCPA	11.602	12.348f	1108947	11806561	<MDL	1.217 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 20:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:07:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

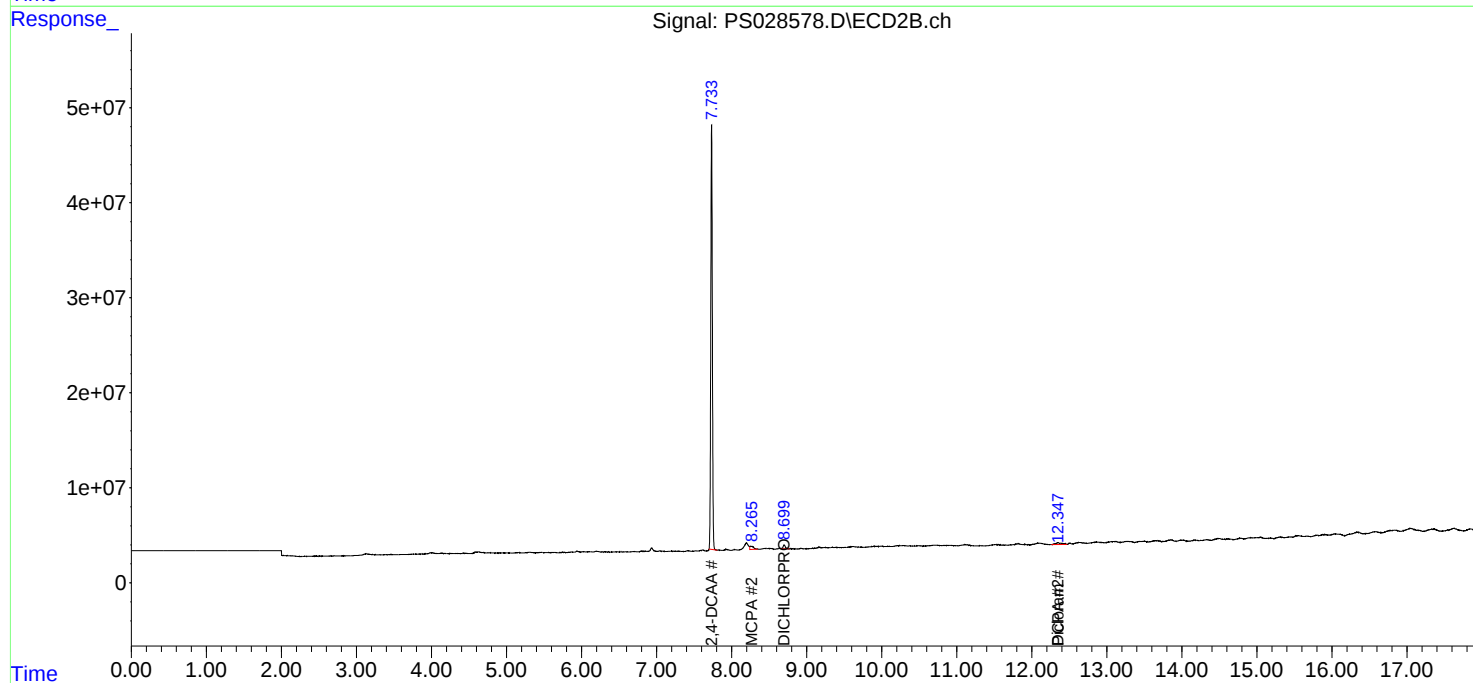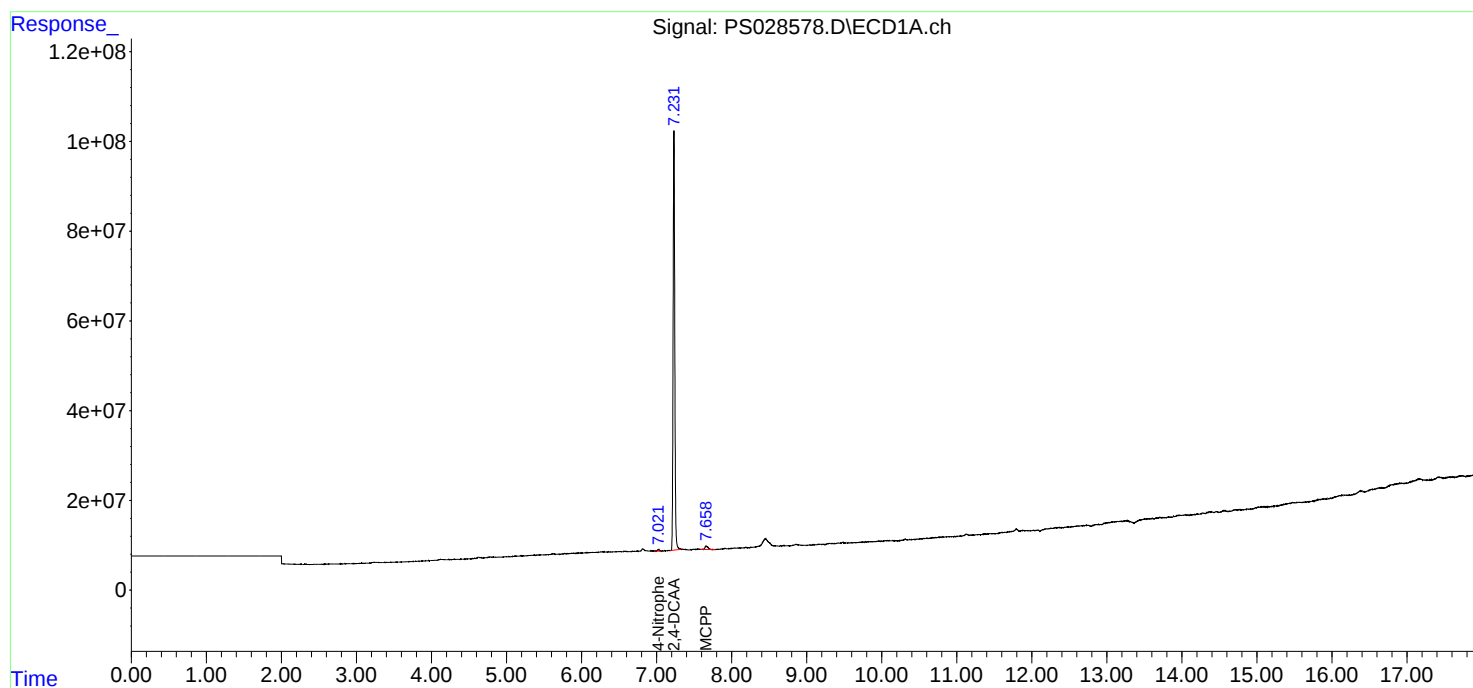


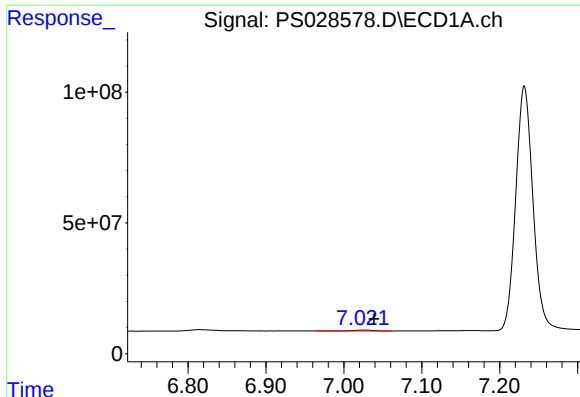

#3 4-Nitrophenol


R.T.: 7.025 min
Delta R.T.: -0.014 min
Response: 6670882
Conc: 3.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

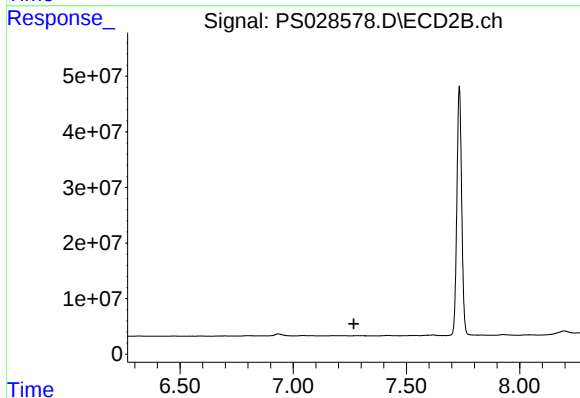


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

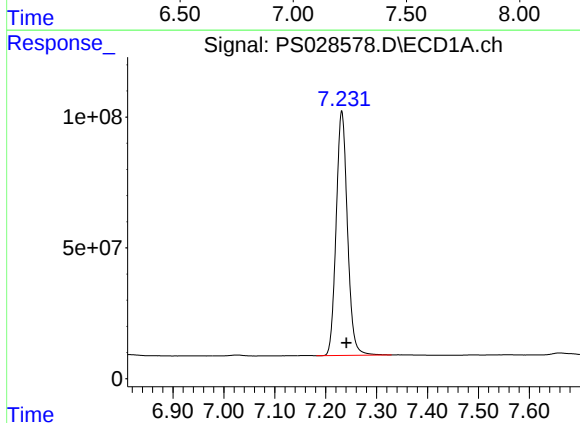


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.009 min
Response: 1438063248
Conc: 562.65 ng/ml

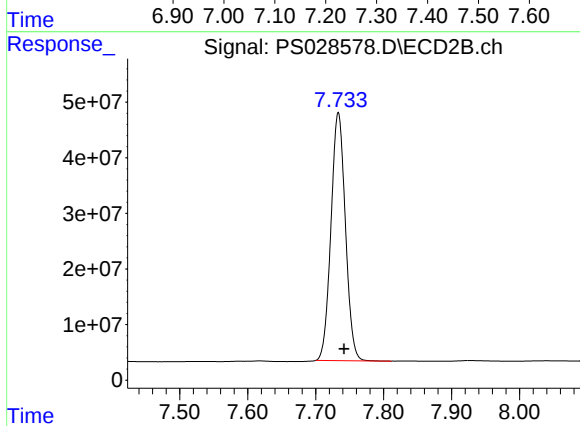

#4 2,4-DCAA


R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 656708413
Conc: 508.17 ng/ml

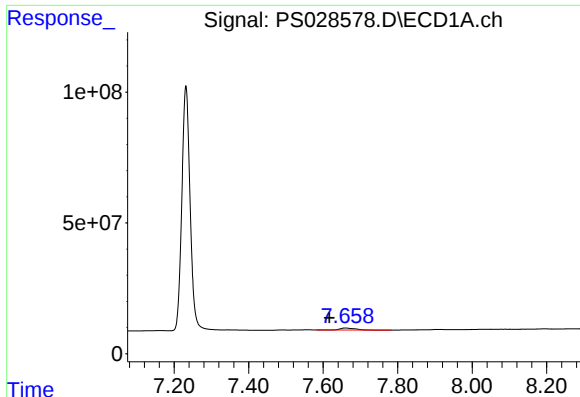

#6 MCPP


R.T.: 7.659 min
Delta R.T.: 0.042 min
Response: 21234446
Conc: 3.02 ug/ml

Instrument :
ECD_S
ClientSampleId :

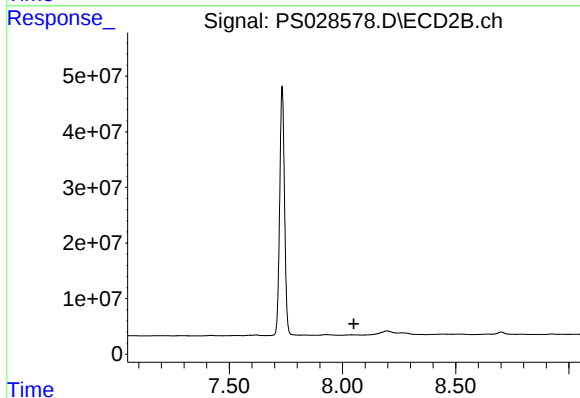


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

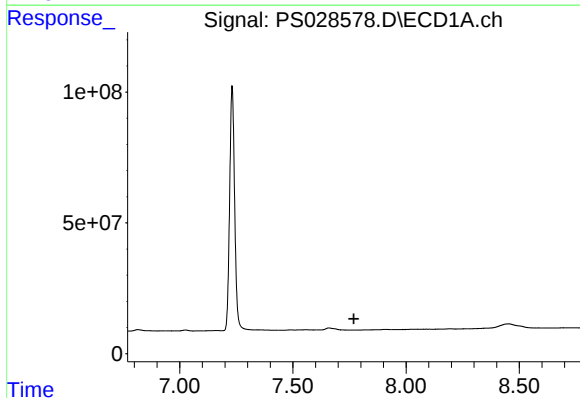


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.769 min
Response: 0
Conc: N.D.

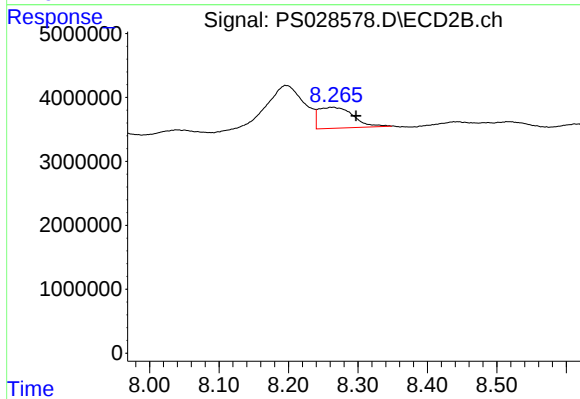

#7 MCPA


R.T.: 8.265 min
Delta R.T.: -0.033 min
Response: 11231783
Conc: 1.81 ug/ml

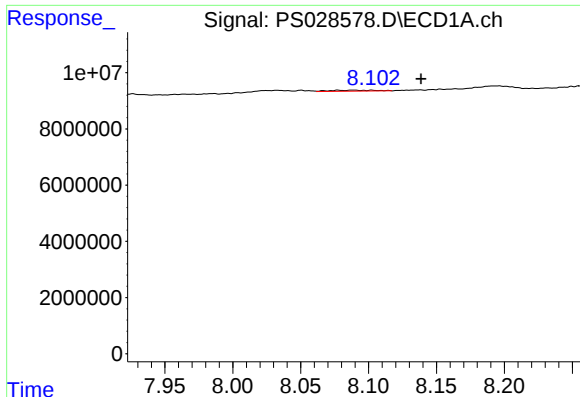

#8 DICHLORPROP


R.T.: 8.089 min
Delta R.T.: -0.050 min
Response: 800164
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

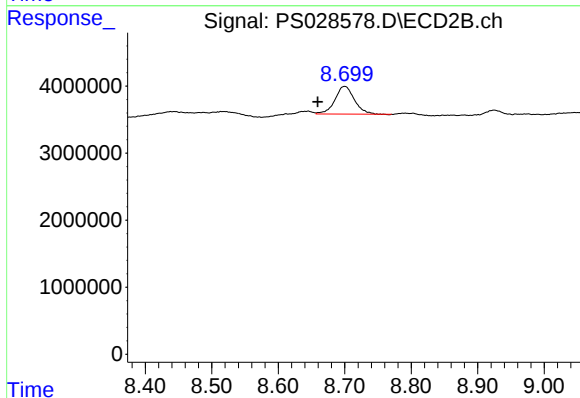


#8 DICHLORPROP

R.T.: 8.700 min
Delta R.T.: 0.040 min
Response: 8437156
Conc: 5.78 ng/ml

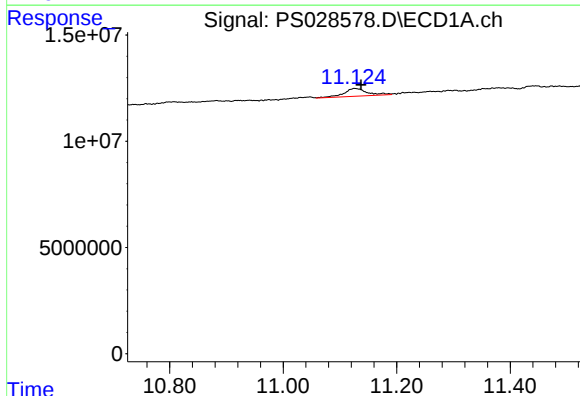


#15 Picloram

R.T.: 11.127 min
Delta R.T.: -0.011 min
Response: 10617163
Conc: N.D.

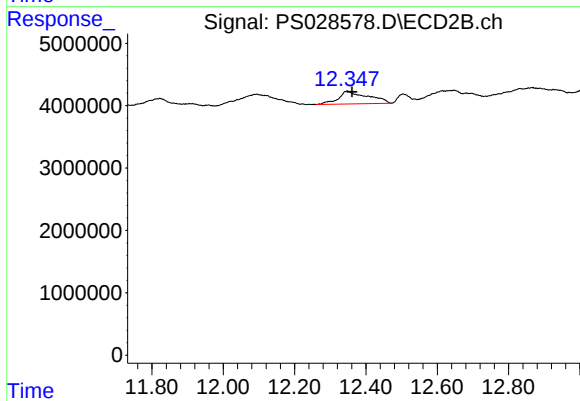

#15 Picloram


R.T.: 12.348 min
Delta R.T.: -0.013 min
Response: 11806561
Conc: 1.04 ng/ml

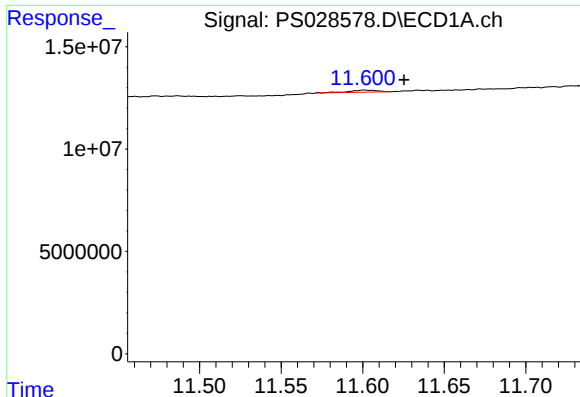

#16 DCPA

R.T.: 11.602 min
Delta R.T.: -0.023 min
Response: 1108947
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

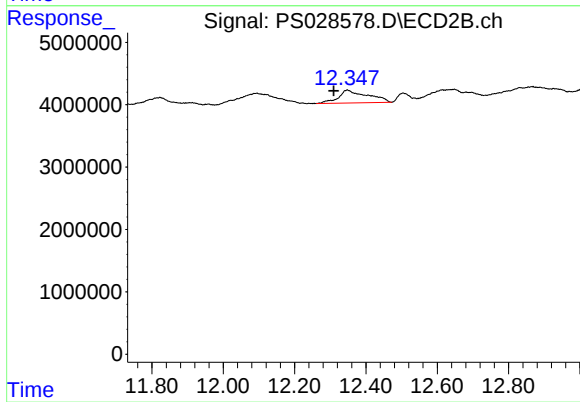

#16 DCPA

R.T.: 12.348 min
Delta R.T.: 0.038 min
Response: 11806561
Conc: 1.22 ng/ml