

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
 Data File : PS028586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 00:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:23:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	7.733	1450.4E6	665.1E6	567.462	514.675
Target Compounds							
1) T	Dalapon	2.635	0.000	1101196	0	<MDL	N.D. #
3) T	4-Nitroph...	7.027	0.000	4880957	0	2.874	N.D. #
5) T	DICAMBA	0.000	7.928	0	2770083	N.D.	<MDL
6) T	MCPD	7.658f	0.000	18543385	0	2.636	N.D. #
7) T	MCPA	0.000	8.252f	0	11903567	N.D.	1.922
8) T	DICHLORPROP	0.000	8.699f	0	6964408	N.D.	4.768
10) T	Pentachlo...	8.625f	9.510	7880475	5384018	<MDL	<MDL #
11) T	2,4,5-TP ...	9.218f	0.000	618121	0	<MDL	N.D. #
12) T	2,4,5-T	9.532	0.000	851675	0	<MDL	N.D. #
13) T	2,4-DB	10.089f	0.000	1140147	0	<MDL	N.D. #
14) T	DINOSEB	11.325	0.000	3518833	0	<MDL	N.D. #
15) T	Picloram	11.124	12.365	13443675	8645222	<MDL	<MDL #
16) T	DCPA	11.593f	0.000	1560380	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112024\
Data File : PS028586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 00:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:23:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

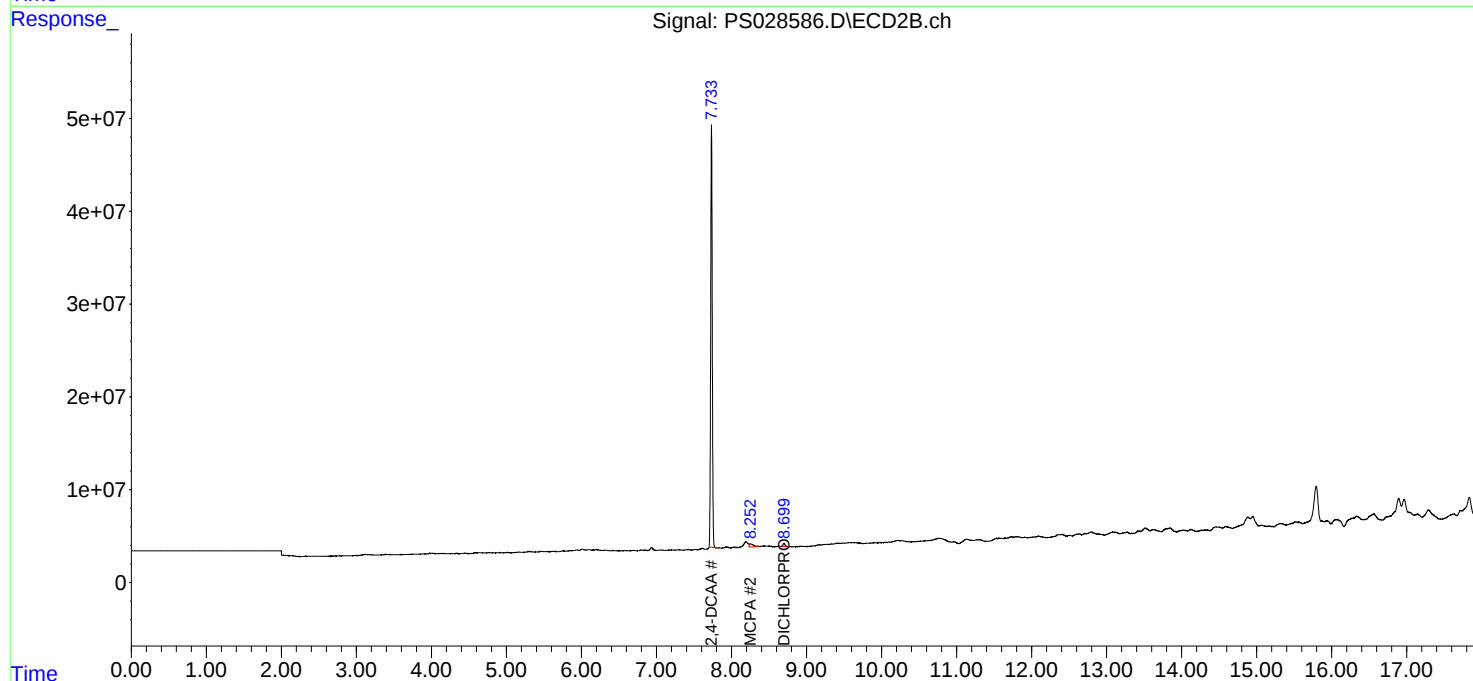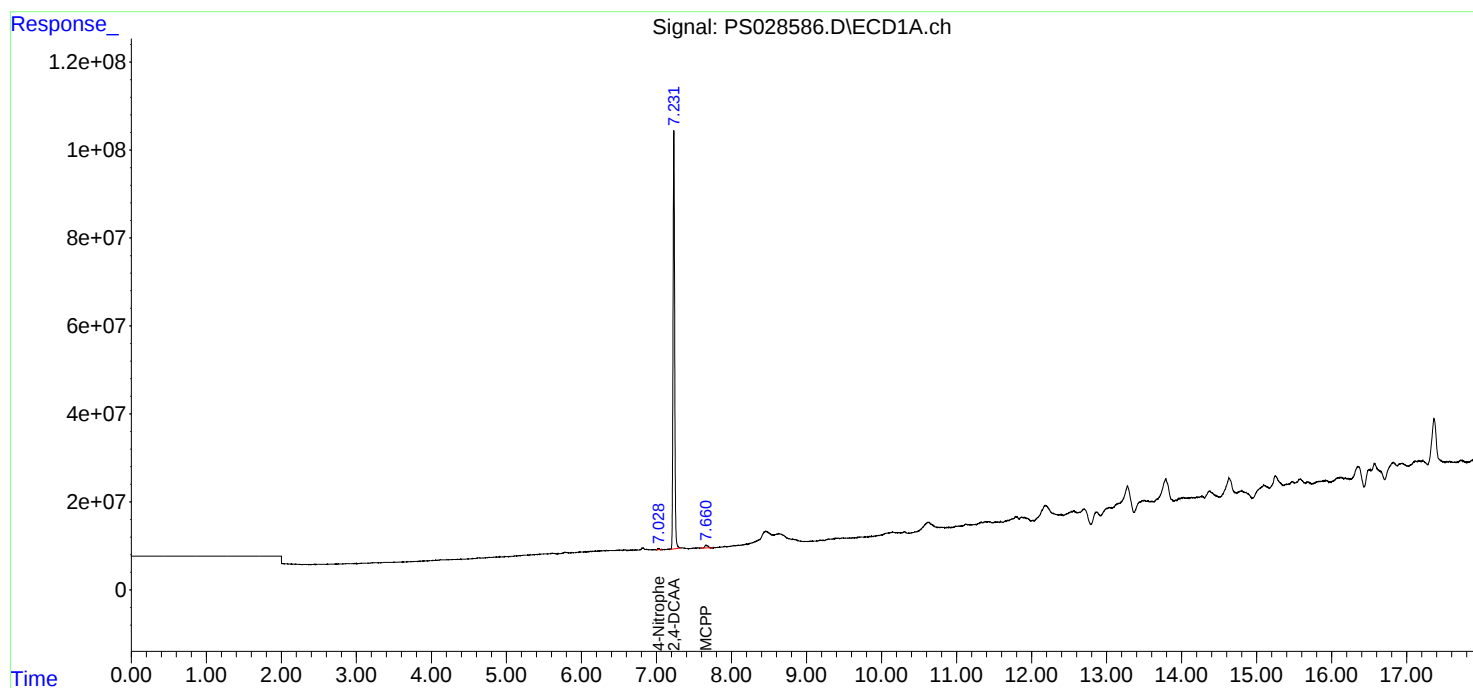


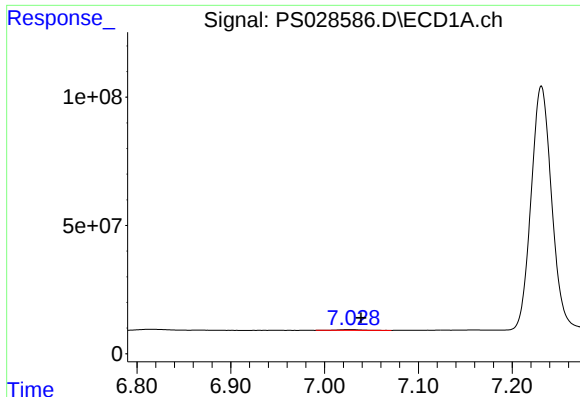

#3 4-Nitrophenol


R.T.: 7.027 min
Delta R.T.: -0.012 min
Response: 4880957
Conc: 2.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

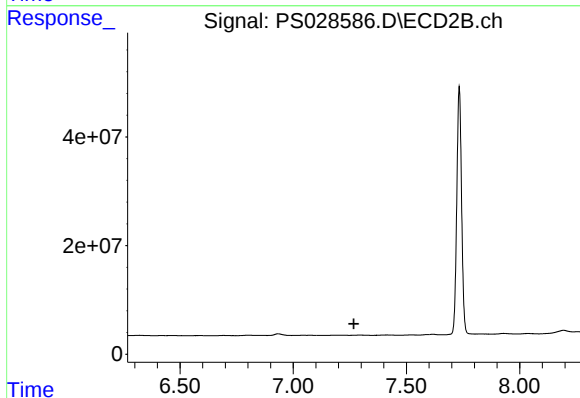


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

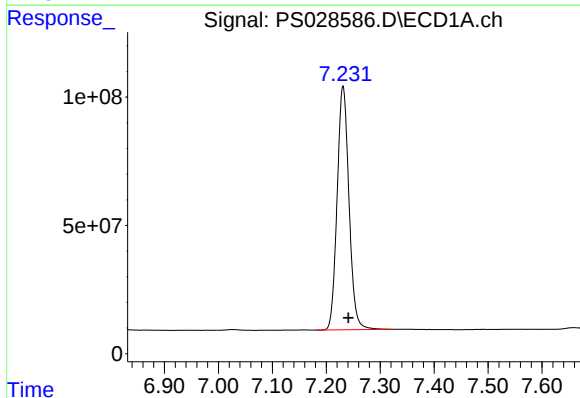


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.010 min
Response: 1450367106
Conc: 567.46 ng/ml

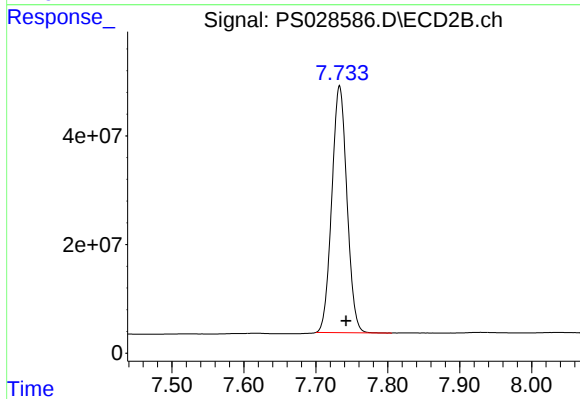

#4 2,4-DCAA


R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 665117173
Conc: 514.68 ng/ml

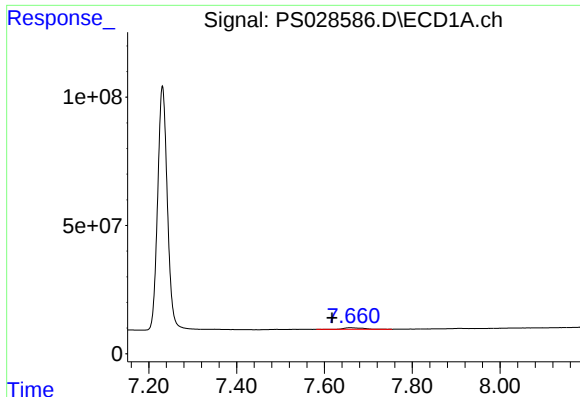

#6 MCPP


R.T.: 7.658 min
Delta R.T.: 0.041 min
Response: 18543385
Conc: 2.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

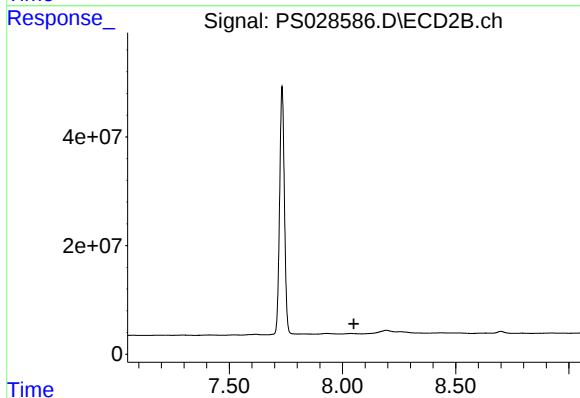


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

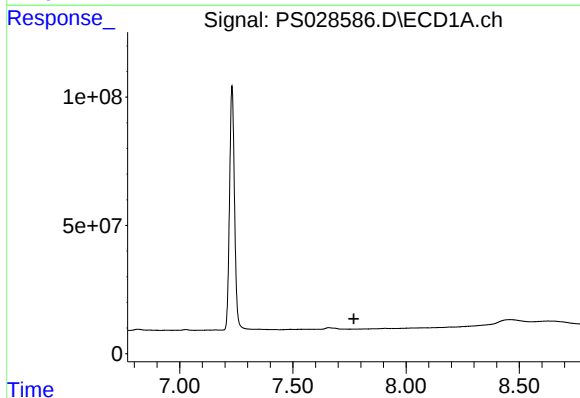


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.769 min
Response: 0
Conc: N.D.

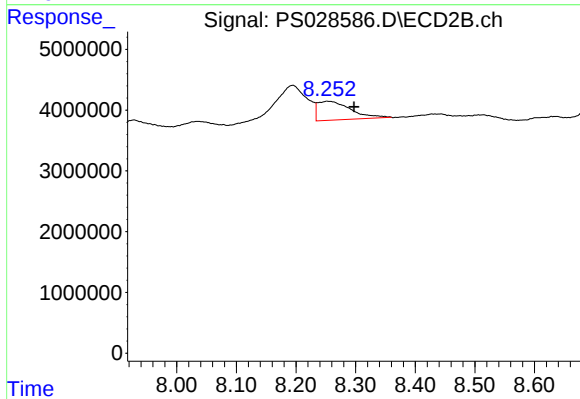

#7 MCPA


R.T.: 8.252 min
Delta R.T.: -0.045 min
Response: 11903567
Conc: 1.92 ug/ml

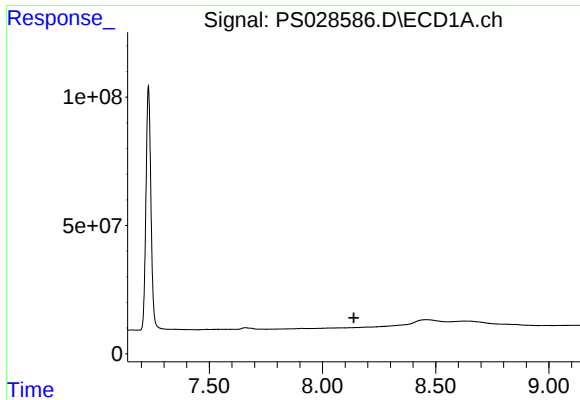

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

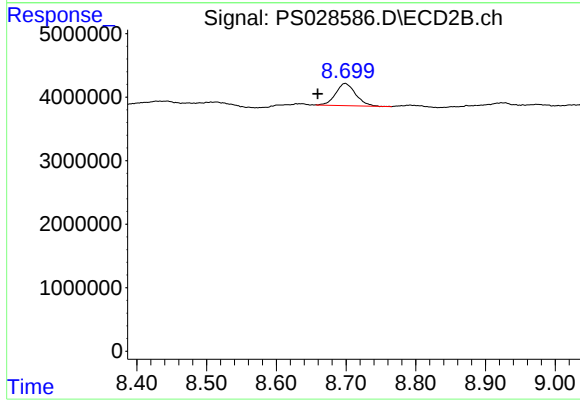

#8 DICHLORPROP

R.T.: 8.699 min
Delta R.T.: 0.039 min
Response: 6964408
Conc: 4.77 ng/ml