

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112025\
 Data File : PS032499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2025 10:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 04:08:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.624	1710.1E6	1970.3E6	377.410	540.489 #
Target Compounds							
1) T	Dalapon	2.702f	0.000	41267828	0	5.749	N.D. #
2) T	3,5-DICHL...	6.443	0.000	31726977	0	4.907	N.D. #
3) T	4-Nitroph...	7.129f	0.000	92213	0	<MDL	N.D. #
6) T	MCP	7.676f	7.911	173594	47307473	<MDL	3.557 #
7) T	MCPA	0.000	8.107f	0	2716900	N.D.	<MDL
9) T	2,4-D	0.000	8.876	0	4050241	N.D.	<MDL
10) T	Pentachlo...	8.712	9.365	4854977	3319384	<MDL	<MDL #
11) T	2,4,5-TP ...	9.272	0.000	3675557	0	<MDL	N.D. #
12) T	2,4,5-T	9.615f	10.142f	6257441	1791390	<MDL	<MDL #
13) T	2,4-DB	10.139	0.000	1824987	0	<MDL	N.D. #
14) T	DINOSEB	11.340	11.122	8156937	1890566	<MDL	<MDL #
15) T	Picloram	11.201	12.227	32304931	28305800	1.522	<MDL #
16) T	DCPA	11.644	0.000	6919289	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112025\
Data File : PS032499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2025 10:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 04:08:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

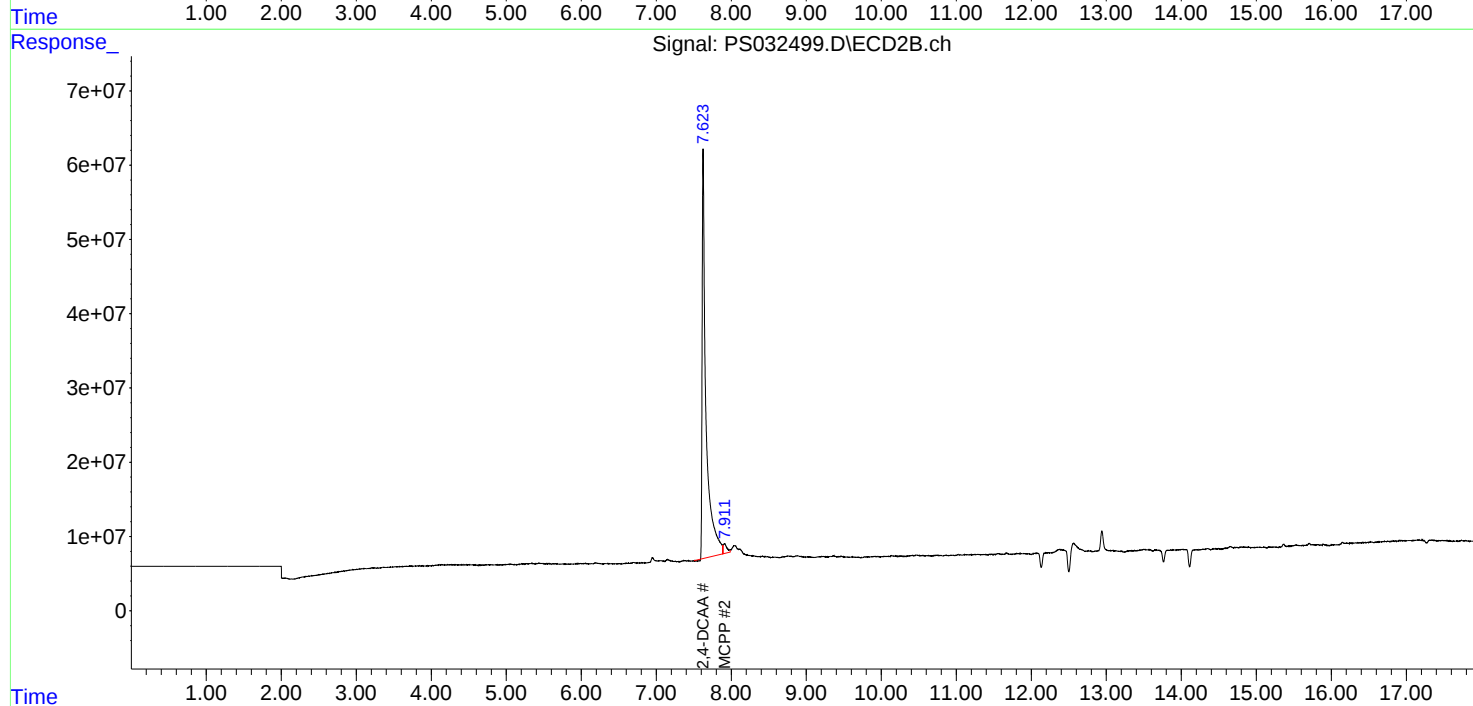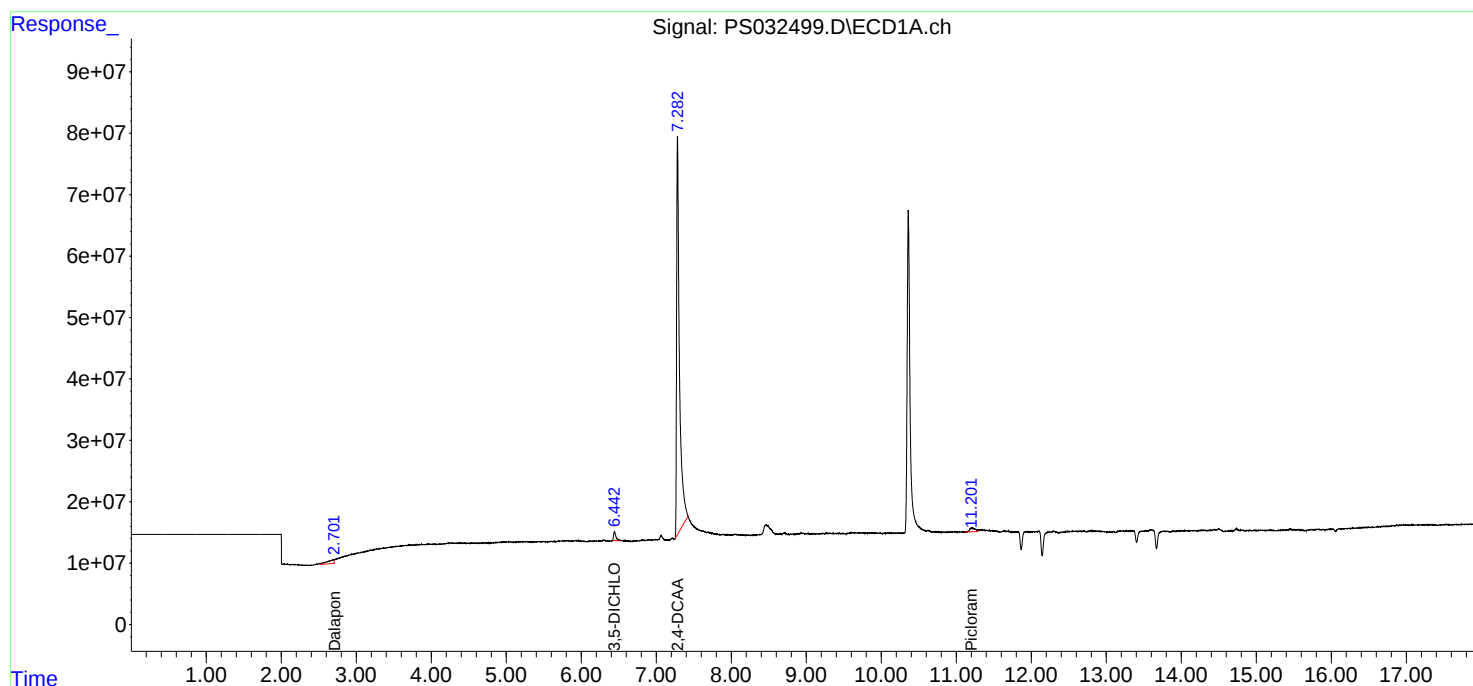


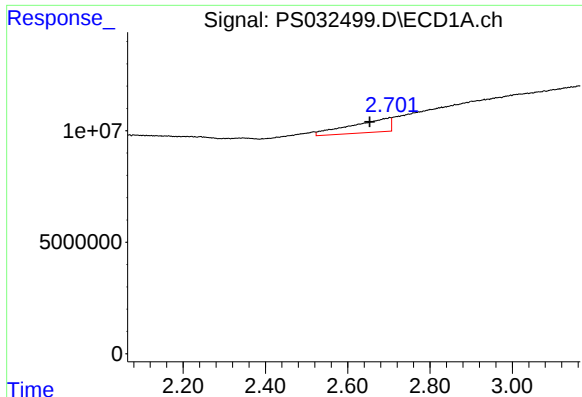

#1 Dalapon


R.T.: 2.702 min
Delta R.T.: 0.048 min
Response: 41267828
Conc: 5.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

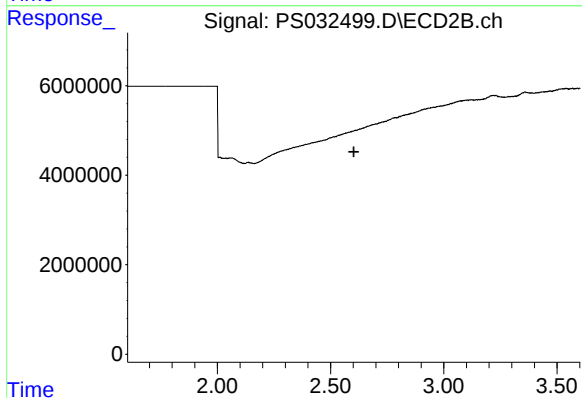


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.603 min
Response: 0
Conc: N.D.

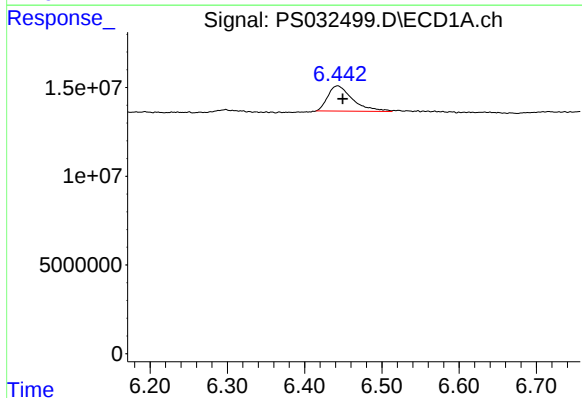


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.443 min
Delta R.T.: -0.006 min
Response: 31726977
Conc: 4.91 ng/ml

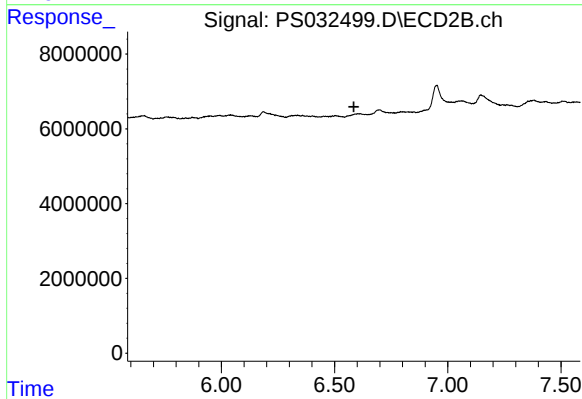

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

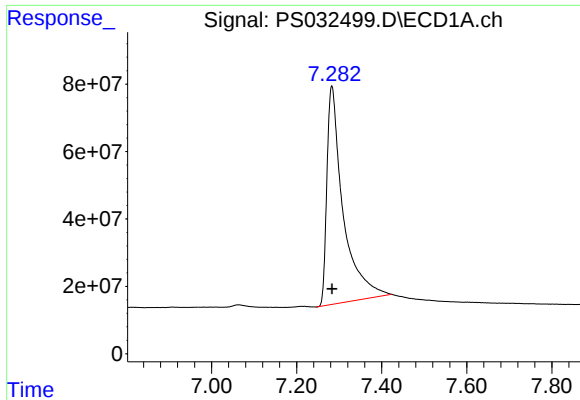

#4 2,4-DCAA


R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1710149319
Conc: 377.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

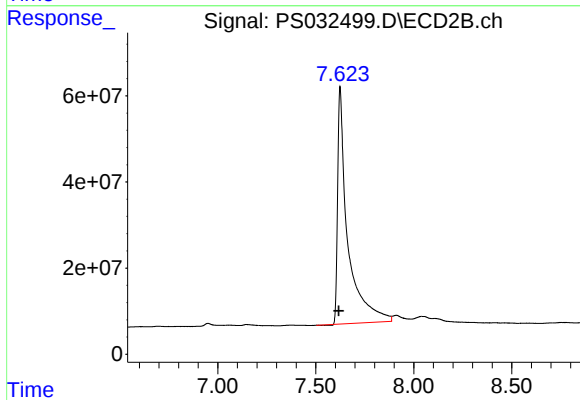


#4 2,4-DCAA

R.T.: 7.624 min
Delta R.T.: 0.007 min
Response: 1970349038
Conc: 540.49 ng/ml

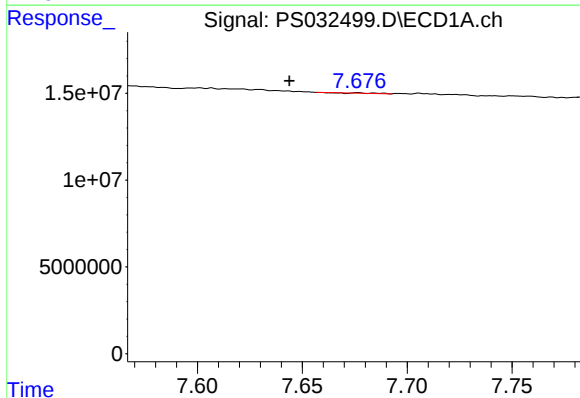


#6 MCPP

R.T.: 7.676 min
Delta R.T.: 0.033 min
Response: 173594
Conc: N.D.

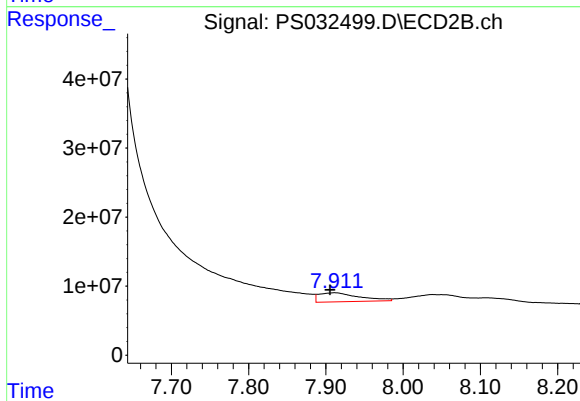

#6 MCPP


R.T.: 7.911 min
Delta R.T.: 0.006 min
Response: 47307473
Conc: 3.56 ug/ml

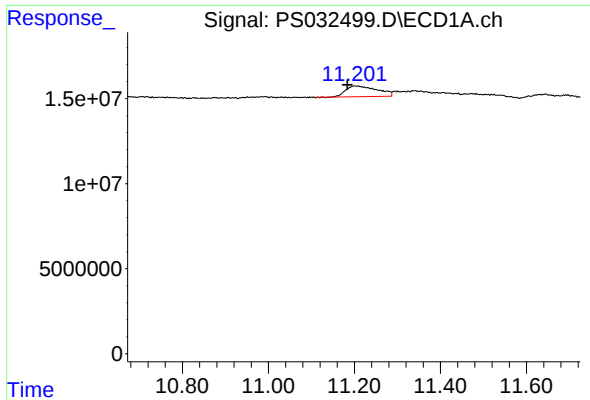

#15 Picloram

R.T.: 11.201 min
Delta R.T.: 0.017 min
Response: 32304931
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

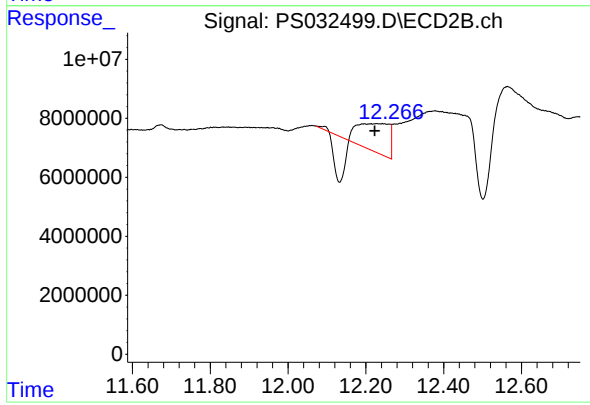

#15 Picloram

R.T.: 12.227 min
Delta R.T.: 0.004 min
Response: 28305800
Conc: N.D.