

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112025\
 Data File : PS032508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2025 20:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 04:10:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.276	7.618	1810.2E6	1893.4E6	399.492	519.377 #
Target Compounds							
2) T	3,5-DICHL...	6.436	0.000	7700650	0	1.191	N.D. #
7) T	MCPA	7.789	0.000	4175640	0	<MDL	N.D. #
8) T	DICHLORPROP	8.163	0.000	154220	0	<MDL	N.D. #
9) T	2,4-D	0.000	8.857	0	9359973	N.D.	1.784
10) T	Pentachlo...	8.711	9.361	3344555	3379744	<MDL	<MDL #
11) T	2,4,5-TP ...	9.278	0.000	8485376	0	<MDL	N.D. #
12) T	2,4,5-T	9.576	10.141f	1624908	6238834	<MDL	<MDL #
13) T	2,4-DB	10.161	0.000	9046742	0	3.433	N.D. #
14) T	DINOSEB	11.342	0.000	2389058	0	<MDL	N.D. #
15) T	Picloram	11.157f	12.271f	20801495	298.6E6	<MDL	8.032 #
16) T	DCPA	11.632	12.095f	706735	54770474	<MDL	1.719 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112025\
Data File : PS032508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2025 20:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 04:10:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

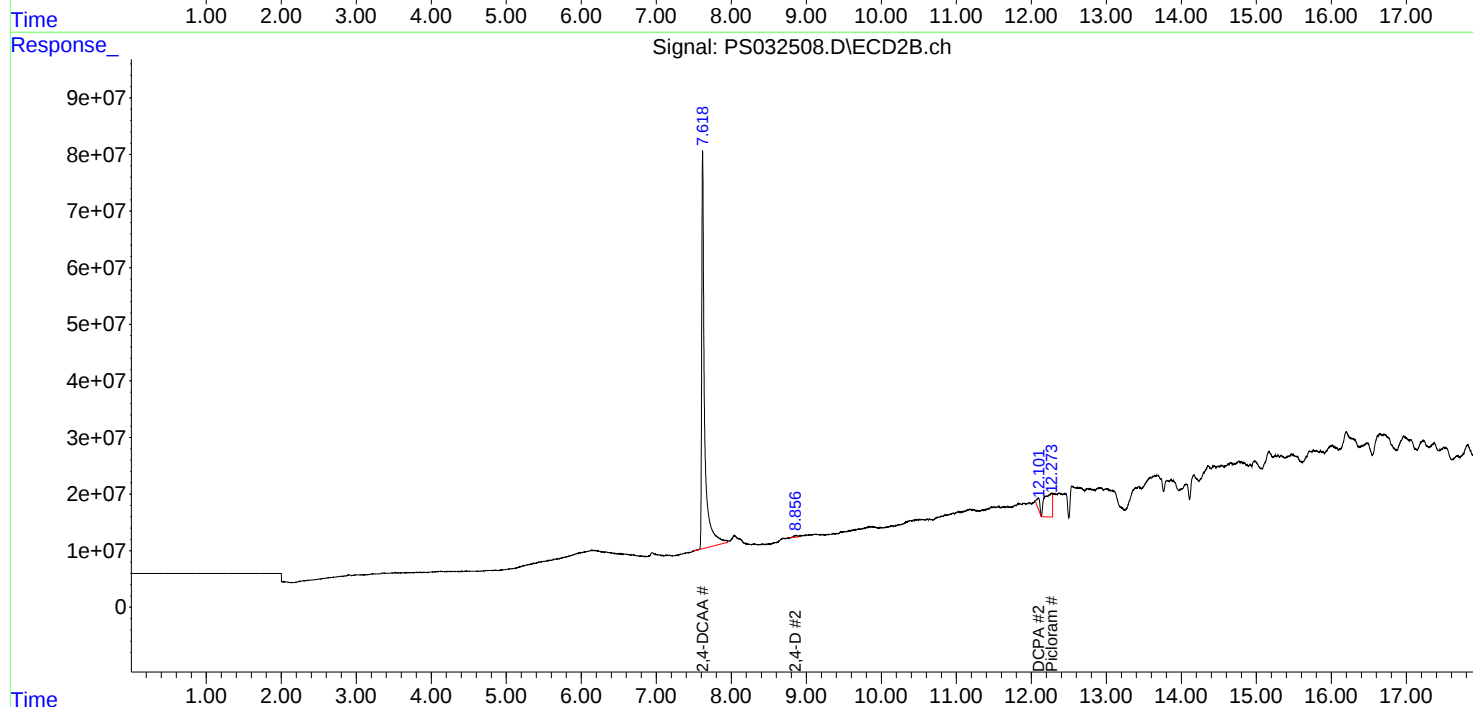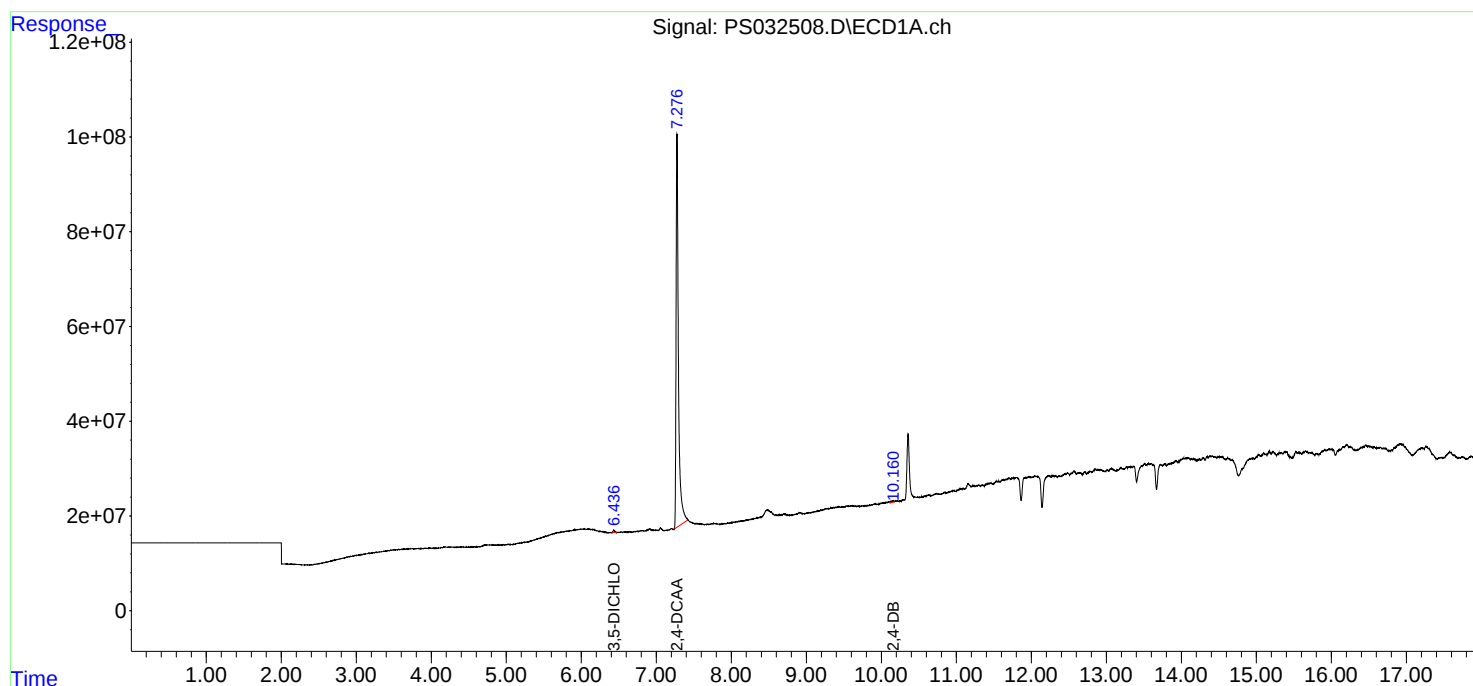


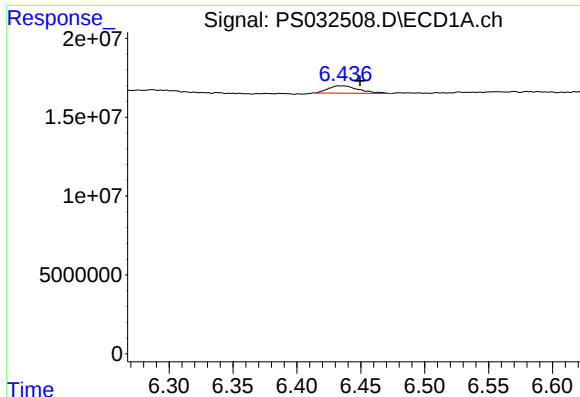

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.436 min
Delta R.T.: -0.014 min
Response: 7700650
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

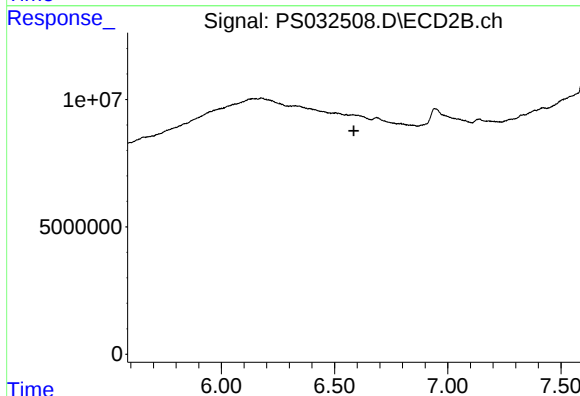


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

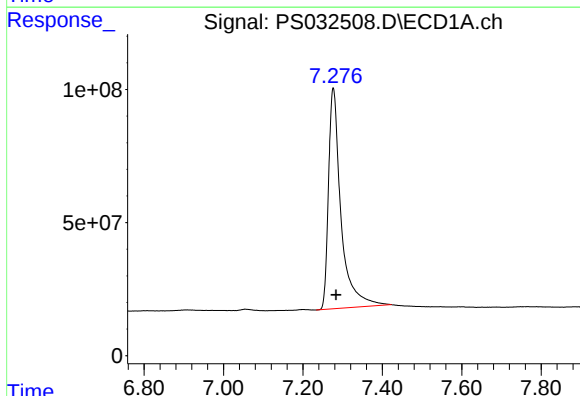


#4 2,4-DCAA

R.T.: 7.276 min
Delta R.T.: -0.007 min
Response: 1810209645
Conc: 399.49 ng/ml

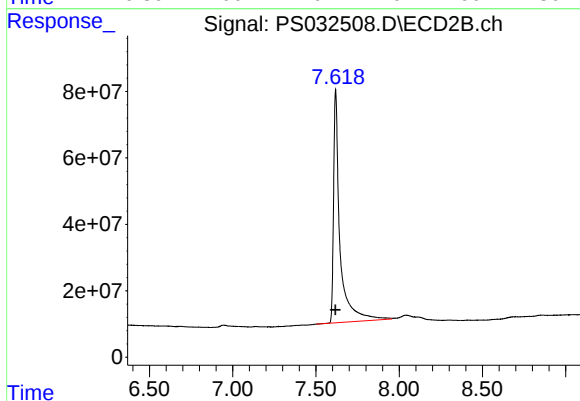

#4 2,4-DCAA


R.T.: 7.618 min
Delta R.T.: 0.000 min
Response: 1893387230
Conc: 519.38 ng/ml

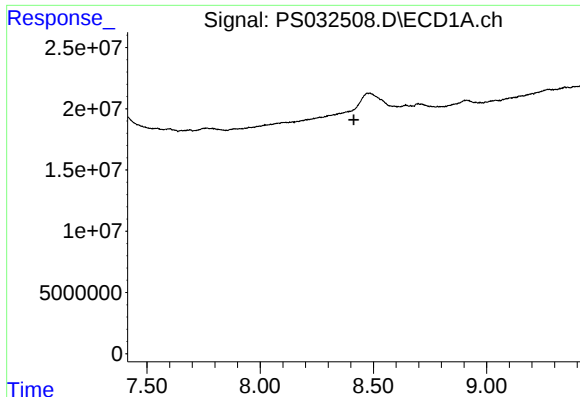

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

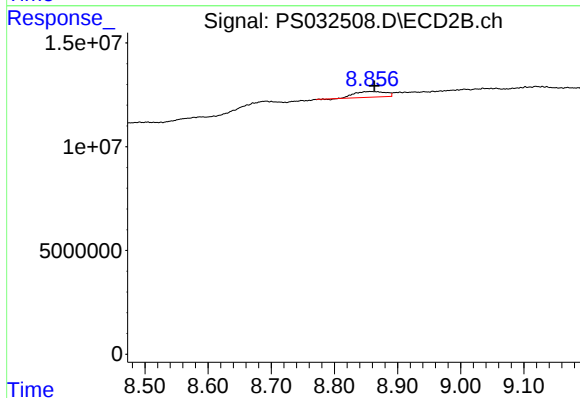


#9 2,4-D

R.T.: 8.857 min
Delta R.T.: -0.007 min
Response: 9359973
Conc: 1.78 ng/ml

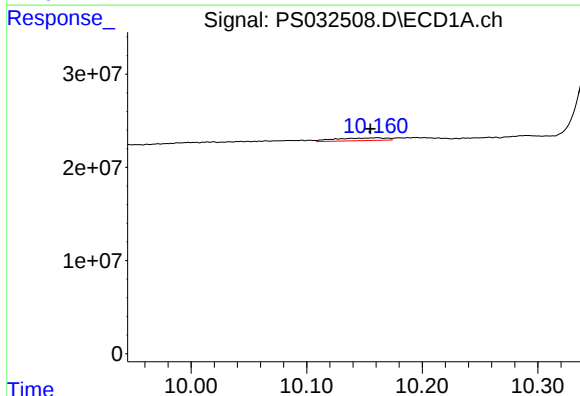


#13 2,4-DB

R.T.: 10.161 min
Delta R.T.: 0.006 min
Response: 9046742
Conc: 3.43 ng/ml

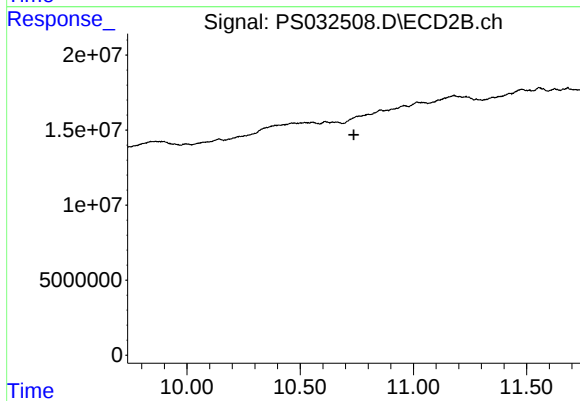

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.737 min
Response: 0
Conc: N.D.

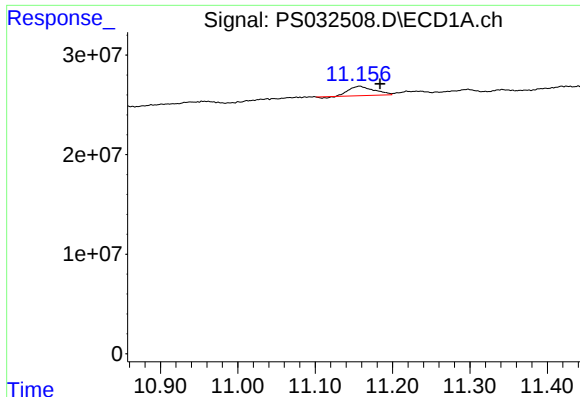

#15 Picloram


R.T.: 11.157 min
Delta R.T.: -0.027 min
Response: 20801495
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

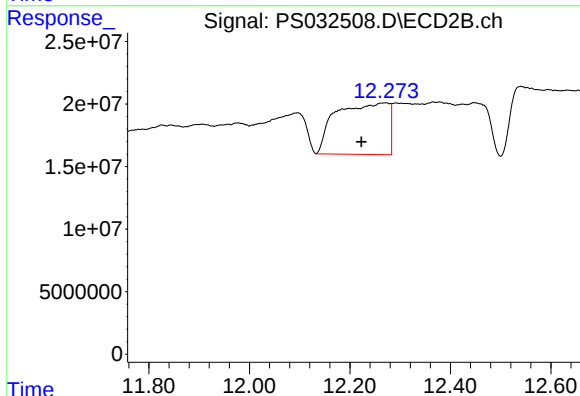


#15 Picloram

R.T.: 12.271 min
Delta R.T.: 0.047 min
Response: 298635399
Conc: 8.03 ng/ml

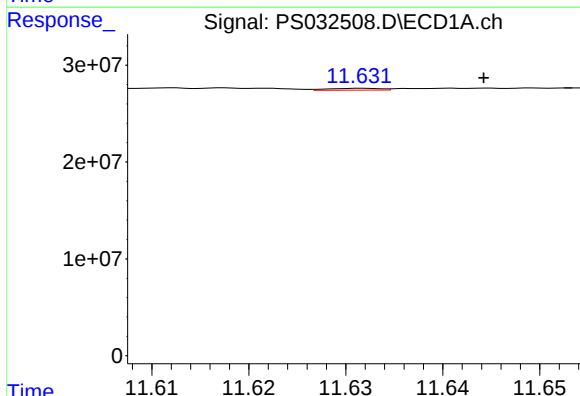

#16 DCPA

R.T.: 11.632 min
Delta R.T.: -0.012 min
Response: 706735
Conc: N.D.

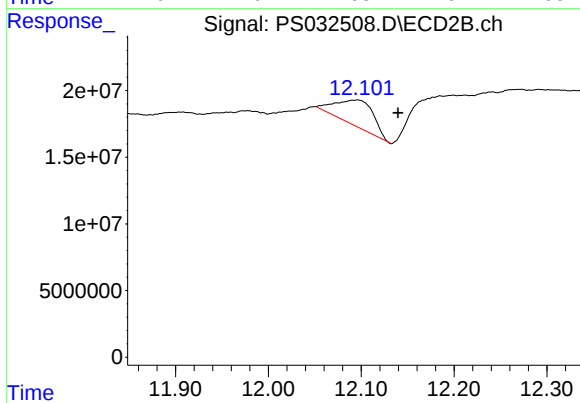

#16 DCPA

R.T.: 12.095 min
Delta R.T.: -0.045 min
Response: 54770474
Conc: 1.72 ng/ml