

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112118\
 Data File : PS002461.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 11:07
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 04:19:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.943	0	66693	N.D.	0.182 #
Target Compounds							
3) T	4-Nitroph...	11.007	10.076	4057167	140818	25.005	0.804 #
5) T	DICAMBA	0.000	11.215	0	198044	N.D.	0.146 #
6) T	MCP	0.000	11.451	0	447176	N.D.	0.493 #
8) T	DICHLORPROP	0.000	12.347	0	116915	N.D.	0.353 #
9) T	2,4-D	0.000	12.809	0	47381	N.D.	0.119 #
10) T	Pentachlo...	0.000	13.396	0	98494	N.D.	0.019 #
11) T	2,4,5-TP ...	0.000	13.938	0	193930	N.D.	0.096 #
14) T	DINOSEB	0.000	15.603	0	158085	N.D.	0.106 #
15) T	Picloram	0.000	16.804	0	795707	N.D.	0.299 #
16) T	DCPA	0.000	16.817	0	538930	N.D.	0.225 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112118\
Data File : PS002461.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 11:07
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 04:19:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

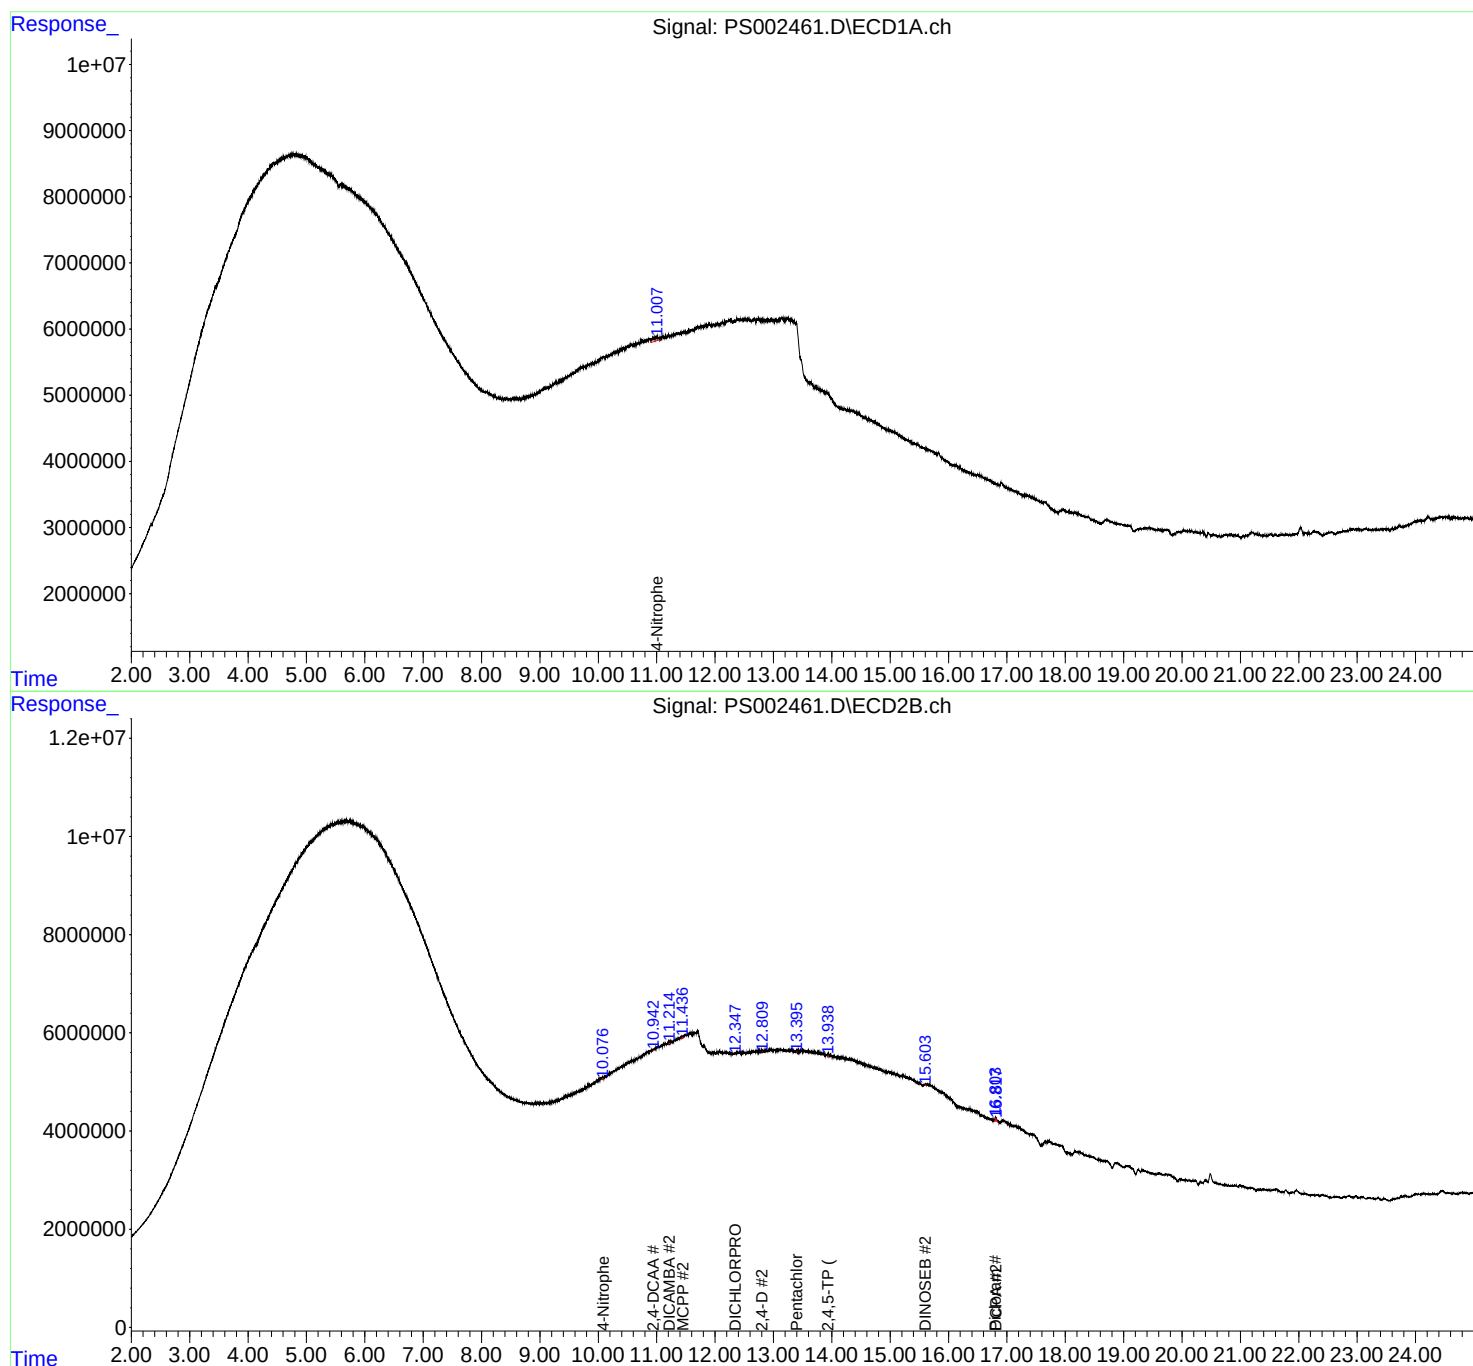


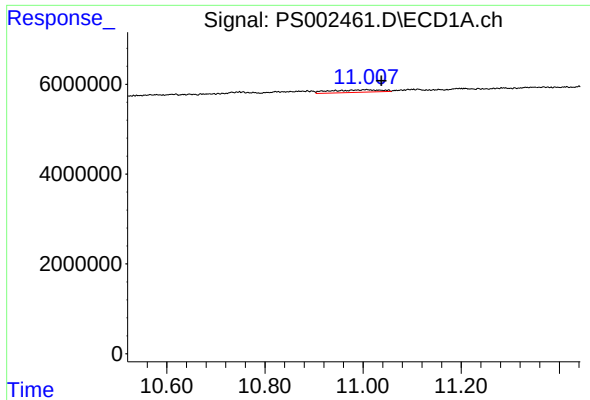

#3 4-Nitrophenol


R.T.: 11.007 min
Delta R.T.: -0.030 min
Response: 4057167
Conc: 25.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

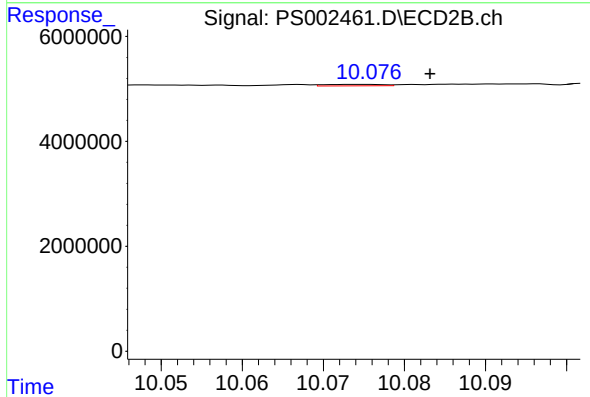


#3 4-Nitrophenol

R.T.: 10.076 min
Delta R.T.: -0.008 min
Response: 140818
Conc: 0.80 ng/ml

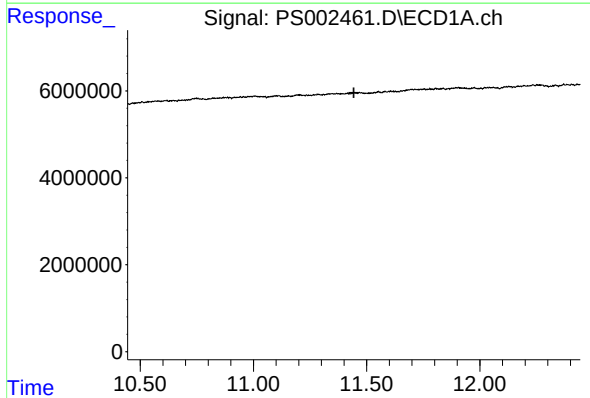


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.444 min
Response: 0
Conc: N.D.

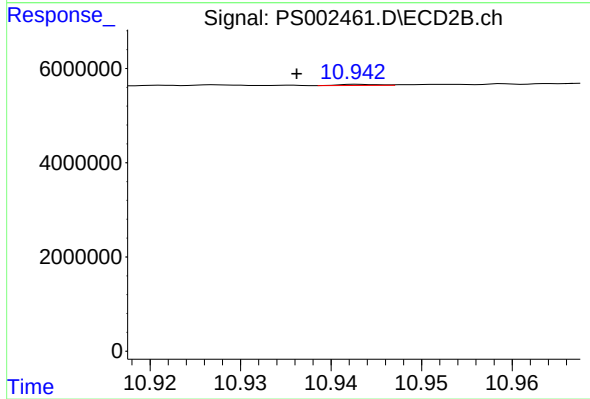

#4 2,4-DCAA


R.T.: 10.943 min
Delta R.T.: 0.007 min
Response: 66693
Conc: 0.18 ng/ml

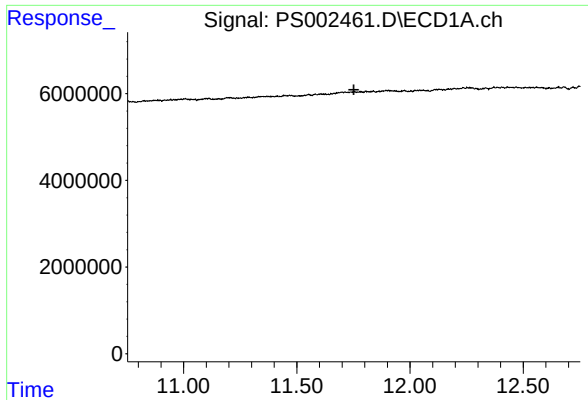

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

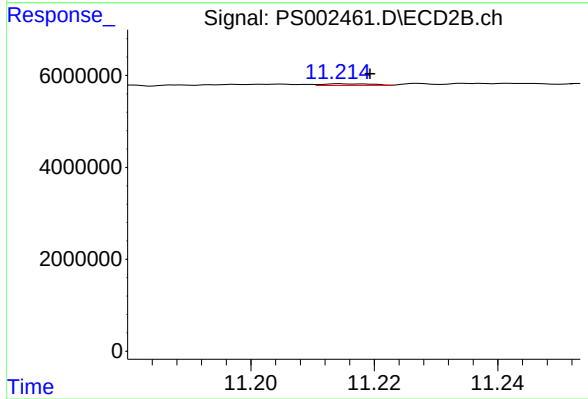


#5 DICAMBA

R.T.: 11.215 min
Delta R.T.: -0.005 min
Response: 198044
Conc: 0.15 ng/ml

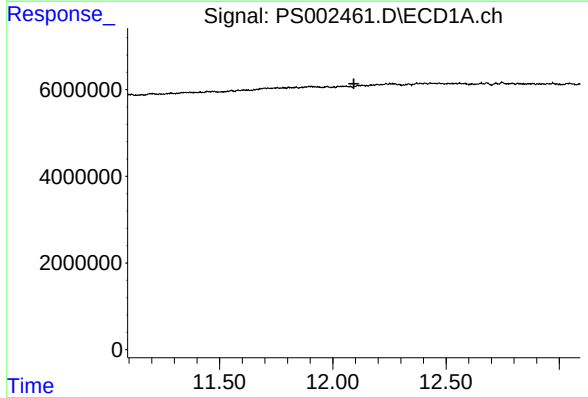


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.093 min
Response: 0
Conc: N.D.

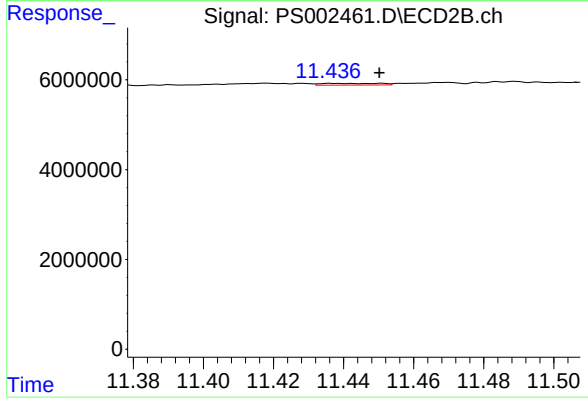

#6 MCP


R.T.: 11.451 min
Delta R.T.: 0.000 min
Response: 447176
Conc: 0.49 ug/ml

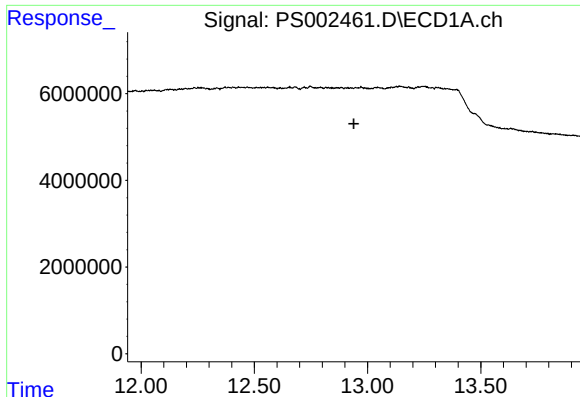

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

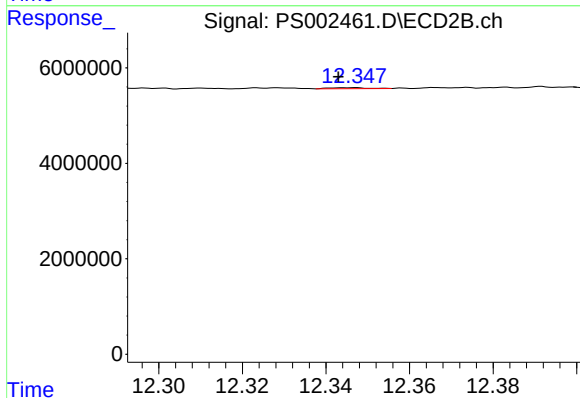


#8 DICHLORPROP

R.T.: 12.347 min
Delta R.T.: 0.004 min
Response: 116915
Conc: 0.35 ng/ml

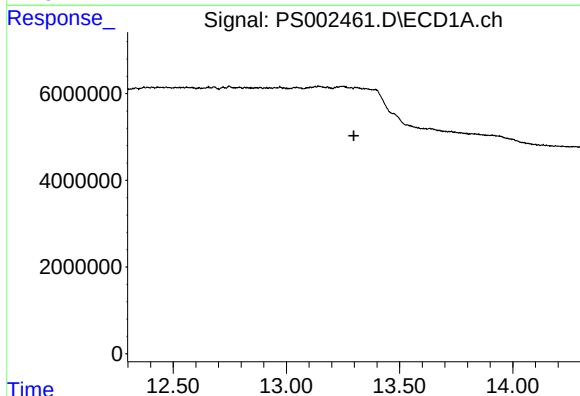


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

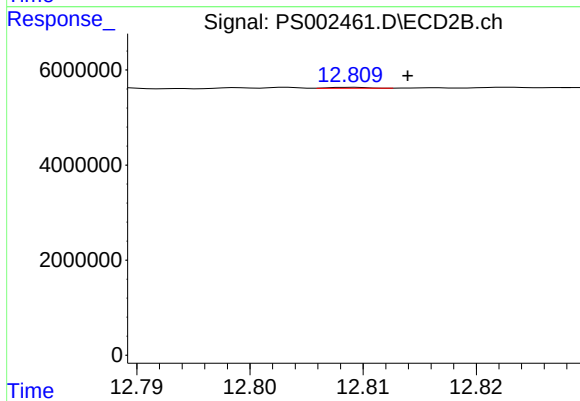

#9 2,4-D


R.T.: 12.809 min
Delta R.T.: -0.005 min
Response: 47381
Conc: 0.12 ng/ml

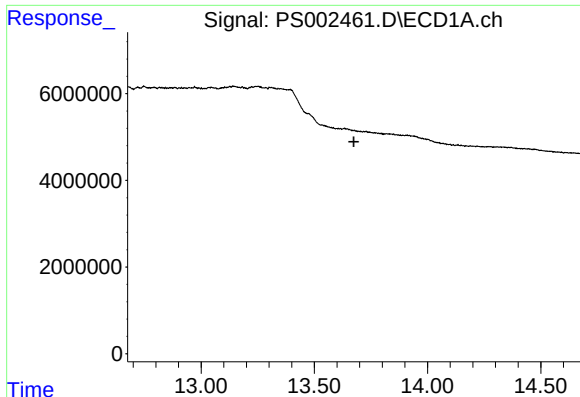

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

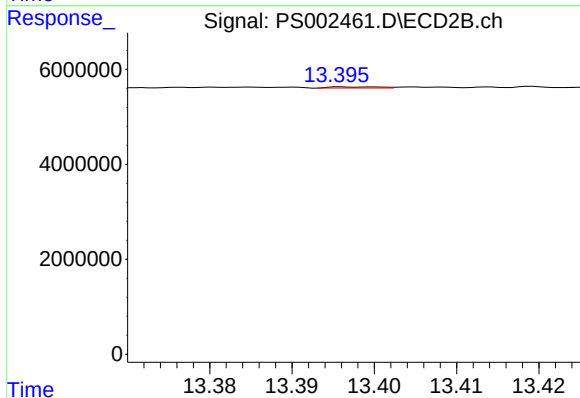


#10 Pentachlorophenol

R.T.: 13.396 min
Delta R.T.: 0.037 min
Response: 98494
Conc: 0.02 ng/ml

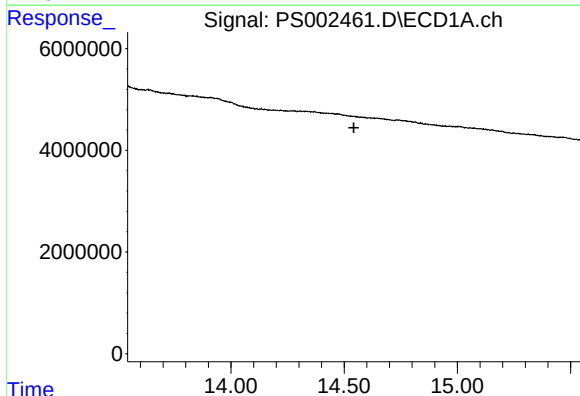


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.543 min
Response: 0
Conc: N.D.

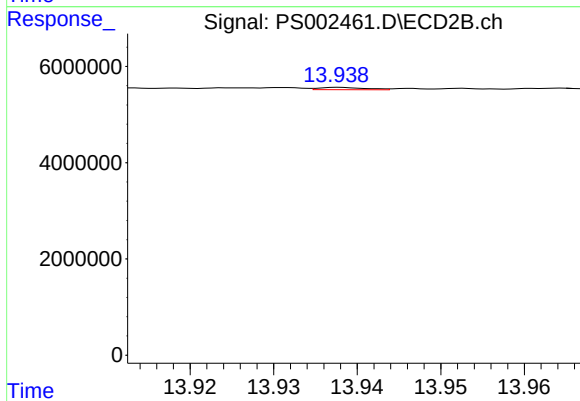

#11 2,4,5-TP (SILVEX)


R.T.: 13.938 min
Delta R.T.: -0.039 min
Response: 193930
Conc: 0.10 ng/ml

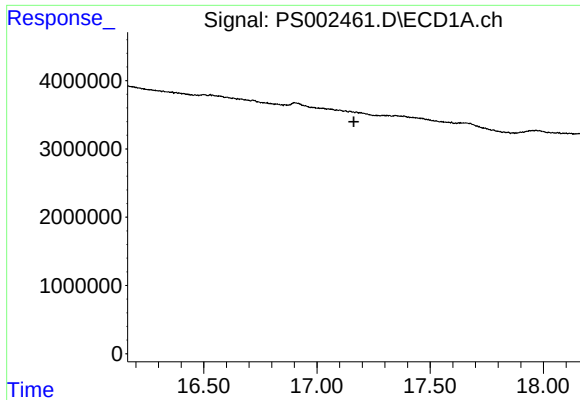

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

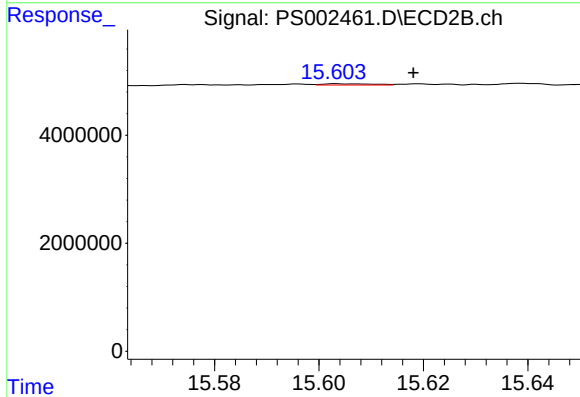


#14 DINOSEB

R.T.: 15.603 min
Delta R.T.: -0.015 min
Response: 158085
Conc: 0.11 ng/ml

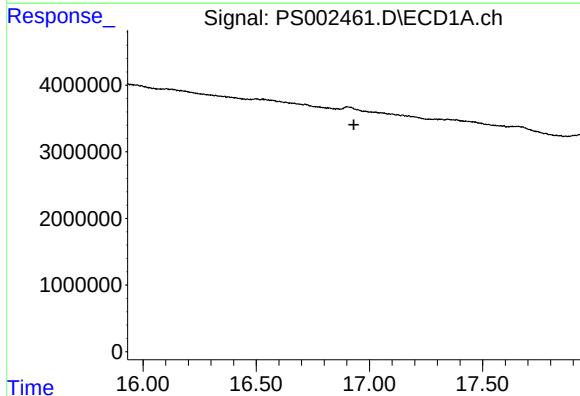


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

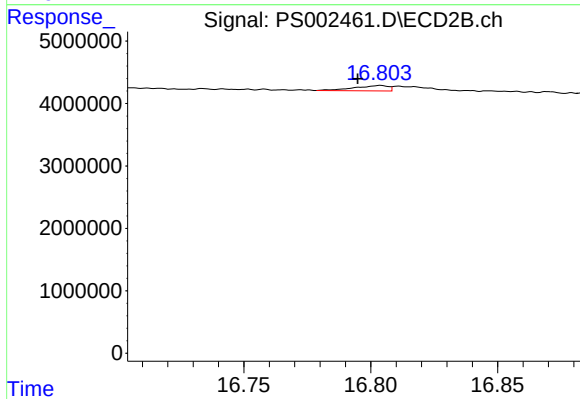

#15 Picloram


R.T.: 16.804 min
Delta R.T.: 0.009 min
Response: 795707
Conc: 0.30 ng/ml

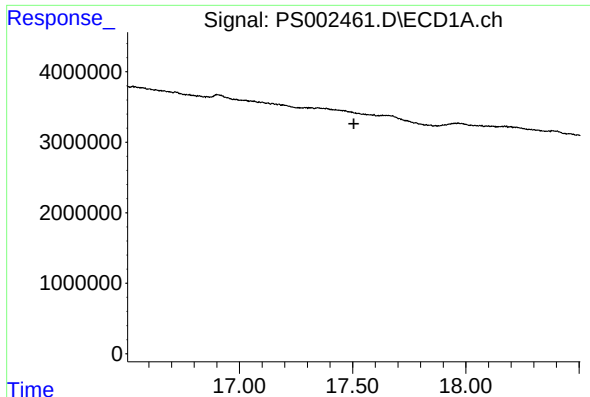

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

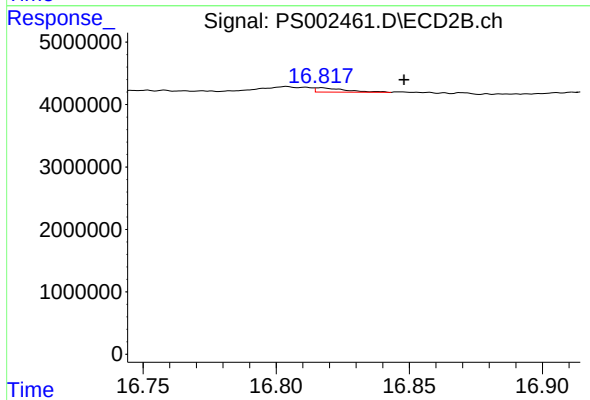

#16 DCPA

R.T.: 16.817 min
Delta R.T.: -0.031 min
Response: 538930
Conc: 0.22 ng/ml