

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112118\
 Data File : PS002462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2018 11:38
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 04:19:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.410	10.902	141.7E6	144.9E6	465.076	396.098
Target Compounds							
3) T	4-Nitroph...	0.000	10.034	0	50763	N.D.	0.290 #
7) T	MCPA	0.000	11.820	0	97476	N.D.	0.069 #
15) T	Picloram	0.000	16.844	0	97160	N.D.	0.037 #
16) T	DCPA	0.000	16.844	0	97160	N.D.	0.041 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112118\
Data File : PS002462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2018 11:38
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 04:19:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

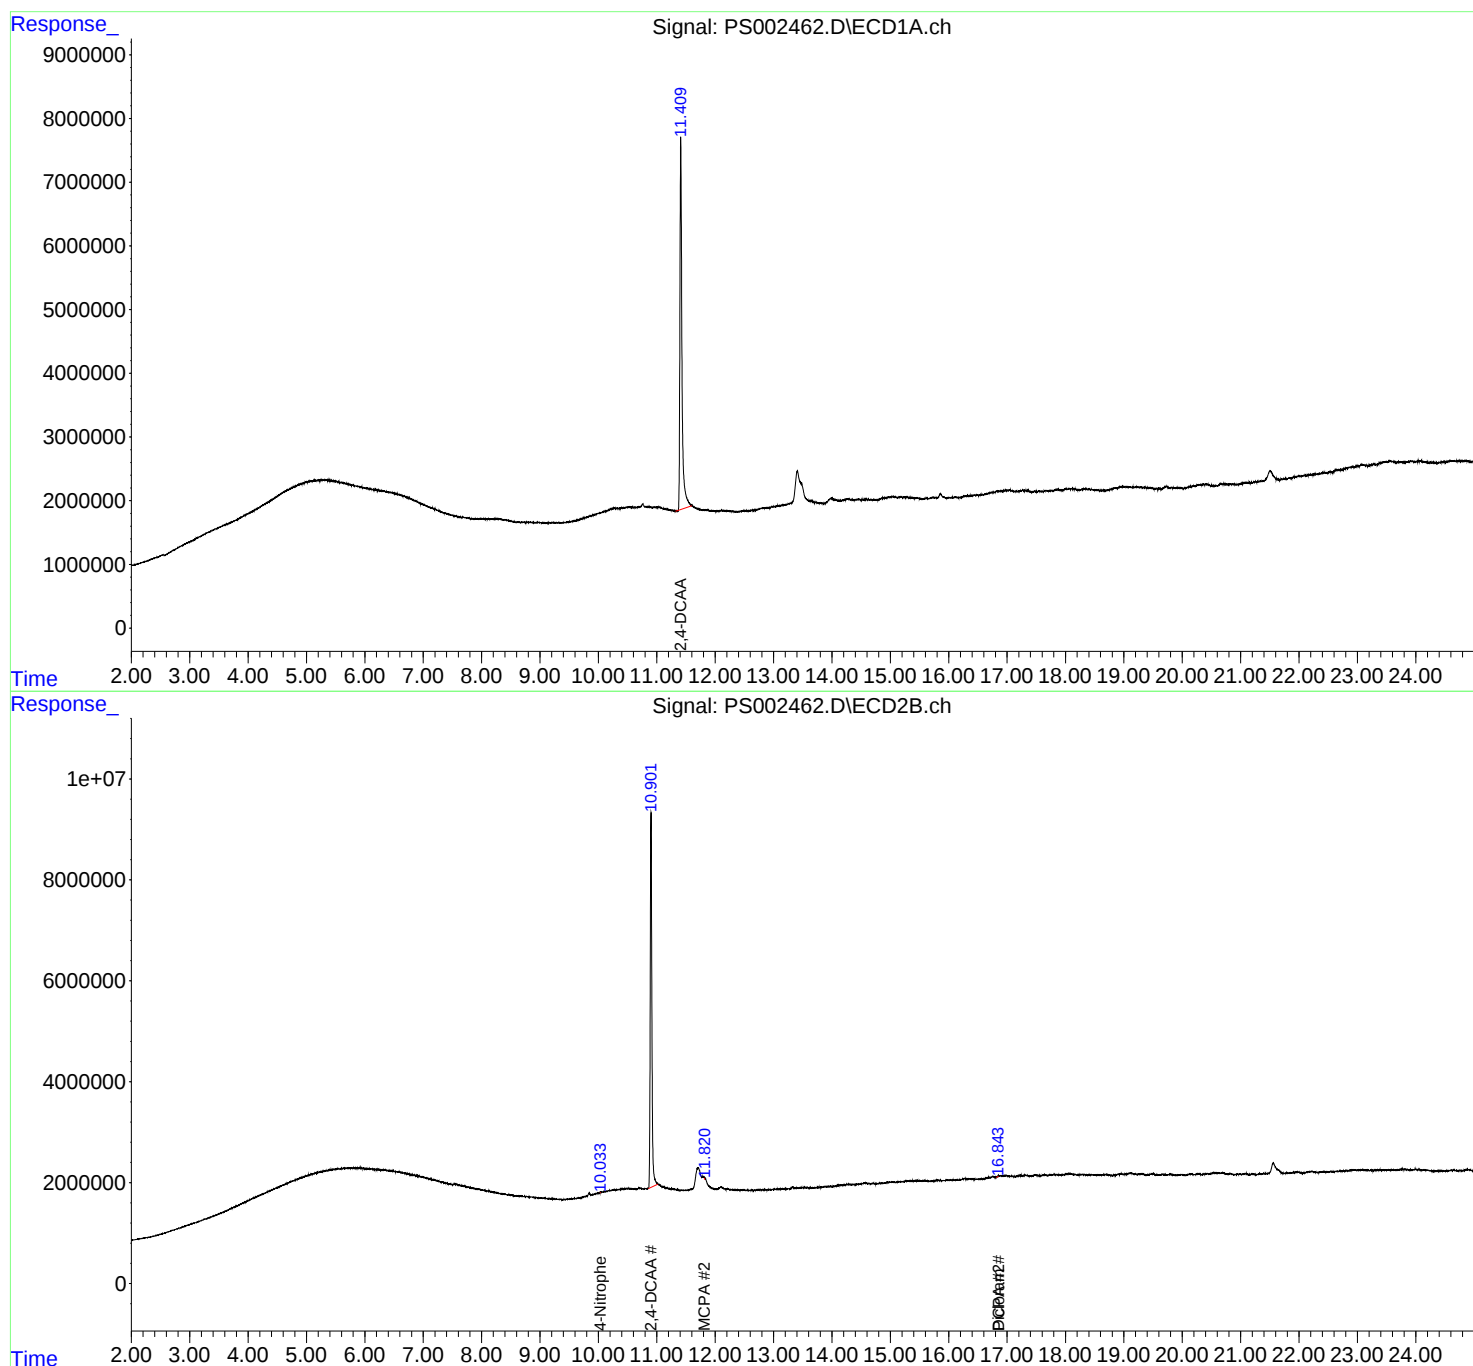


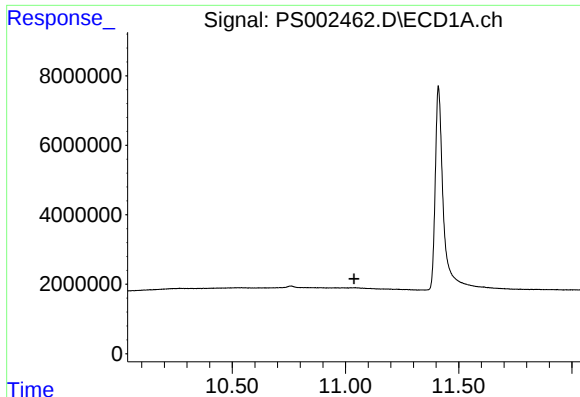

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

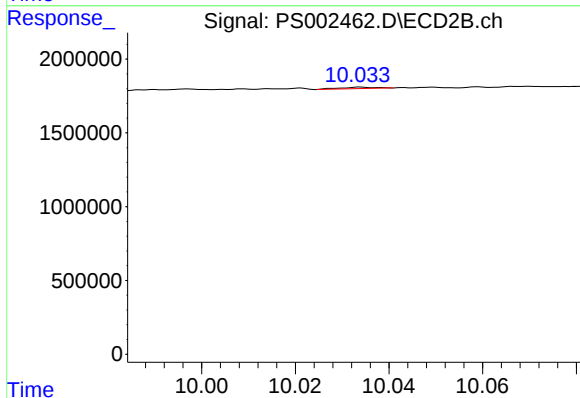


#3 4-Nitrophenol

R.T.: 10.034 min
Delta R.T.: -0.049 min
Response: 50763
Conc: 0.29 ng/ml

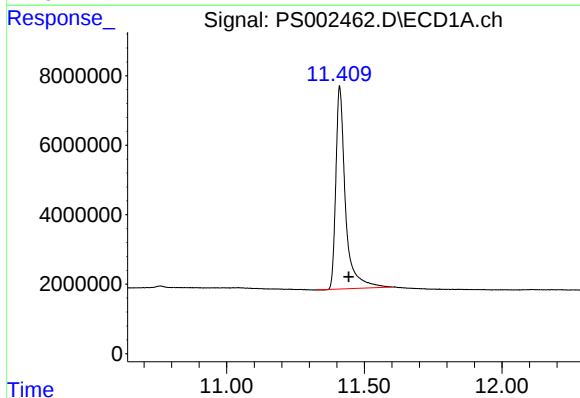


#4 2,4-DCAA

R.T.: 11.410 min
Delta R.T.: -0.033 min
Response: 141661999
Conc: 465.08 ng/ml

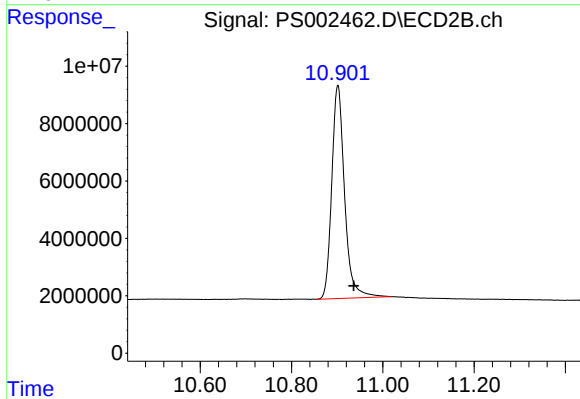

#4 2,4-DCAA


R.T.: 10.902 min
Delta R.T.: -0.034 min
Response: 144937273
Conc: 396.10 ng/ml

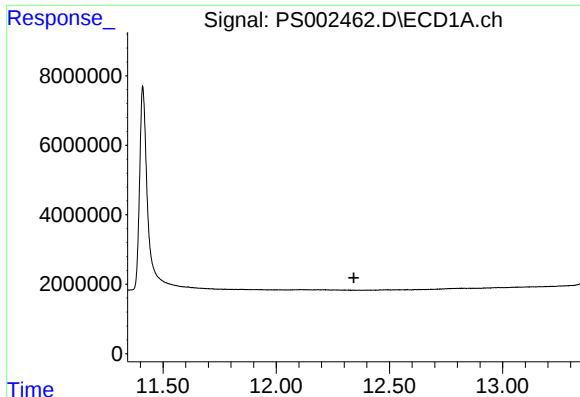

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

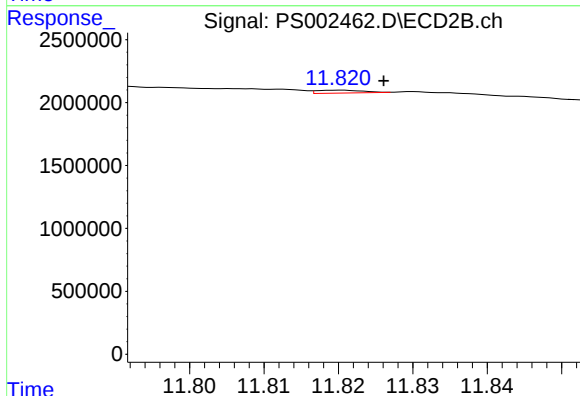


#7 MCPA

R.T.: 11.820 min
Delta R.T.: -0.006 min
Response: 97476
Conc: 0.07 ug/ml

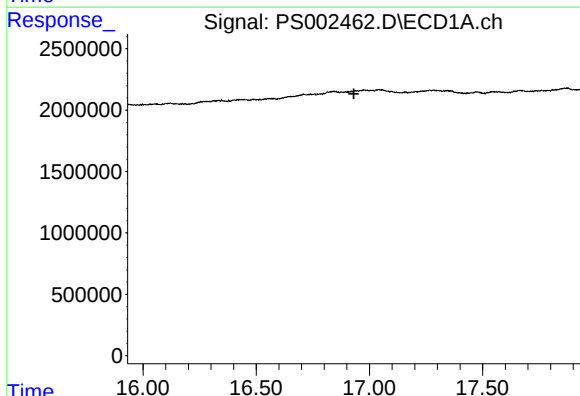


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

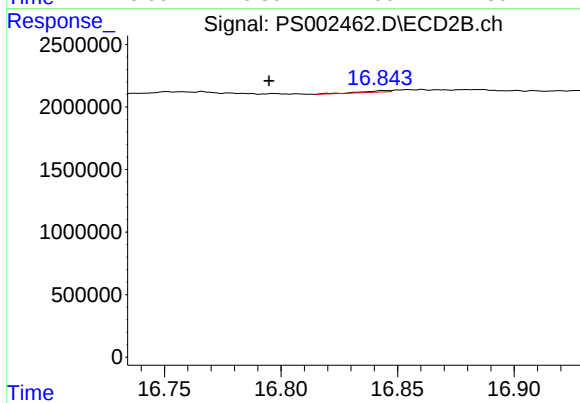

#15 Picloram


R.T.: 16.844 min
Delta R.T.: 0.049 min
Response: 97160
Conc: 0.04 ng/ml

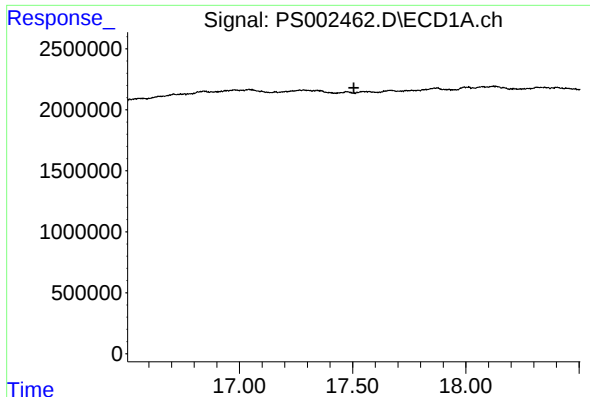

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

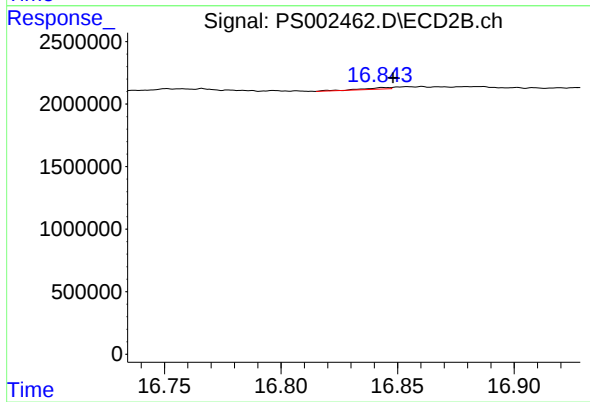

#16 DCPA

R.T.: 16.844 min
Delta R.T.: -0.005 min
Response: 97160
Conc: 0.04 ng/ml