

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112119\
 Data File : PS007772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2019 11:18
 Operator : SM\AJ
 Sample : K5933-05RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WC-COMP-01RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 11:40:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.465	5.187	239.2E6	154.2E6	173.710	219.451 #
Target Compounds							
1) T	Dalapon	2.023	1.730	82823417	314.9E6	45.780	265.181 #
2) T	3,5-DICHL...	0.000	4.477	0	7627049	N.D.	8.442
3) T	4-Nitroph...	0.000	4.862	0	17882546	N.D.	43.458
7) T	MCPA	0.000	5.494	0	56232492	N.D.	18.709
10) T	Pentachlo...	0.000	6.396	0	17532679	N.D.	1.790
11) T	2,4,5-TP ...	0.000	6.789	0	15392439	N.D.	3.931
15) T	Picloram	0.000	8.944	0	9872646	N.D.	1.685



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112119\
Data File : PS007772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2019 11:18
Operator : SM\AJ
Sample : K5933-05RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WC-COMP-01RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 11:40:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

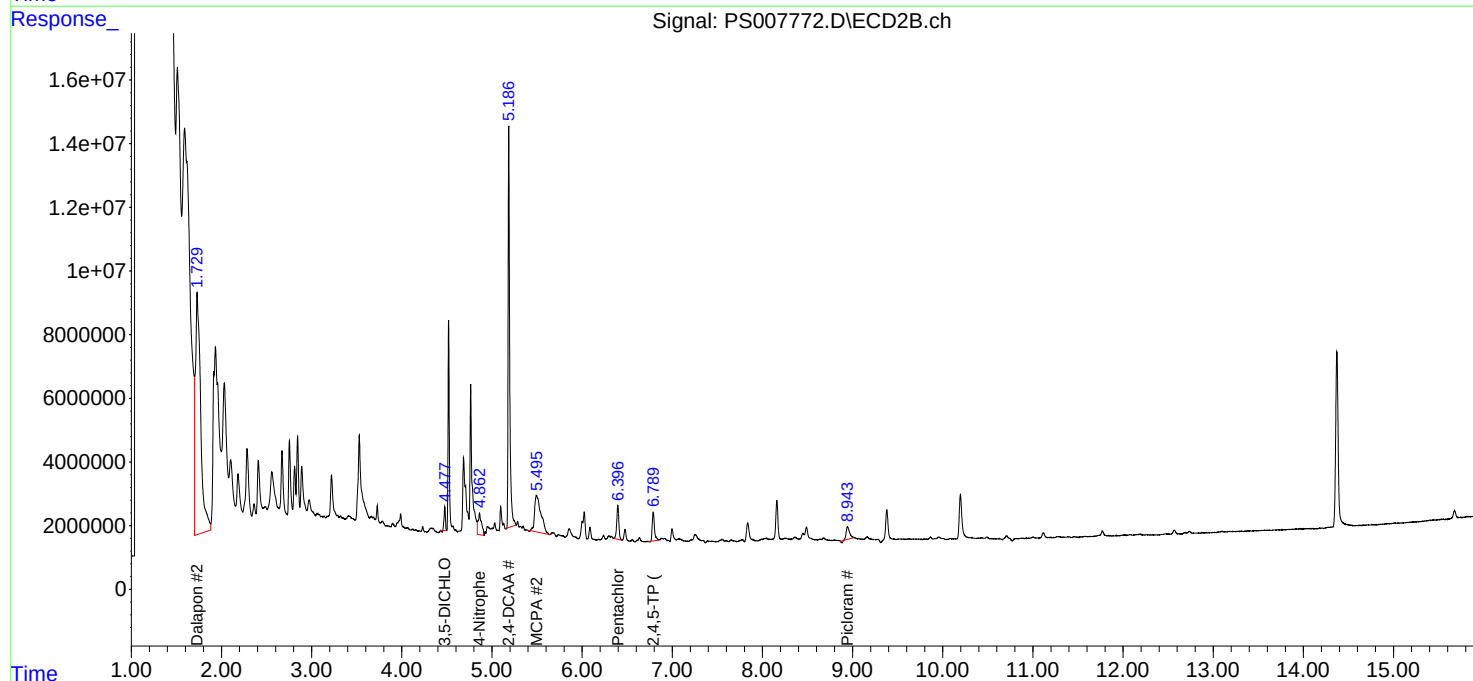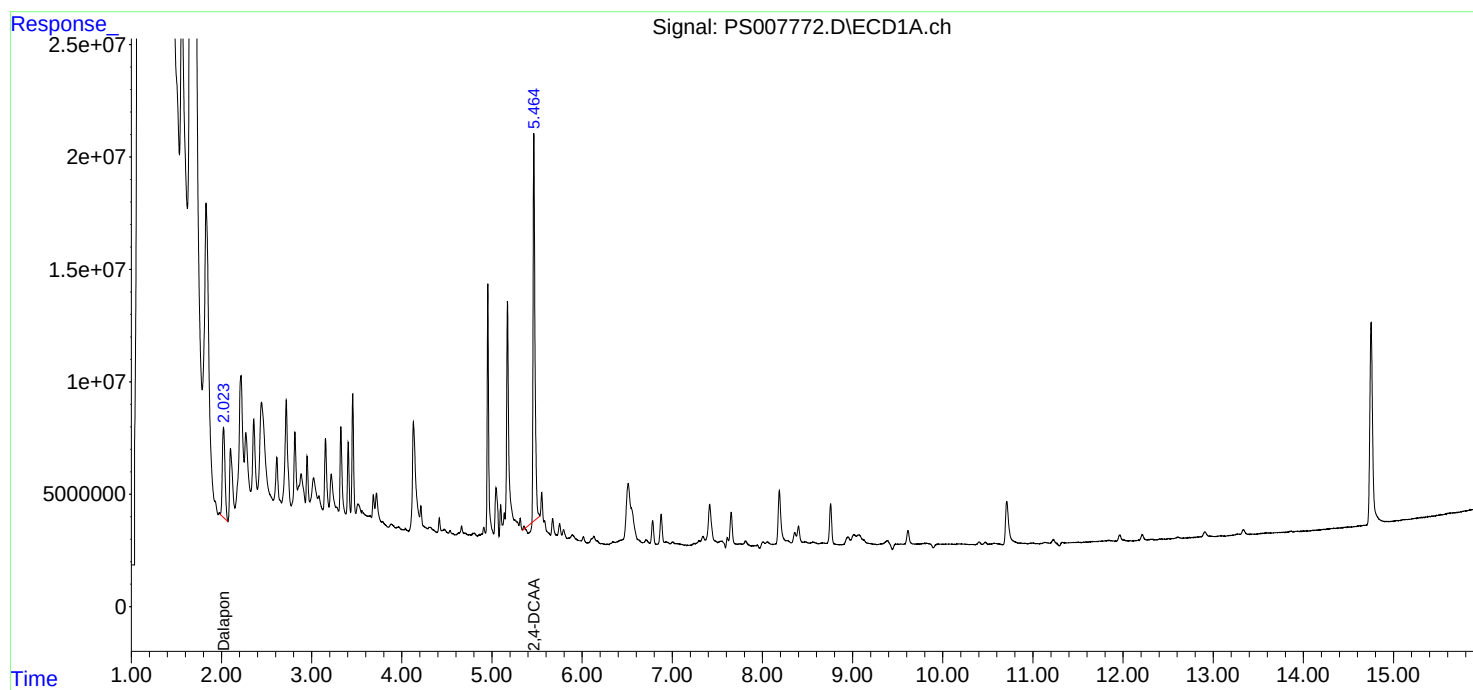


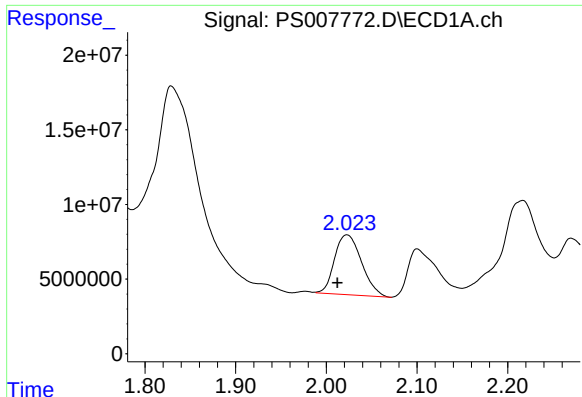

#1 Dalapon


R.T.: 2.023 min
Delta R.T.: 0.011 min
Response: 82823417
Conc: 45.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-COMP-01RE

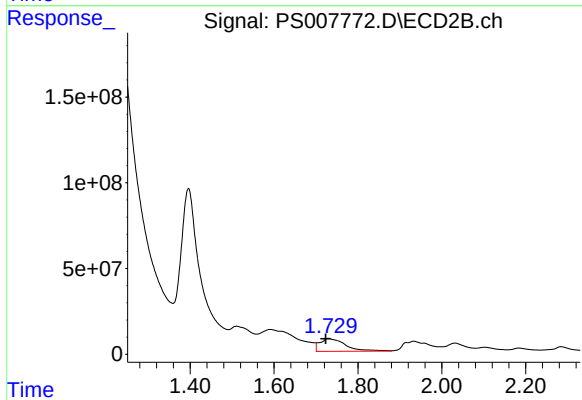


#1 Dalapon

R.T.: 1.730 min
Delta R.T.: 0.007 min
Response: 314876786
Conc: 265.18 ng/ml

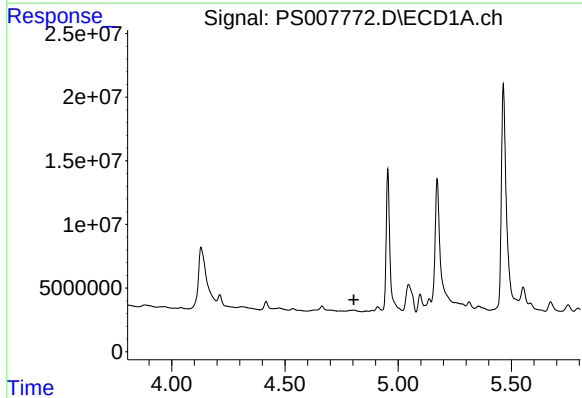


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

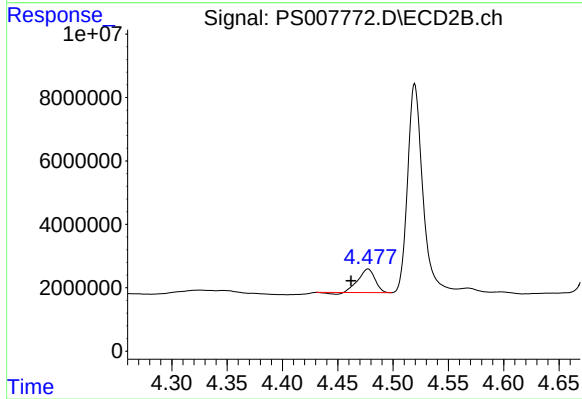

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.477 min
Delta R.T.: 0.015 min
Response: 7627049
Conc: 8.44 ng/ml

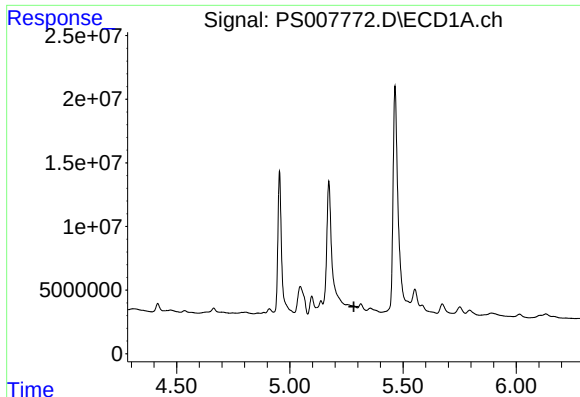

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-COMP-01RE

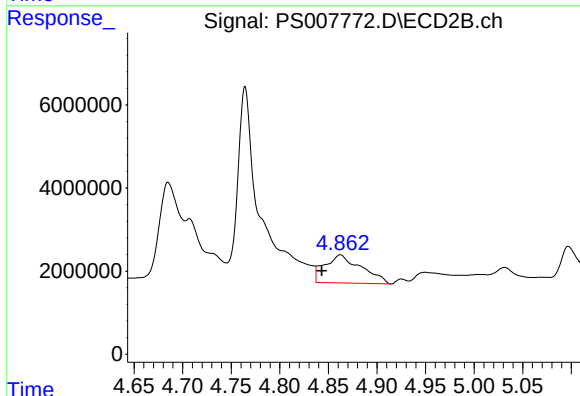


#3 4-Nitrophenol

R.T.: 4.862 min
Delta R.T.: 0.019 min
Response: 17882546
Conc: 43.46 ng/ml

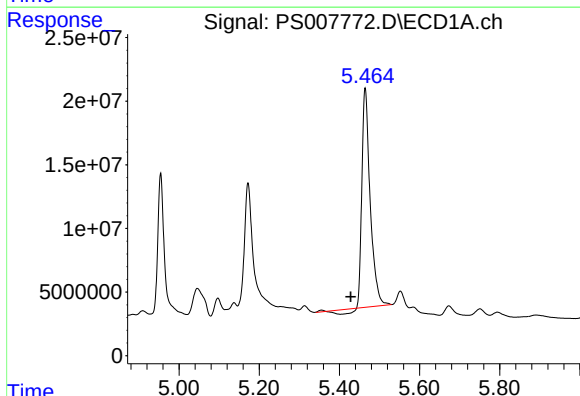


#4 2,4-DCAA

R.T.: 5.465 min
Delta R.T.: 0.036 min
Response: 239231384
Conc: 173.71 ng/ml

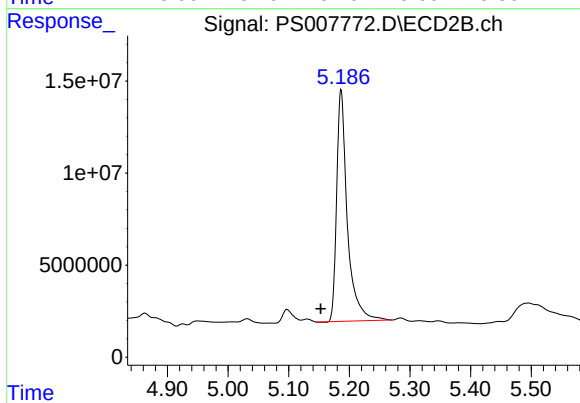

#4 2,4-DCAA


R.T.: 5.187 min
Delta R.T.: 0.034 min
Response: 154178320
Conc: 219.45 ng/ml

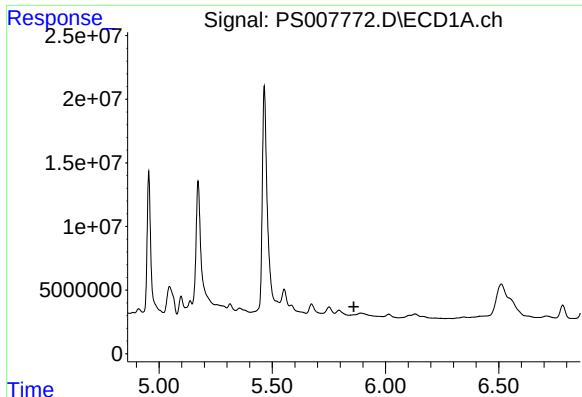

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-COMP-01RE

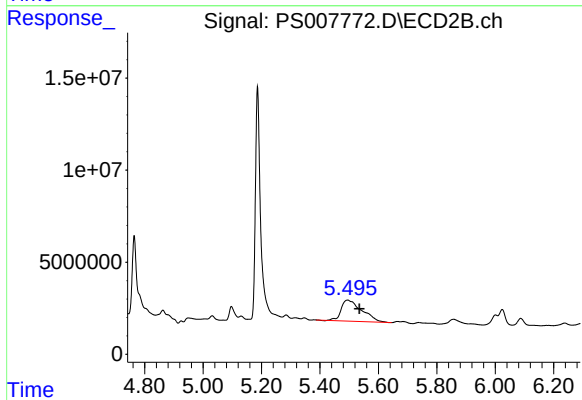


#7 MCPA

R.T.: 5.494 min
Delta R.T.: -0.041 min
Response: 56232492
Conc: 18.71 ug/ml

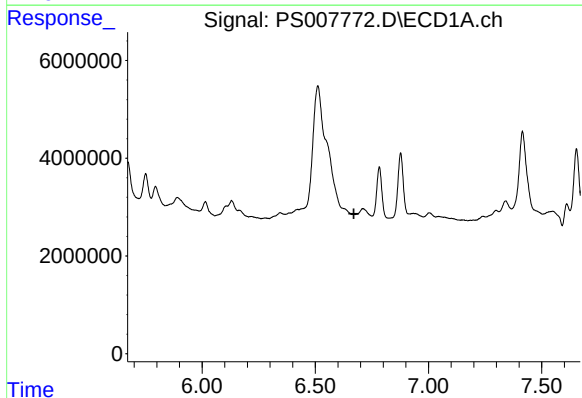


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

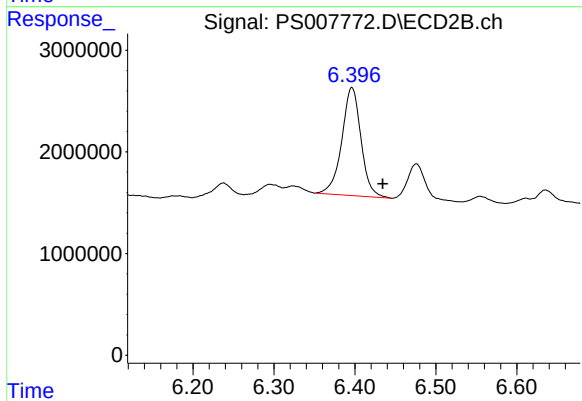

#10 Pentachlorophenol


R.T.: 6.396 min
Delta R.T.: -0.038 min
Response: 17532679
Conc: 1.79 ng/ml

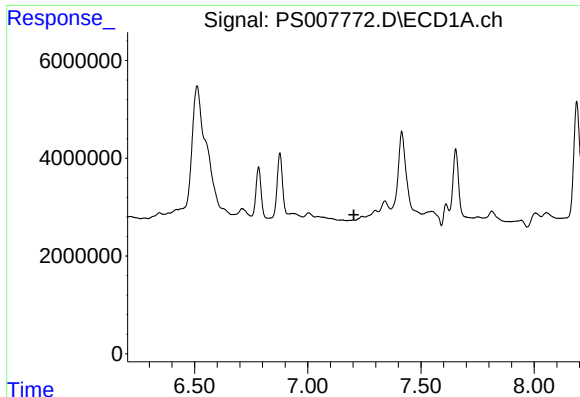

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-COMP-01RE

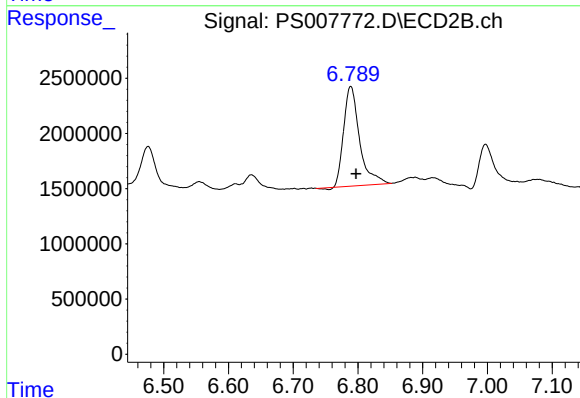


#11 2,4,5-TP (SILVEX)

R.T.: 6.789 min
Delta R.T.: -0.008 min
Response: 15392439
Conc: 3.93 ng/ml

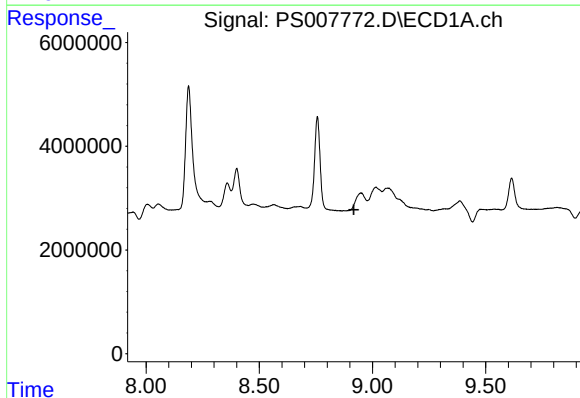

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

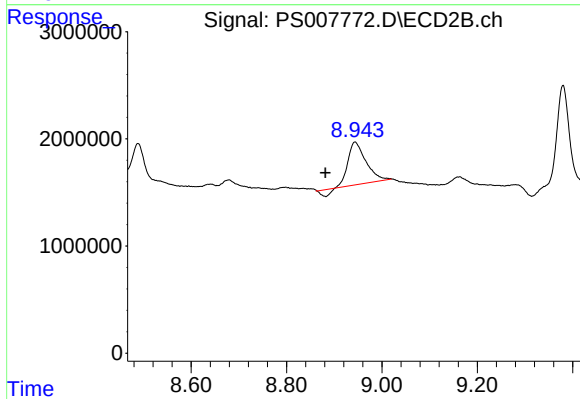

#15 Picloram

R.T.: 8.944 min
Delta R.T.: 0.062 min
Response: 9872646
Conc: 1.69 ng/ml