

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112119\
 Data File : PS007774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2019 12:02
 Operator : SM\AJ
 Sample : K5934-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 13:08:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.432	0.000	394.9E6	0	286.737	N.D. #
Target Compounds							
1) T	Dalapon	1.992	1.700	94917527	239.8E6	52.464	201.982 #
2) T	3,5-DICHL...	0.000	4.447	0	6805428	N.D.	7.533
5) T	DICAMBA	5.521	0.000	39747063	0	7.813	N.D. #
7) T	MCPA	0.000	5.473	0	62054556	N.D.	20.646
9) T	2,4-D	6.482	0.000	119.0E6	0	84.814	N.D. #
10) T	Pentachlo...	0.000	6.366	0	19322714	N.D.	1.973
11) T	2,4,5-TP ...	0.000	6.757	0	14722644	N.D.	3.760



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112119\
Data File : PS007774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2019 12:02
Operator : SM\AJ
Sample : K5934-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 13:08:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

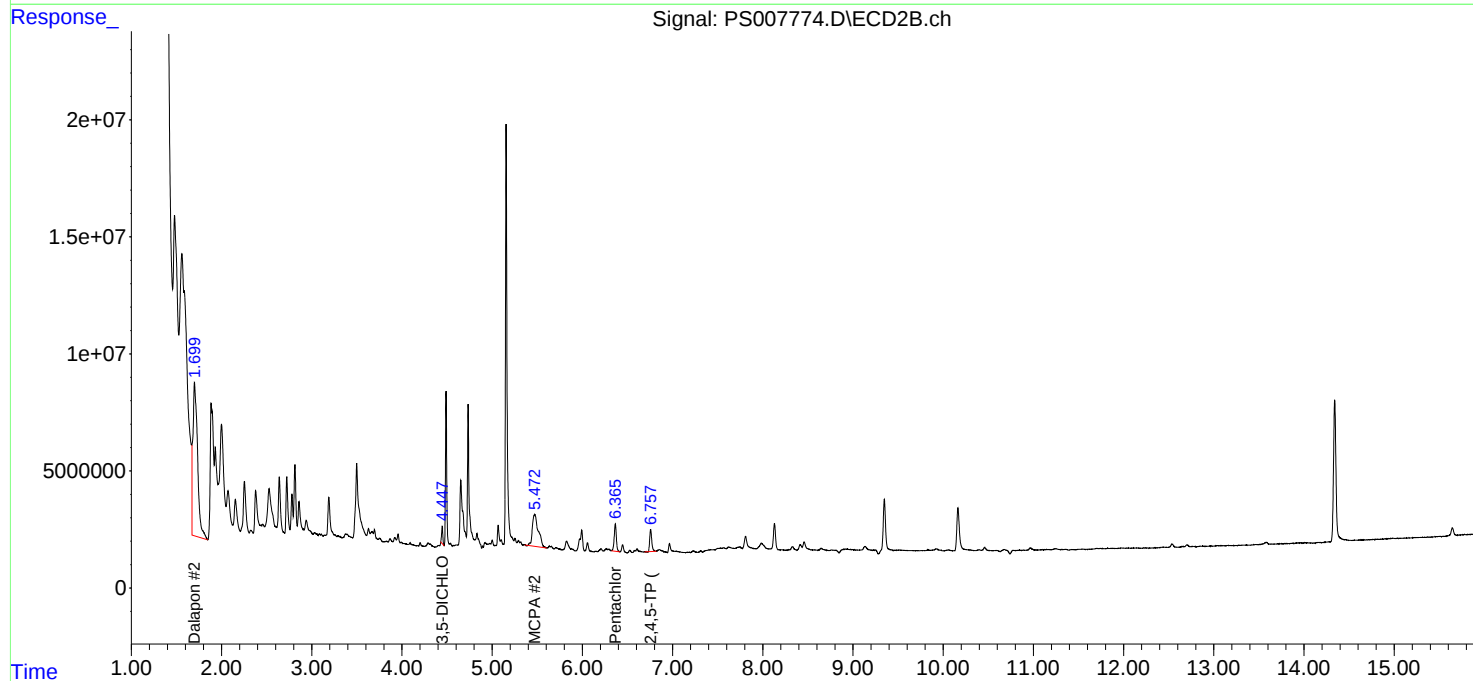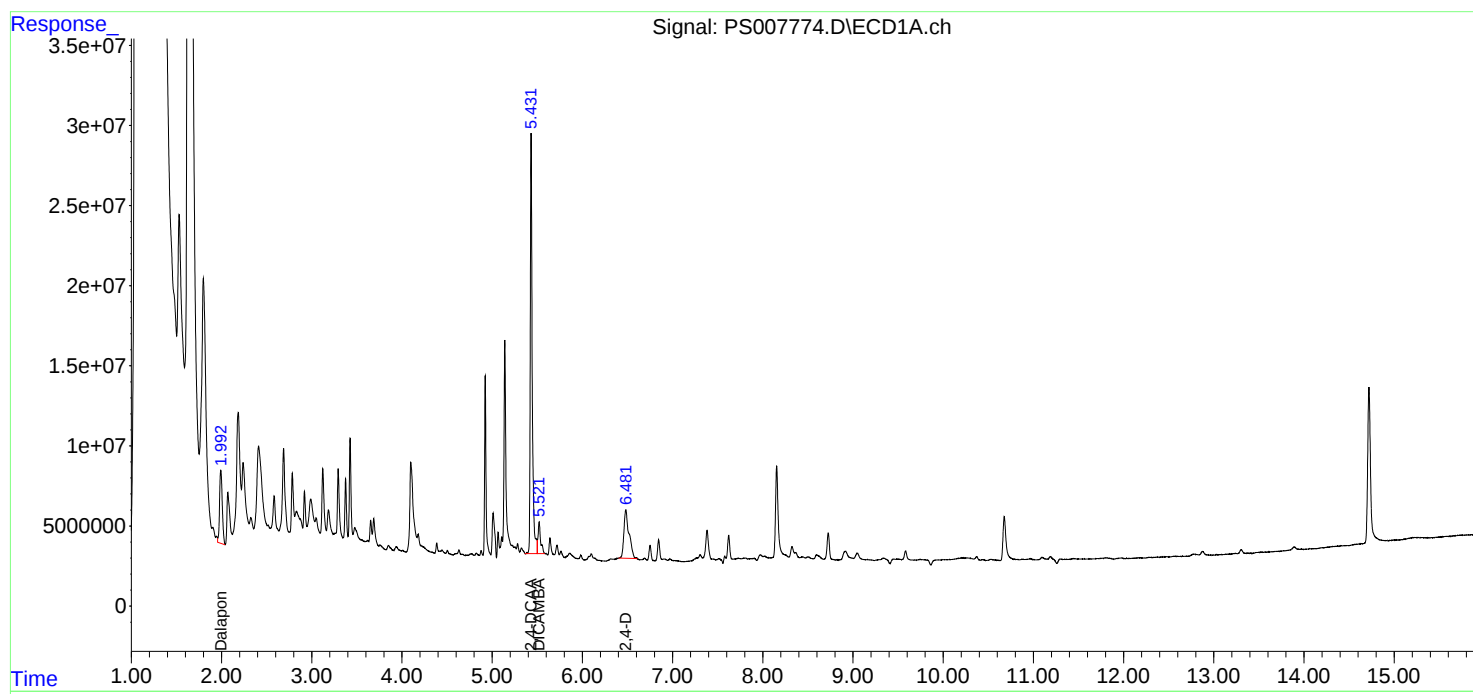


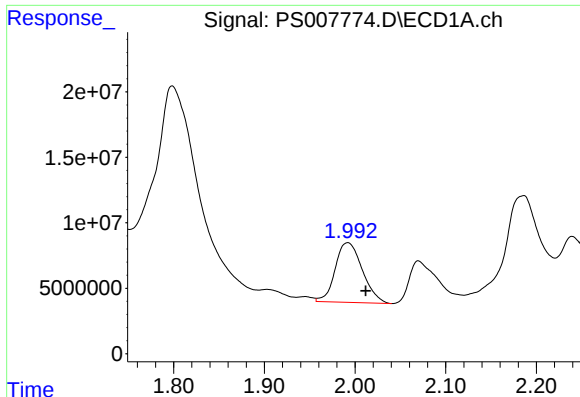

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.020 min
Response: 94917527
Conc: 52.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

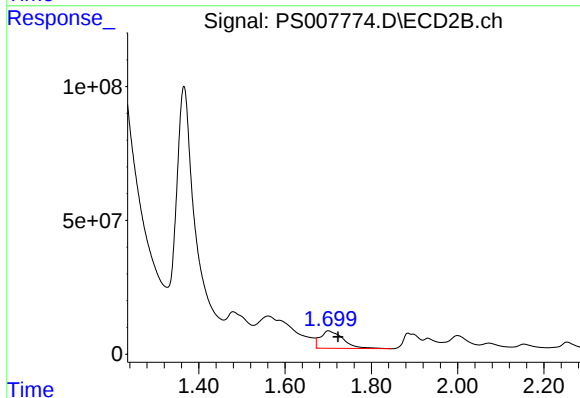


#1 Dalapon

R.T.: 1.700 min
Delta R.T.: -0.023 min
Response: 239833731
Conc: 201.98 ng/ml

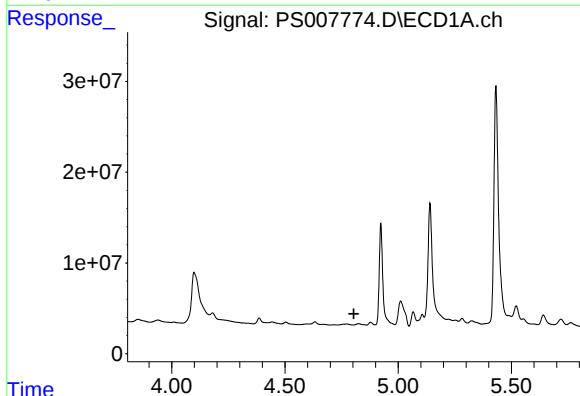


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

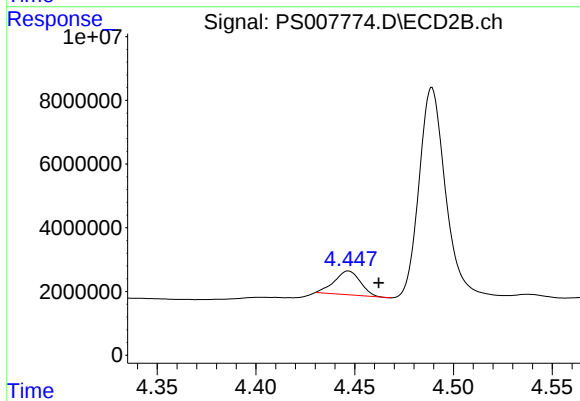

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min
Delta R.T.: -0.015 min
Response: 6805428
Conc: 7.53 ng/ml

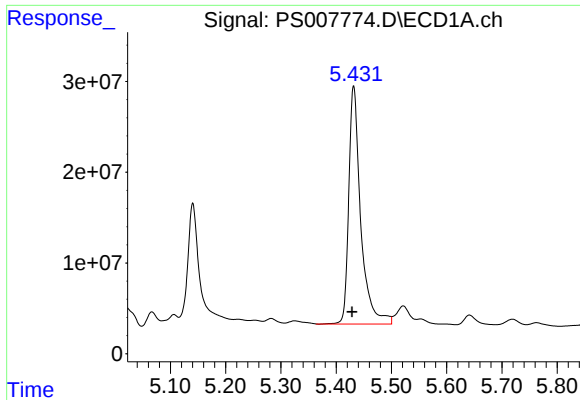

#4 2,4-DCAA


R.T.: 5.432 min
Delta R.T.: 0.003 min
Response: 394889930
Conc: 286.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

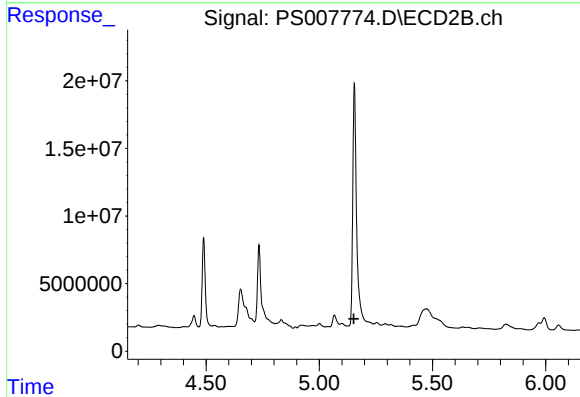


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.153 min
Response: 0
Conc: N.D.

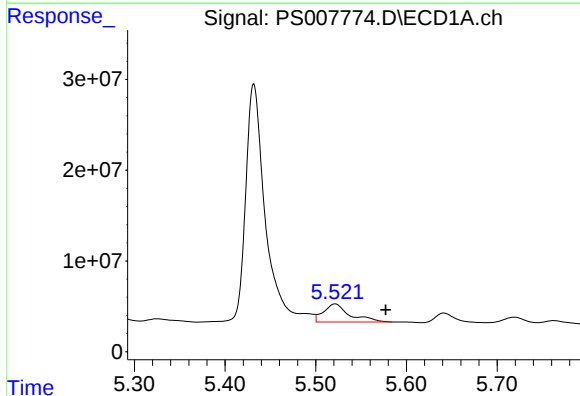


#5 DICAMBA

R.T.: 5.521 min
Delta R.T.: -0.056 min
Response: 39747063
Conc: 7.81 ng/ml

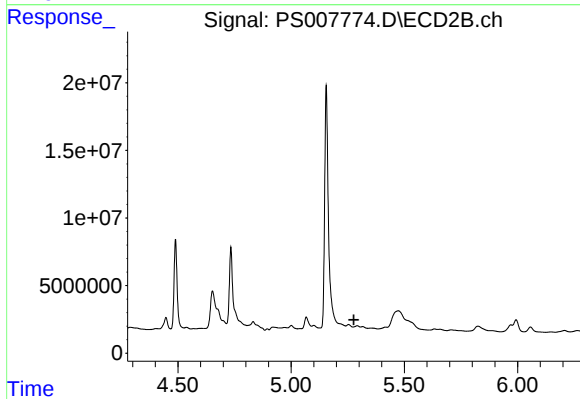

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

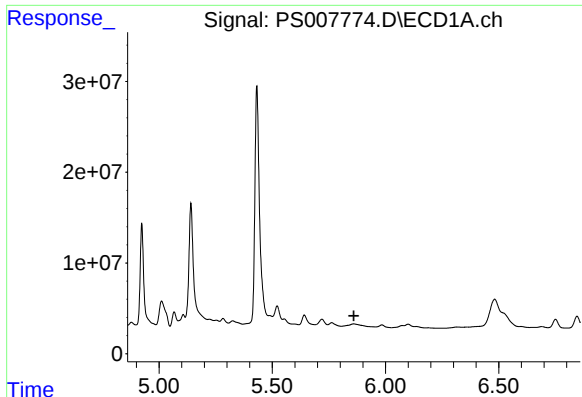

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

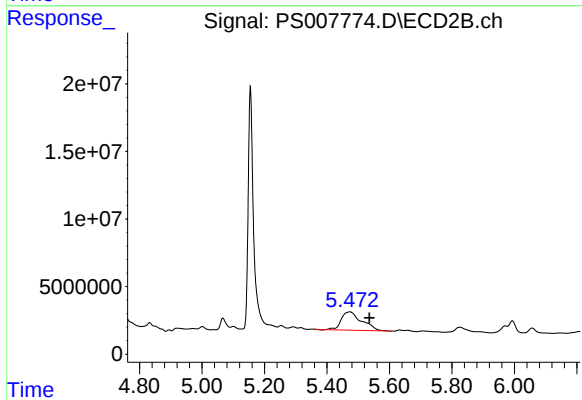


#7 MCPA

R.T.: 5.473 min
Delta R.T.: -0.063 min
Response: 62054556
Conc: 20.65 ug/ml

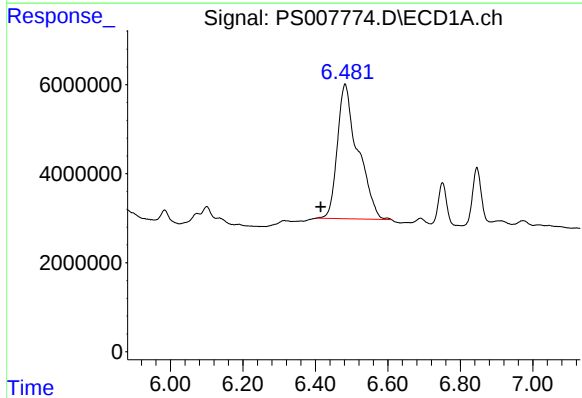


#9 2,4-D

R.T.: 6.482 min
Delta R.T.: 0.068 min
Response: 118955041
Conc: 84.81 ng/ml

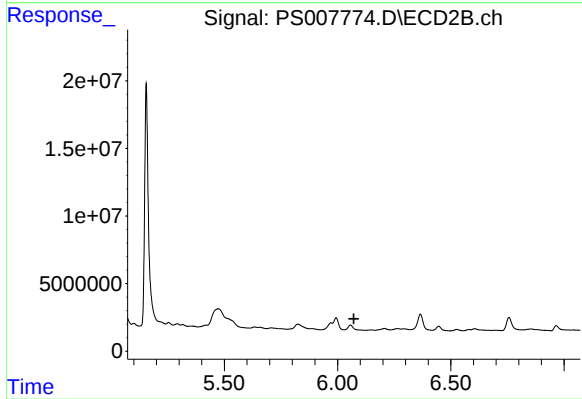

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

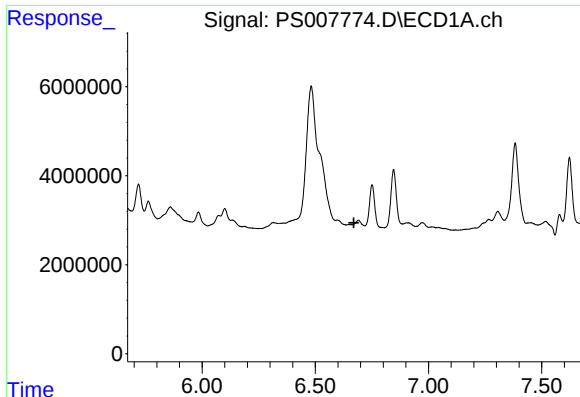

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

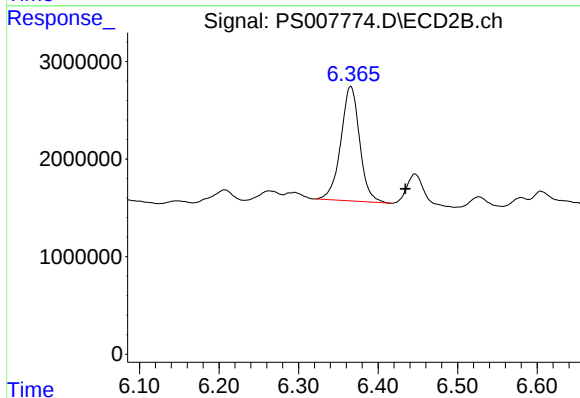


#10 Pentachlorophenol

R.T.: 6.366 min
Delta R.T.: -0.069 min
Response: 19322714
Conc: 1.97 ng/ml

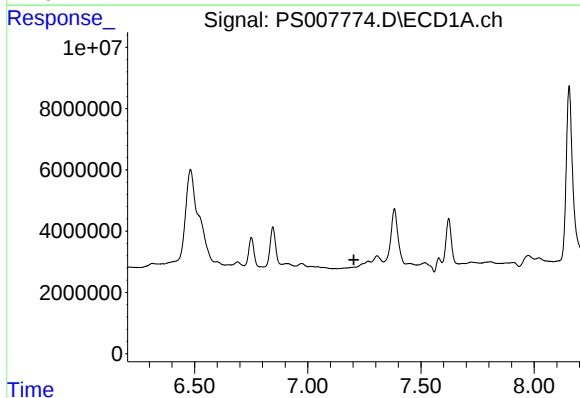

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

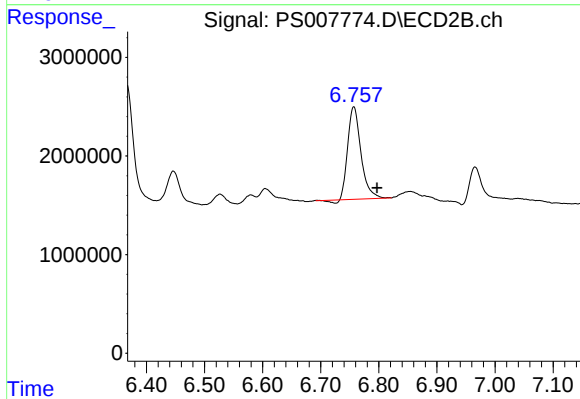

#11 2,4,5-TP (SILVEX)

R.T.: 6.757 min
Delta R.T.: -0.040 min
Response: 14722644
Conc: 3.76 ng/ml