

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112123\
 Data File : PS024887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 09:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 22:52:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.356	6.773	1173.8E6	383.9E6	574.971	569.070
Target Compounds						
1) T Dalapon	0.000	2.565	0	3663529	N.D.	3.477
3) T 4-Nitroph...	6.198	6.370	7330236	666965	5.655	1.519 #
6) T MCPP	6.679	0.000	3540843	0	<MDL	N.D. #
7) T MCPA	0.000	7.167f	0	22746175	N.D.	7.378
8) T DICHLORPROP	0.000	7.561	0	3924978	N.D.	5.373
9) T 2,4-D	0.000	7.773f	0	972928	N.D.	1.087
12) T 2,4,5-T	0.000	8.986	0	333996	N.D.	<MDL
15) T Picloram	9.678	10.764	26020318	8394045	1.463	1.382
16) T DCPA	0.000	10.764	0	8394045	N.D.	1.670



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112123\
Data File : PS024887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 09:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 22:52:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

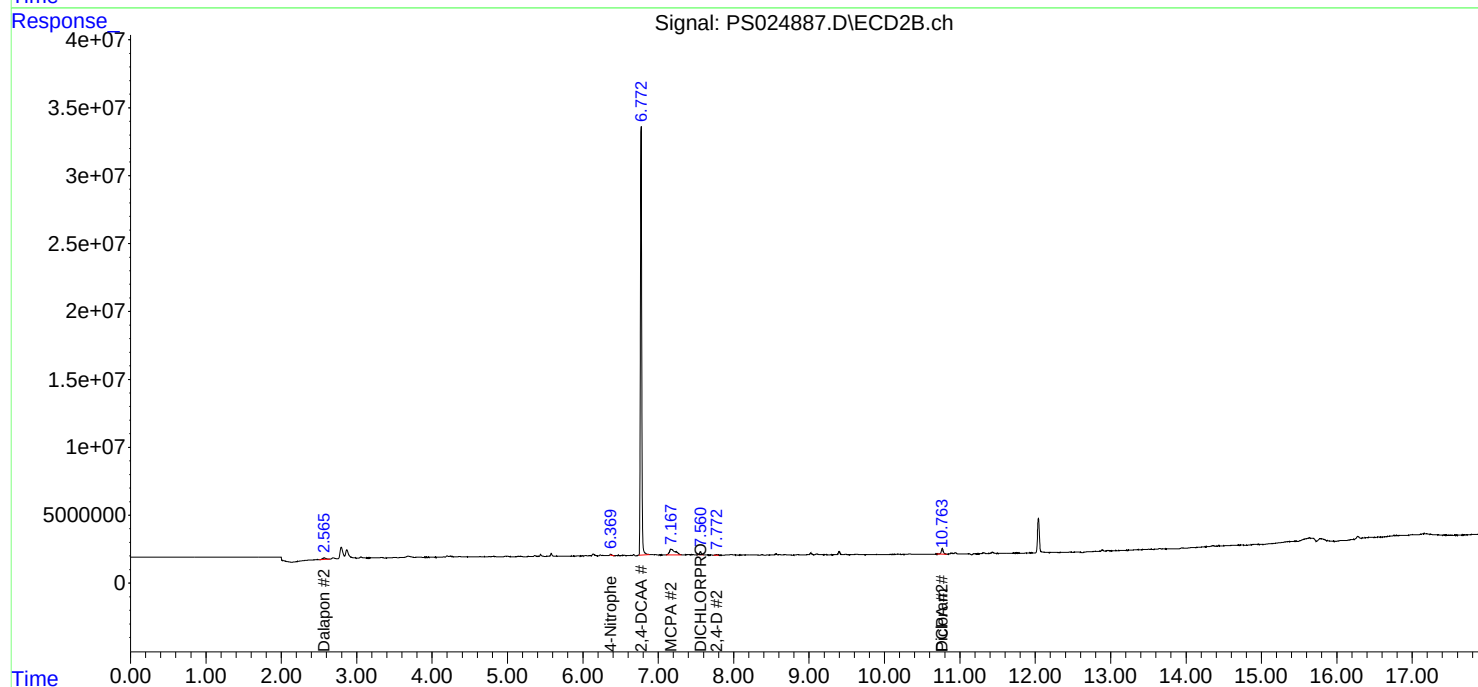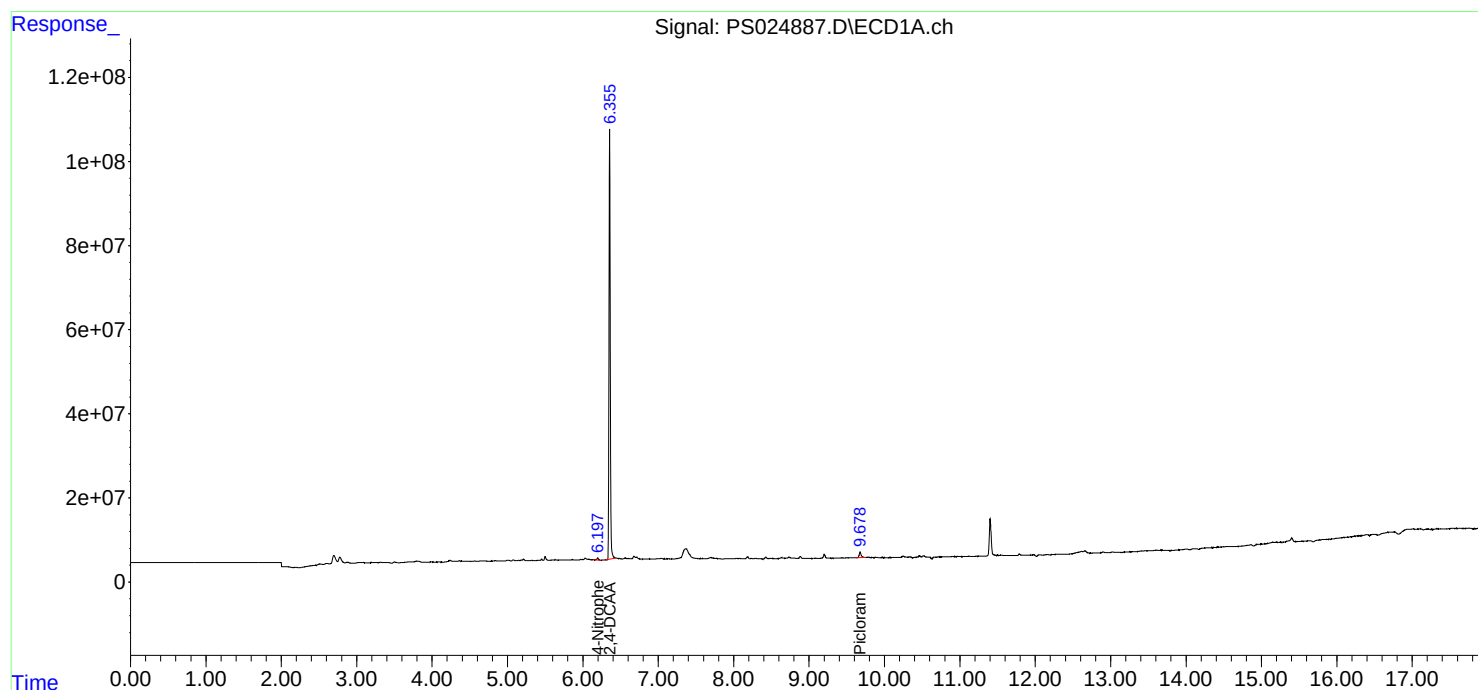


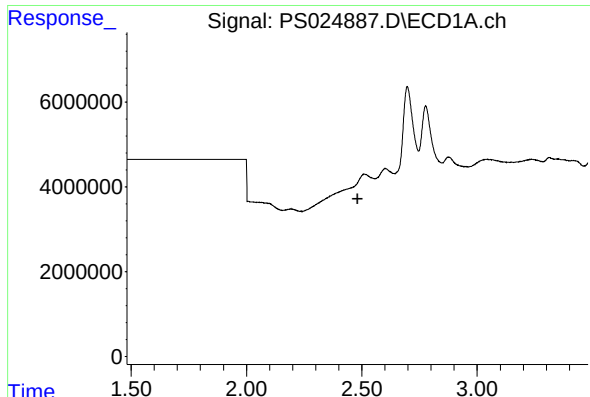

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

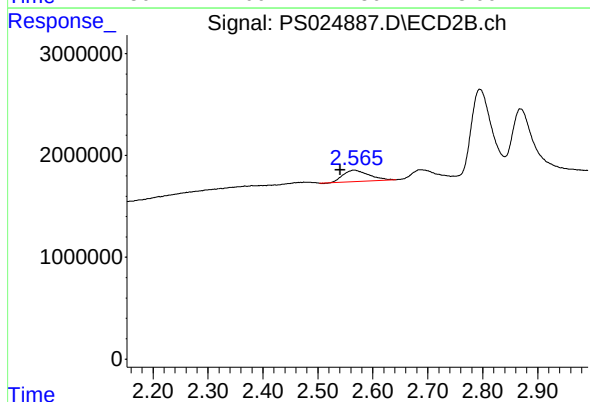


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.025 min
Response: 3663529
Conc: 3.48 ng/ml

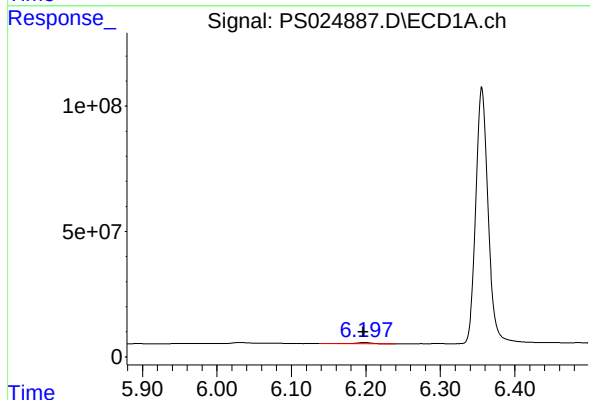


#3 4-Nitrophenol

R.T.: 6.198 min
Delta R.T.: 0.002 min
Response: 7330236
Conc: 5.66 ng/ml

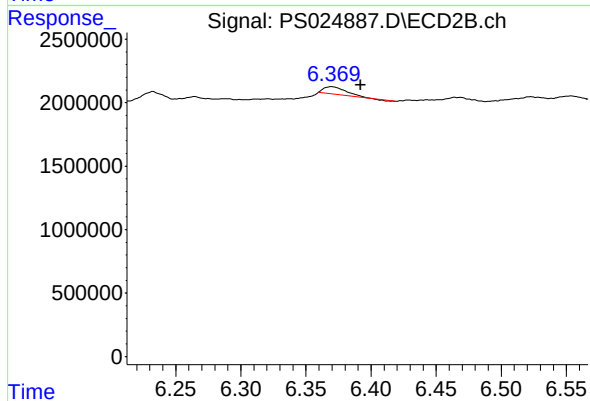

#3 4-Nitrophenol


R.T.: 6.370 min
Delta R.T.: -0.022 min
Response: 666965
Conc: 1.52 ng/ml

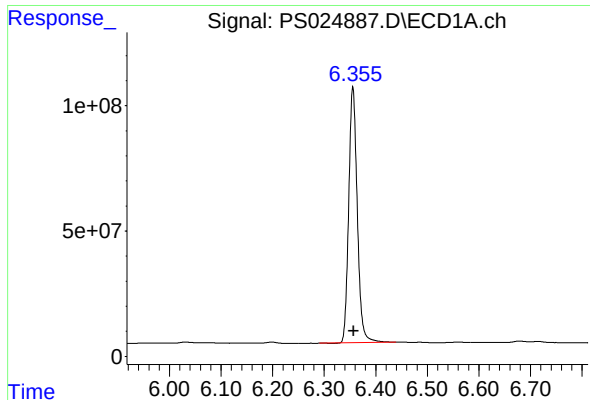

#4 2,4-DCAA


R.T.: 6.356 min
Delta R.T.: -0.002 min
Response: 1173805267
Conc: 574.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

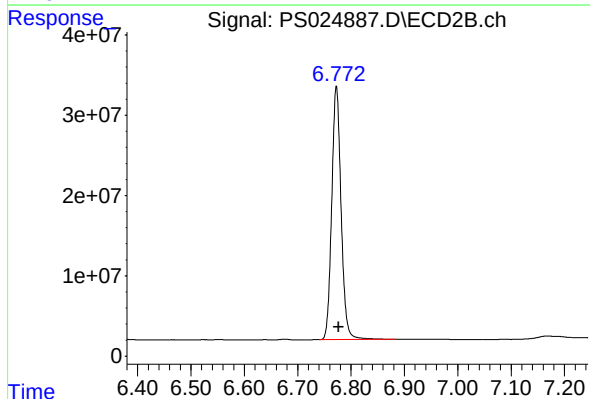


#4 2,4-DCAA

R.T.: 6.773 min
Delta R.T.: -0.004 min
Response: 383894002
Conc: 569.07 ng/ml

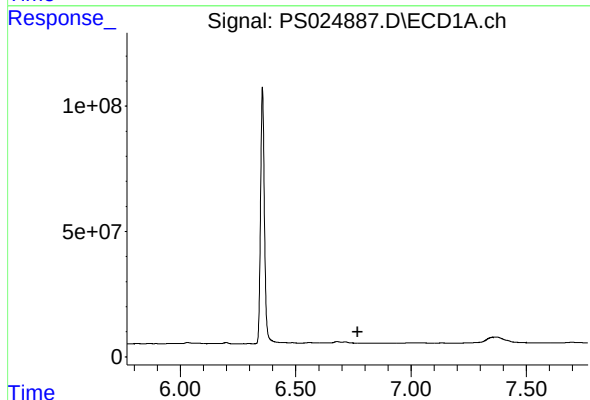


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

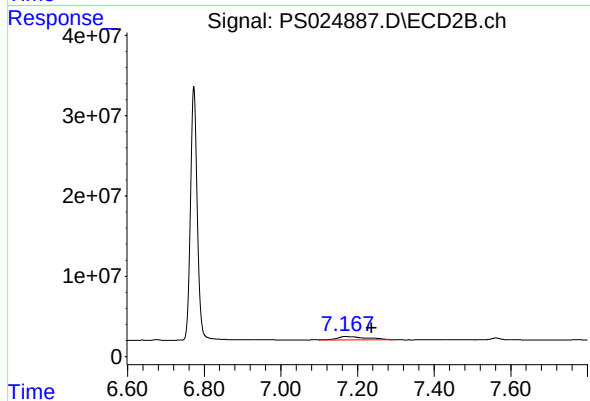

#7 MCPA


R.T.: 7.167 min
Delta R.T.: -0.070 min
Response: 22746175
Conc: 7.38 ug/ml

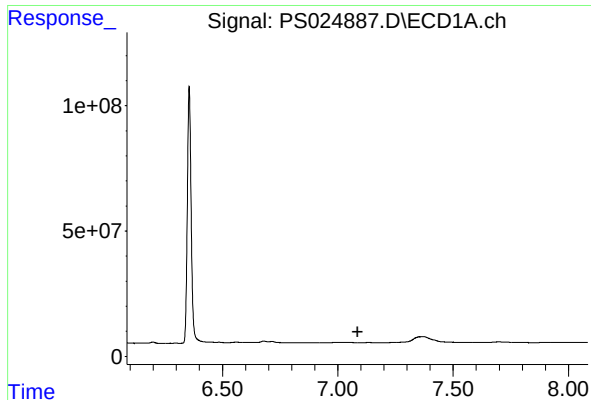

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

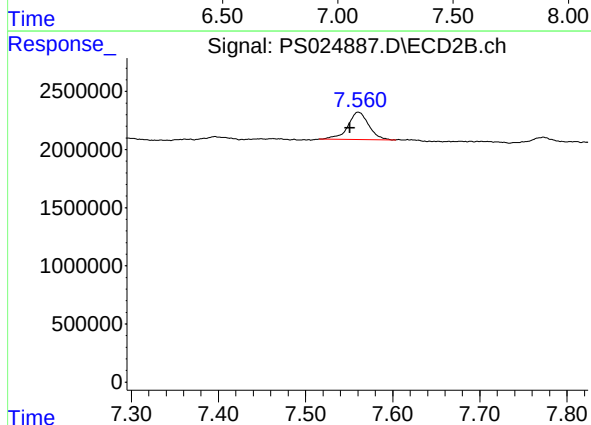


#8 DICHLORPROP

R.T.: 7.561 min
Delta R.T.: 0.009 min
Response: 3924978
Conc: 5.37 ng/ml

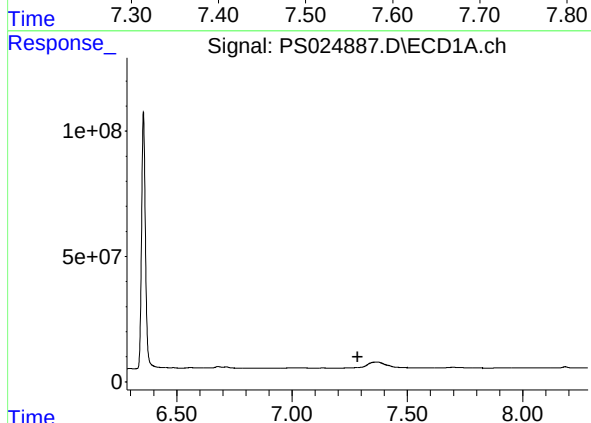


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

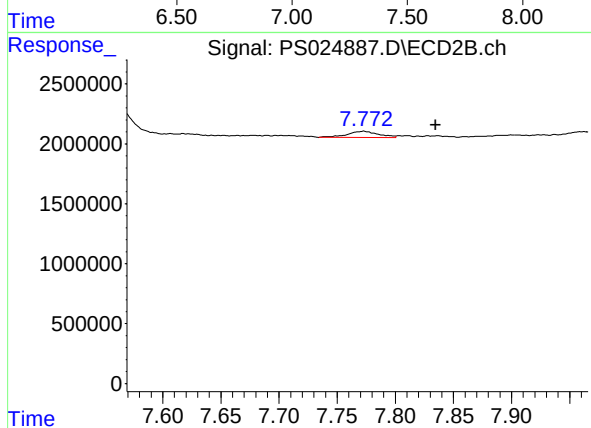

#9 2,4-D


R.T.: 7.773 min
Delta R.T.: -0.062 min
Response: 972928
Conc: 1.09 ng/ml

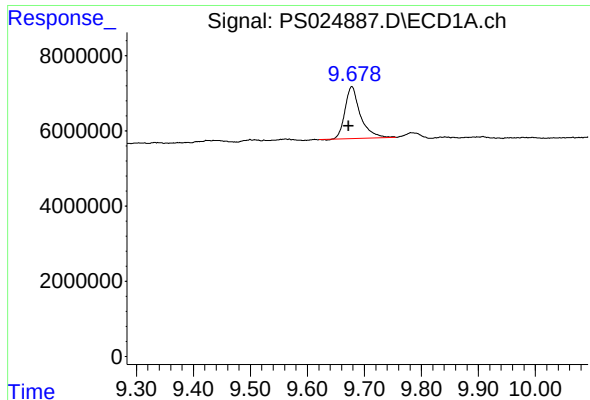

#15 Picloram


R.T.: 9.678 min
Delta R.T.: 0.006 min
Response: 26020318
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

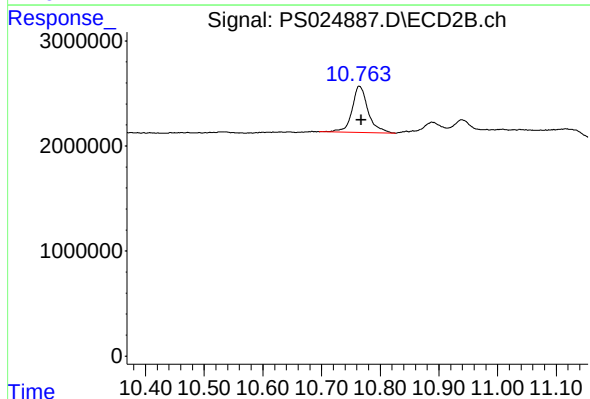


#15 Picloram

R.T.: 10.764 min
Delta R.T.: -0.003 min
Response: 8394045
Conc: 1.38 ng/ml

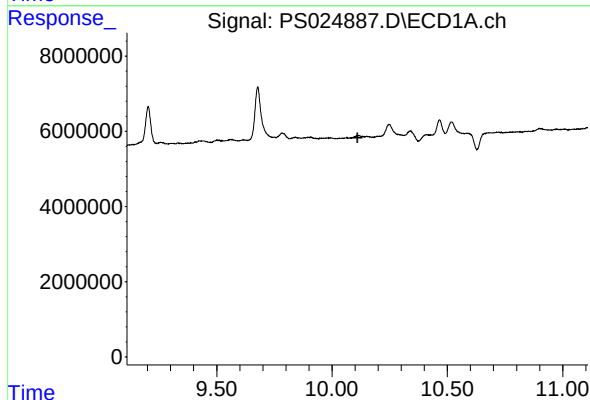

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

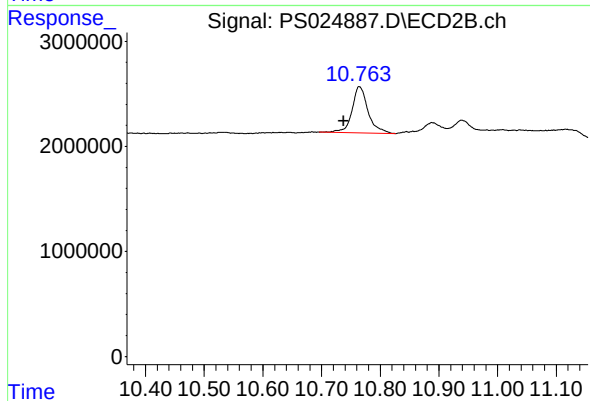

#16 DCPA

R.T.: 10.764 min
Delta R.T.: 0.026 min
Response: 8394045
Conc: 1.67 ng/ml