

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112123\  
 Data File : PS024899.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 21 Nov 2023 14:23  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 21 22:55:04 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110323.M  
 Quant Title : 8080.M  
 QLast Update : Fri Nov 03 15:07:01 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-------|--------|----------|----------|---------|---------|
| -----                       |       |        |          |          |         |         |
| System Monitoring Compounds |       |        |          |          |         |         |
| 4) S 2,4-DCAA               | 6.355 | 6.773  | 1189.3E6 | 391.1E6  | 582.555 | 579.732 |
| Target Compounds            |       |        |          |          |         |         |
| 1) T Dalapon                | 0.000 | 2.568  | 0        | 3207348  | N.D.    | 3.044   |
| 6) T MCPP                   | 6.679 | 0.000  | 7004042  | 0        | 1.124   | N.D. #  |
| 7) T MCPA                   | 0.000 | 7.167f | 0        | 30826434 | N.D.    | 9.999   |
| 8) T DICHLORPROP            | 0.000 | 7.560  | 0        | 5683571  | N.D.    | 7.780   |
| 9) T 2,4-D                  | 0.000 | 7.771f | 0        | 209789   | N.D.    | <MDL    |
| 12) T 2,4,5-T               | 0.000 | 8.983  | 0        | 436192   | N.D.    | <MDL    |
| 13) T 2,4-DB                | 0.000 | 9.488  | 0        | 868087   | N.D.    | 1.780   |
| 15) T Picloram              | 0.000 | 10.766 | 0        | 3276862  | N.D.    | <MDL    |
| 16) T DCPA                  | 0.000 | 10.766 | 0        | 3276862  | N.D.    | <MDL    |
| -----                       |       |        |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112123\  
Data File : PS024899.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 21 Nov 2023 14:23  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 21 22:55:04 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110323.M  
Quant Title : 8080.M  
QLast Update : Fri Nov 03 15:07:01 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

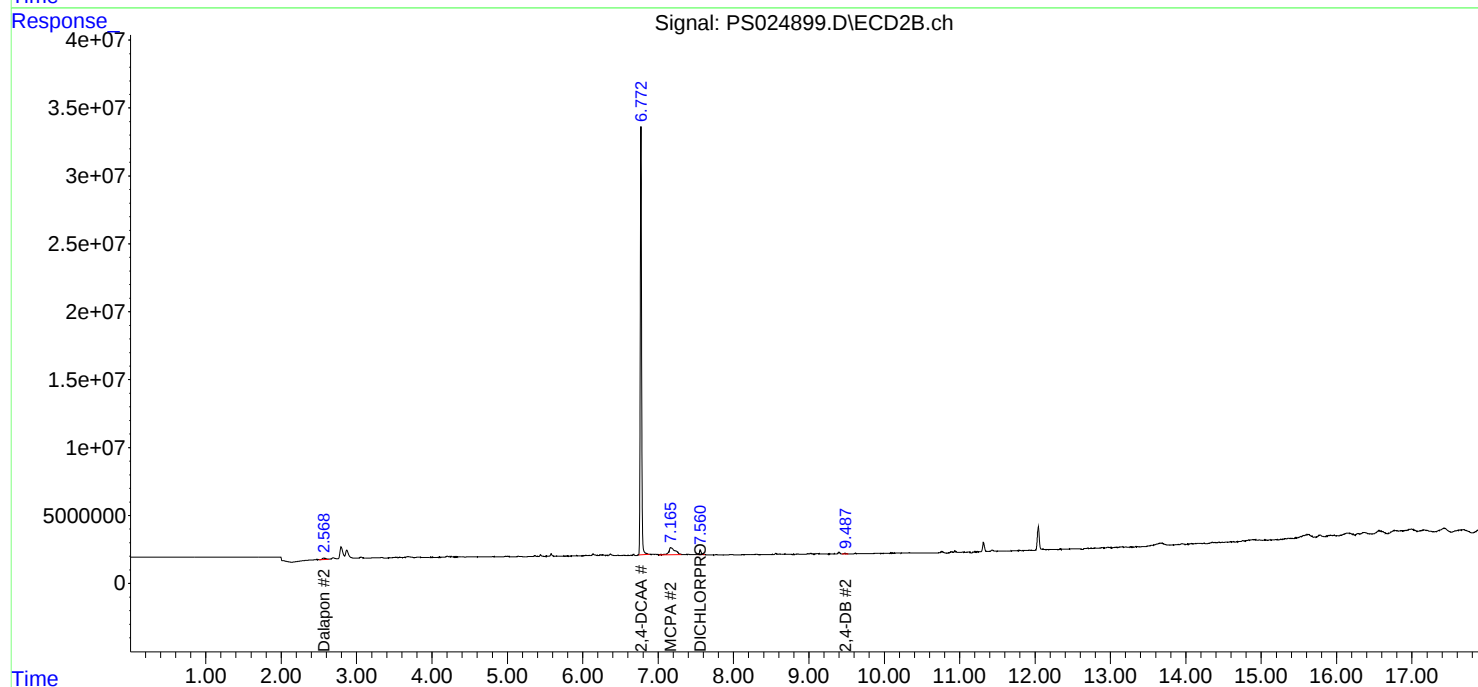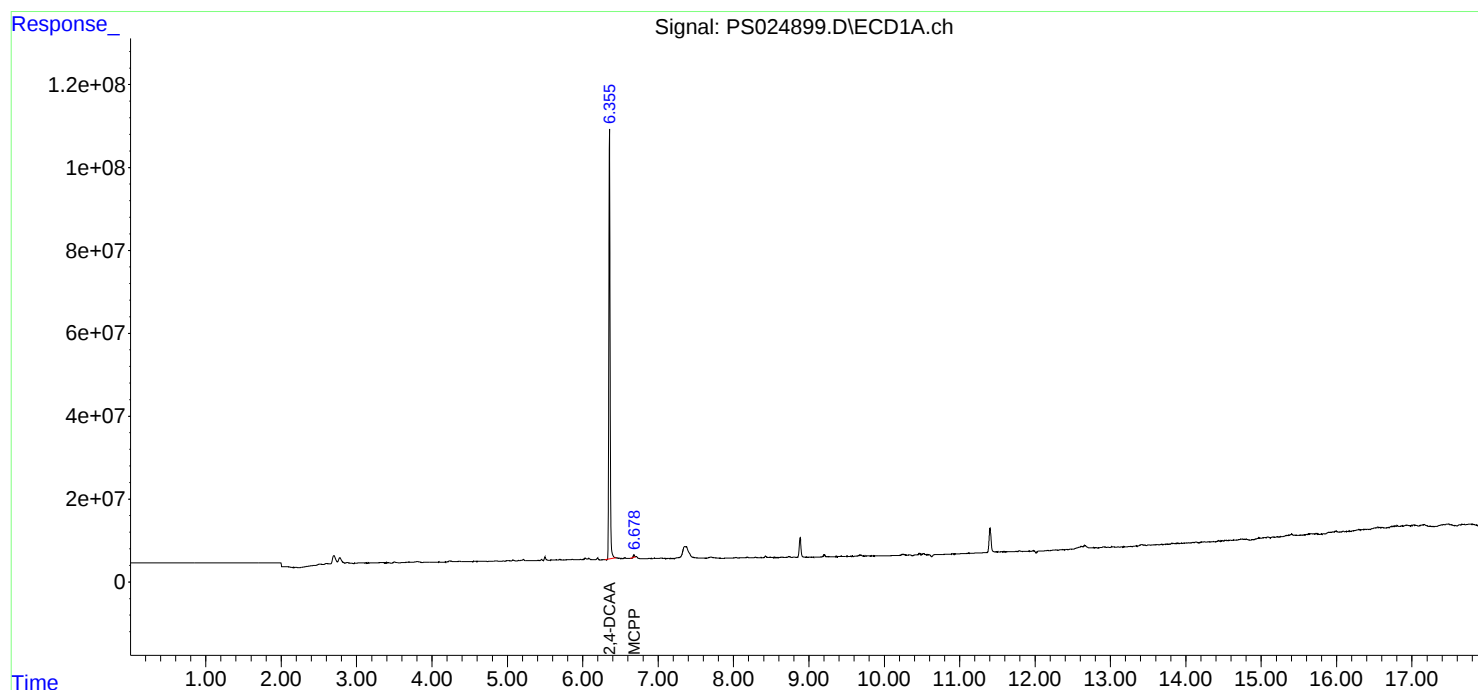


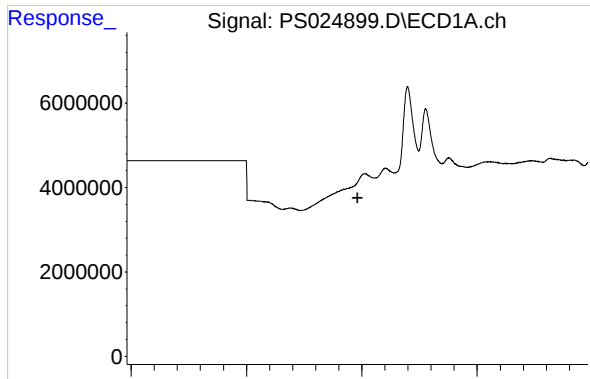

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 2.481 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

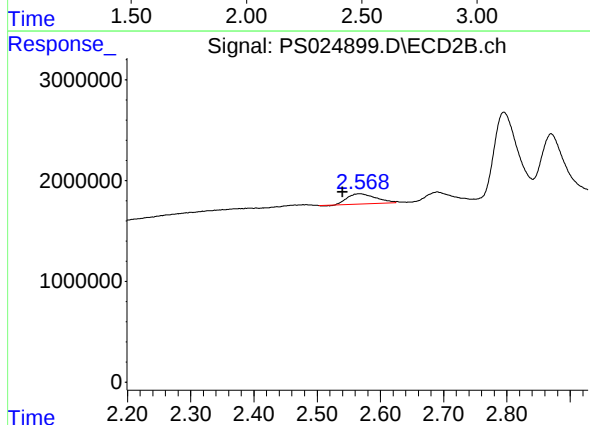


#1 Dalapon

R.T.: 2.568 min  
Delta R.T.: 0.028 min  
Response: 3207348  
Conc: 3.04 ng/ml

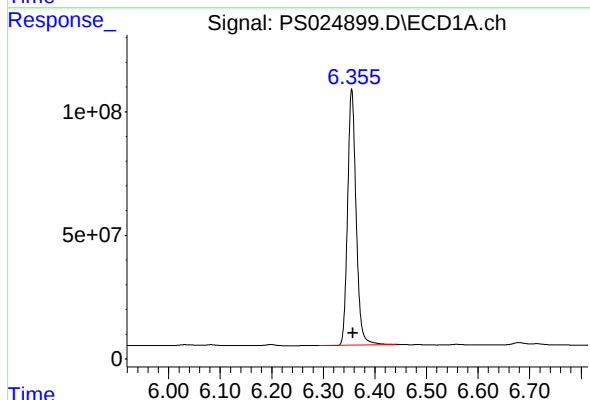


#4 2,4-DCAA

R.T.: 6.355 min  
Delta R.T.: -0.002 min  
Response: 1189288347  
Conc: 582.56 ng/ml

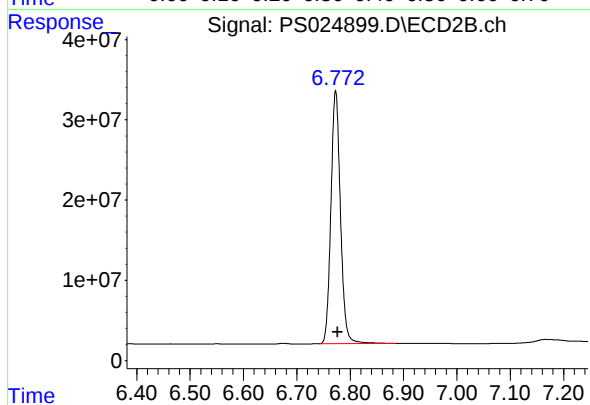

#4 2,4-DCAA


R.T.: 6.773 min  
Delta R.T.: -0.004 min  
Response: 391086574  
Conc: 579.73 ng/ml

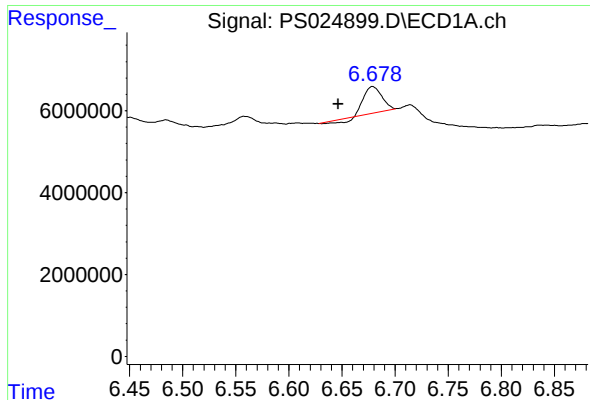

#6 MCPP


R.T.: 6.679 min  
Delta R.T.: 0.032 min  
Response: 7004042  
Conc: 1.12 ug/ml

Instrument :  
ECD\_S  
ClientSampleId :

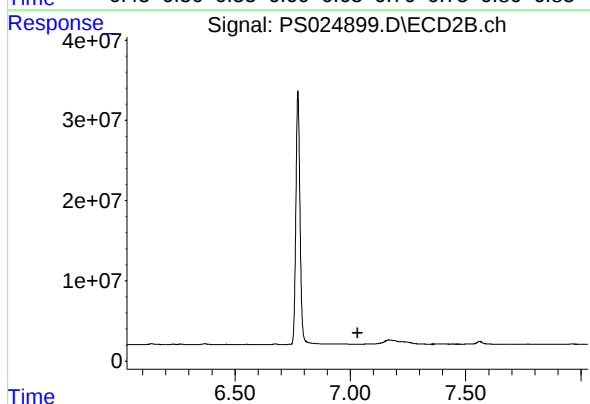


#6 MCPP

R.T.: 0.000 min  
Exp R.T. : 7.031 min  
Response: 0  
Conc: N.D.

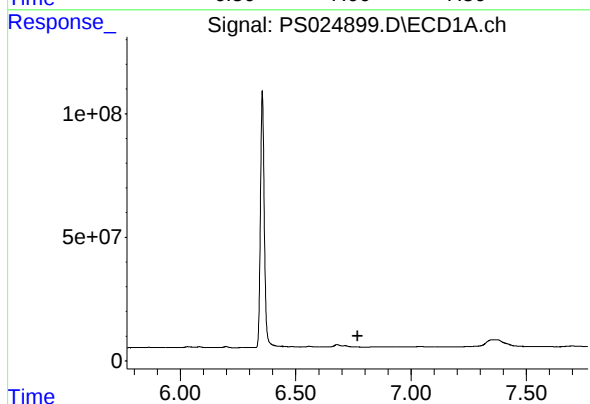


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 6.768 min  
Response: 0  
Conc: N.D.

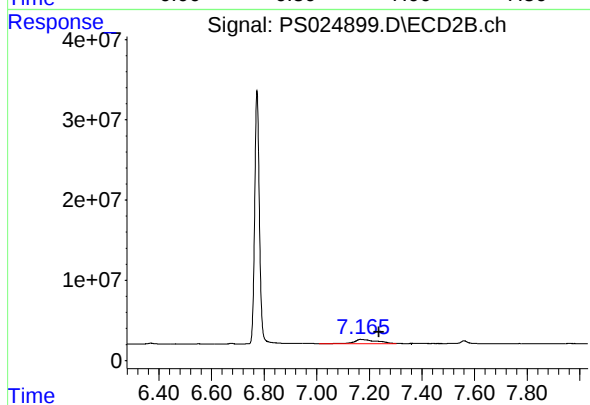

#7 MCPA


R.T.: 7.167 min  
Delta R.T.: -0.070 min  
Response: 30826434  
Conc: 10.00 ug/ml

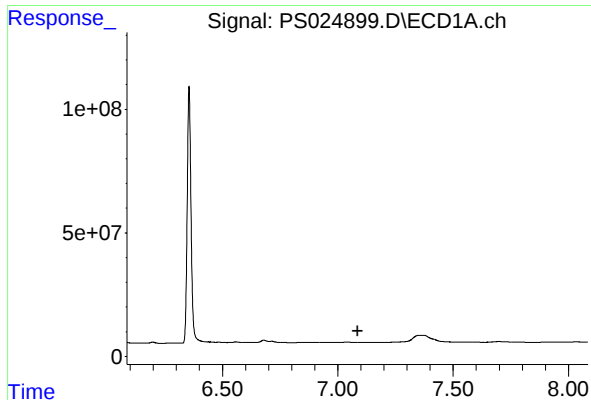

#8 DICHLORPROP


R.T.: 0.000 min  
Exp R.T.: 7.085 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

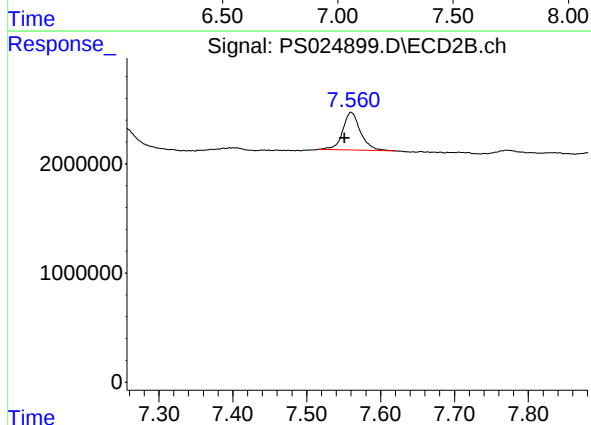


#8 DICHLORPROP

R.T.: 7.560 min  
Delta R.T.: 0.009 min  
Response: 5683571  
Conc: 7.78 ng/ml

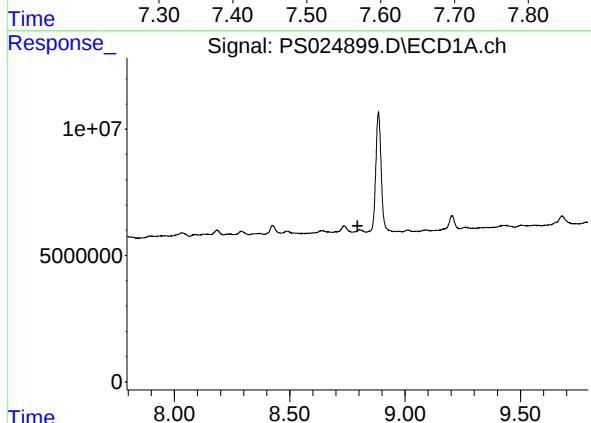

#13 2,4-DB

R.T.: 0.000 min  
Exp R.T.: 8.794 min  
Response: 0  
Conc: N.D.

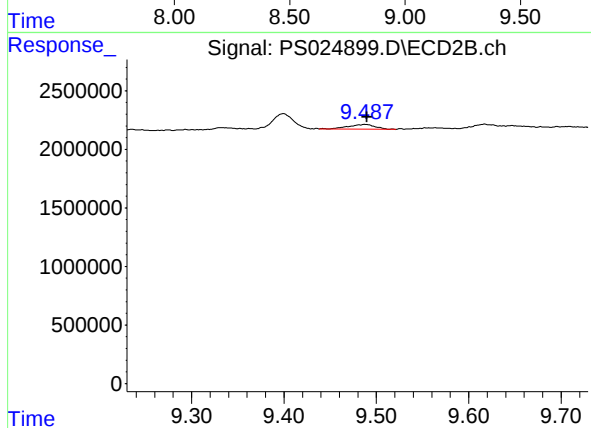

#13 2,4-DB

R.T.: 9.488 min  
Delta R.T.: -0.002 min  
Response: 868087  
Conc: 1.78 ng/ml