

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112124\
 Data File : PS028588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 13:18
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:18:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.669f	0.000	2069262	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.019	0.000	6059857	0	3.568	N.D.	#
5) T	DICAMBA	7.423	7.923	1201394	3282474	<MDL	<MDL	#
6) T	MCP	7.661f	0.000	5303865	0	<MDL	N.D.	#
8) T	DICHLORPROP	0.000	8.695f	0	3666516	N.D.	2.510	
9) T	2,4-D	8.385	0.000	32948928	0	10.306	N.D.	#
10) T	Pentachlo...	8.660	0.000	2334298	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.243	0.000	422649	0	<MDL	N.D.	#
12) T	2,4,5-T	9.538	10.307	3089094	7955432	<MDL	<MDL	#
14) T	DINOSEB	11.321	0.000	1483343	0	<MDL	N.D.	#
15) T	Picloram	11.133	12.344	93903021	24381055	3.335	2.154	#
16) T	DCPA	11.576f	12.344f	7325954	24381055	<MDL	2.514	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112124\
Data File : PS028588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 13:18
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:18:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

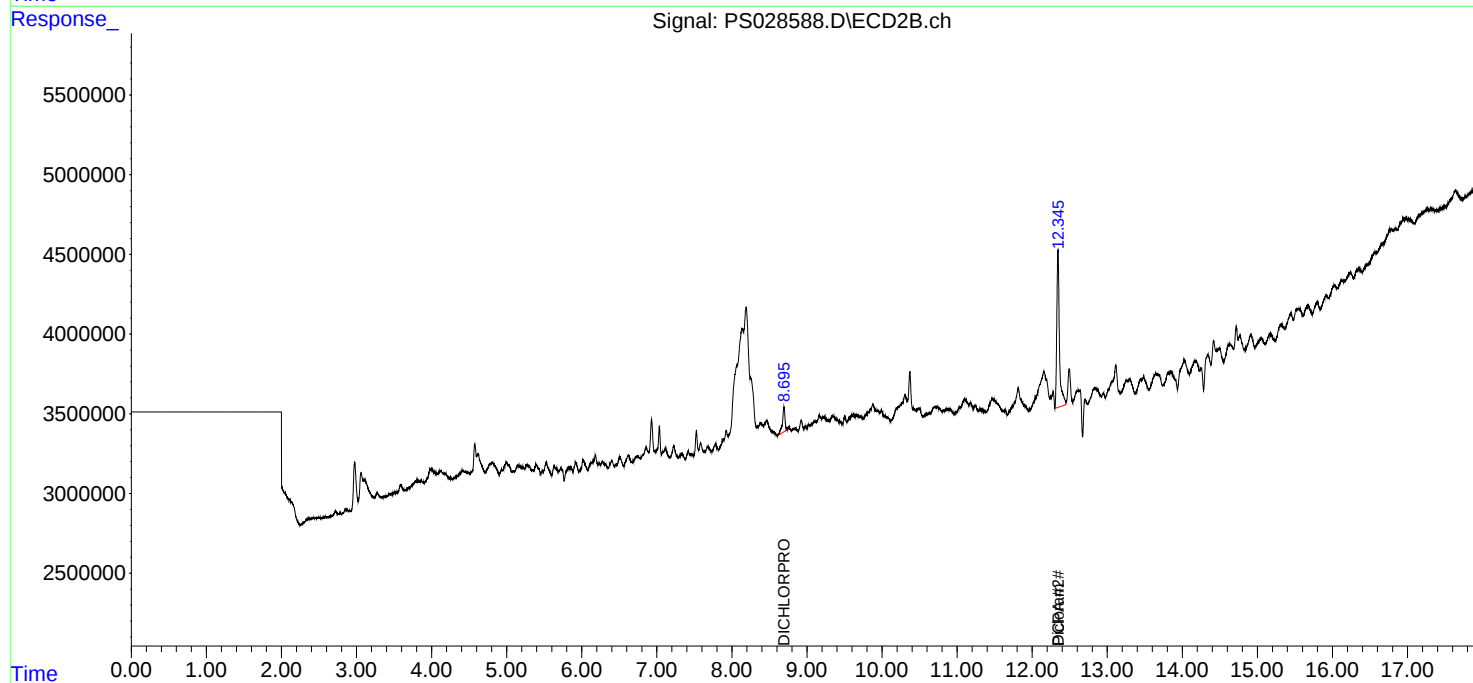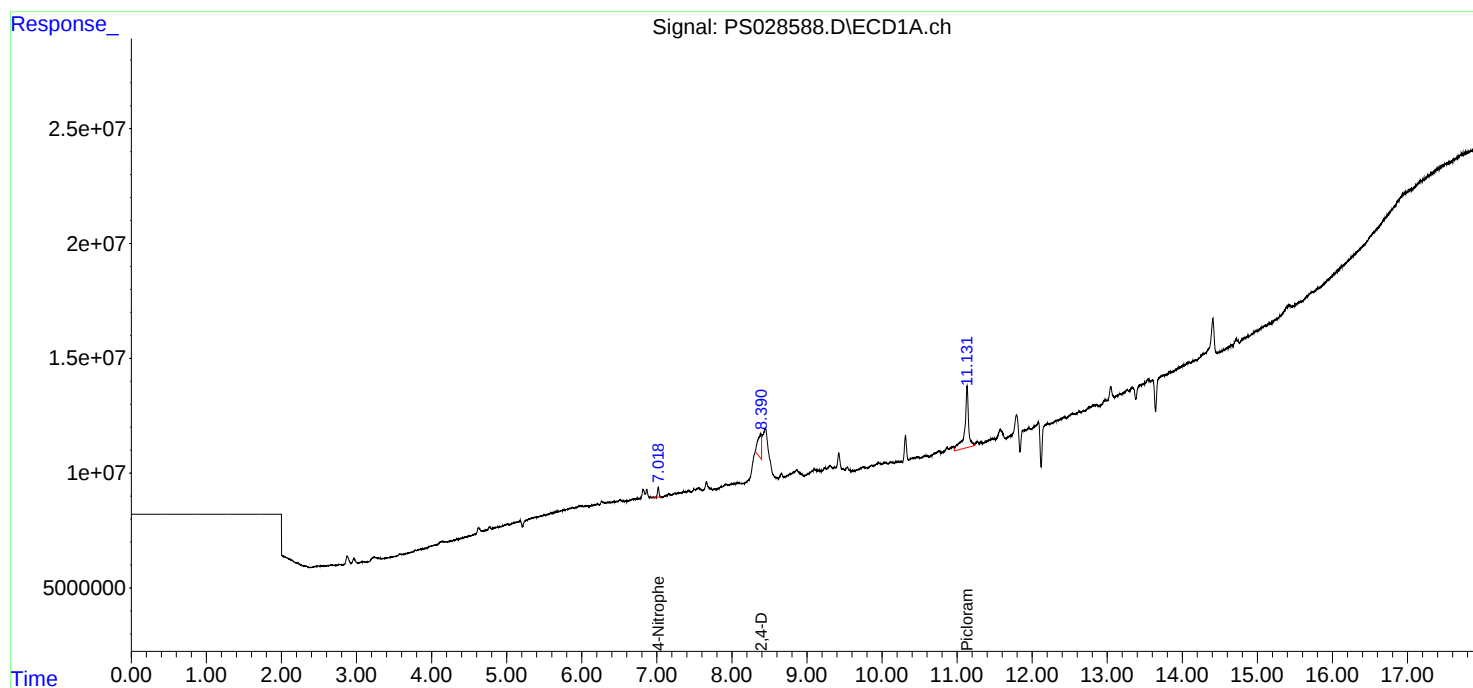


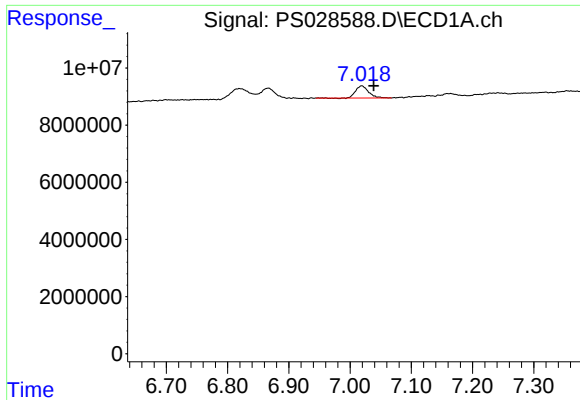

#3 4-Nitrophenol


R.T.: 7.019 min
Delta R.T.: -0.020 min
Response: 6059857
Conc: 3.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

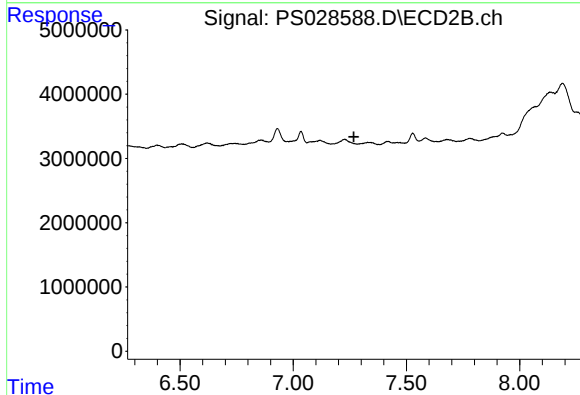


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

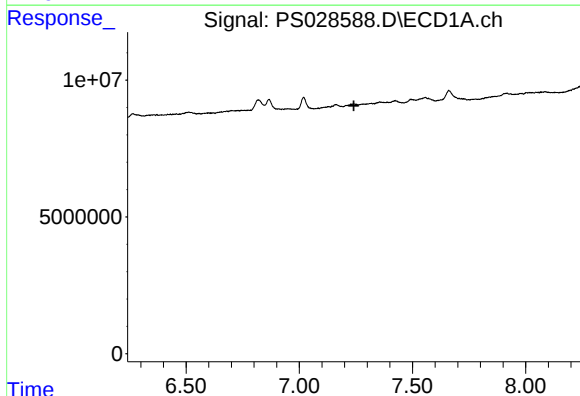


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: -106350
Conc: N.D.

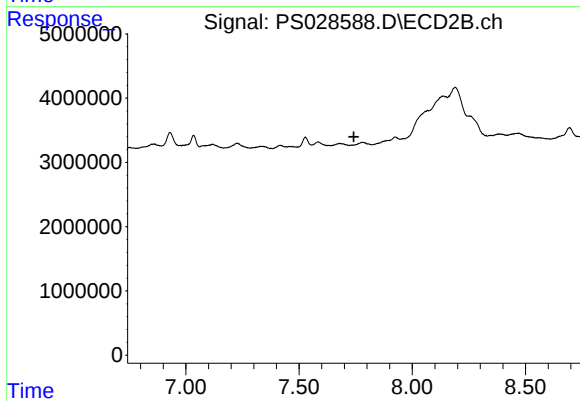

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.742 min
Response: 0
Conc: N.D.

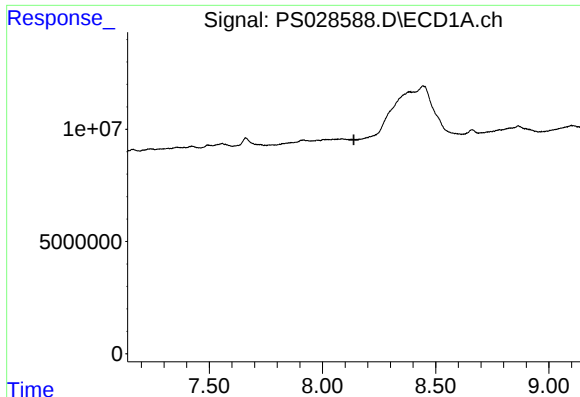

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

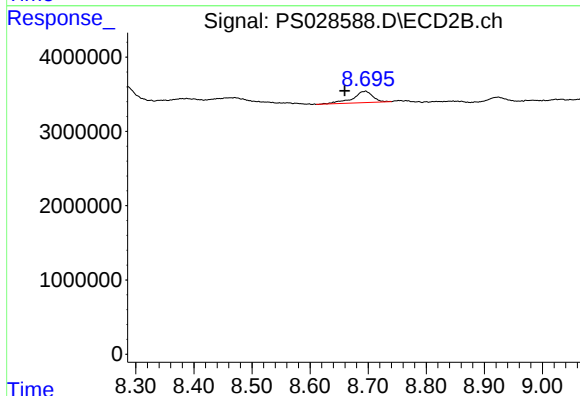


#8 DICHLORPROP

R.T.: 8.695 min
Delta R.T.: 0.036 min
Response: 3666516
Conc: 2.51 ng/ml

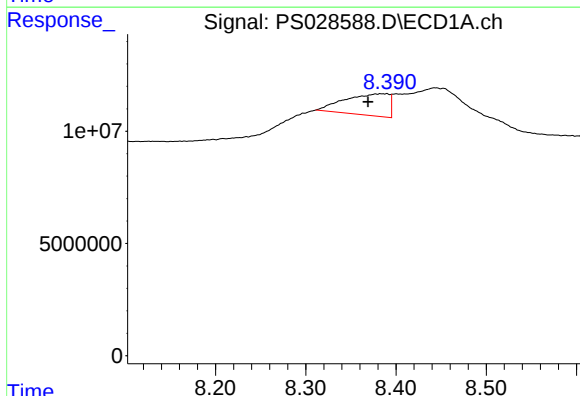


#9 2,4-D

R.T.: 8.385 min
Delta R.T.: 0.016 min
Response: 32948928
Conc: 10.31 ng/ml

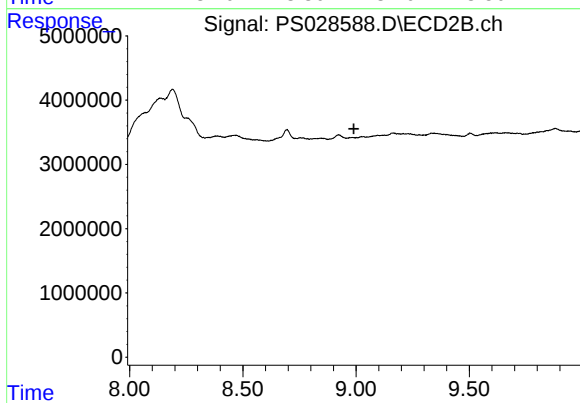

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.990 min
Response: 0
Conc: N.D.

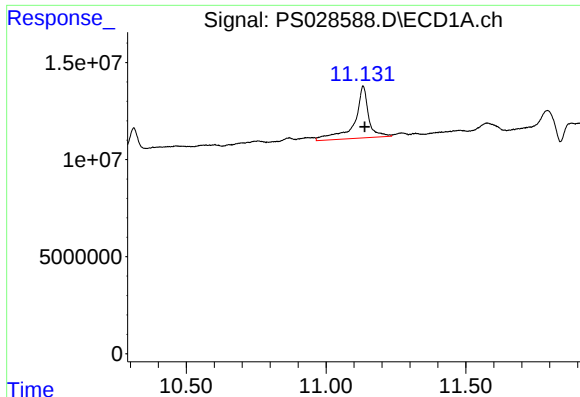

#15 Picloram


R.T.: 11.133 min
Delta R.T.: -0.005 min
Response: 93903021
Conc: 3.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

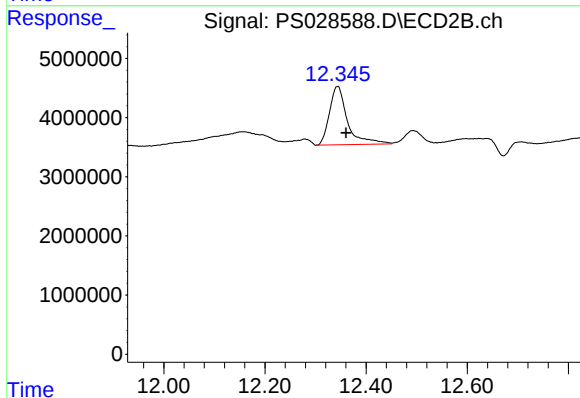


#15 Picloram

R.T.: 12.344 min
Delta R.T.: -0.017 min
Response: 24381055
Conc: 2.15 ng/ml

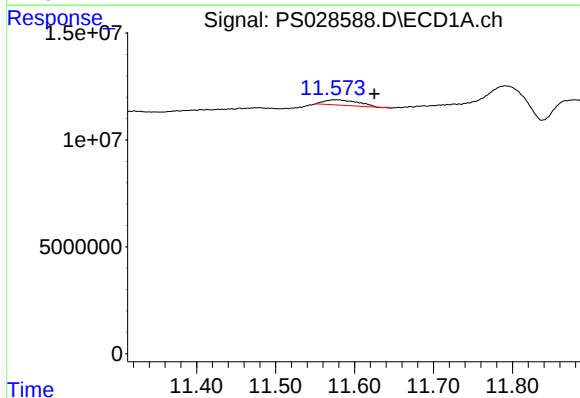

#16 DCPA

R.T.: 11.576 min
Delta R.T.: -0.049 min
Response: 7325954
Conc: N.D.

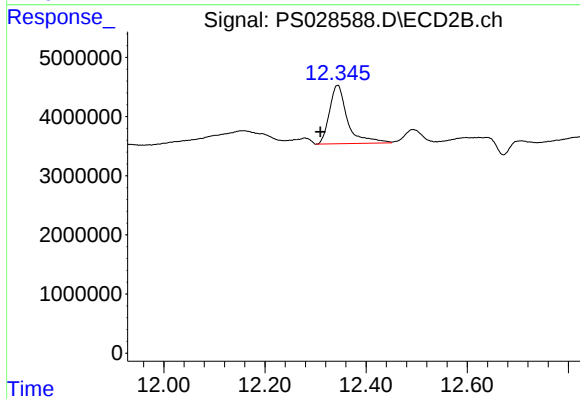

#16 DCPA

R.T.: 12.344 min
Delta R.T.: 0.034 min
Response: 24381055
Conc: 2.51 ng/ml