

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112124\
 Data File : PS028589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 13:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:19:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.732	1491.2E6	661.5E6	583.431	511.903
Target Compounds							
1) T	Dalapon	2.626	0.000	529075	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.437f	0.000	542696	0	<MDL	N.D. #
3) T	4-Nitroph...	7.028	0.000	5494474	0	3.235	N.D. #
7) T	MCPA	0.000	8.259f	0	10599423	N.D.	1.711
8) T	DICHLORPROP	0.000	8.699f	0	3019978	N.D.	2.068
12) T	2,4,5-T	9.539	0.000	1853672	0	<MDL	N.D. #
14) T	DINOSEB	11.315	0.000	2030106	0	<MDL	N.D. #
15) T	Picloram	11.131	12.347	36492137	19330046	1.296	1.708 #
16) T	DCPA	11.598f	12.347f	3339514	19330046	<MDL	1.993 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112124\
Data File : PS028589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 13:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:19:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

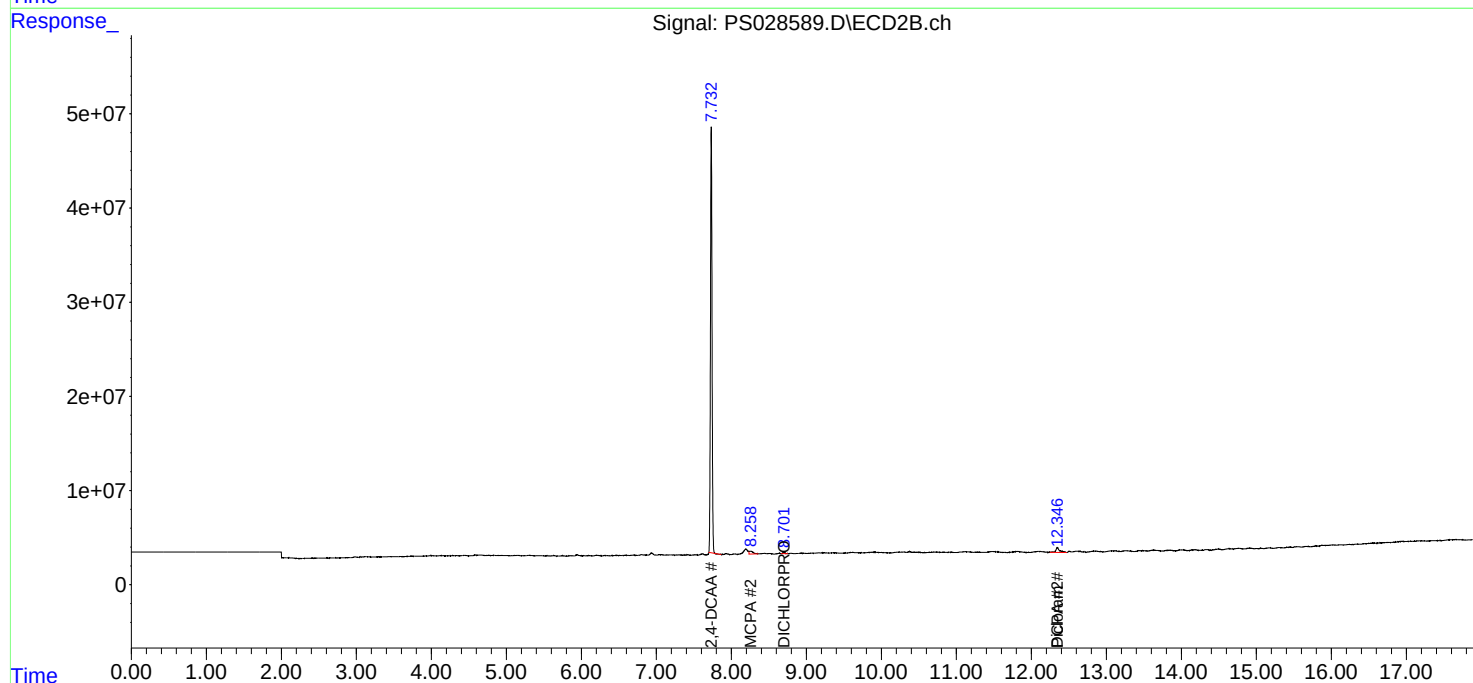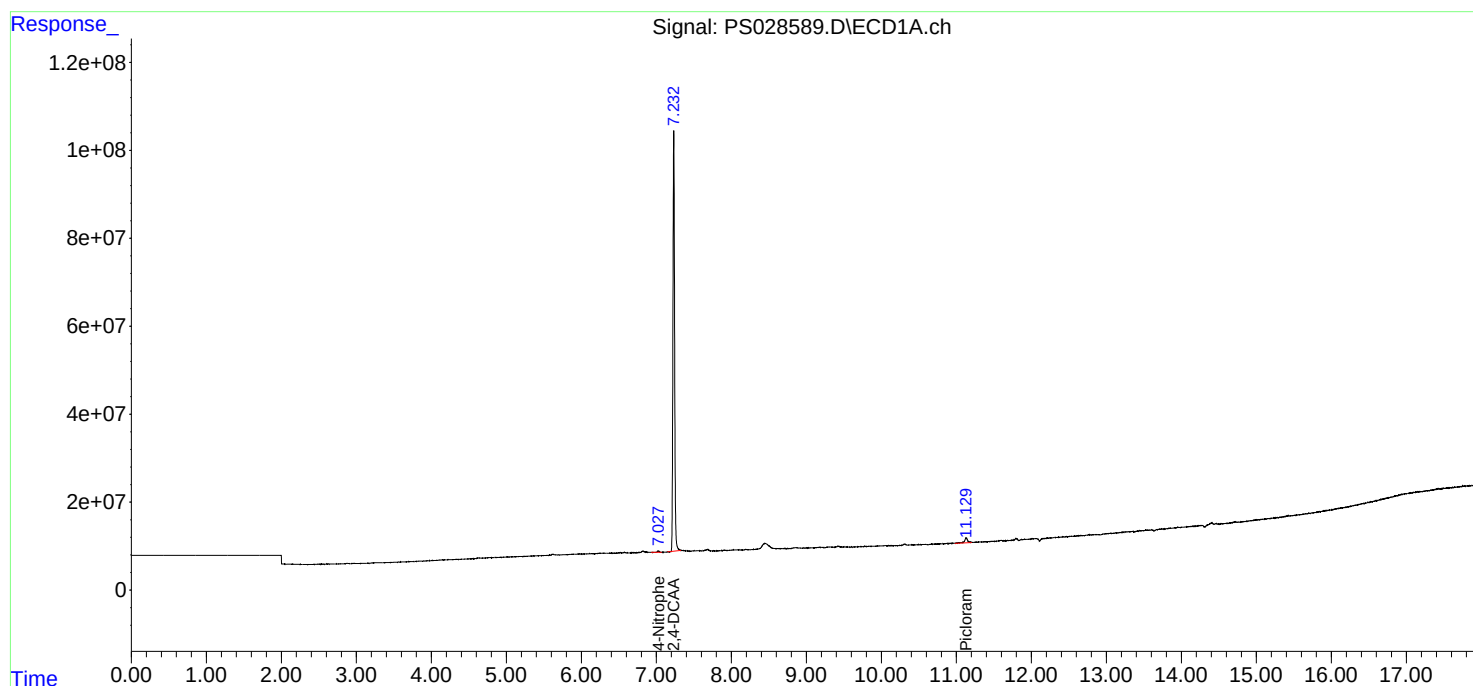


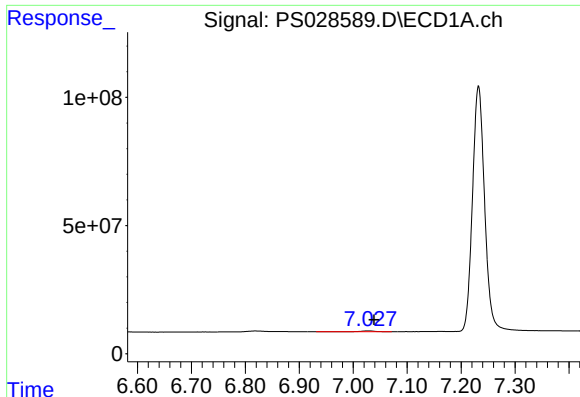

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.011 min
Response: 5494474
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

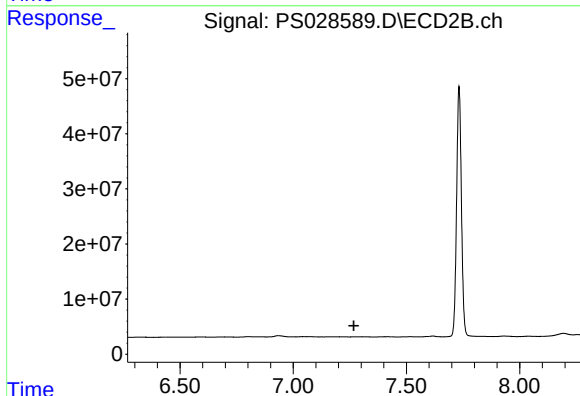


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

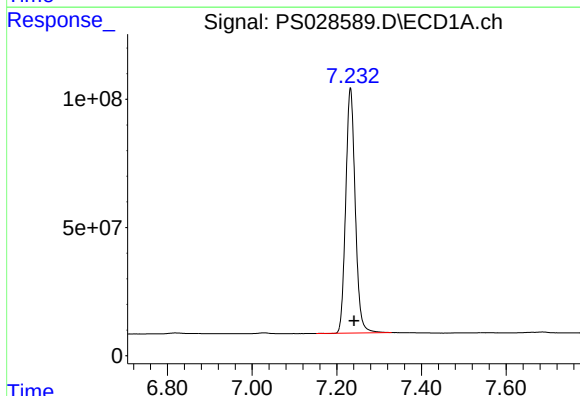


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.009 min
Response: 1491182013
Conc: 583.43 ng/ml

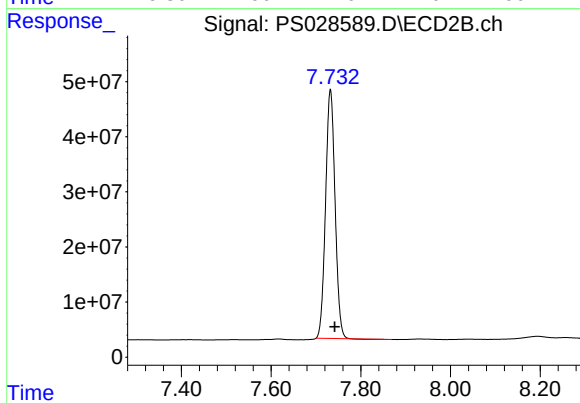

#4 2,4-DCAA


R.T.: 7.732 min
Delta R.T.: -0.010 min
Response: 661534439
Conc: 511.90 ng/ml

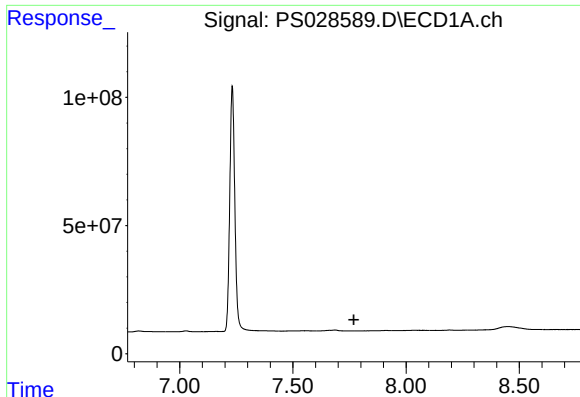

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.769 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

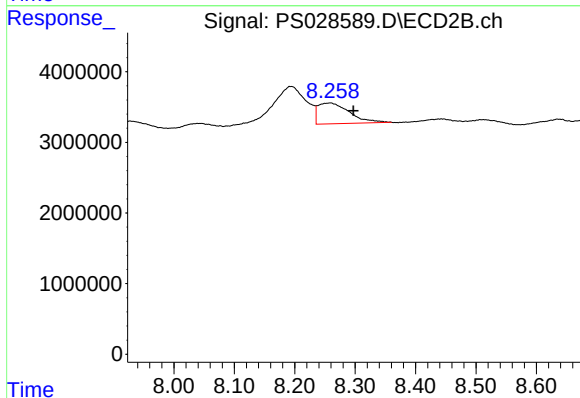


#7 MCPA

R.T.: 8.259 min
Delta R.T.: -0.038 min
Response: 10599423
Conc: 1.71 ug/ml

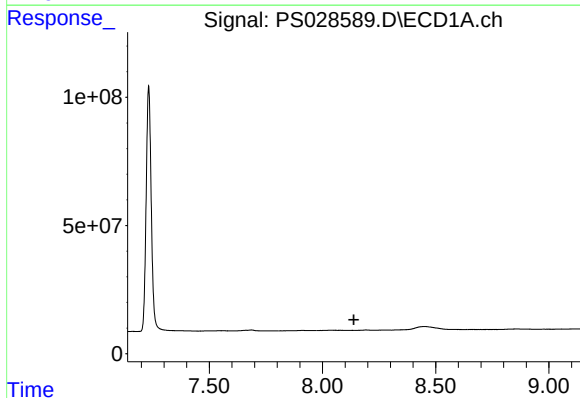


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

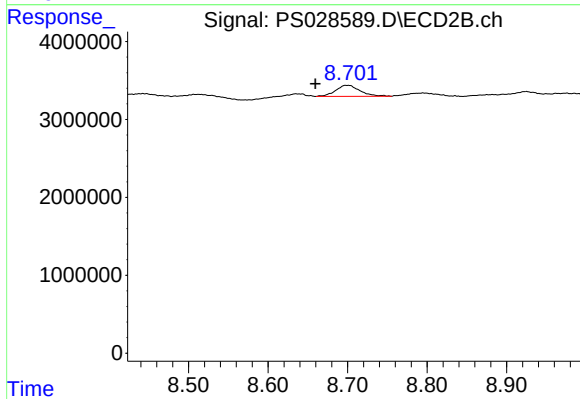

#8 DICHLORPROP


R.T.: 8.699 min
Delta R.T.: 0.040 min
Response: 3019978
Conc: 2.07 ng/ml

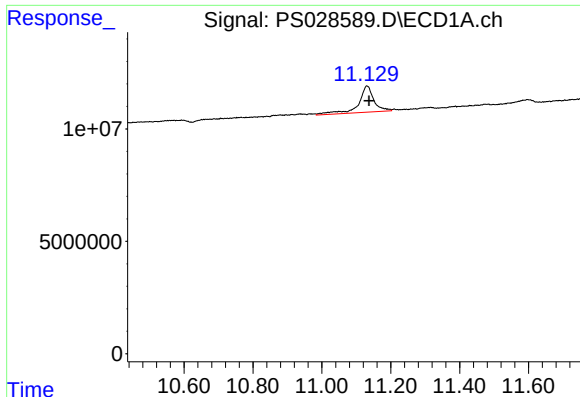

#15 Picloram


R.T.: 11.131 min
Delta R.T.: -0.007 min
Response: 36492137
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

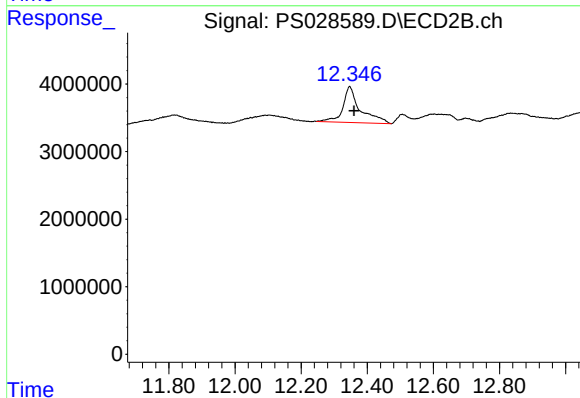


#15 Picloram

R.T.: 12.347 min
Delta R.T.: -0.014 min
Response: 19330046
Conc: 1.71 ng/ml

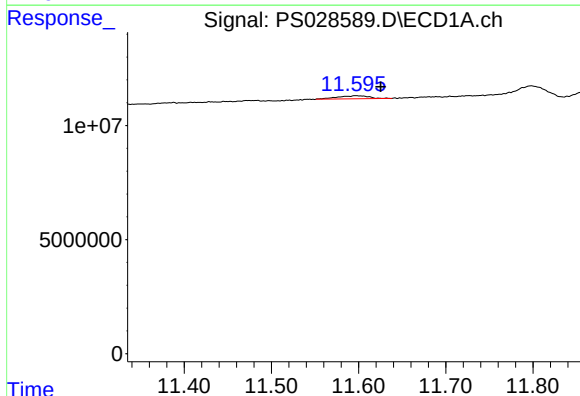

#16 DCPA

R.T.: 11.598 min
Delta R.T.: -0.028 min
Response: 3339514
Conc: N.D.

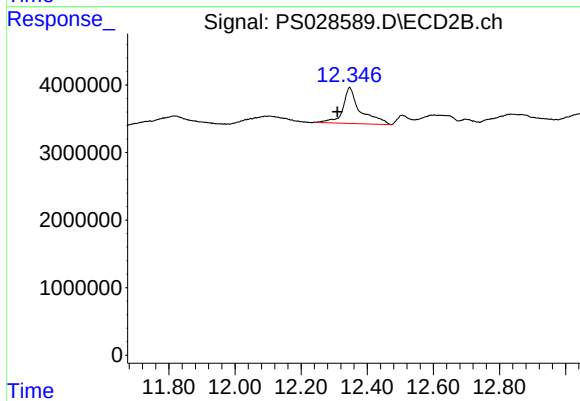

#16 DCPA

R.T.: 12.347 min
Delta R.T.: 0.037 min
Response: 19330046
Conc: 1.99 ng/ml