

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112124\
 Data File : PS028592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 14:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:21:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.733	1490.3E6	665.9E6	583.089	515.299
Target Compounds							
2) T	3,5-DICHL...	6.422	0.000	194158	0	<MDL	N.D. #
3) T	4-Nitroph...	7.028	0.000	5481641	0	3.227	N.D. #
5) T	DICAMBA	0.000	7.930	0	3225674	N.D.	<MDL
6) T	MCP	7.661f	0.000	15443364	0	2.195	N.D. #
7) T	MCPA	0.000	8.258f	0	12162514	N.D.	1.964
8) T	DICHLORPROP	0.000	8.700f	0	5788439	N.D.	3.963
12) T	2,4,5-T	9.537	0.000	790683	0	<MDL	N.D. #
14) T	DINOSEB	11.301f	0.000	2317233	0	<MDL	N.D. #
15) T	Picloram	11.131	12.347	28132641	13667754	<MDL	1.208 #
16) T	DCPA	11.599f	12.347f	2705872	13667754	<MDL	1.409 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112124\
Data File : PS028592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 14:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:21:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

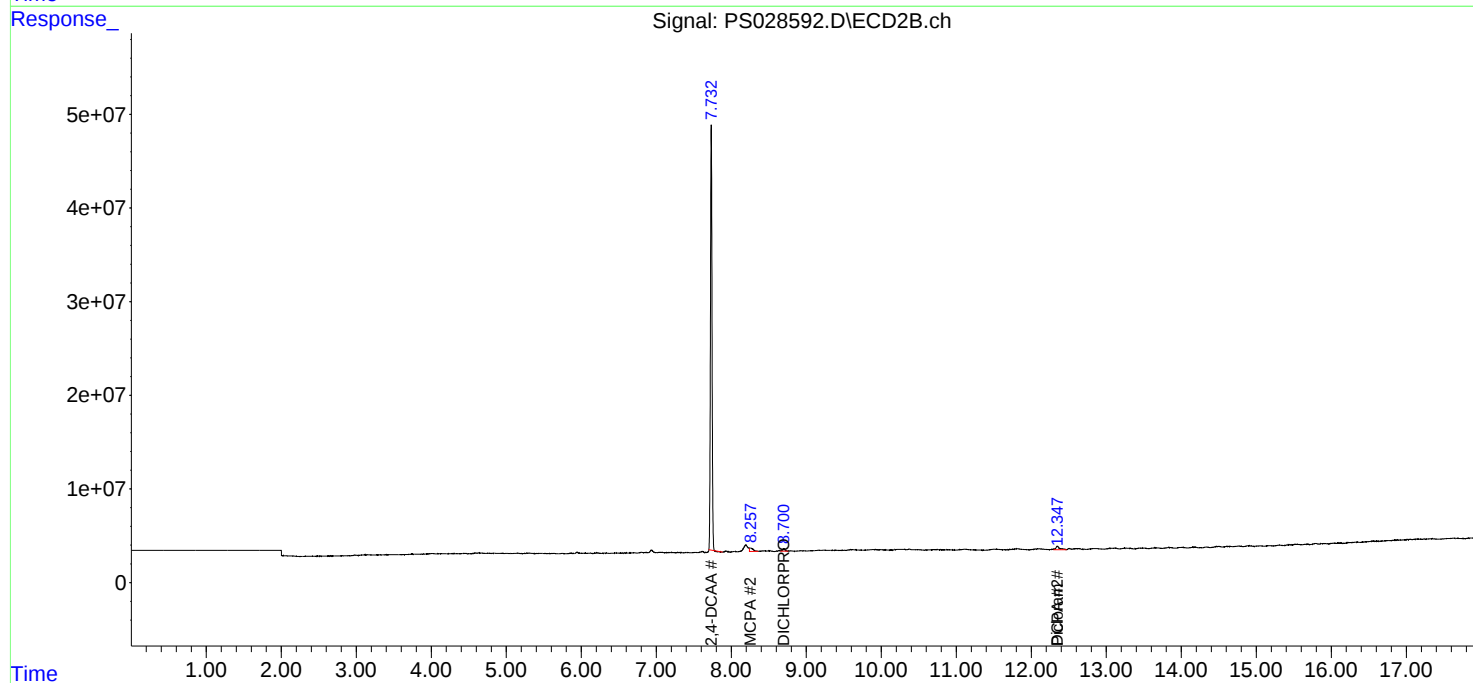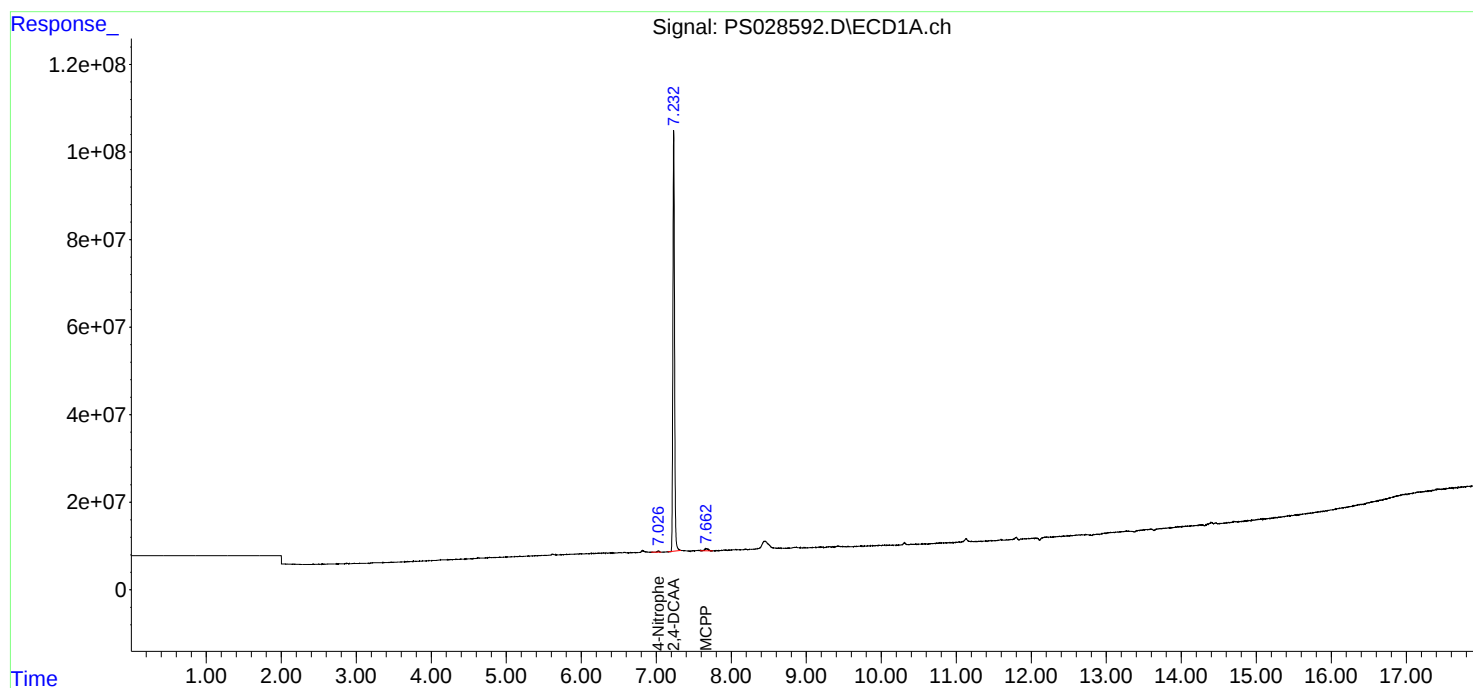


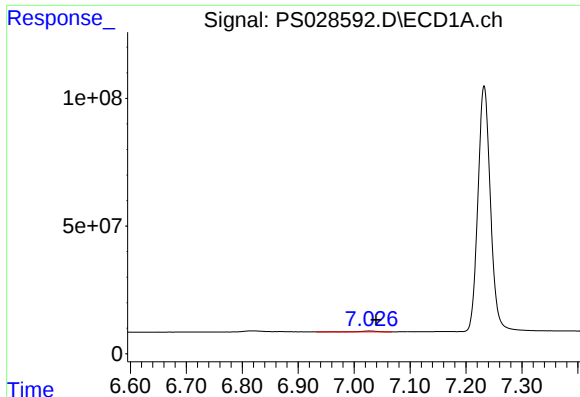

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.011 min
Response: 5481641
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

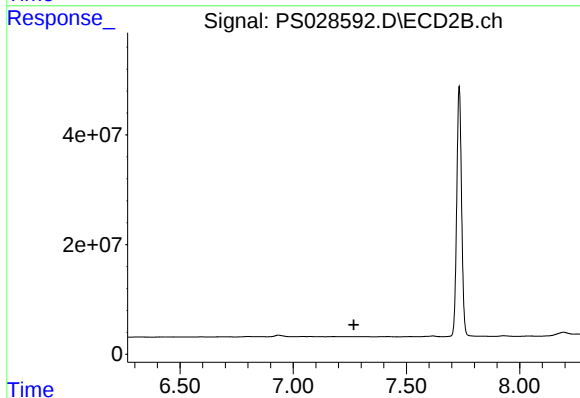


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

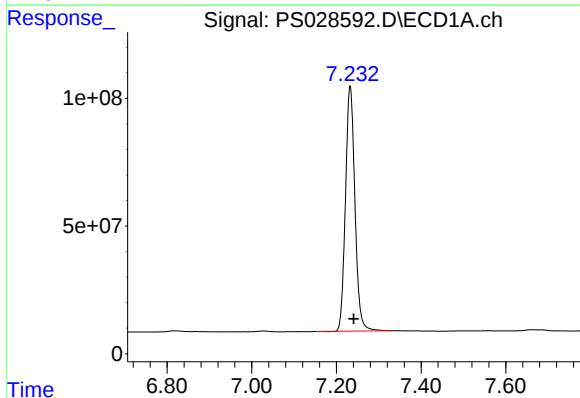


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.008 min
Response: 1490305578
Conc: 583.09 ng/ml

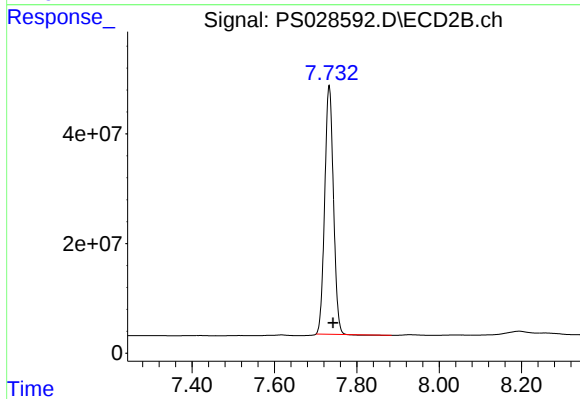

#4 2,4-DCAA


R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 665923252
Conc: 515.30 ng/ml

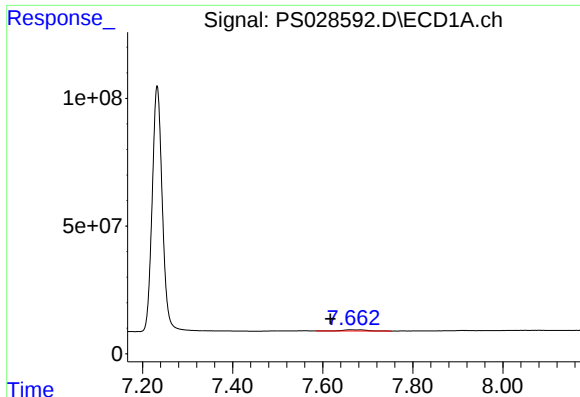

#6 MCPP


R.T.: 7.661 min
Delta R.T.: 0.044 min
Response: 15443364
Conc: 2.20 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

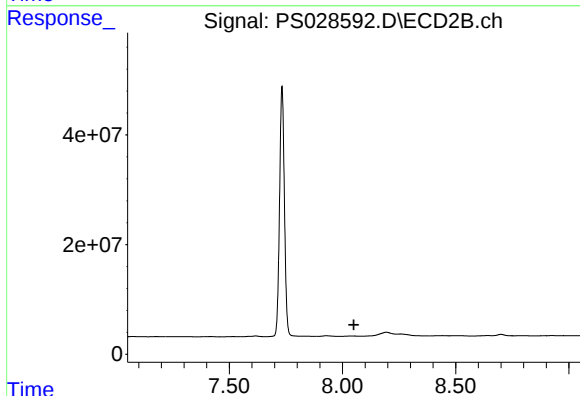


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

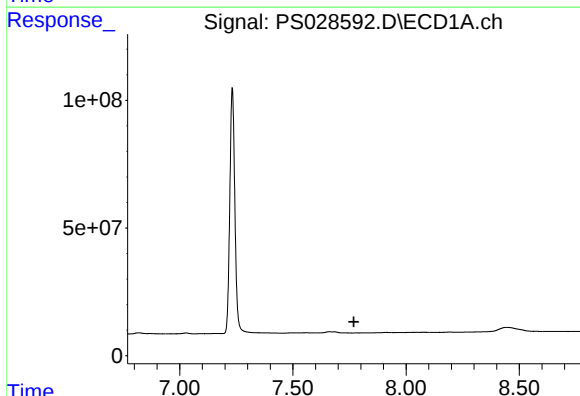


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.769 min
Response: 0
Conc: N.D.

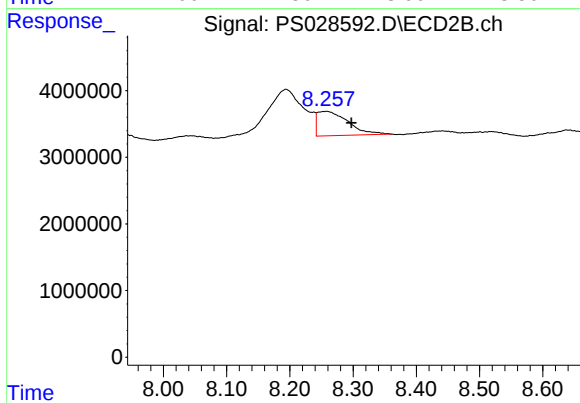

#7 MCPA


R.T.: 8.258 min
Delta R.T.: -0.040 min
Response: 12162514
Conc: 1.96 ug/ml

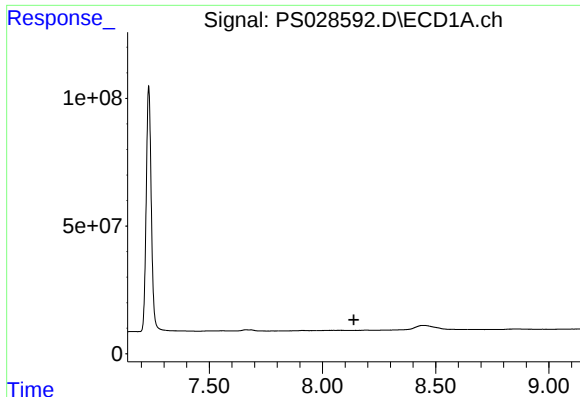

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

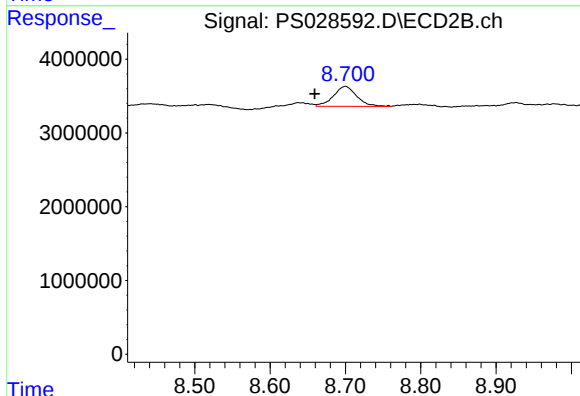


#8 DICHLORPROP

R.T.: 8.700 min
Delta R.T.: 0.040 min
Response: 5788439
Conc: 3.96 ng/ml

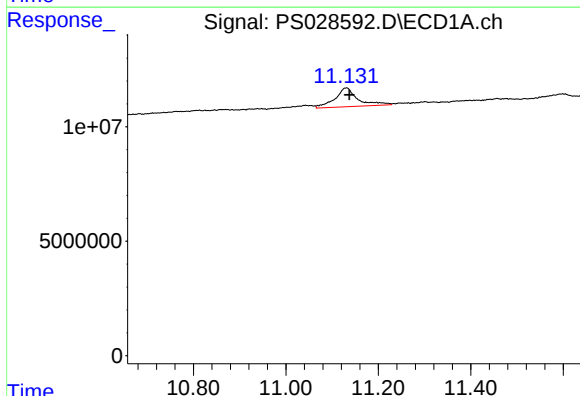


#15 Picloram

R.T.: 11.131 min
Delta R.T.: -0.007 min
Response: 28132641
Conc: N.D.

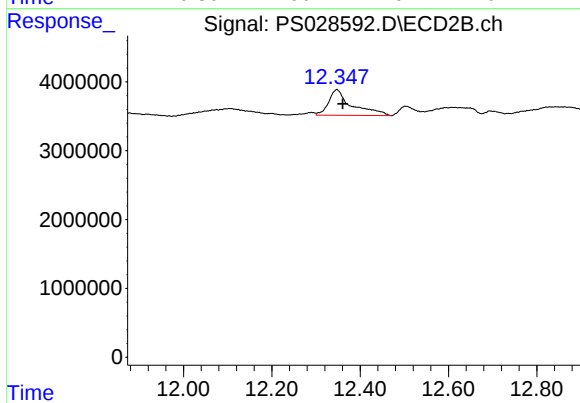

#15 Picloram


R.T.: 12.347 min
Delta R.T.: -0.013 min
Response: 13667754
Conc: 1.21 ng/ml

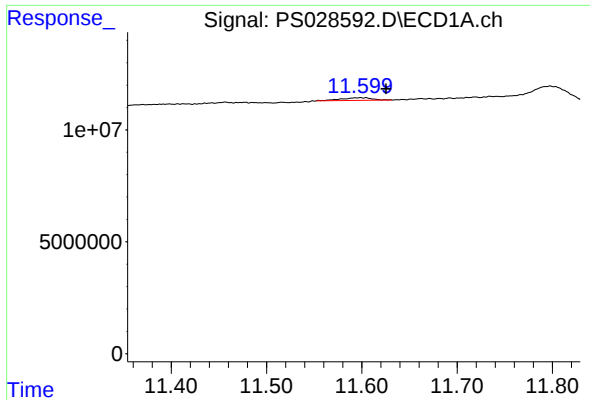

#16 DCPA

R.T.: 11.599 min
Delta R.T.: -0.026 min
Response: 2705872
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

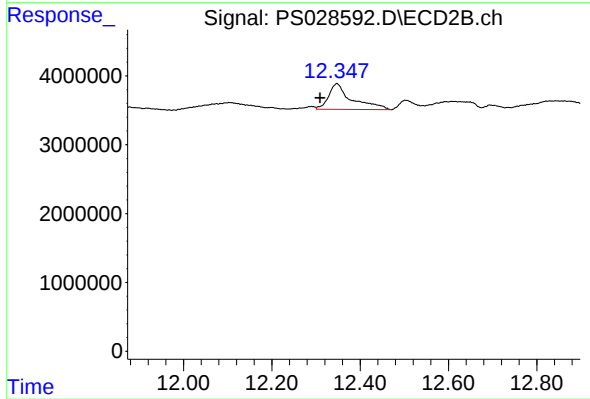

#16 DCPA

R.T.: 12.347 min
Delta R.T.: 0.038 min
Response: 13667754
Conc: 1.41 ng/ml