

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
 Data File : PS007781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 12:00
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 01:30:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.430	0.000	648.5E6	0	470.863	N.D. #
Target Compounds							
7) T	MCPA	0.000	5.473	0	41626269	N.D.	13.849
9) T	2,4-D	6.479	0.000	67874118	0	48.393	N.D. #
14) T	DINOSEB	9.024	0.000	79705931	0	13.272	N.D. #
15) T	Picloram	0.000	8.926	0	86643714	N.D.	14.788



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
Data File : PS007781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 12:00
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 01:30:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

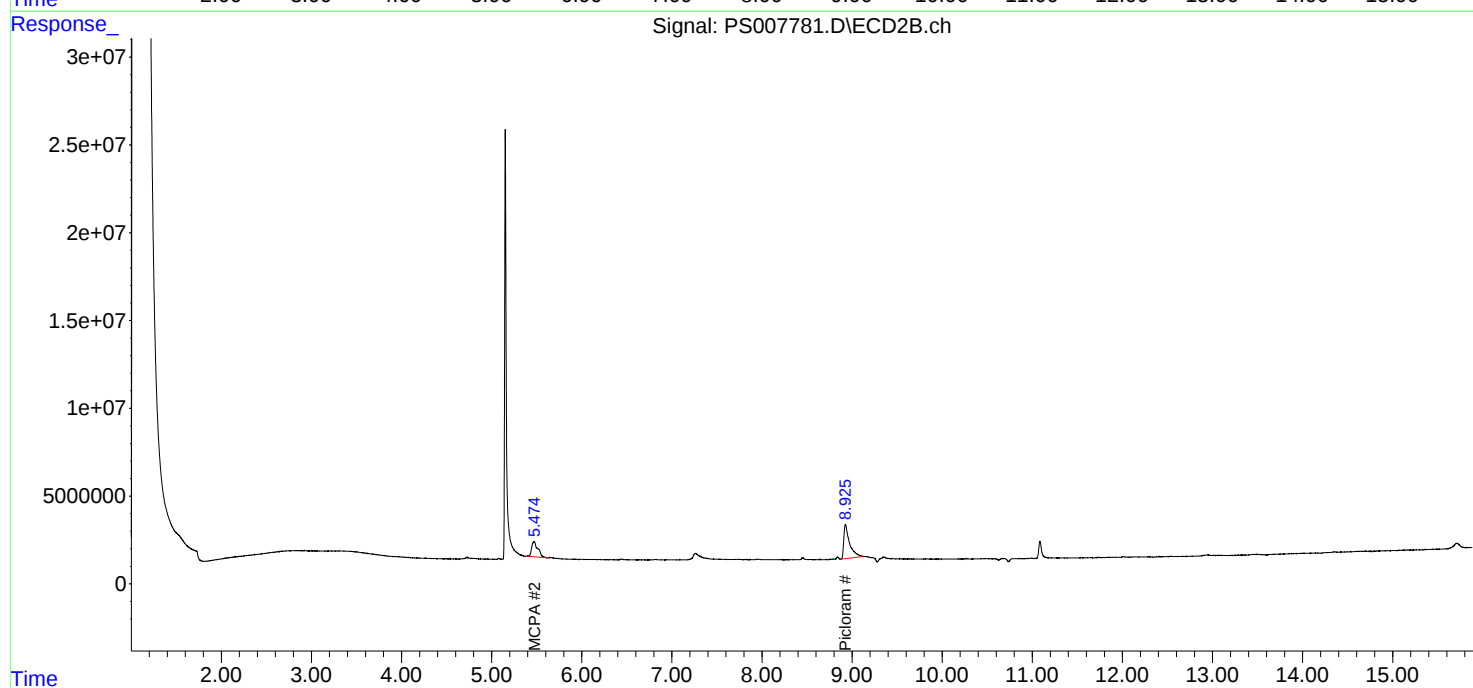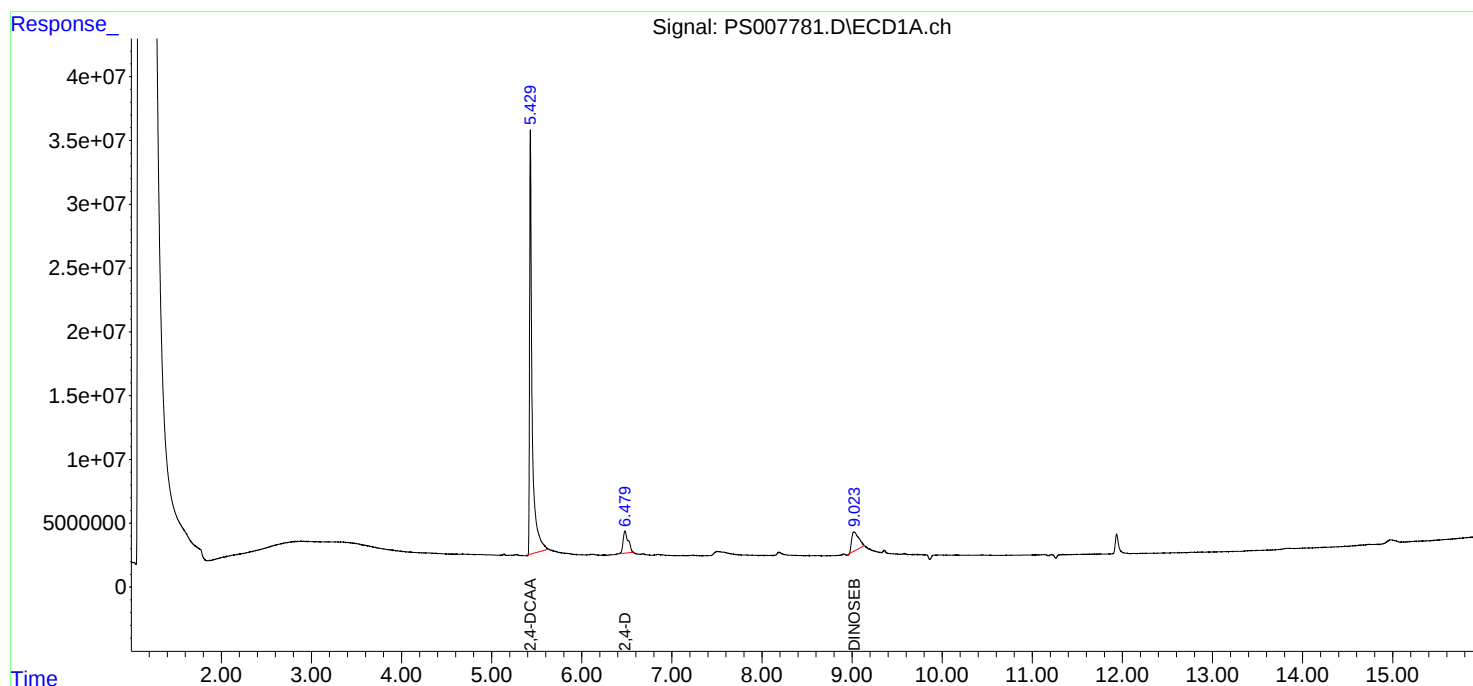


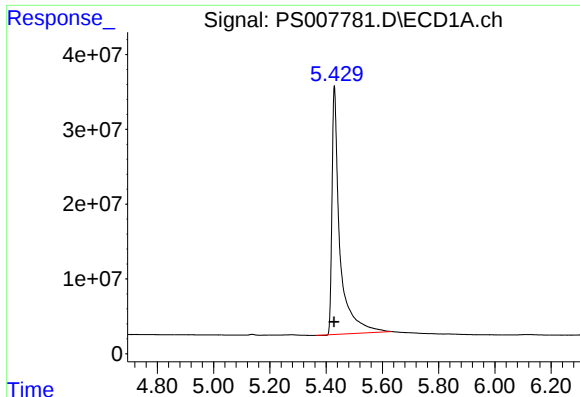

#4 2,4-DCAA


R.T.: 5.430 min
Delta R.T.: 0.001 min
Response: 648464960
Conc: 470.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

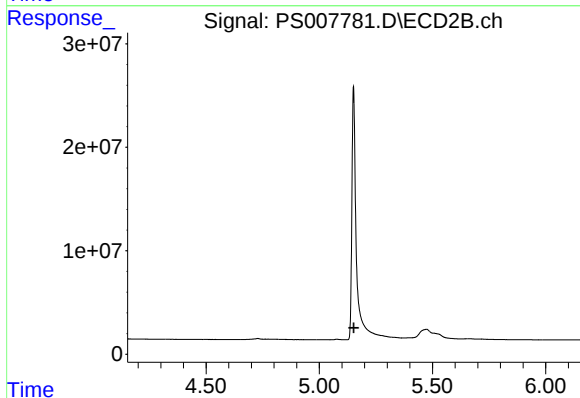


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.153 min
Response: 0
Conc: N.D.

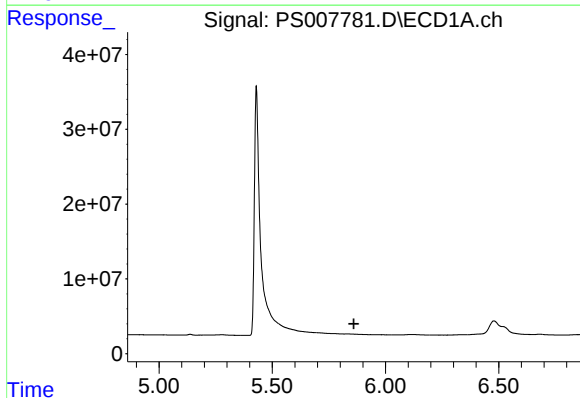


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

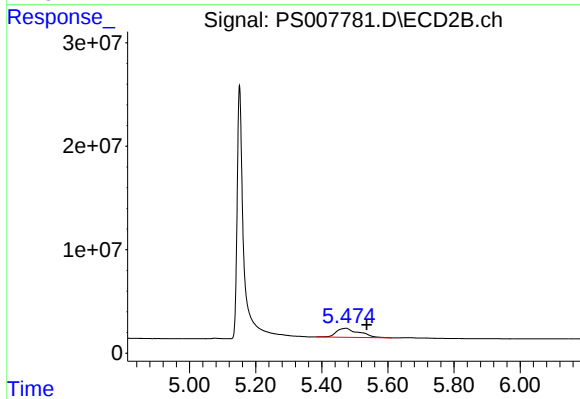

#7 MCPA


R.T.: 5.473 min
Delta R.T.: -0.063 min
Response: 41626269
Conc: 13.85 ug/ml

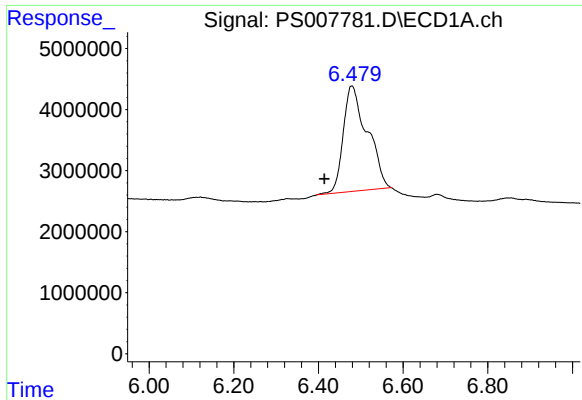

#9 2,4-D


R.T.: 6.479 min
Delta R.T.: 0.065 min
Response: 67874118
Conc: 48.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

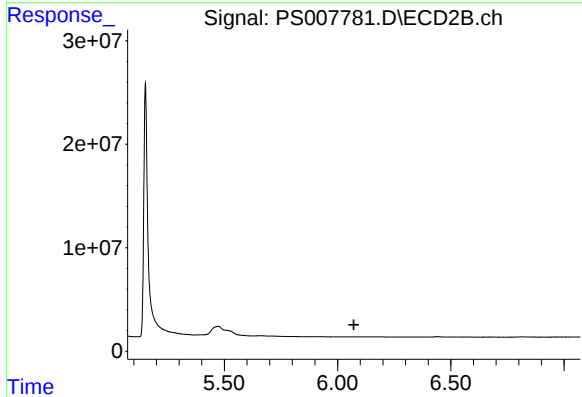


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

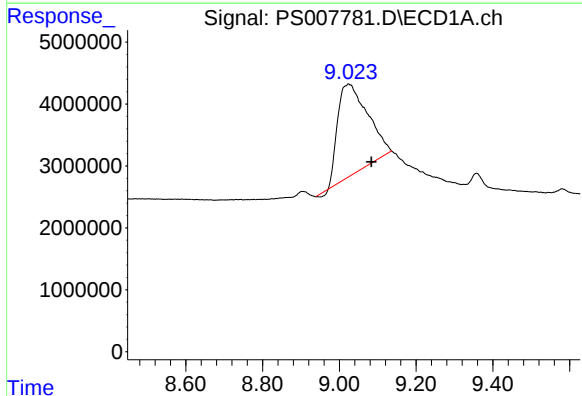


#14 DINOSEB

R.T.: 9.024 min
Delta R.T.: -0.059 min
Response: 79705931
Conc: 13.27 ng/ml

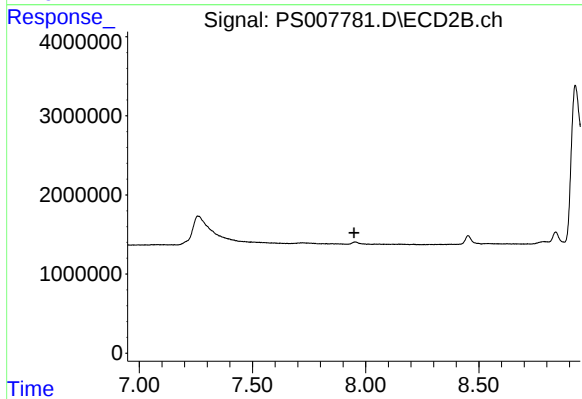

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 7.948 min
Response: 0
Conc: N.D.

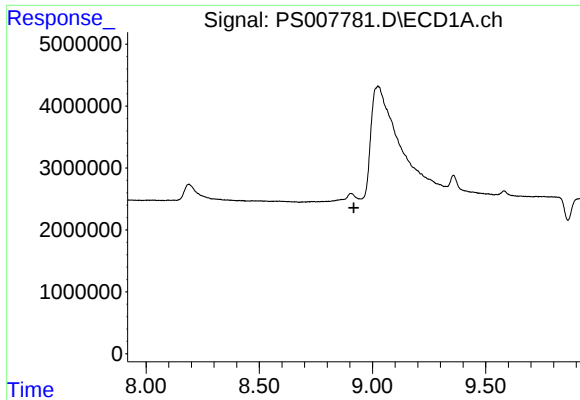

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

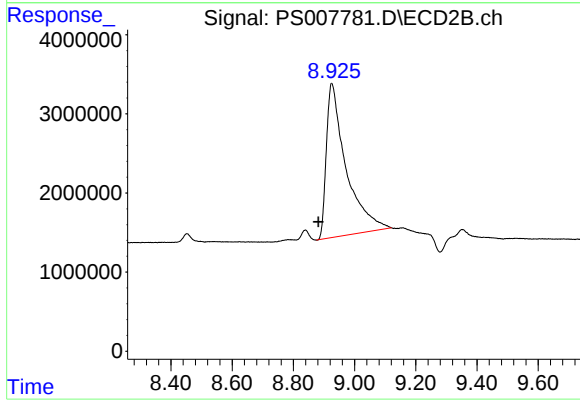

#15 Picloram

R.T.: 8.926 min
Delta R.T.: 0.044 min
Response: 86643714
Conc: 14.79 ng/ml