

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
 Data File : PS007783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 16:31
 Operator : SM\AJ
 Sample : PB125023BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125023BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 01:30:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.429	0.000	648.5E6	0	470.920	N.D. #
Target Compounds							
1) T	Dalapon	1.990	1.697	113.1E6	106.0E6	62.530	89.308 #
2) T	3,5-DICHL...	0.000	4.489	0	24598927	N.D.	27.228
5) T	DICAMBA	5.519	0.000	46382006	0	9.117	N.D. #
7) T	MCPA	5.895	5.521	32530008	32734672	5.910	10.891 #
9) T	2,4-D	6.480	6.055	91554154	6620916	65.277	8.210 #
10) T	Pentachlo...	0.000	6.365	0	21492066	N.D.	2.195
11) T	2,4,5-TP ...	0.000	6.759	0	26303157	N.D.	6.717
15) T	Picloram	0.000	8.913	0	88152471	N.D.	15.046



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
Data File : PS007783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 16:31
Operator : SM\AJ
Sample : PB125023BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125023BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 01:30:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

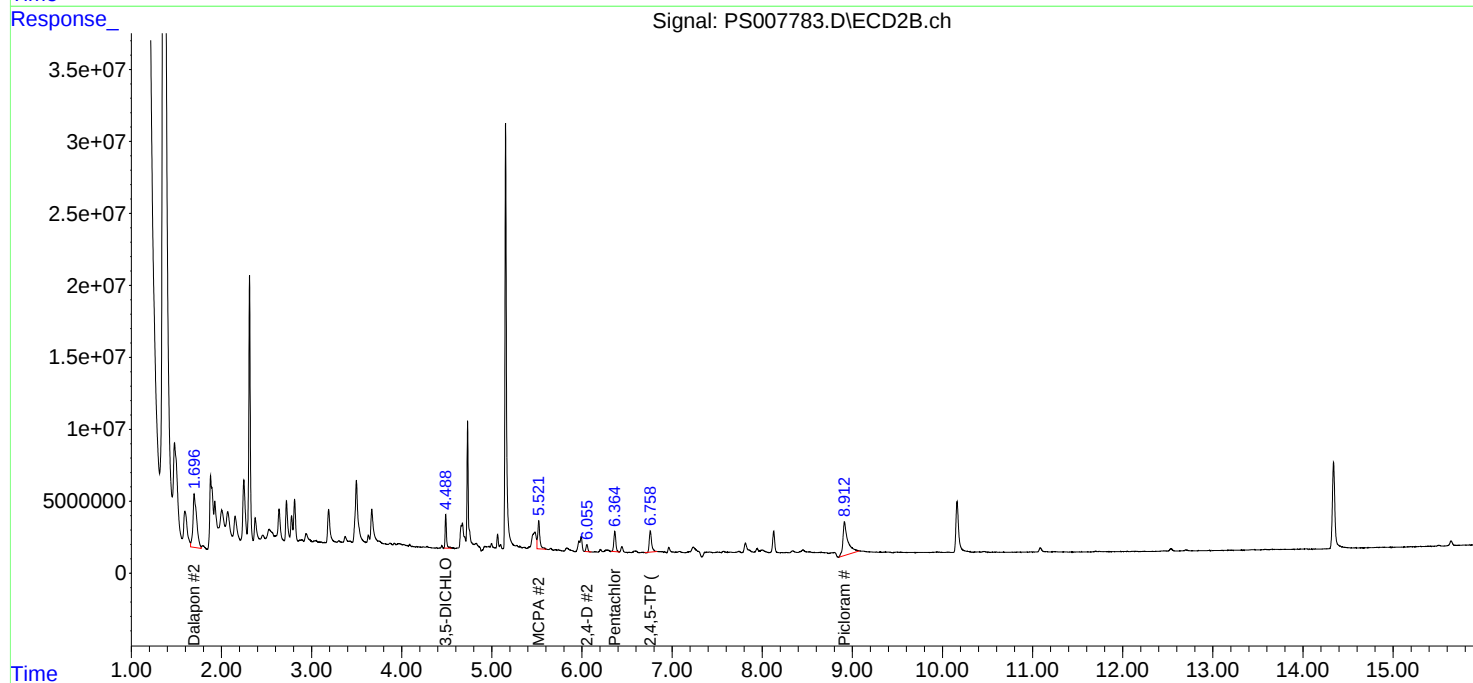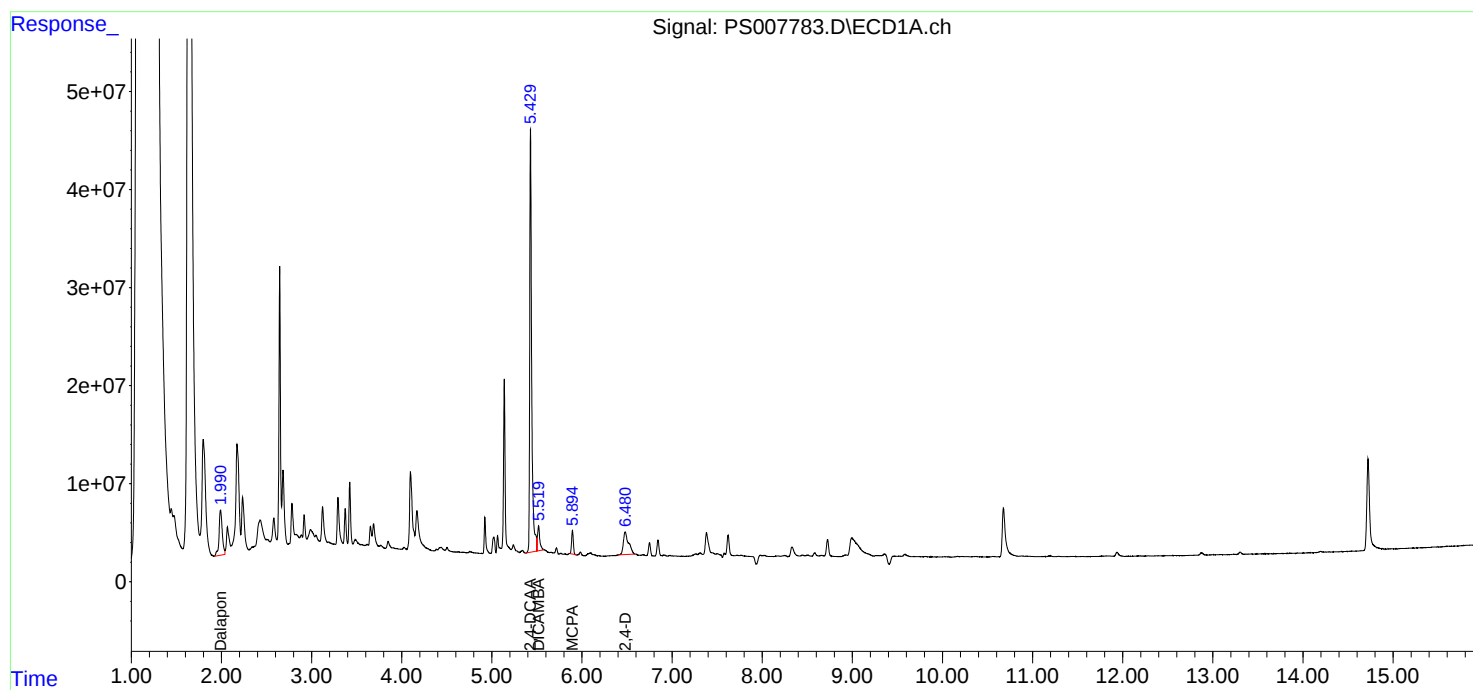


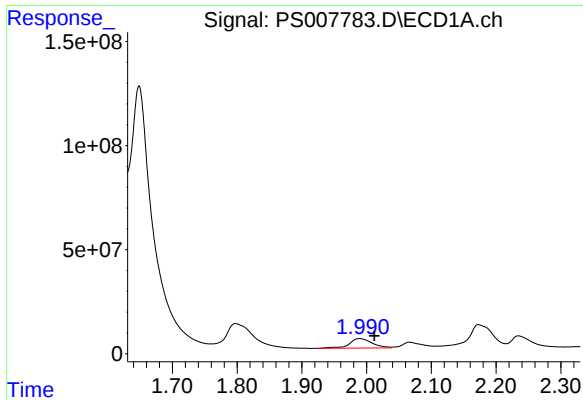

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.022 min
Response: 113128061
Conc: 62.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125023BL

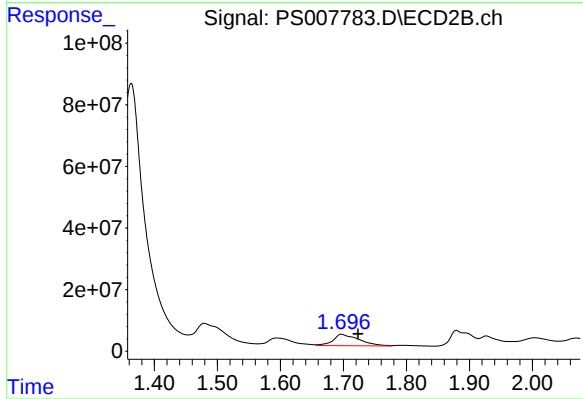


#1 Dalapon

R.T.: 1.697 min
Delta R.T.: -0.026 min
Response: 106044316
Conc: 89.31 ng/ml

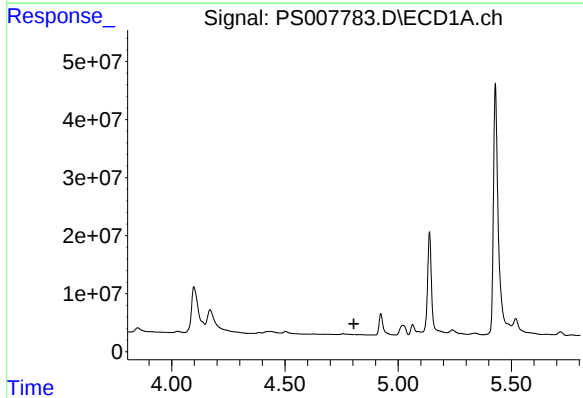


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

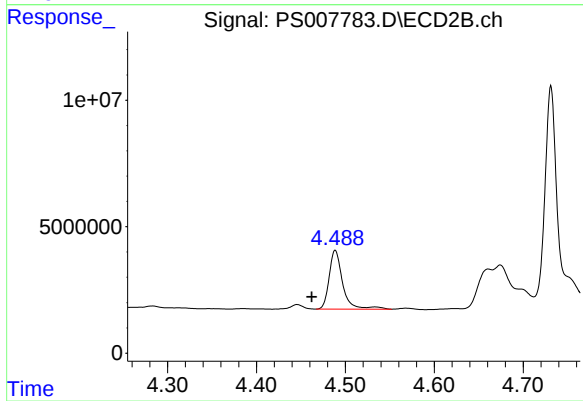

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.027 min
Response: 24598927
Conc: 27.23 ng/ml

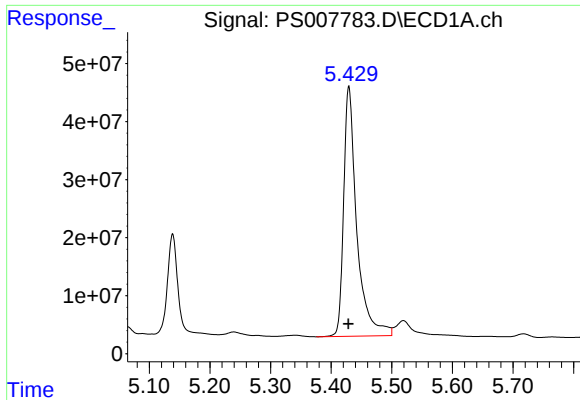

#4 2,4-DCAA


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 648543922
Conc: 470.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125023BL

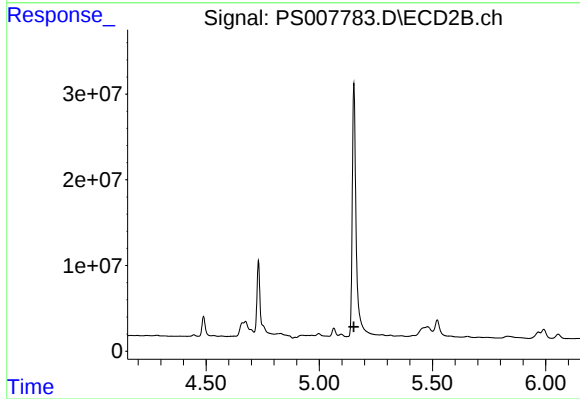


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.153 min
Response: 0
Conc: N.D.

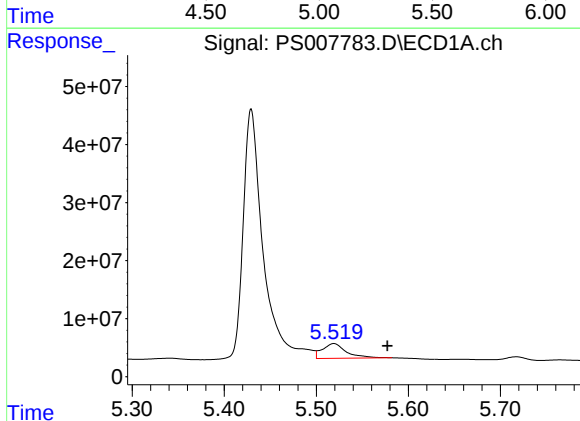


#5 DICAMBA

R.T.: 5.519 min
Delta R.T.: -0.058 min
Response: 46382006
Conc: 9.12 ng/ml

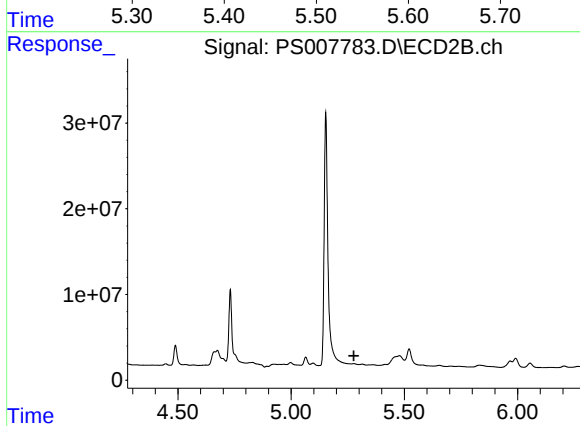

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

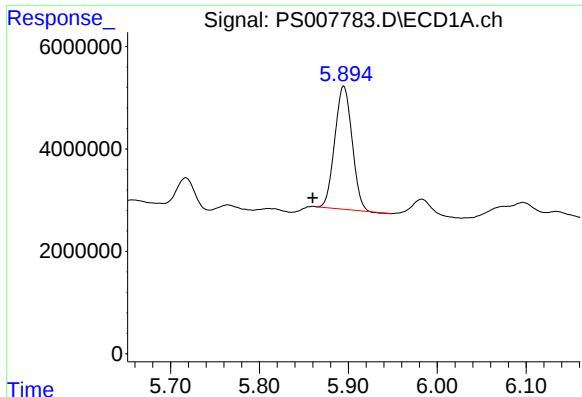

#7 MCPA


R.T.: 5.895 min
Delta R.T.: 0.035 min
Response: 32530008
Conc: 5.91 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125023BL

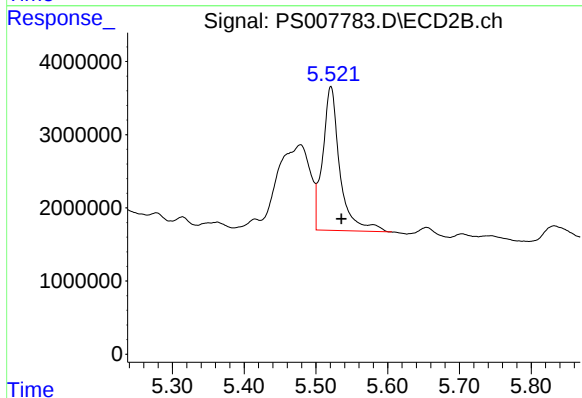


#7 MCPA

R.T.: 5.521 min
Delta R.T.: -0.015 min
Response: 32734672
Conc: 10.89 ug/ml

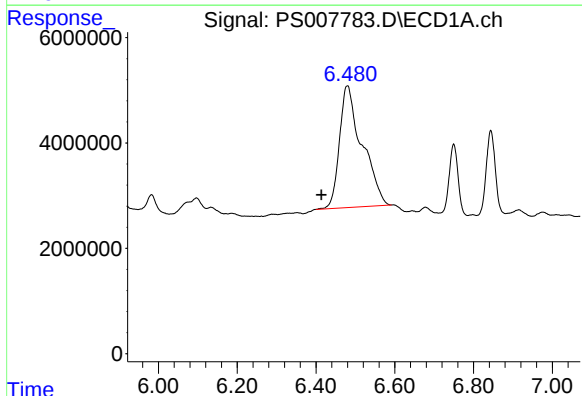


#9 2,4-D

R.T.: 6.480 min
Delta R.T.: 0.065 min
Response: 91554154
Conc: 65.28 ng/ml

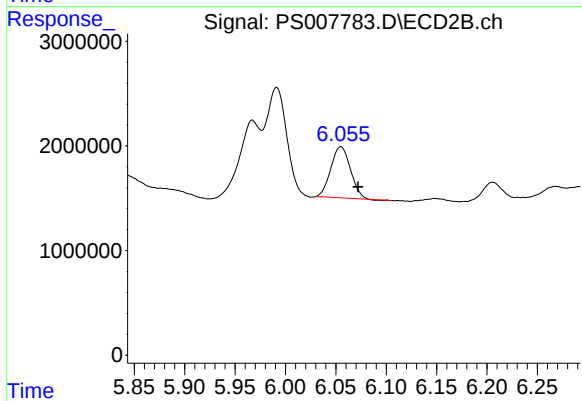

#9 2,4-D


R.T.: 6.055 min
Delta R.T.: -0.017 min
Response: 6620916
Conc: 8.21 ng/ml

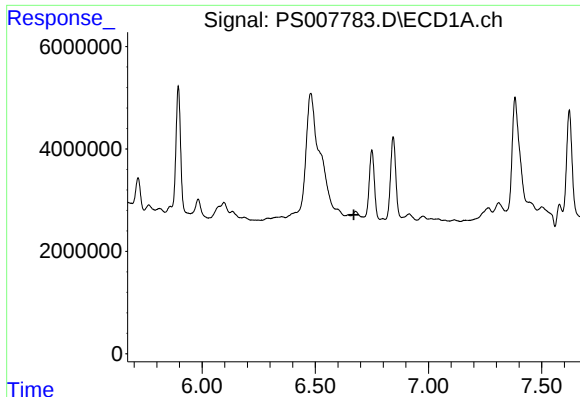

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125023BL

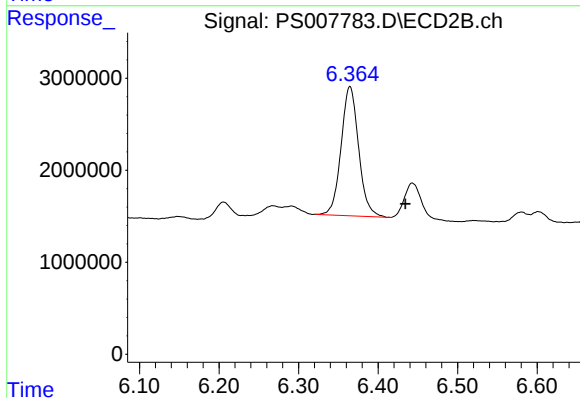


#10 Pentachlorophenol

R.T.: 6.365 min
Delta R.T.: -0.070 min
Response: 21492066
Conc: 2.19 ng/ml

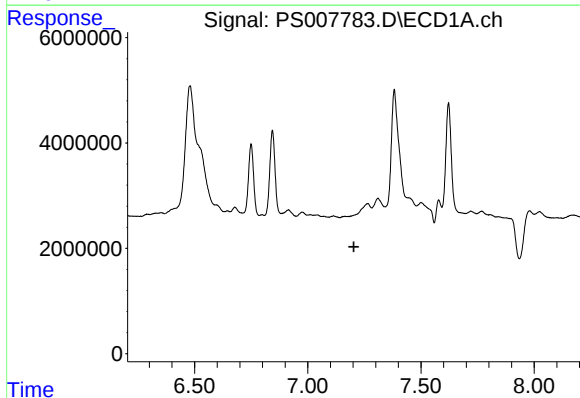


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

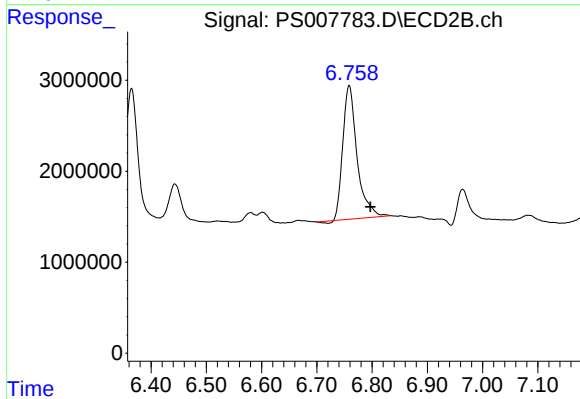

#11 2,4,5-TP (SILVEX)


R.T.: 6.759 min
Delta R.T.: -0.038 min
Response: 26303157
Conc: 6.72 ng/ml

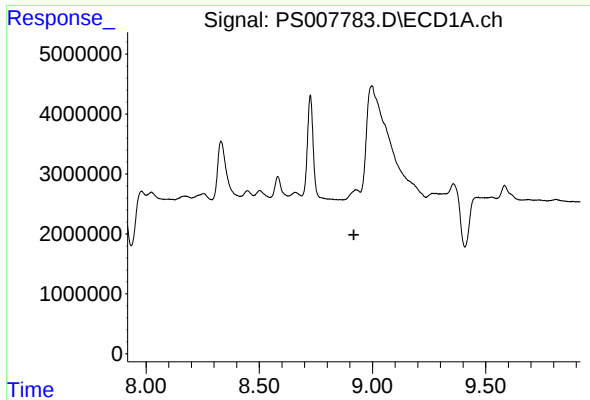

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125023BL

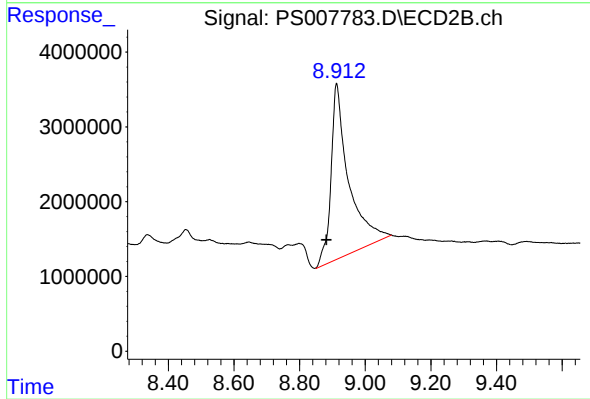

#15 Picloram

R.T.: 8.913 min
Delta R.T.: 0.031 min
Response: 88152471
Conc: 15.05 ng/ml