

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
 Data File : PS007808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2019 01:39
 Operator : SM\AJ
 Sample : K5676-30
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-03-112019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 03:36:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.429	5.153	682.0E6	341.7E6	495.206	486.377
Target Compounds							
1) T	Dalapon	1.991	1.700	94638308	113.2E6	52.310	95.331 #
2) T	3,5-DICHL...	0.000	4.447	0	5609111	N.D.	6.209
3) T	4-Nitroph...	0.000	4.831	0	13892139	N.D.	33.760
5) T	DICAMBA	5.520	0.000	47259847	0	9.290	N.D. #
7) T	MCPA	0.000	5.475	0	43469123	N.D.	14.462
8) T	DICHLORPROP	0.000	5.822	0	8072700	N.D.	12.310
9) T	2,4-D	6.481	0.000	76669034	0	54.664	N.D. #
10) T	Pentachlo...	0.000	6.442	0	10435824	N.D.	1.066
11) T	2,4,5-TP ...	0.000	6.752	0	69612838	N.D.	17.777



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
Data File : PS007808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2019 01:39
Operator : SM\AJ
Sample : K5676-30
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-03-112019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 03:36:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

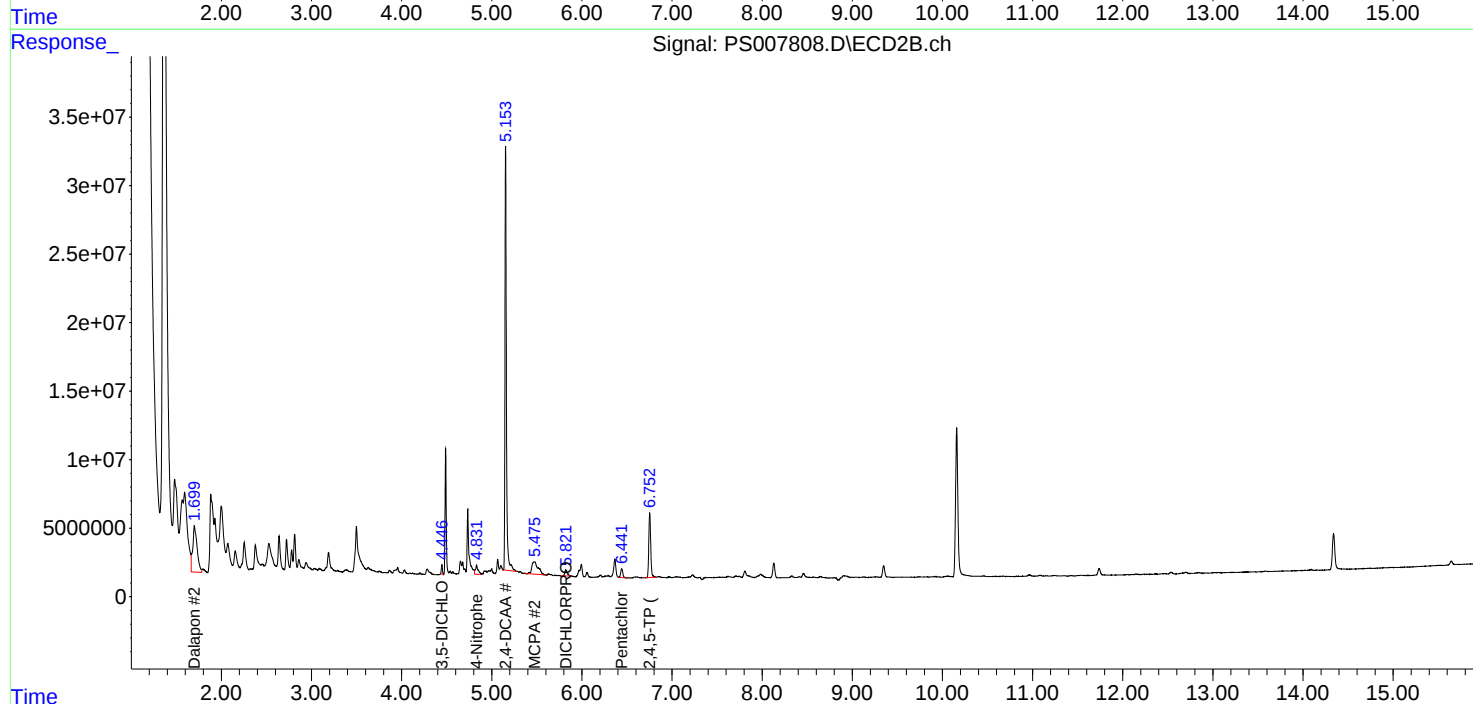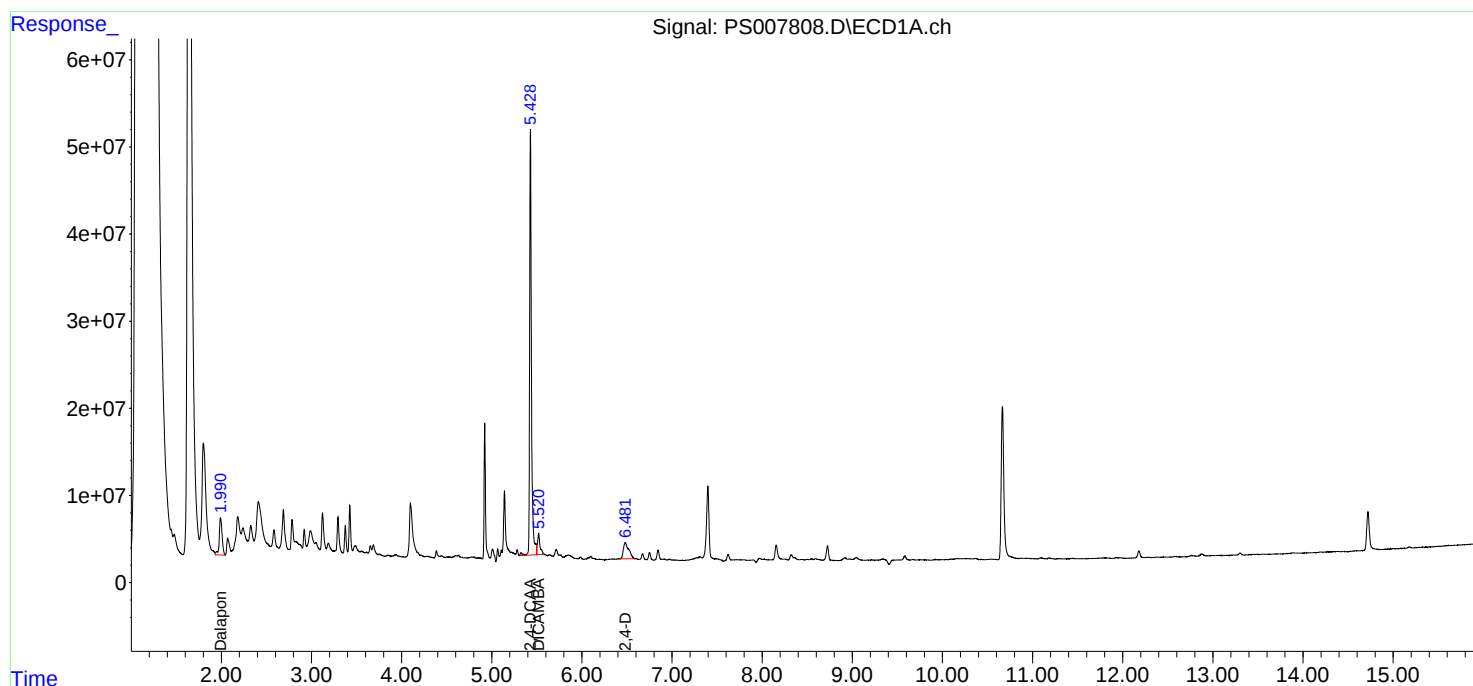


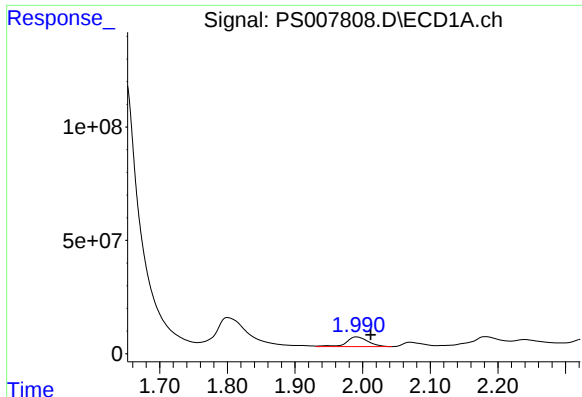

#1 Dalapon


R.T.: 1.991 min
Delta R.T.: -0.021 min
Response: 94638308
Conc: 52.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-03-112019

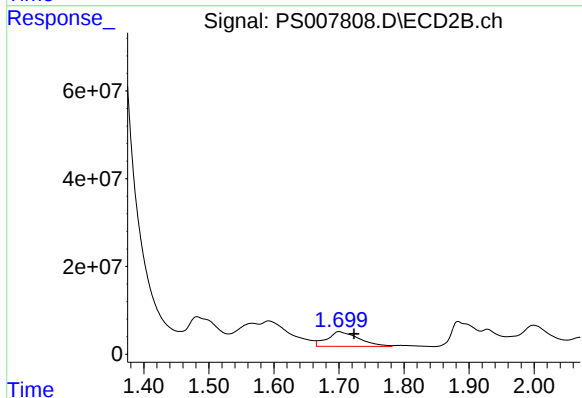


#1 Dalapon

R.T.: 1.700 min
Delta R.T.: -0.023 min
Response: 113196781
Conc: 95.33 ng/ml

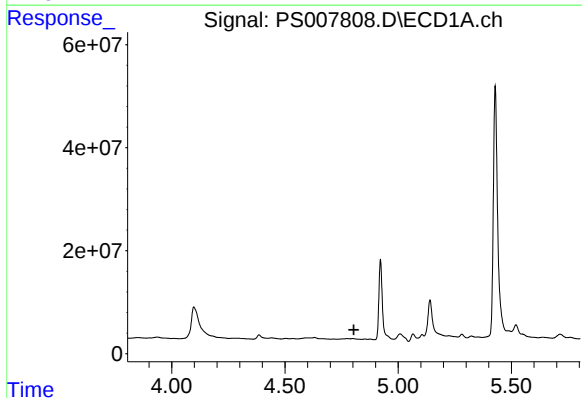


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

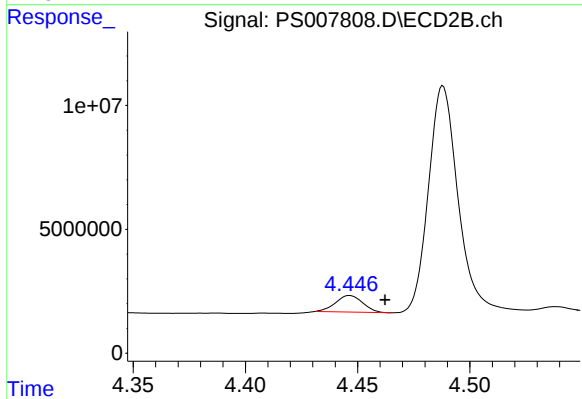

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min
Delta R.T.: -0.016 min
Response: 5609111
Conc: 6.21 ng/ml

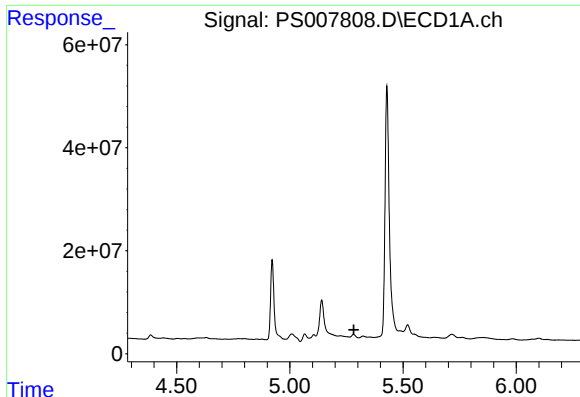

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-112019

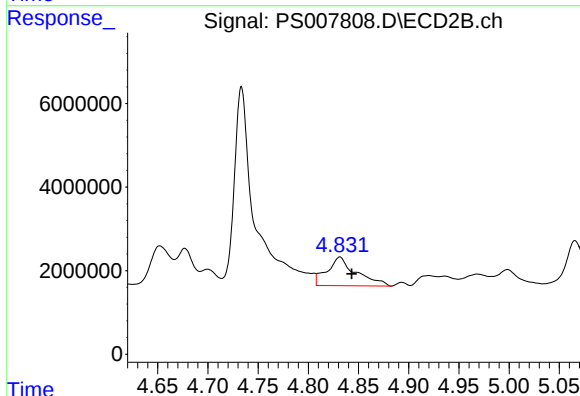


#3 4-Nitrophenol

R.T.: 4.831 min
Delta R.T.: -0.012 min
Response: 13892139
Conc: 33.76 ng/ml

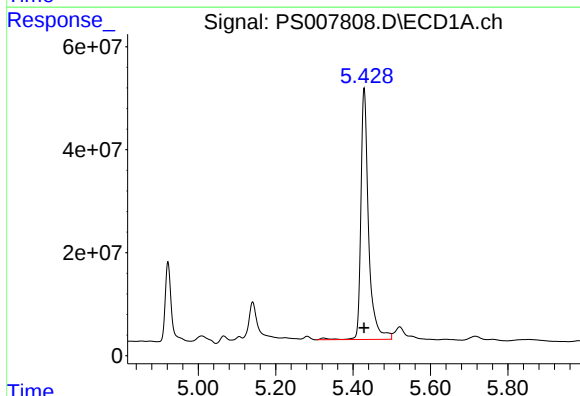


#4 2,4-DCAA

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 681990393
Conc: 495.21 ng/ml

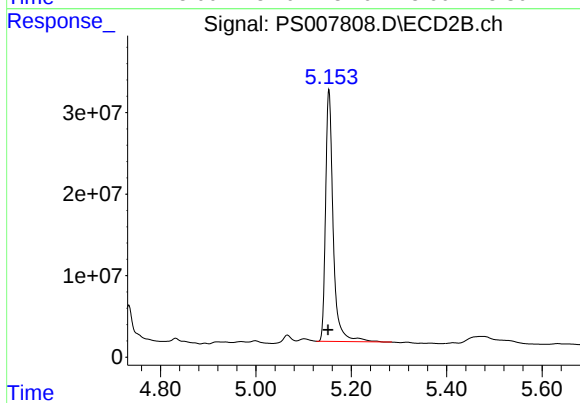

#4 2,4-DCAA


R.T.: 5.153 min
Delta R.T.: 0.002 min
Response: 341710897
Conc: 486.38 ng/ml

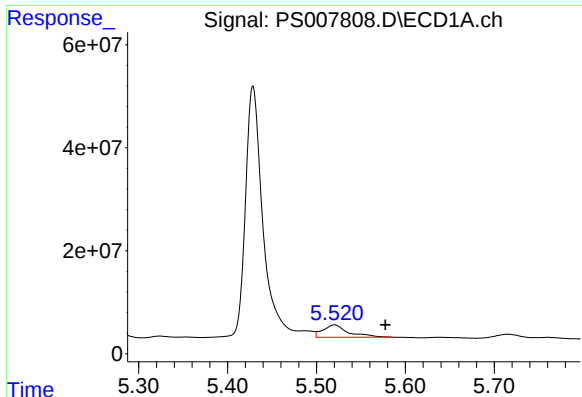

#5 DICAMBA


R.T.: 5.520 min
Delta R.T.: -0.057 min
Response: 47259847
Conc: 9.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-03-112019

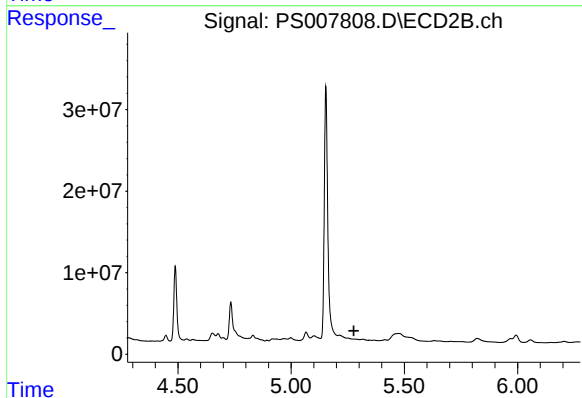


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

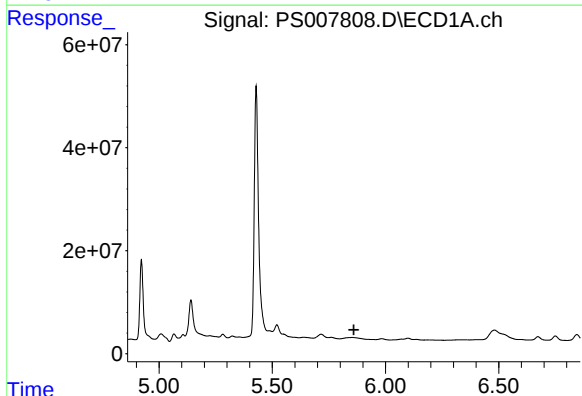


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

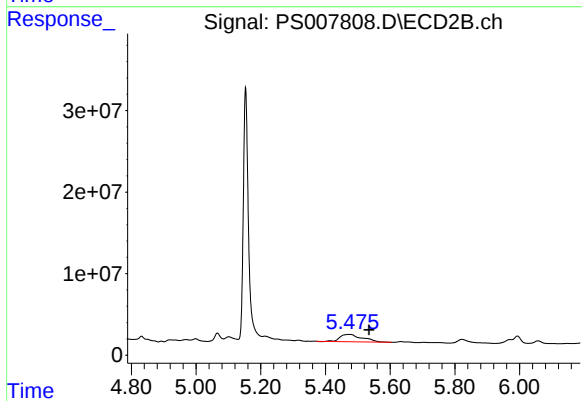

#7 MCPA


R.T.: 5.475 min
Delta R.T.: -0.060 min
Response: 43469123
Conc: 14.46 ug/ml

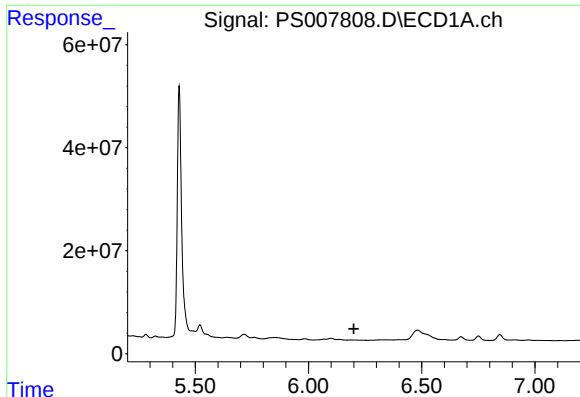

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-112019

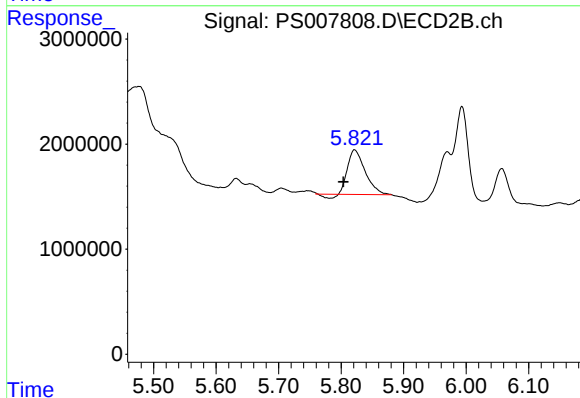


#8 DICHLORPROP

R.T.: 5.822 min
Delta R.T.: 0.018 min
Response: 8072700
Conc: 12.31 ng/ml

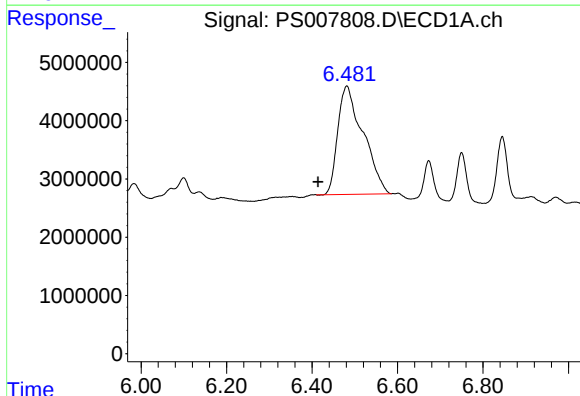


#9 2,4-D

R.T.: 6.481 min
Delta R.T.: 0.067 min
Response: 76669034
Conc: 54.66 ng/ml

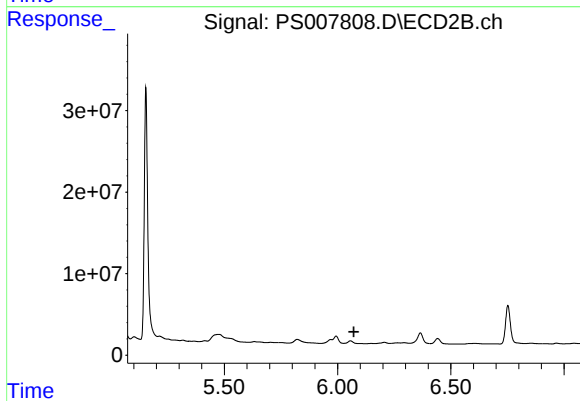

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

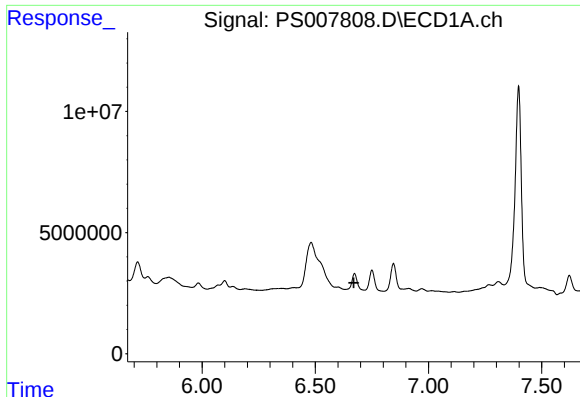

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-03-112019

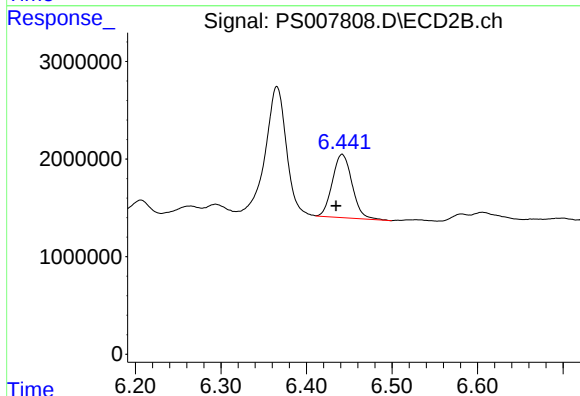


#10 Pentachlorophenol

R.T.: 6.442 min
Delta R.T.: 0.007 min
Response: 10435824
Conc: 1.07 ng/ml

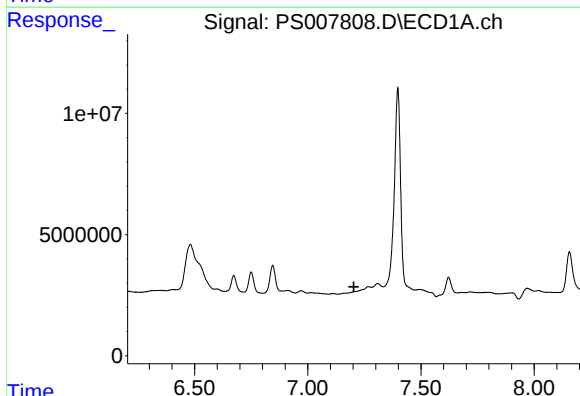

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

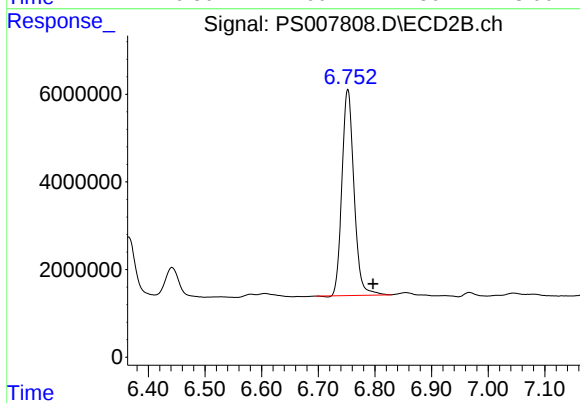

#11 2,4,5-TP (SILVEX)

R.T.: 6.752 min
Delta R.T.: -0.045 min
Response: 69612838
Conc: 17.78 ng/ml