

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
 Data File : PS007812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2019 03:07
 Operator : SM\AJ
 Sample : K5973-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DUCT-BANK-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 03:37:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.427	5.152	207.1E6	93997859	150.373	133.793
Target Compounds							
1) T	Dalapon	1.989	1.696	88080935	363.7E6	48.686	306.291 #
2) T	3,5-DICHL...	4.866	4.487	22560568	51699407	12.645	57.226 #
3) T	4-Nitroph...	0.000	4.829	0	8871140	N.D.	21.558
5) T	DICAMBA	5.519	5.265	43797058	13195269	8.609	4.986 #
7) T	MCPA	5.895	5.521	28111980	43757808	5.107	14.558 #
8) T	DICHLORPROP	0.000	5.810	0	18326687	N.D.	27.946
9) T	2,4-D	6.476	6.057	32212829	5919283	22.967	7.340 #
10) T	Pentachlo...	0.000	6.438	0	15280180	N.D.	1.560
11) T	2,4,5-TP ...	0.000	6.750	0	22809953	N.D.	5.825
14) T	DINOSEB	0.000	7.941	0	18592635	N.D.	6.396
15) T	Picloram	0.000	8.899	0	29540506	N.D.	5.042
16) T	DCPA	0.000	8.899	0	29540506	N.D.	5.653



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
Data File : PS007812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2019 03:07
Operator : SM\AJ
Sample : K5973-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 03:37:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

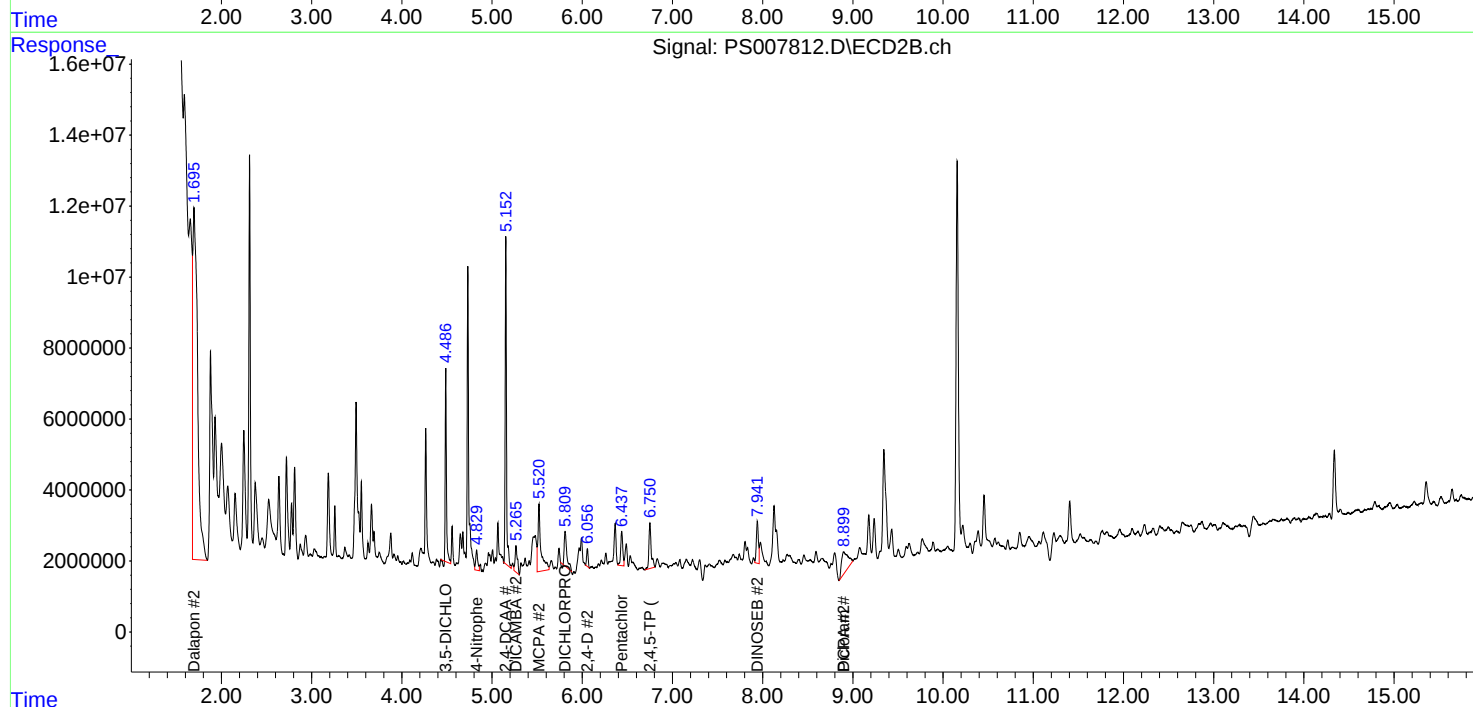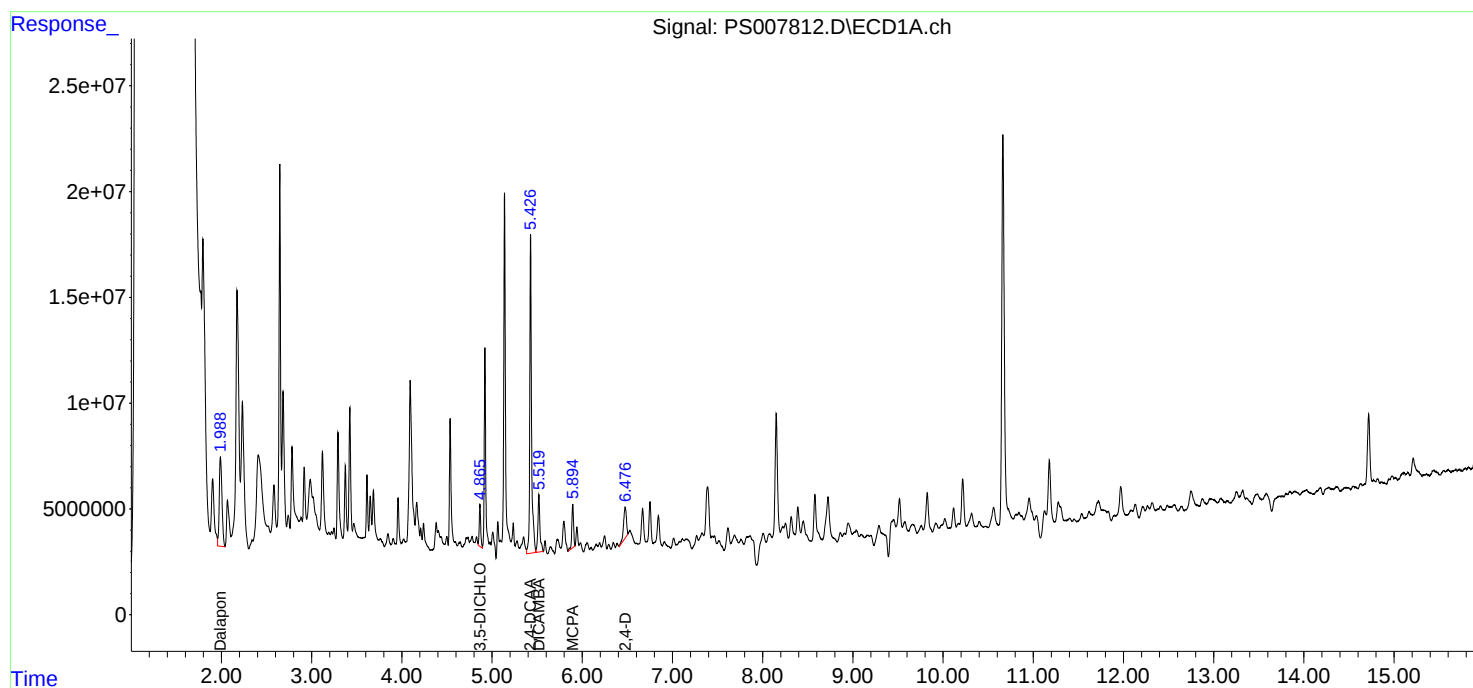


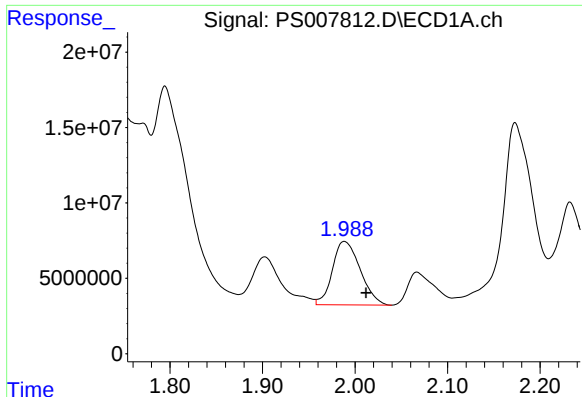

#1 Dalapon


R.T.: 1.989 min
Delta R.T.: -0.023 min
Response: 88080935
Conc: 48.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

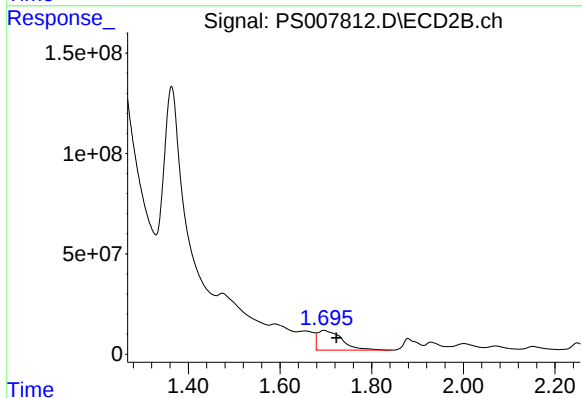


#1 Dalapon

R.T.: 1.696 min
Delta R.T.: -0.027 min
Response: 363690310
Conc: 306.29 ng/ml

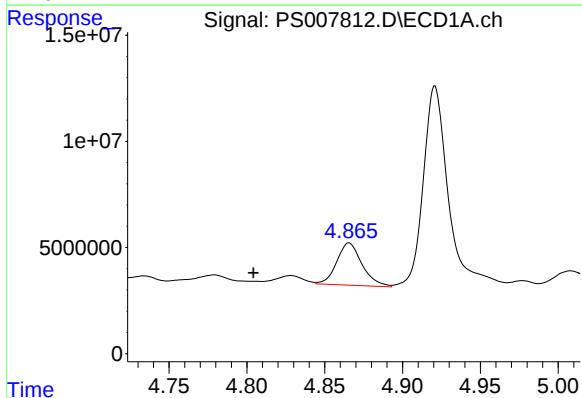


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.866 min
Delta R.T.: 0.061 min
Response: 22560568
Conc: 12.65 ng/ml

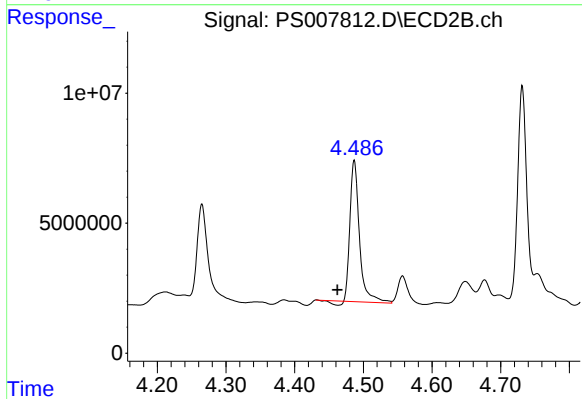

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.487 min
Delta R.T.: 0.025 min
Response: 51699407
Conc: 57.23 ng/ml

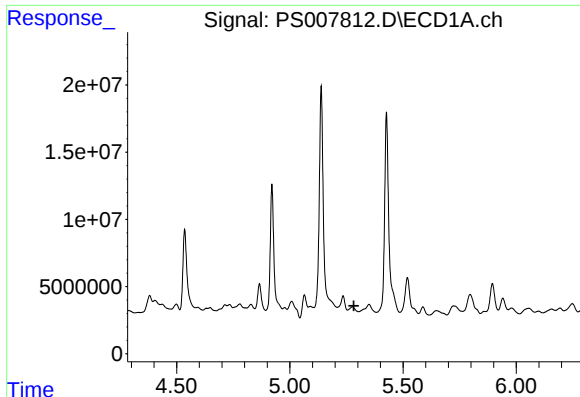

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

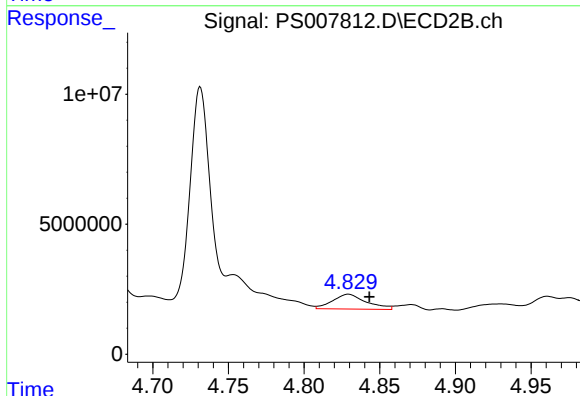


#3 4-Nitrophenol

R.T.: 4.829 min
Delta R.T.: -0.014 min
Response: 8871140
Conc: 21.56 ng/ml

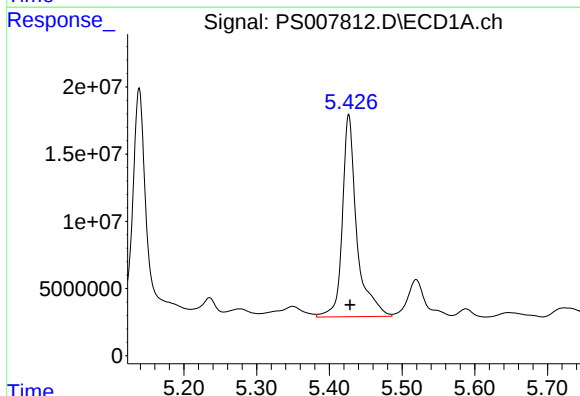


#4 2,4-DCAA

R.T.: 5.427 min
Delta R.T.: -0.002 min
Response: 207091203
Conc: 150.37 ng/ml

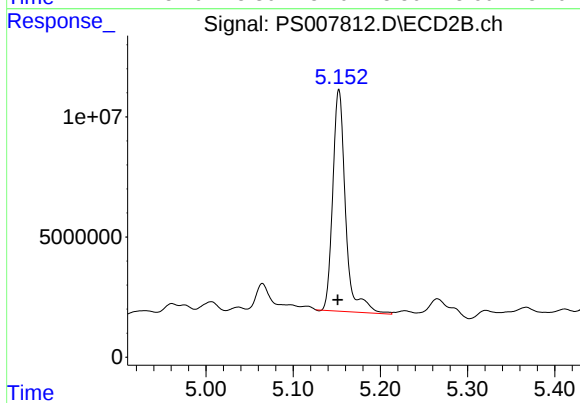

#4 2,4-DCAA


R.T.: 5.152 min
Delta R.T.: 0.001 min
Response: 93997859
Conc: 133.79 ng/ml

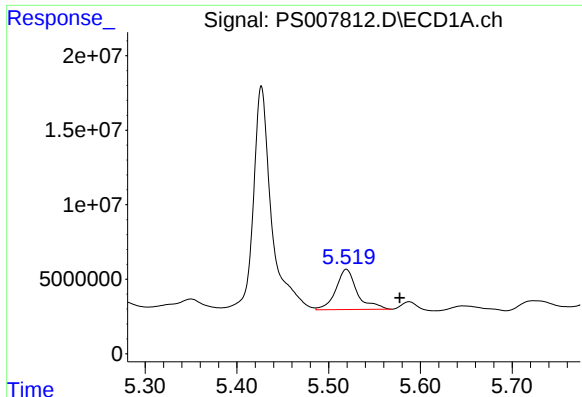

#5 DICAMBA


R.T.: 5.519 min
Delta R.T.: -0.058 min
Response: 43797058
Conc: 8.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

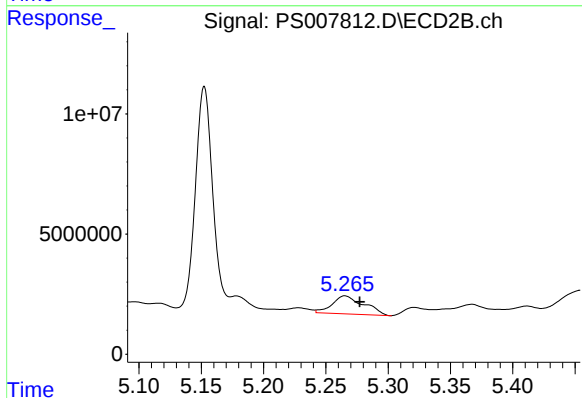


#5 DICAMBA

R.T.: 5.265 min
Delta R.T.: -0.012 min
Response: 13195269
Conc: 4.99 ng/ml

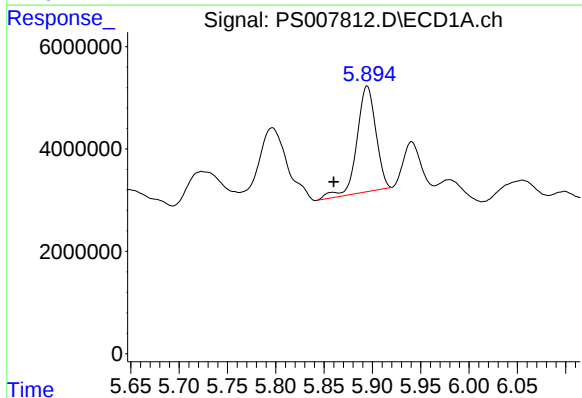


#7 MCPA

R.T.: 5.895 min
Delta R.T.: 0.035 min
Response: 28111980
Conc: 5.11 ug/ml

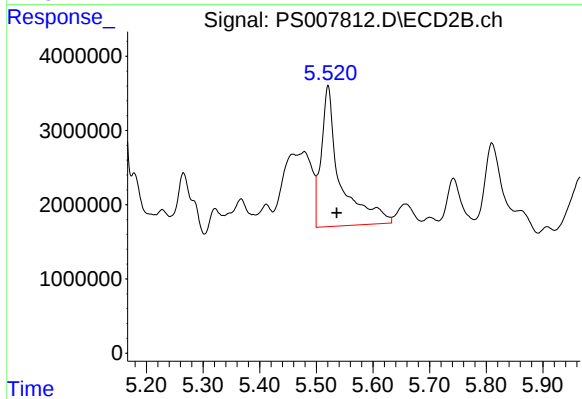

#7 MCPA


R.T.: 5.521 min
Delta R.T.: -0.015 min
Response: 43757808
Conc: 14.56 ug/ml

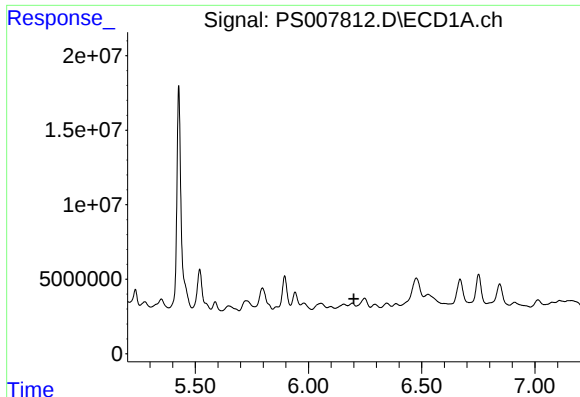

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

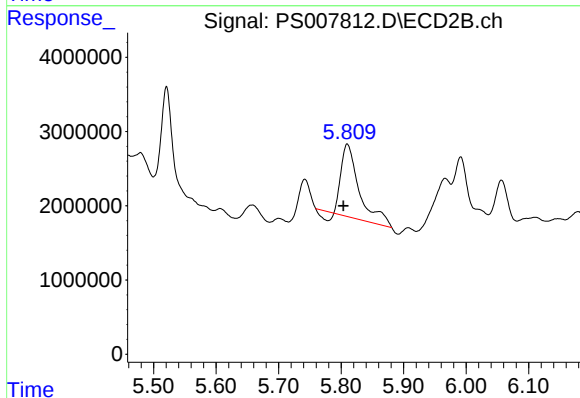


#8 DICHLORPROP

R.T.: 5.810 min
Delta R.T.: 0.006 min
Response: 18326687
Conc: 27.95 ng/ml

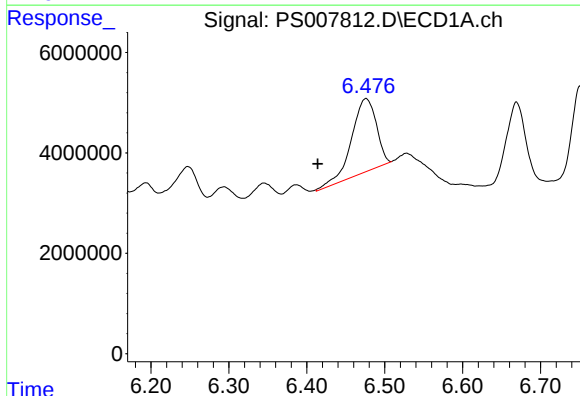


#9 2,4-D

R.T.: 6.476 min
Delta R.T.: 0.062 min
Response: 32212829
Conc: 22.97 ng/ml

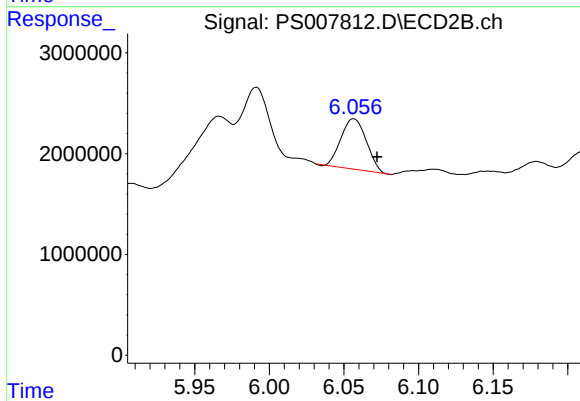

#9 2,4-D


R.T.: 6.057 min
Delta R.T.: -0.016 min
Response: 5919283
Conc: 7.34 ng/ml

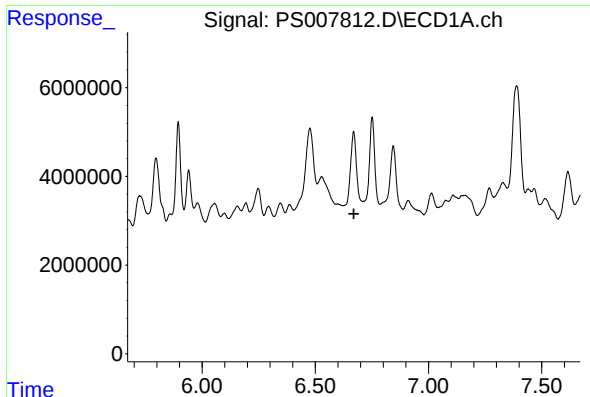

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

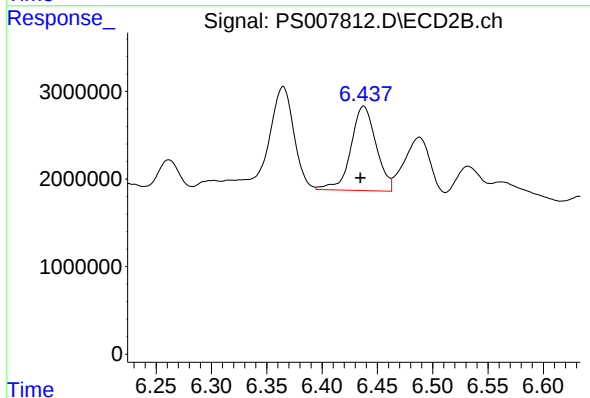


#10 Pentachlorophenol

R.T.: 6.438 min
Delta R.T.: 0.003 min
Response: 15280180
Conc: 1.56 ng/ml

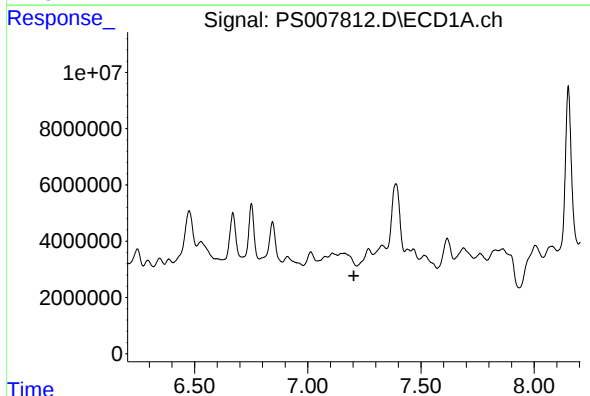


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

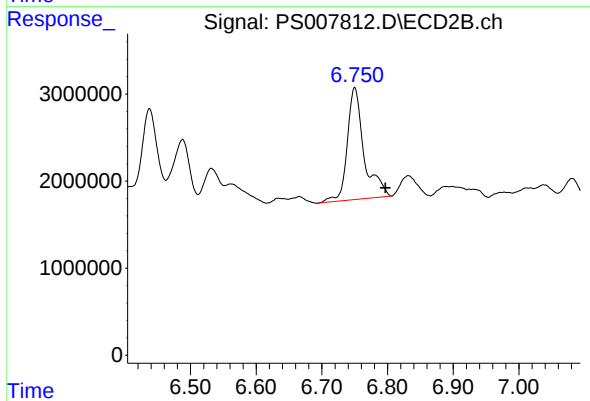

#11 2,4,5-TP (SILVEX)


R.T.: 6.750 min
Delta R.T.: -0.047 min
Response: 22809953
Conc: 5.83 ng/ml

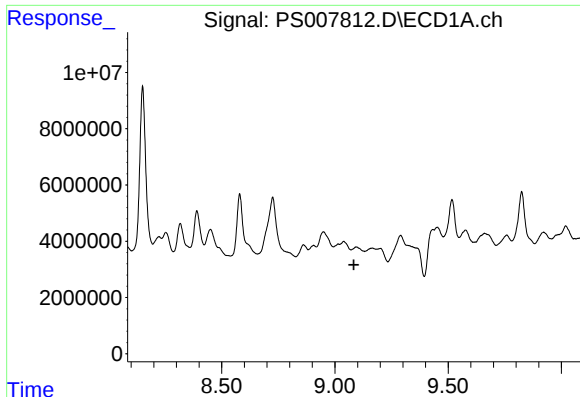

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

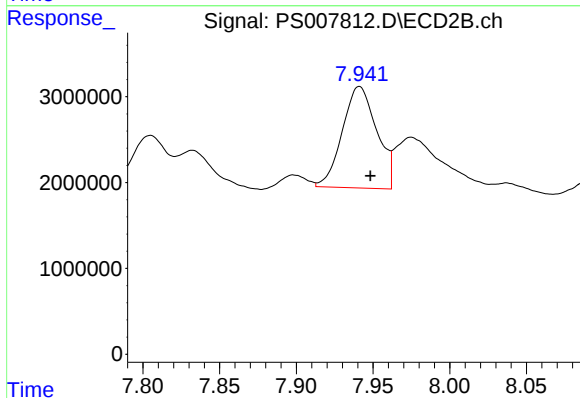


#14 DINOSEB

R.T.: 7.941 min
Delta R.T.: -0.007 min
Response: 18592635
Conc: 6.40 ng/ml

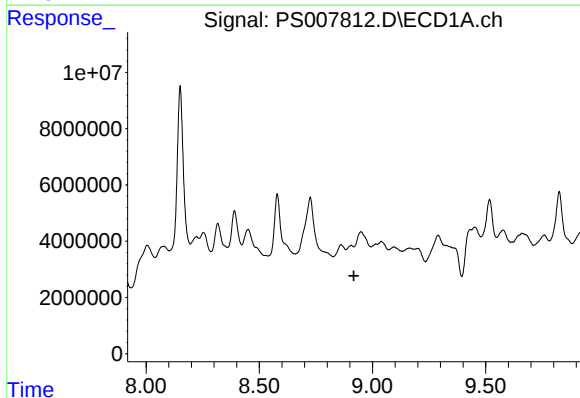


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

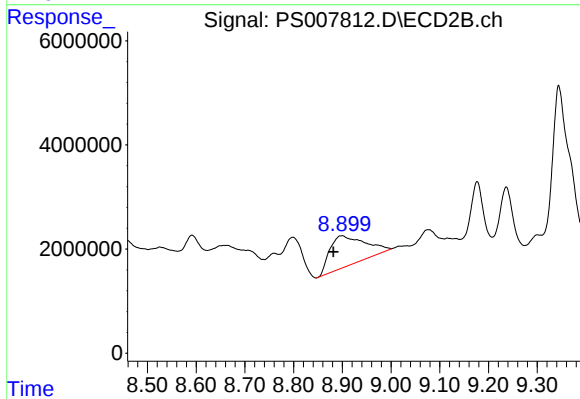

#15 Picloram


R.T.: 8.899 min
Delta R.T.: 0.017 min
Response: 29540506
Conc: 5.04 ng/ml

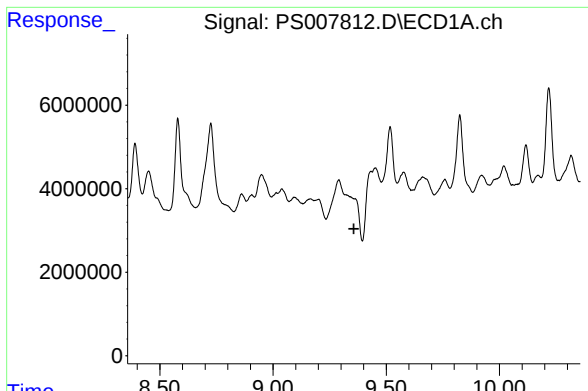

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-1

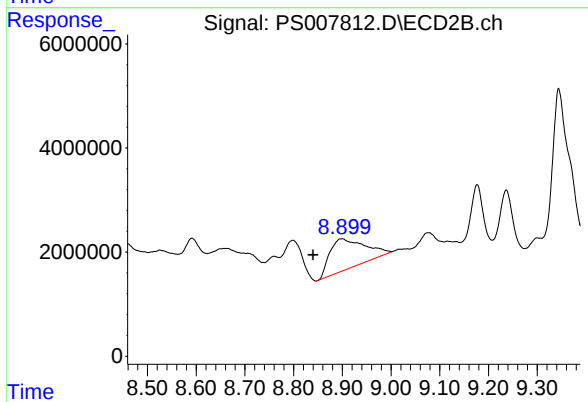

#16 DCPA

R.T.: 8.899 min
Delta R.T.: 0.059 min
Response: 29540506
Conc: 5.65 ng/ml