

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
 Data File : PS007814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2019 03:51
 Operator : SM\AJ
 Sample : K5973-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 04:48:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.432	5.158	164.0E6	62349623	119.073	88.746 #
Target Compounds							
1) T	Dalapon	1.994	1.662	100.3E6	849.5E6	55.447	715.400 #
2) T	3,5-DICHL...	4.871	4.492	24173708	56670473	13.550	62.728 #
5) T	DICAMBA	5.525	5.291	53621889	12251249	10.540	4.630 #
6) T	MCP	0.000	5.291	0	12251249	N.D.	6.306
7) T	MCPA	5.898	5.526	29625769	27989161	5.382	9.312 #
8) T	DICHLORPROP	0.000	5.818	0	4462967	N.D.	6.805
9) T	2,4-D	6.480	6.062	31675894	5147906	22.585	6.384 #
10) T	Pentachlo...	0.000	6.495	0	11922437	N.D.	1.218
11) T	2,4,5-TP ...	0.000	6.755	0	23046980	N.D.	5.886
13) T	2,4-DB	8.068	7.663	-10636595	22519646	N.D.	46.066
14) T	DINOSEB	0.000	7.946	0	9837649	N.D.	3.384
15) T	Picloram	0.000	8.936	0	34119300	N.D.	5.823
16) T	DCPA	0.000	8.798	0	26711458	N.D.	5.112



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112219\
Data File : PS007814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2019 03:51
Operator : SM\AJ
Sample : K5973-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 04:48:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

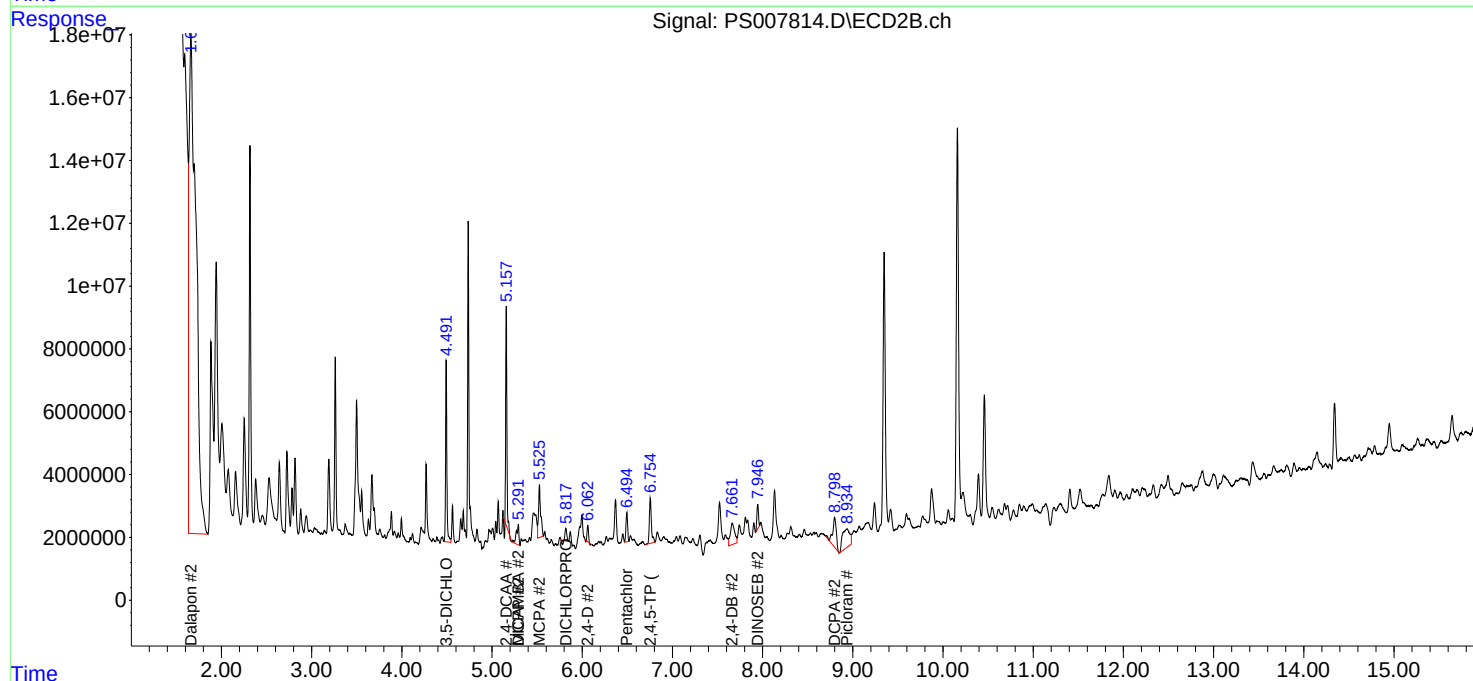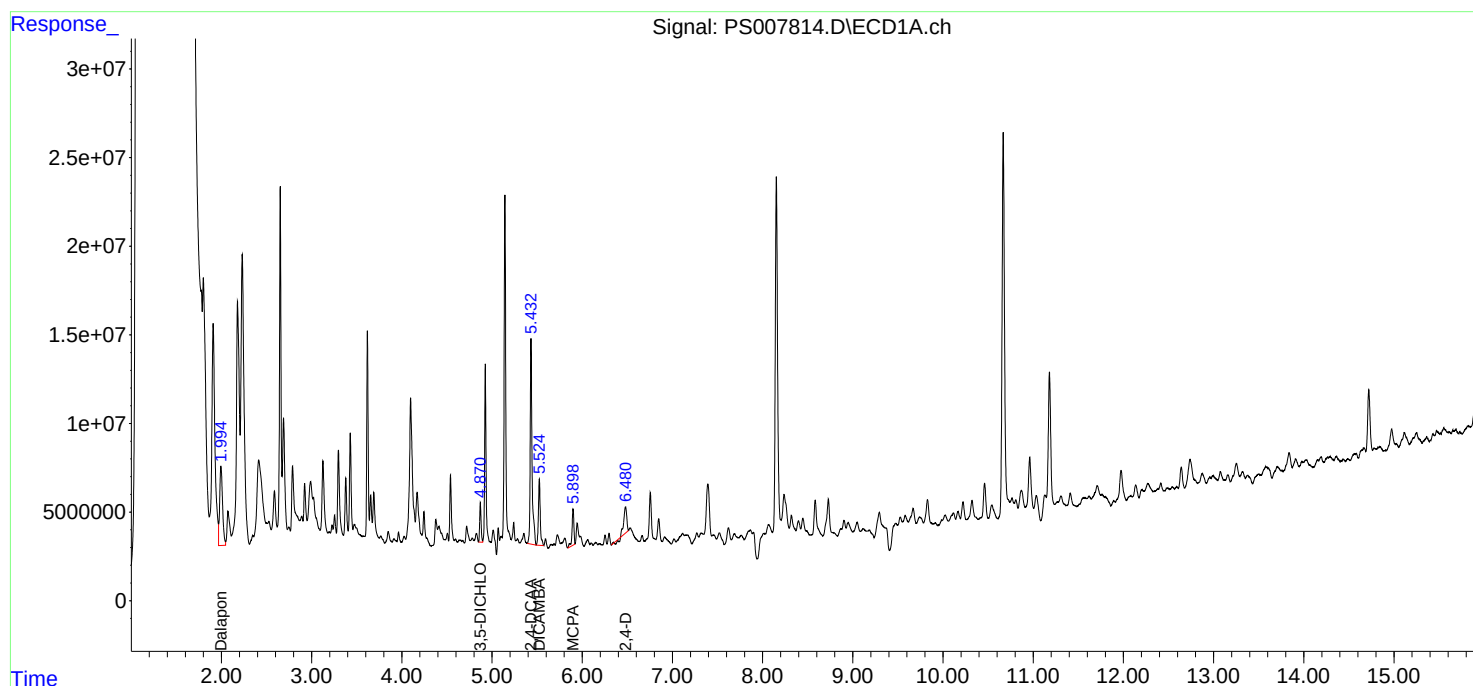


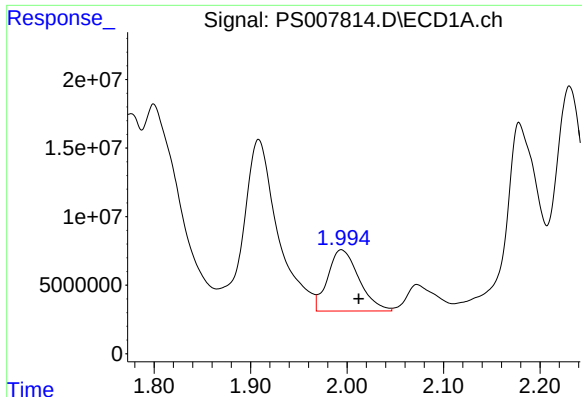

#1 Dalapon


R.T.: 1.994 min
Delta R.T.: -0.018 min
Response: 100314204
Conc: 55.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

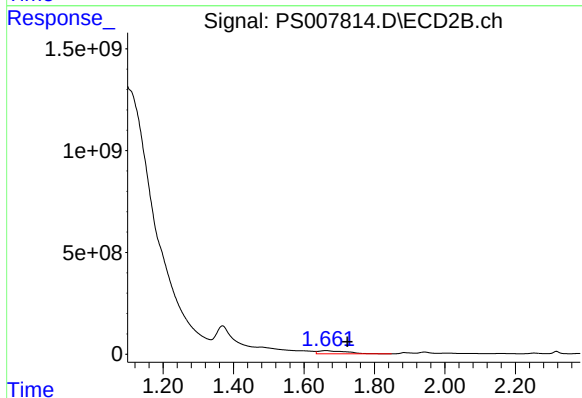


#1 Dalapon

R.T.: 1.662 min
Delta R.T.: -0.061 min
Response: 849467490
Conc: 715.40 ng/ml

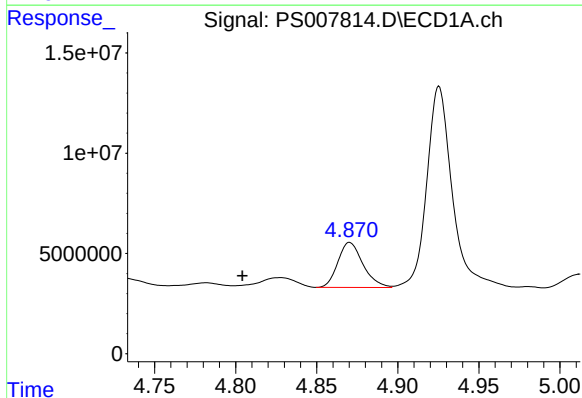


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.871 min
Delta R.T.: 0.066 min
Response: 24173708
Conc: 13.55 ng/ml

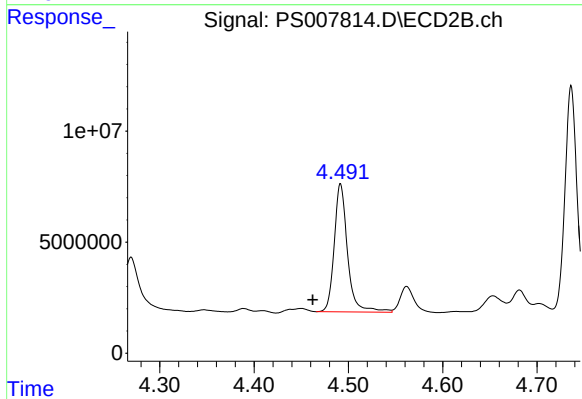

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.492 min
Delta R.T.: 0.030 min
Response: 56670473
Conc: 62.73 ng/ml

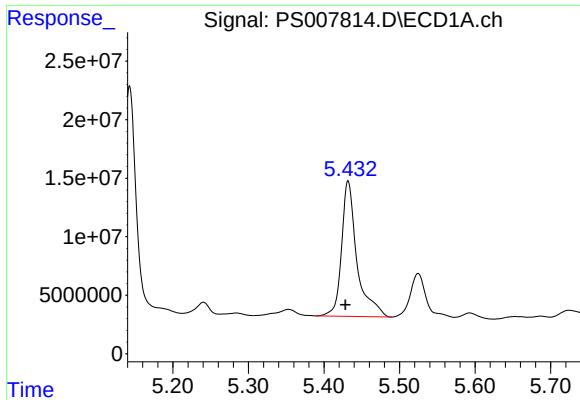

#4 2,4-DCAA


R.T.: 5.432 min
Delta R.T.: 0.004 min
Response: 163985974
Conc: 119.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-7

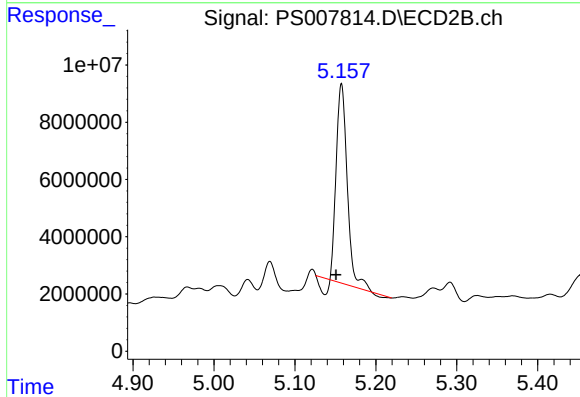


#4 2,4-DCAA

R.T.: 5.158 min
Delta R.T.: 0.007 min
Response: 62349623
Conc: 88.75 ng/ml

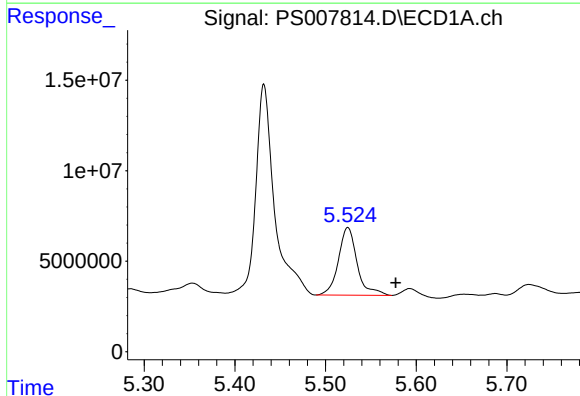


#5 DICAMBA

R.T.: 5.525 min
Delta R.T.: -0.053 min
Response: 53621889
Conc: 10.54 ng/ml

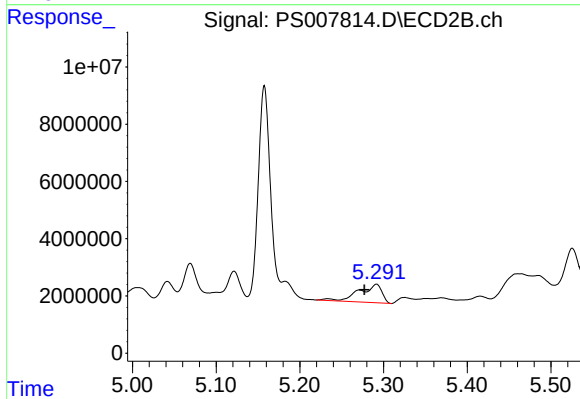

#5 DICAMBA


R.T.: 5.291 min
Delta R.T.: 0.014 min
Response: 12251249
Conc: 4.63 ng/ml

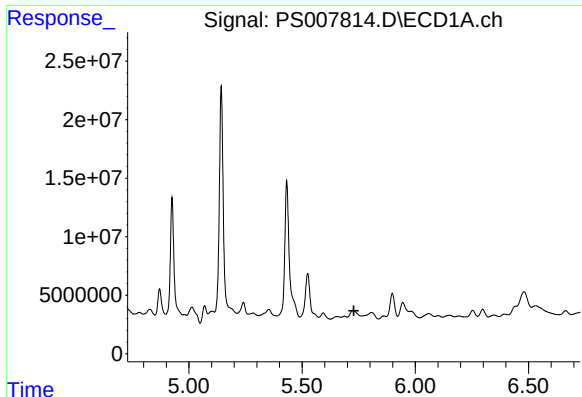

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

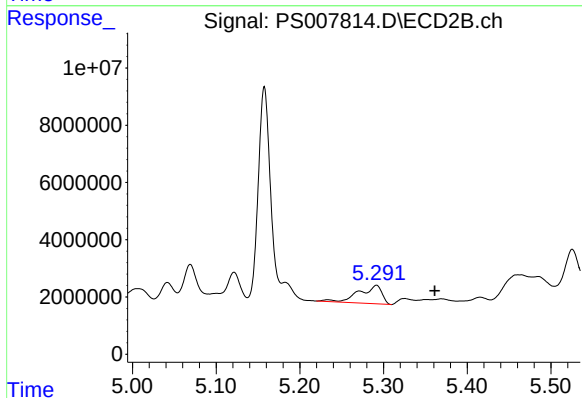


#6 MCPP

R.T.: 5.291 min
Delta R.T.: -0.070 min
Response: 12251249
Conc: 6.31 ug/ml

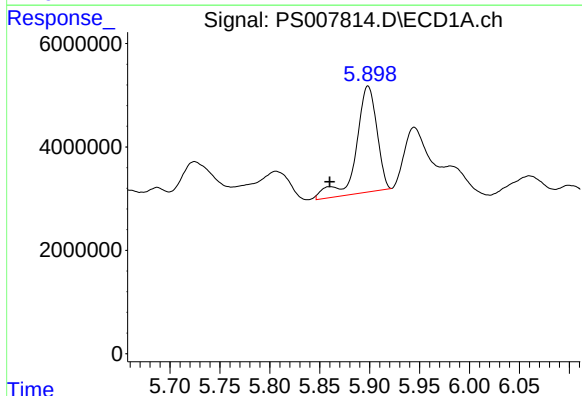


#7 MCPA

R.T.: 5.898 min
Delta R.T.: 0.038 min
Response: 29625769
Conc: 5.38 ug/ml

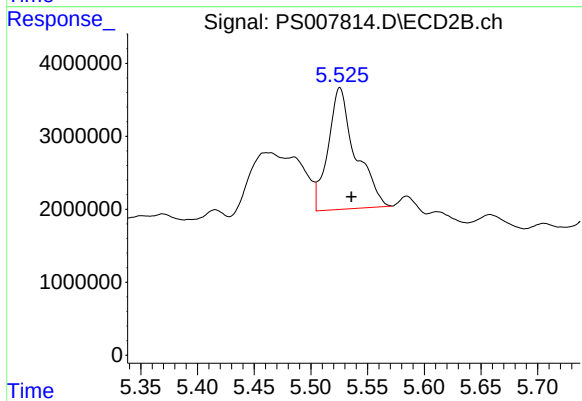

#7 MCPA


R.T.: 5.526 min
Delta R.T.: -0.010 min
Response: 27989161
Conc: 9.31 ug/ml

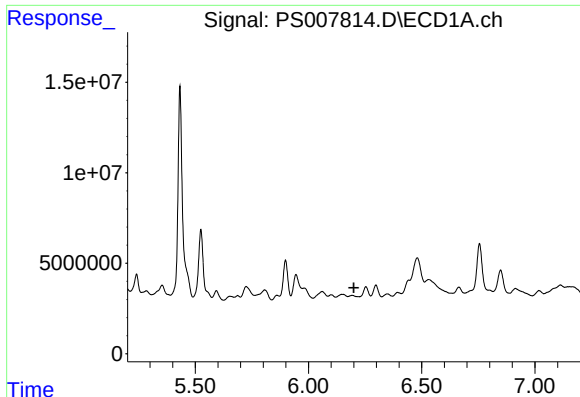

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

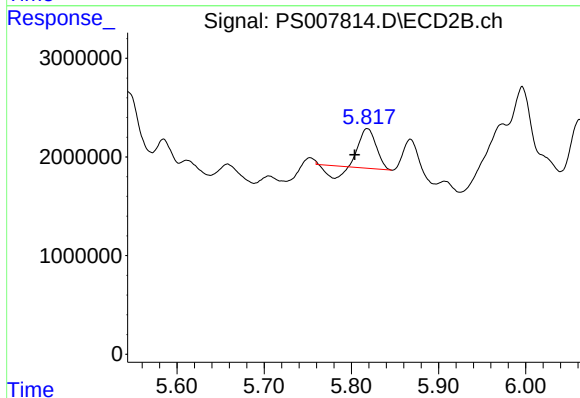


#8 DICHLORPROP

R.T.: 5.818 min
Delta R.T.: 0.015 min
Response: 4462967
Conc: 6.81 ng/ml

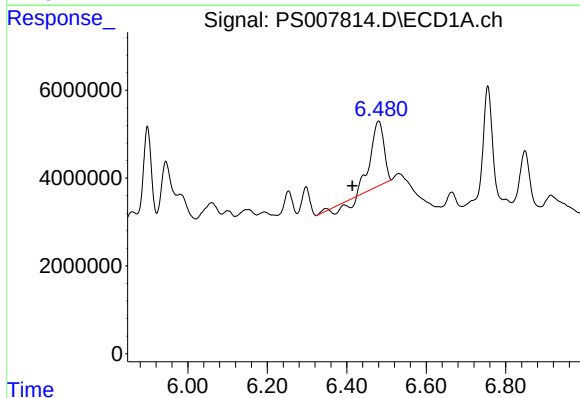


#9 2,4-D

R.T.: 6.480 min
Delta R.T.: 0.066 min
Response: 31675894
Conc: 22.58 ng/ml

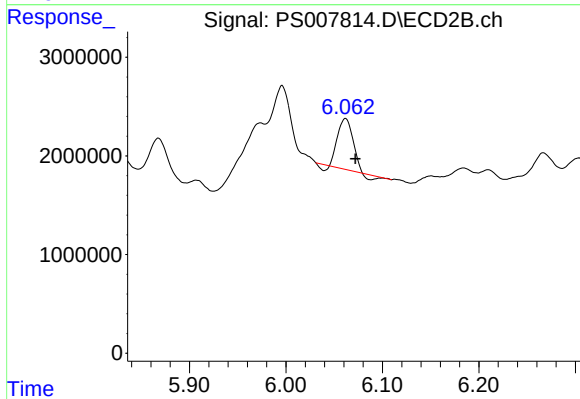

#9 2,4-D


R.T.: 6.062 min
Delta R.T.: -0.011 min
Response: 5147906
Conc: 6.38 ng/ml

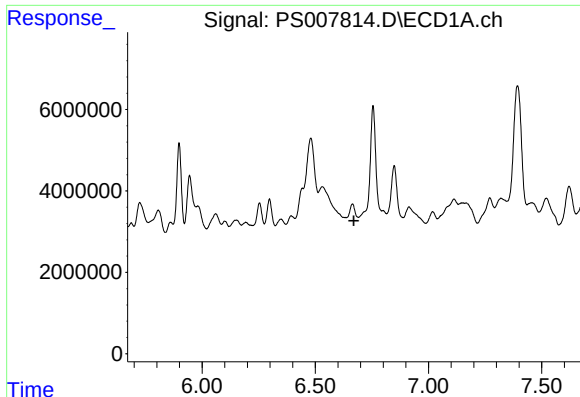

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

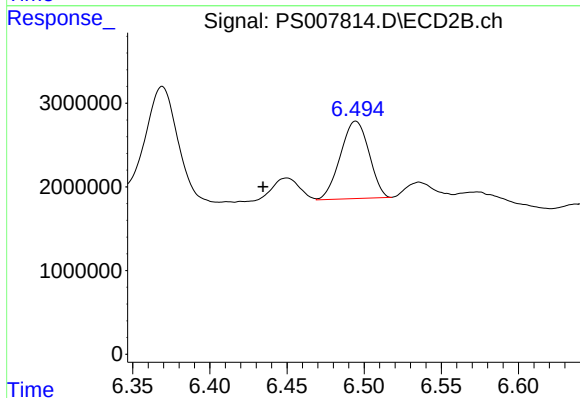


#10 Pentachlorophenol

R.T.: 6.495 min
Delta R.T.: 0.060 min
Response: 11922437
Conc: 1.22 ng/ml

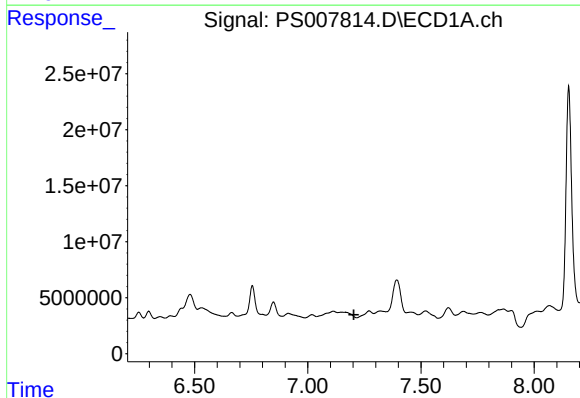


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

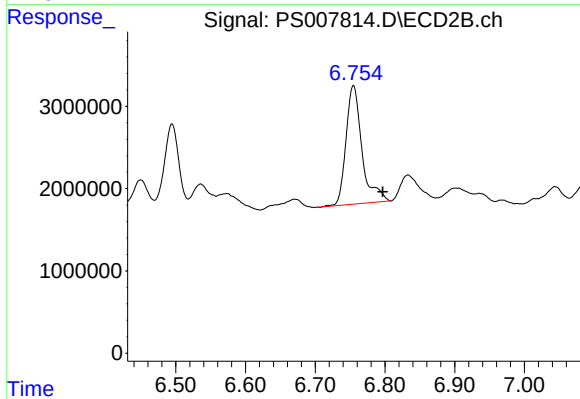

#11 2,4,5-TP (SILVEX)


R.T.: 6.755 min
Delta R.T.: -0.042 min
Response: 23046980
Conc: 5.89 ng/ml

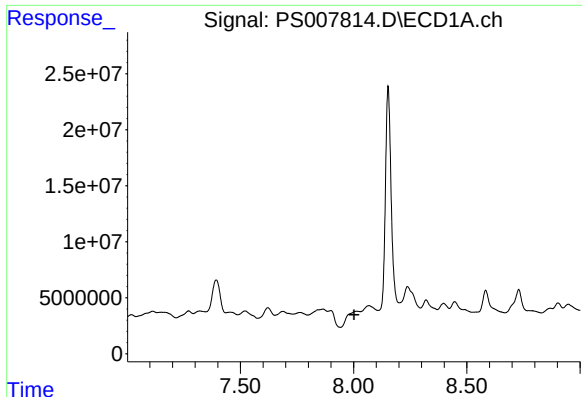

#13 2,4-DB


R.T.: 8.068 min
Delta R.T.: 0.066 min
Response: -10636595
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

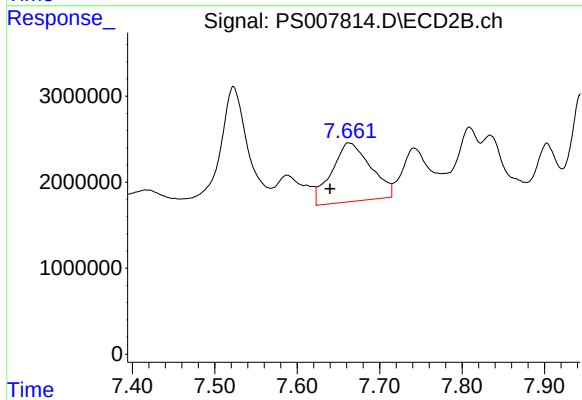


#13 2,4-DB

R.T.: 7.663 min
Delta R.T.: 0.023 min
Response: 22519646
Conc: 46.07 ng/ml

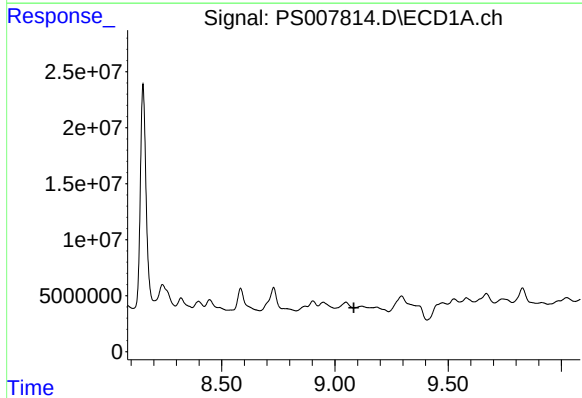


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.083 min
Response: 0
Conc: N.D.

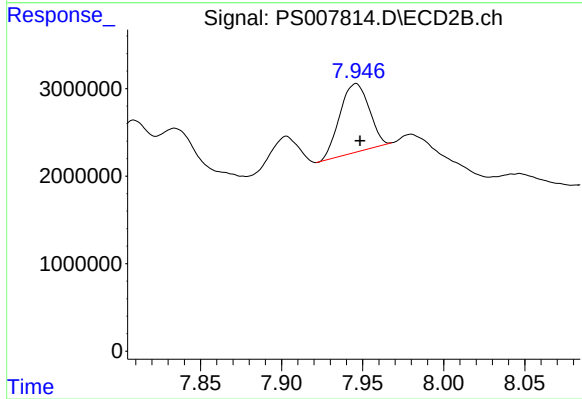

#14 DINOSEB


R.T.: 7.946 min
Delta R.T.: -0.003 min
Response: 9837649
Conc: 3.38 ng/ml

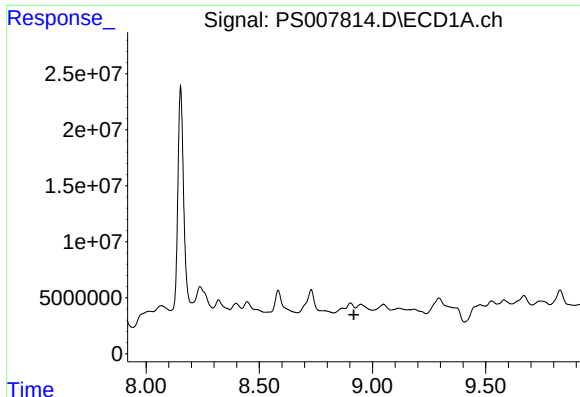

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-7

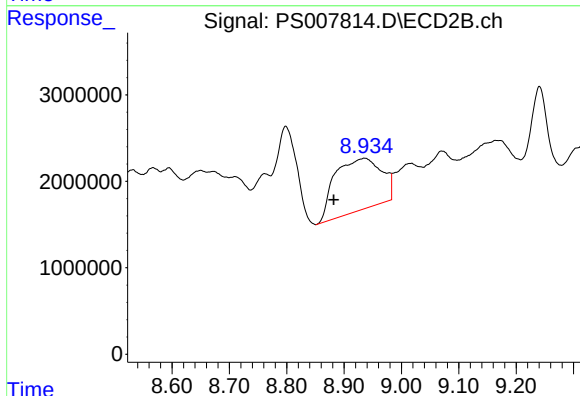


#15 Picloram

R.T.: 8.936 min
Delta R.T.: 0.054 min
Response: 34119300
Conc: 5.82 ng/ml

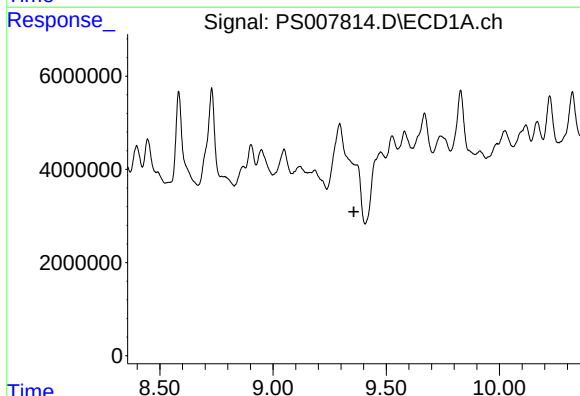

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

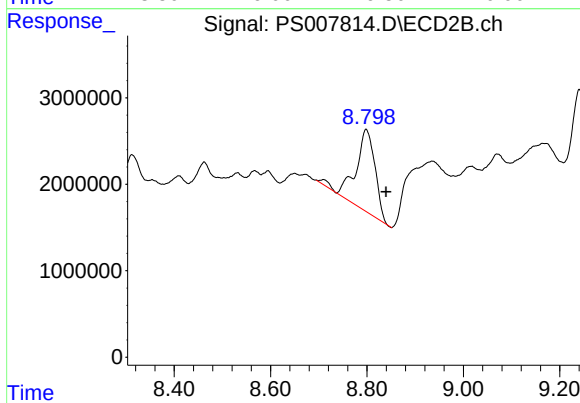

#16 DCPA

R.T.: 8.798 min
Delta R.T.: -0.042 min
Response: 26711458
Conc: 5.11 ng/ml