

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112221\
 Data File : PS017485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2021 17:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 00:37:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.149	6.738	683.3E6	278.0E6	434.597	469.196
Target Compounds							
5) T	DICAMBA	7.338	0.000	11571592	0	1.896	N.D. #
9) T	2,4-D	8.329f	0.000	55025673	0	29.448	N.D. #
10) T	Pentachlo...	8.565	0.000	10452689	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.119	0.000	8493631	0	1.019	N.D. #
12) T	2,4,5-T	9.421	9.036f	16922745	22052990	2.003	6.631 #
14) T	DINOSEB	11.097	0.000	18910250	0	3.037	N.D. #
15) T	Picloram	10.956	10.794	124.1E6	41982964	10.178	9.621
16) T	DCPA	11.365	10.794f	13934235	41982964	1.305	9.528 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112221\
Data File : PS017485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2021 17:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 00:37:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

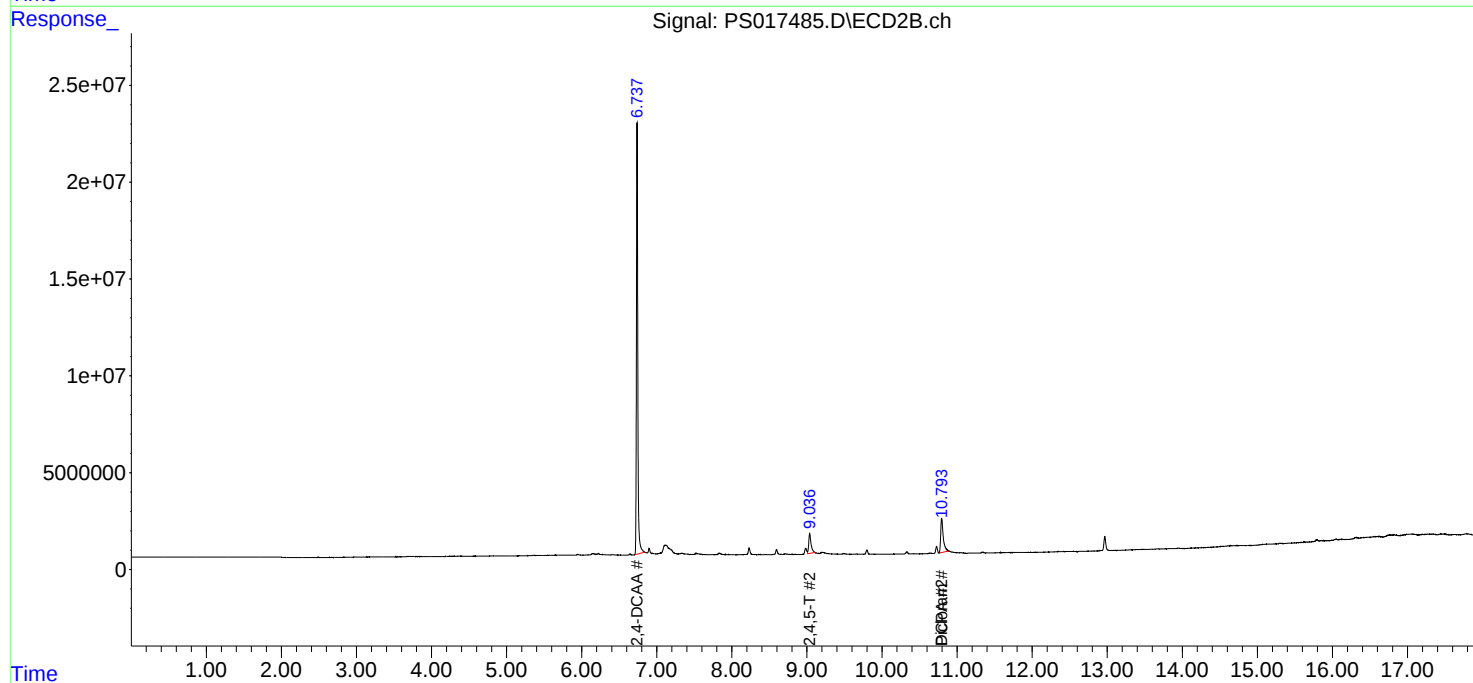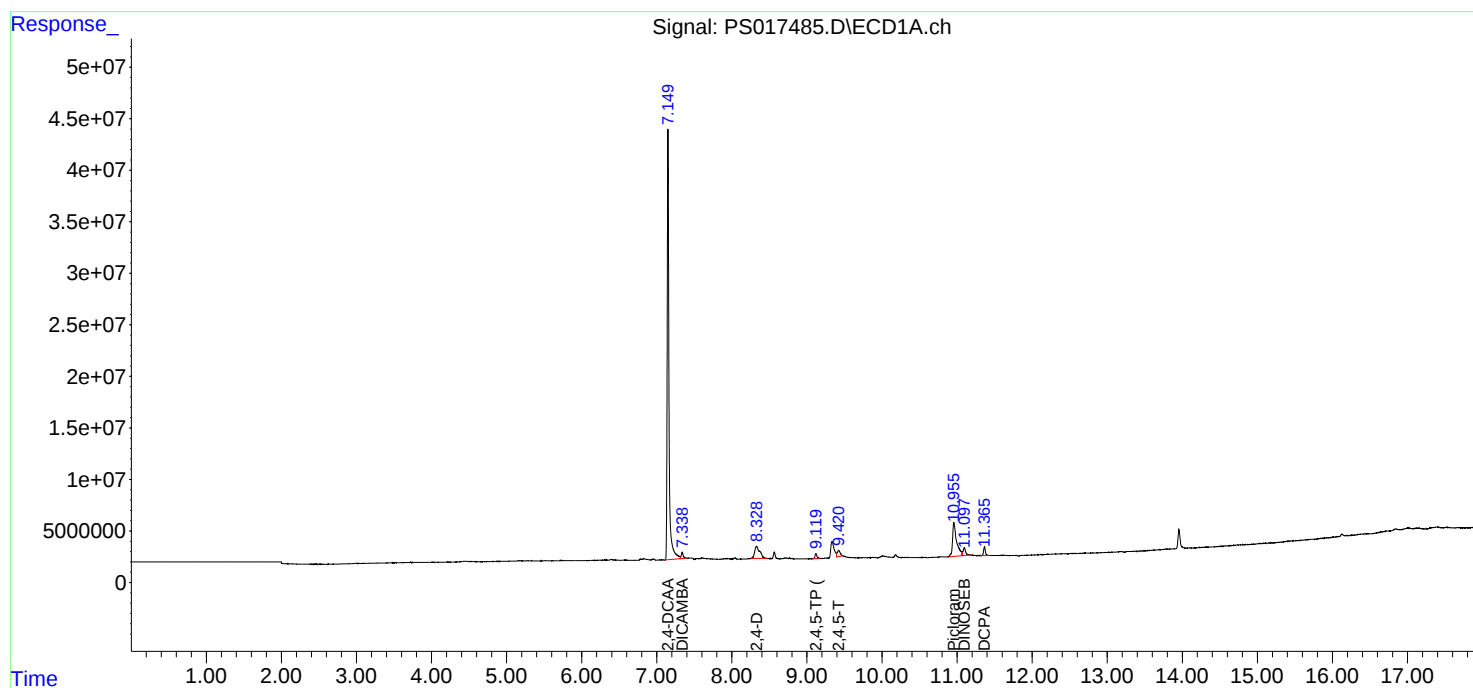


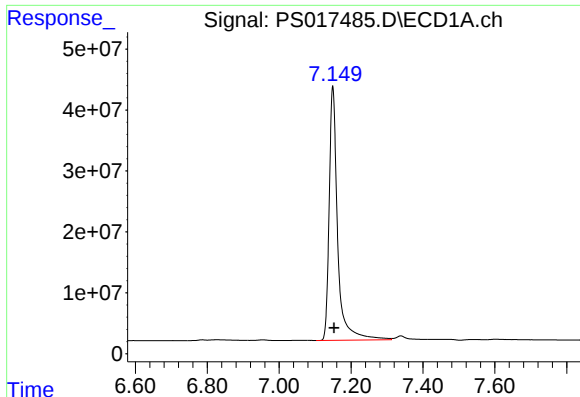

#4 2,4-DCAA


R.T.: 7.149 min
Delta R.T.: -0.003 min
Response: 683270929
Conc: 434.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

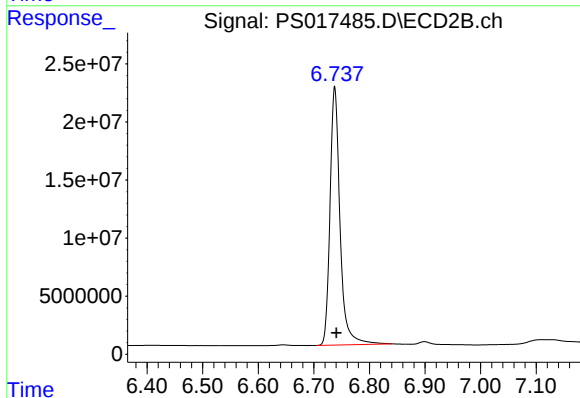


#4 2,4-DCAA

R.T.: 6.738 min
Delta R.T.: -0.003 min
Response: 278035158
Conc: 469.20 ng/ml

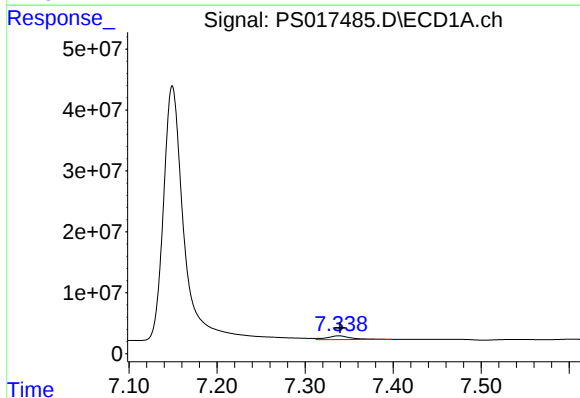


#5 DICAMBA

R.T.: 7.338 min
Delta R.T.: -0.002 min
Response: 11571592
Conc: 1.90 ng/ml

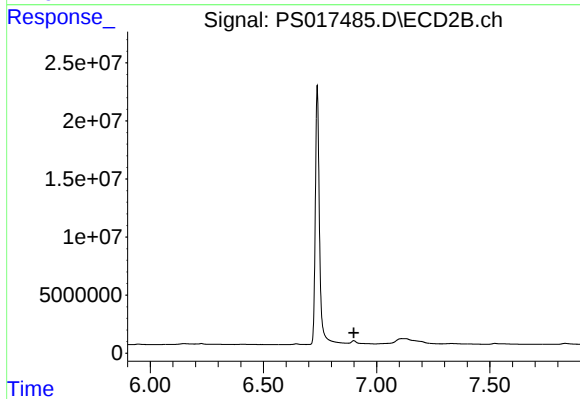

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

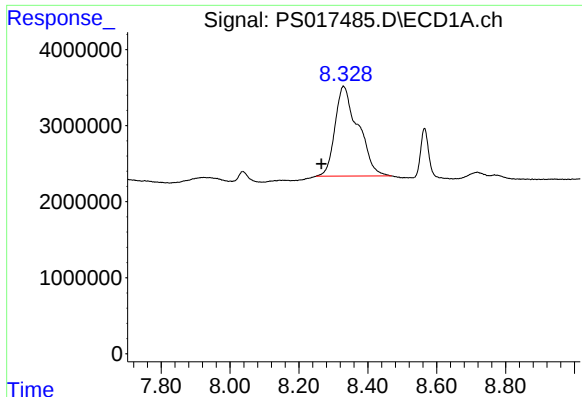

#9 2,4-D


R.T.: 8.329 min
Delta R.T.: 0.064 min
Response: 55025673
Conc: 29.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

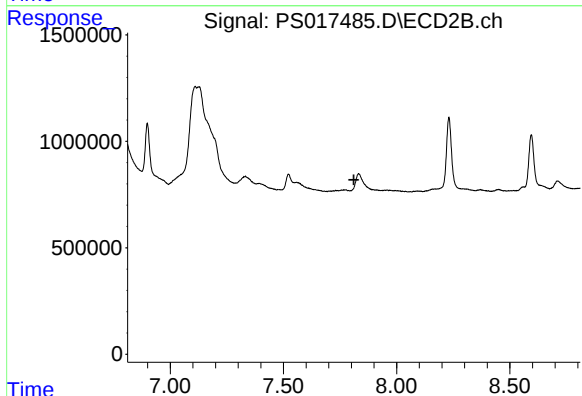


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.

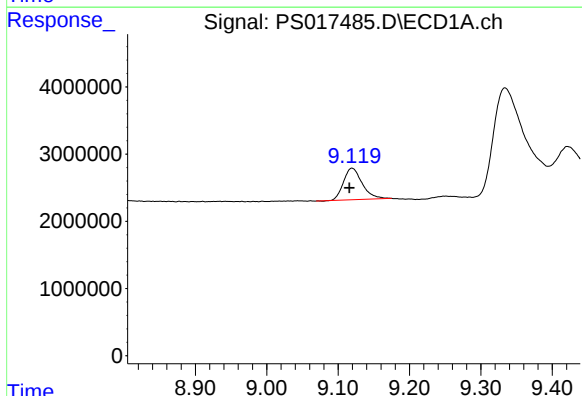


#11 2,4,5-TP (SILVEX)

R.T.: 9.119 min
Delta R.T.: 0.004 min
Response: 8493631
Conc: 1.02 ng/ml

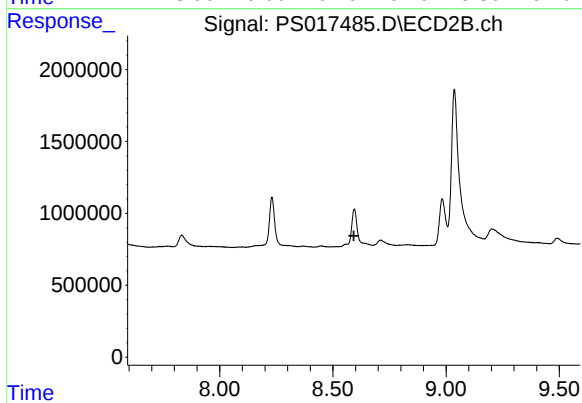

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.593 min
Response: 0
Conc: N.D.

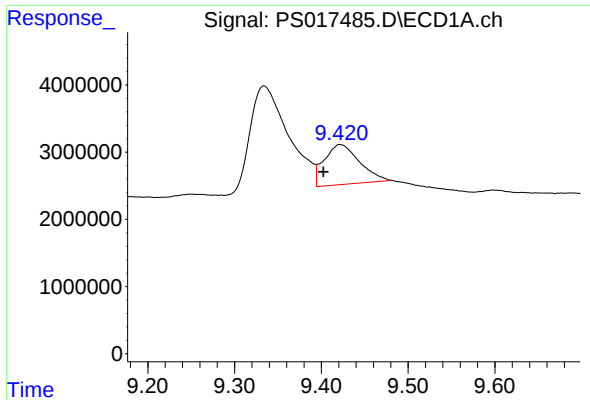

#12 2,4,5-T


R.T.: 9.421 min
Delta R.T.: 0.019 min
Response: 16922745
Conc: 2.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

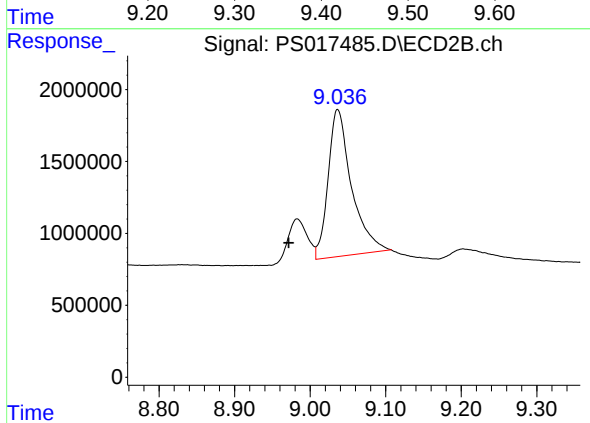


#12 2,4,5-T

R.T.: 9.036 min
Delta R.T.: 0.065 min
Response: 22052990
Conc: 6.63 ng/ml

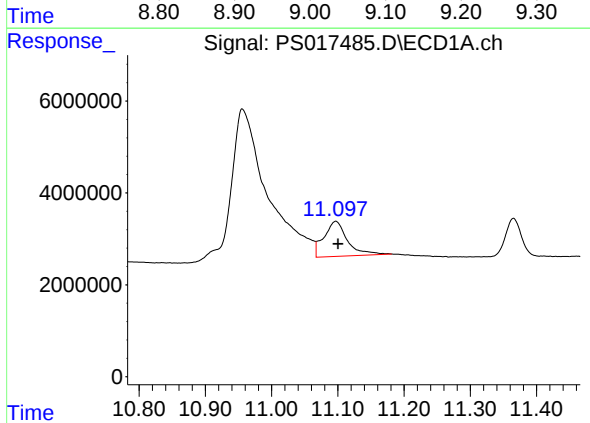


#14 DINOSEB

R.T.: 11.097 min
Delta R.T.: -0.003 min
Response: 18910250
Conc: 3.04 ng/ml

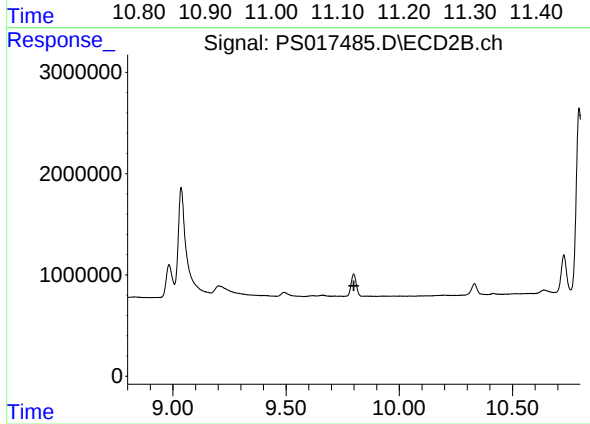

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.799 min
Response: 0
Conc: N.D.

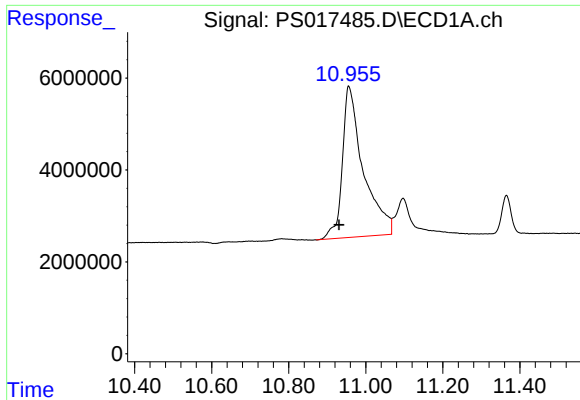

#15 Picloram


R.T.: 10.956 min
Delta R.T.: 0.025 min
Response: 124098285
Conc: 10.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

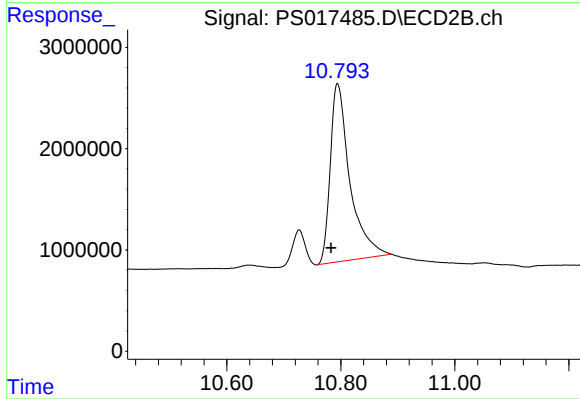


#15 Picloram

R.T.: 10.794 min
Delta R.T.: 0.011 min
Response: 41982964
Conc: 9.62 ng/ml

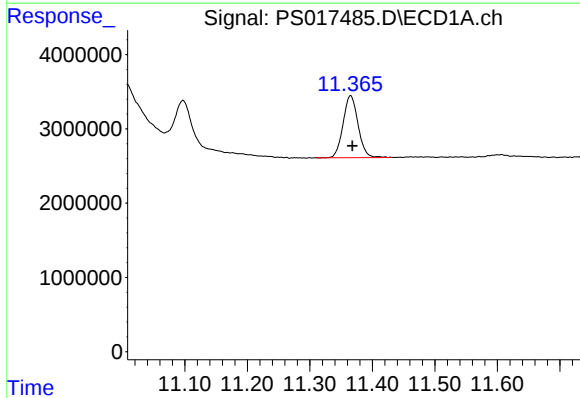

#16 DCPA

R.T.: 11.365 min
Delta R.T.: -0.003 min
Response: 13934235
Conc: 1.30 ng/ml

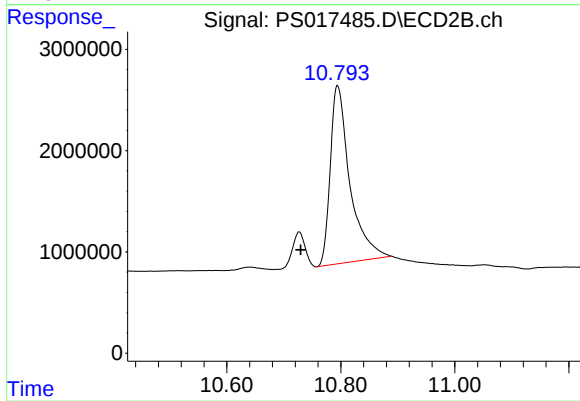

#16 DCPA

R.T.: 10.794 min
Delta R.T.: 0.065 min
Response: 41982964
Conc: 9.53 ng/ml