

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112222\
 Data File : PS021221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 16:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 23:33:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.408	6.843	1015.1E6	807.0E6	466.852	533.660
Target Compounds							
1) T	Dalapon	2.469	0.000	195168	0	<MDL	N.D. #
3) T	4-Nitroph...	6.249	0.000	6039700	0	4.471	N.D. #
7) T	MCPA	6.791f	0.000	7400565	0	<MDL	N.D. #
8) T	DICHLORPROP	7.084f	7.696f	582338	173215	<MDL	<MDL #
10) T	Pentachlo...	7.581	0.000	1286188	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.123	0.000	1859242	0	<MDL	N.D. #
12) T	2,4,5-T	8.371	9.142f	3200865	828333	<MDL	<MDL #
13) T	2,4-DB	8.883	9.544f	1802861	1893467	<MDL	1.617 #
14) T	DINOSEB	9.938	0.000	3313119	0	<MDL	N.D. #
15) T	Picloram	9.782	10.860f	2003463	3076393	<MDL	<MDL #
16) T	DCPA	10.203	10.860	678155	3076393	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112222\
Data File : PS021221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 16:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 23:33:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

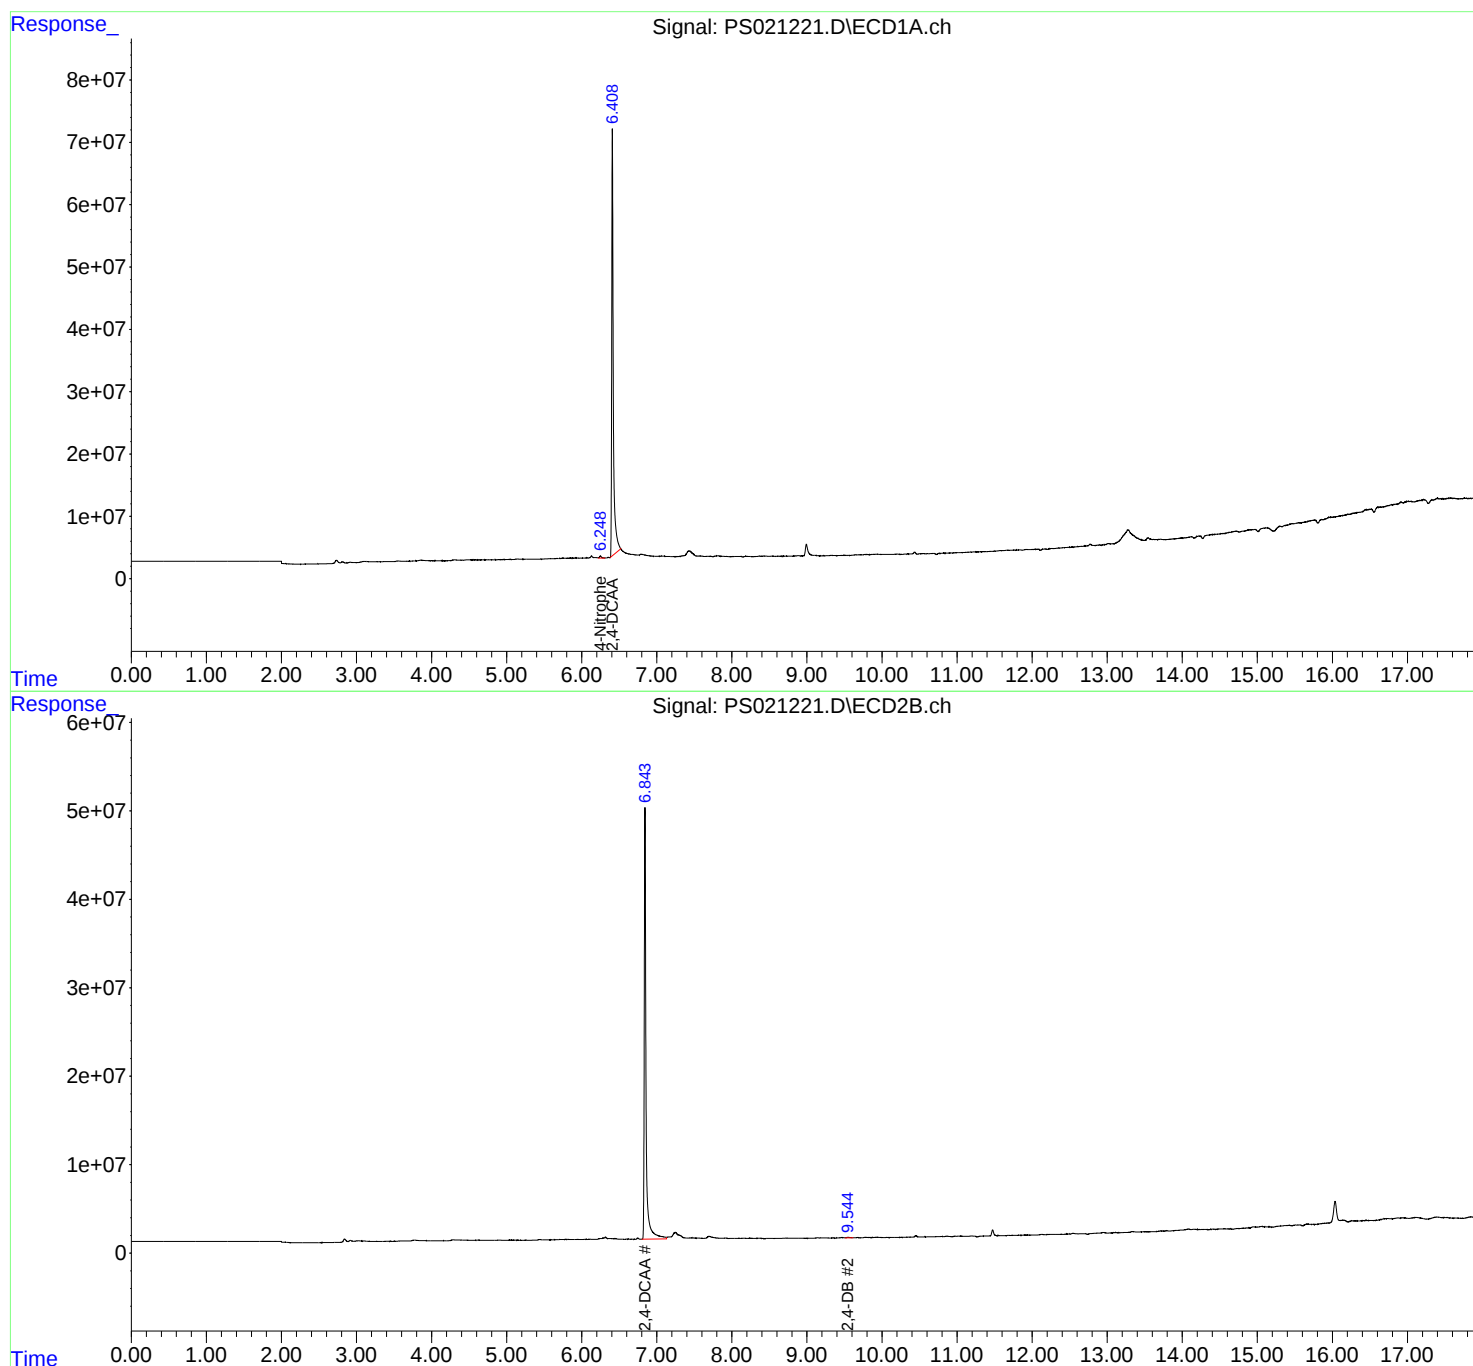


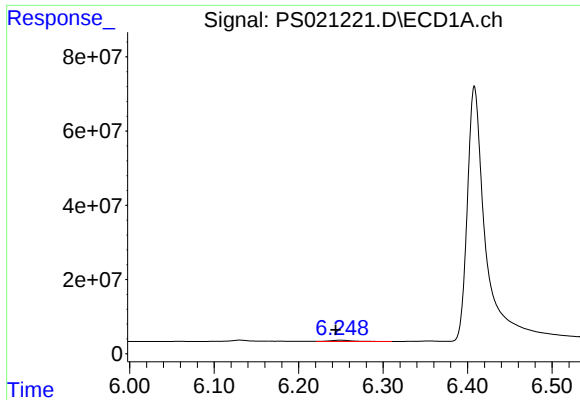

#3 4-Nitrophenol


R.T.: 6.249 min
Delta R.T.: 0.005 min
Response: 6039700
Conc: 4.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

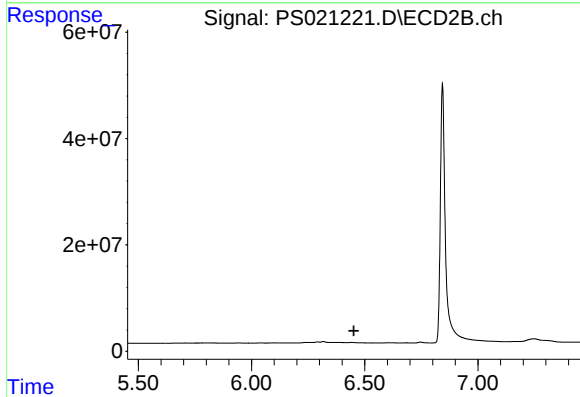


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

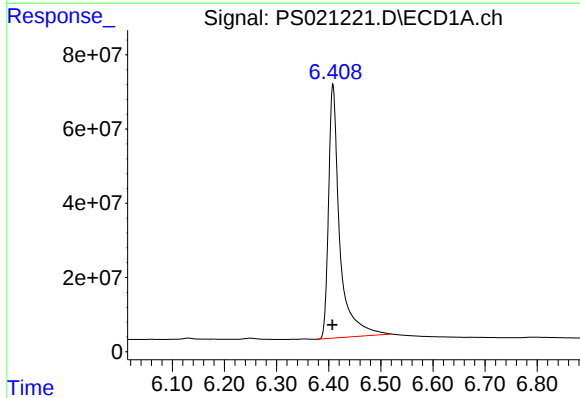


#4 2,4-DCAA

R.T.: 6.408 min
Delta R.T.: 0.002 min
Response: 1015073176
Conc: 466.85 ng/ml

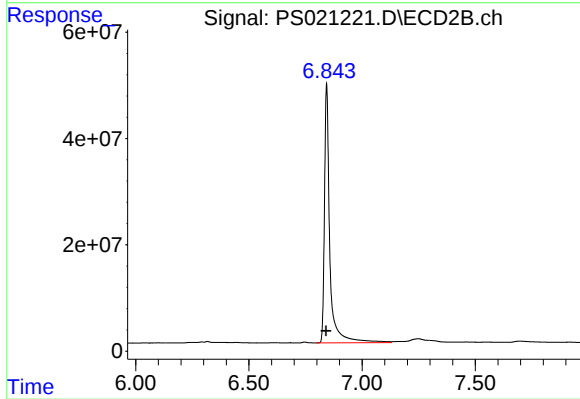

#4 2,4-DCAA


R.T.: 6.843 min
Delta R.T.: 0.001 min
Response: 806956361
Conc: 533.66 ng/ml

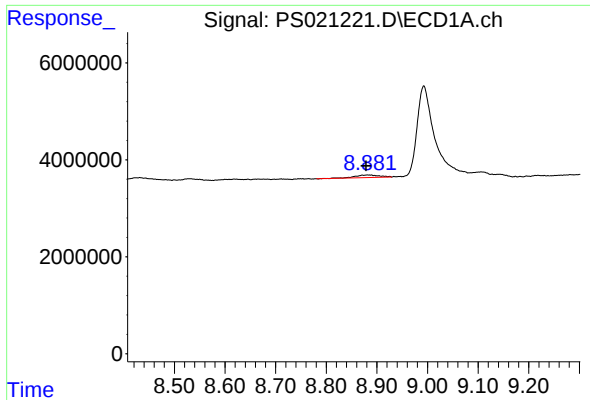

#13 2,4-DB

R.T.: 8.883 min
Delta R.T.: 0.004 min
Response: 1802861
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

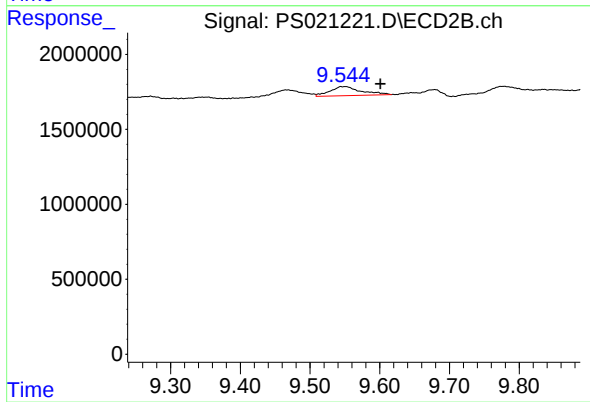

#13 2,4-DB

R.T.: 9.544 min
Delta R.T.: -0.056 min
Response: 1893467
Conc: 1.62 ng/ml