

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
 Data File : PS028595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2024 09:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:56:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	7.732	1488.8E6	647.9E6	582.482	501.318
Target Compounds							
3) T	4-Nitroph...	7.028	0.000	5368724	0	3.161	N.D. #
7) T	MCPA	0.000	8.250f	0	11786684	N.D.	1.903
8) T	DICHLORPROP	0.000	8.702f	0	2689087	N.D.	1.841
10) T	Pentachlo...	8.661	0.000	115446	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.299f	0.000	2843061	0	<MDL	N.D. #
12) T	2,4,5-T	9.541	0.000	625562	0	<MDL	N.D. #
14) T	DINOSEB	11.313	0.000	1321052	0	<MDL	N.D. #
15) T	Picloram	11.134	12.354	18431448	15721635	<MDL	1.389 #
16) T	DCPA	11.603	12.354f	2656402	15721635	<MDL	1.621 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
Data File : PS028595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 09:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:56:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

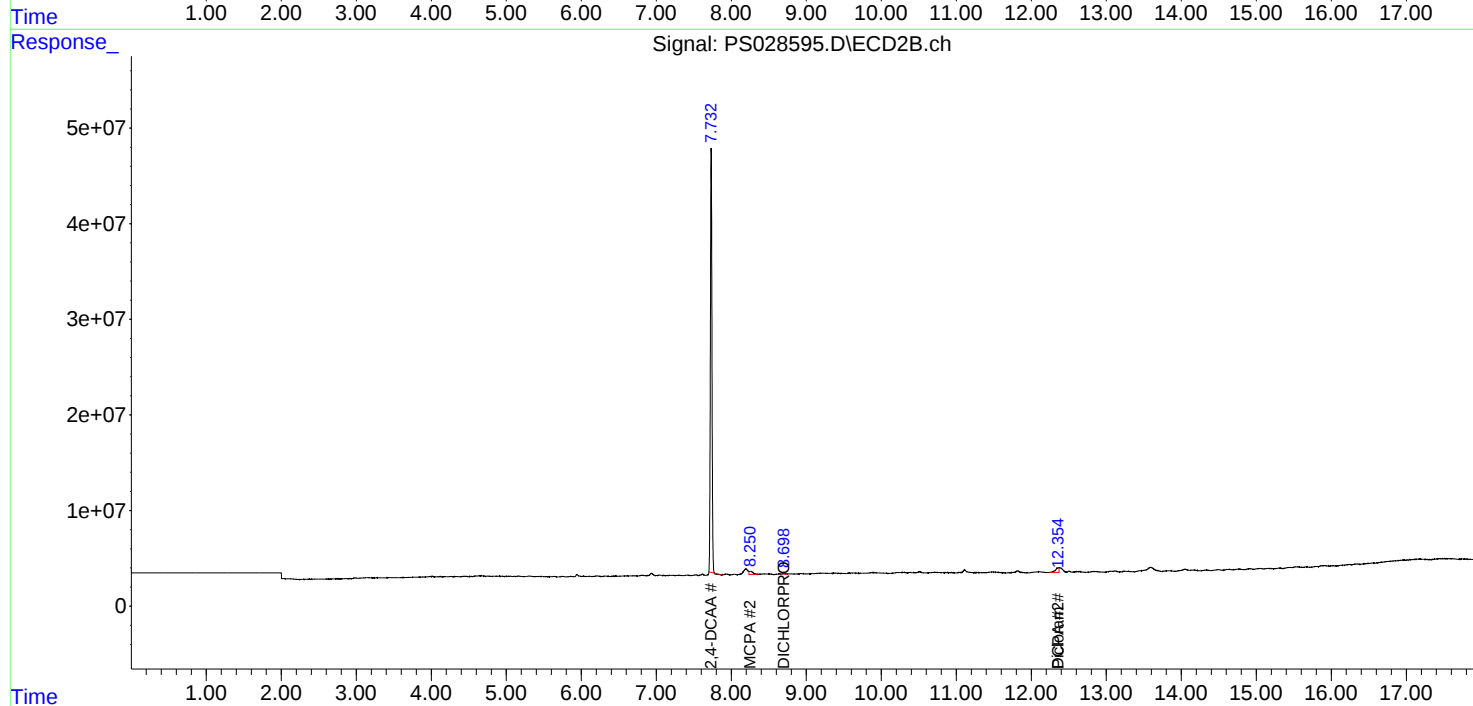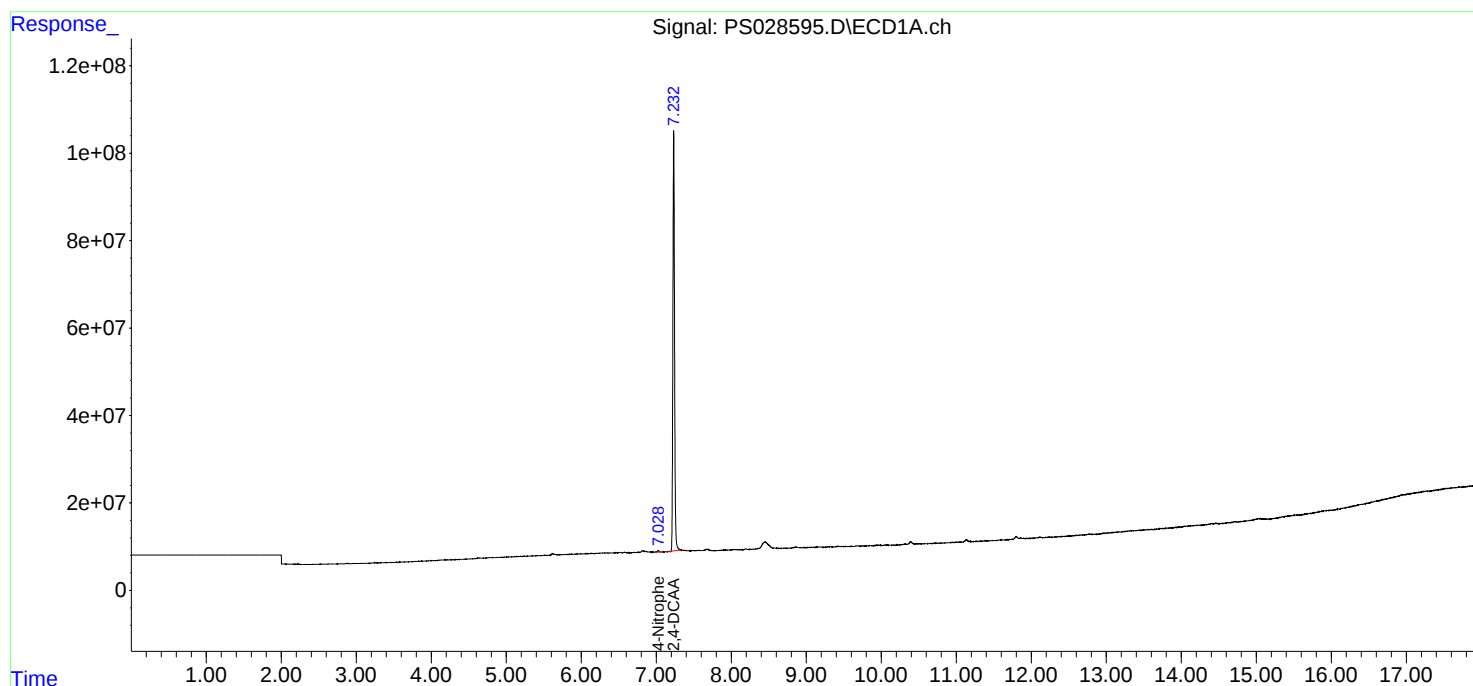


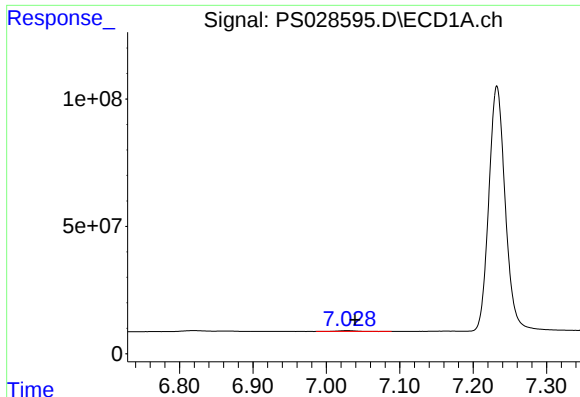

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.011 min
Response: 5368724
Conc: 3.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

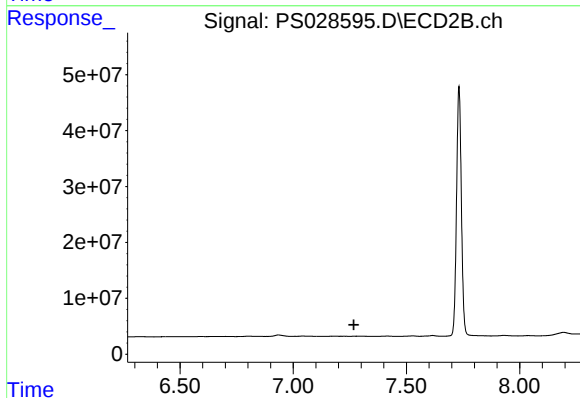


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

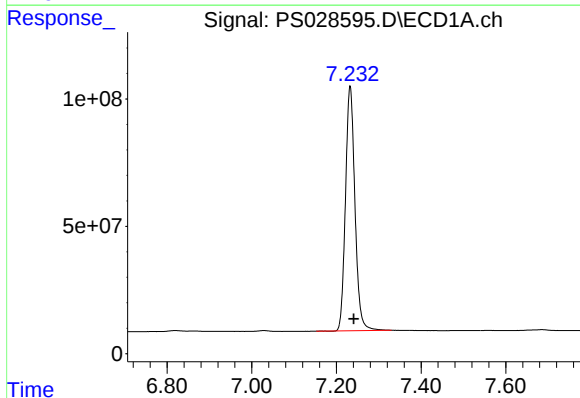


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: -0.009 min
Response: 1488756461
Conc: 582.48 ng/ml

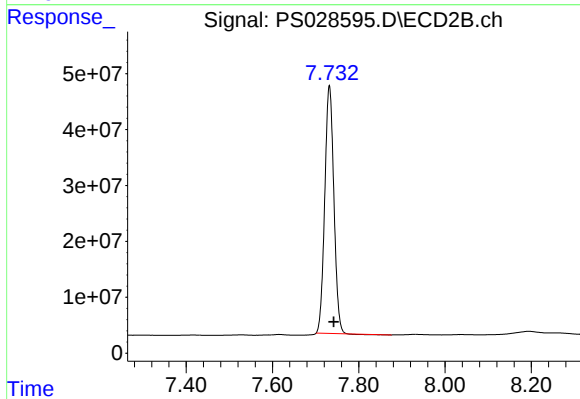

#4 2,4-DCAA


R.T.: 7.732 min
Delta R.T.: -0.010 min
Response: 647855440
Conc: 501.32 ng/ml

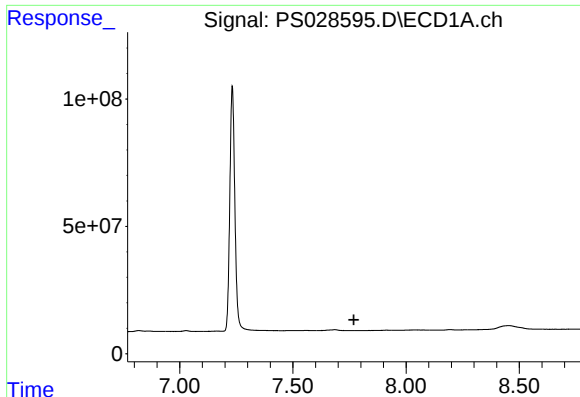

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.769 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

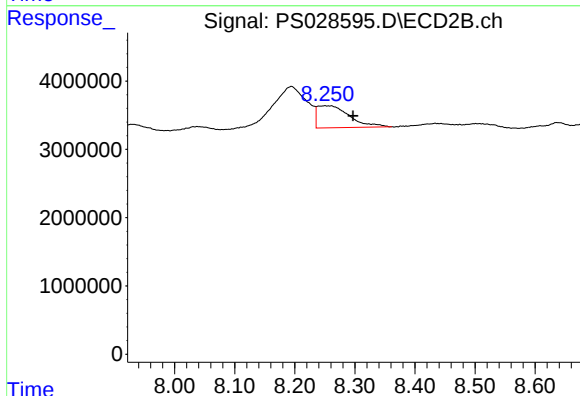


#7 MCPA

R.T.: 8.250 min
Delta R.T.: -0.047 min
Response: 11786684
Conc: 1.90 ug/ml

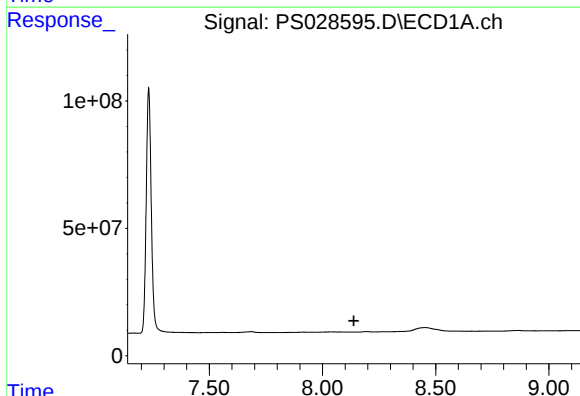


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

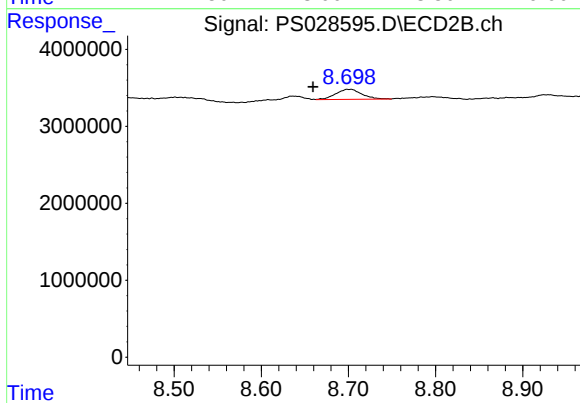

#8 DICHLORPROP


R.T.: 8.702 min
Delta R.T.: 0.043 min
Response: 2689087
Conc: 1.84 ng/ml

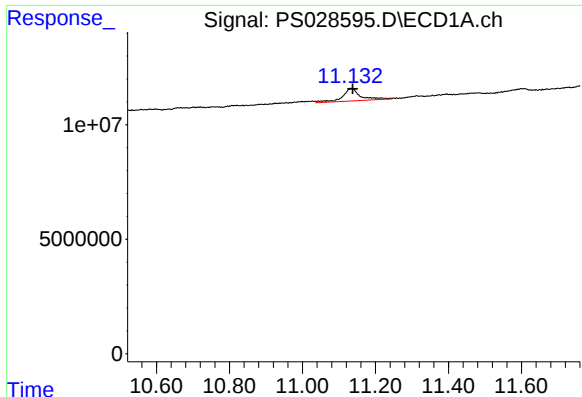

#15 Picloram


R.T.: 11.134 min
Delta R.T.: -0.004 min
Response: 18431448
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

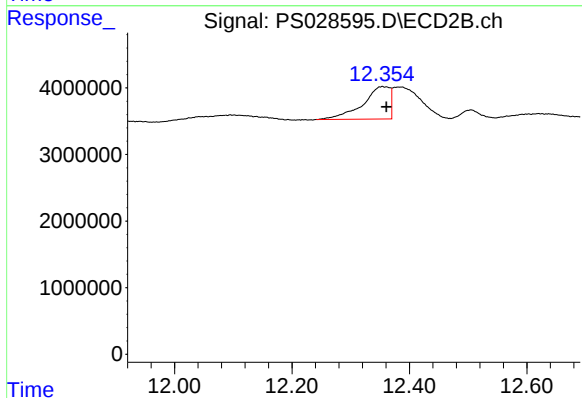


#15 Picloram

R.T.: 12.354 min
Delta R.T.: -0.007 min
Response: 15721635
Conc: 1.39 ng/ml

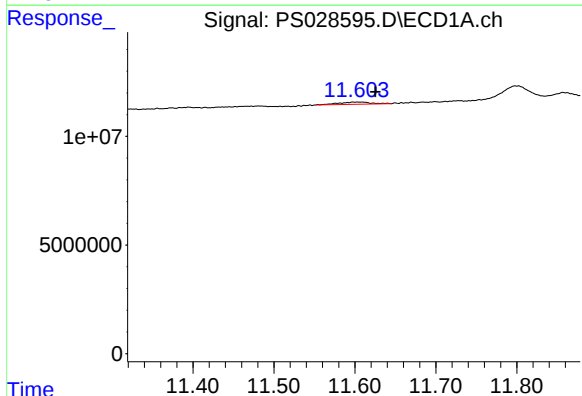

#16 DCPA

R.T.: 11.603 min
Delta R.T.: -0.022 min
Response: 2656402
Conc: N.D.

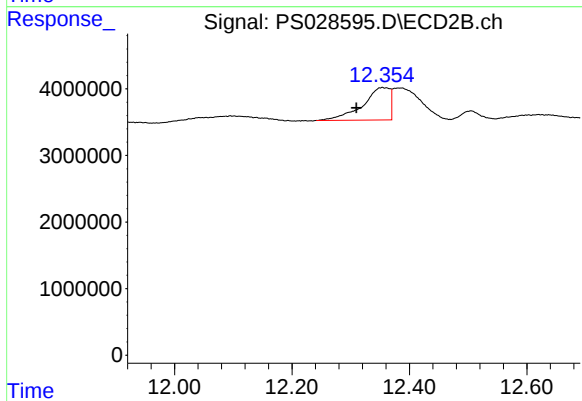

#16 DCPA

R.T.: 12.354 min
Delta R.T.: 0.044 min
Response: 15721635
Conc: 1.62 ng/ml