

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
 Data File : PS028603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2024 13:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 21:04:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	7.731	1461.1E6	654.5E6	571.653	506.423
Target Compounds							
3) T	4-Nitroph...	7.024	0.000	9289332	0	5.469	N.D. #
5) T	DICAMBA	0.000	7.927	0	4070116	N.D.	<MDL
6) T	MCP	7.660f	0.000	28502482	0	4.052	N.D. #
7) T	MCPA	7.774	0.000	334626	0	<MDL	N.D. #
8) T	DICHLORPROP	8.097f	8.698f	1799476	10449032	<MDL	7.154 #
10) T	Pentachlo...	8.657	0.000	350649	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.880	0	2310620	N.D.	<MDL
12) T	2,4,5-T	9.536	0.000	7445475	0	<MDL	N.D. #
14) T	DINOSEB	11.311	0.000	3775474	0	<MDL	N.D. #
15) T	Picloram	11.127	12.345	26903023	11269587	<MDL	<MDL #
16) T	DCPA	11.596f	12.294	8332244	2165632	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
Data File : PS028603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 13:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 21:04:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

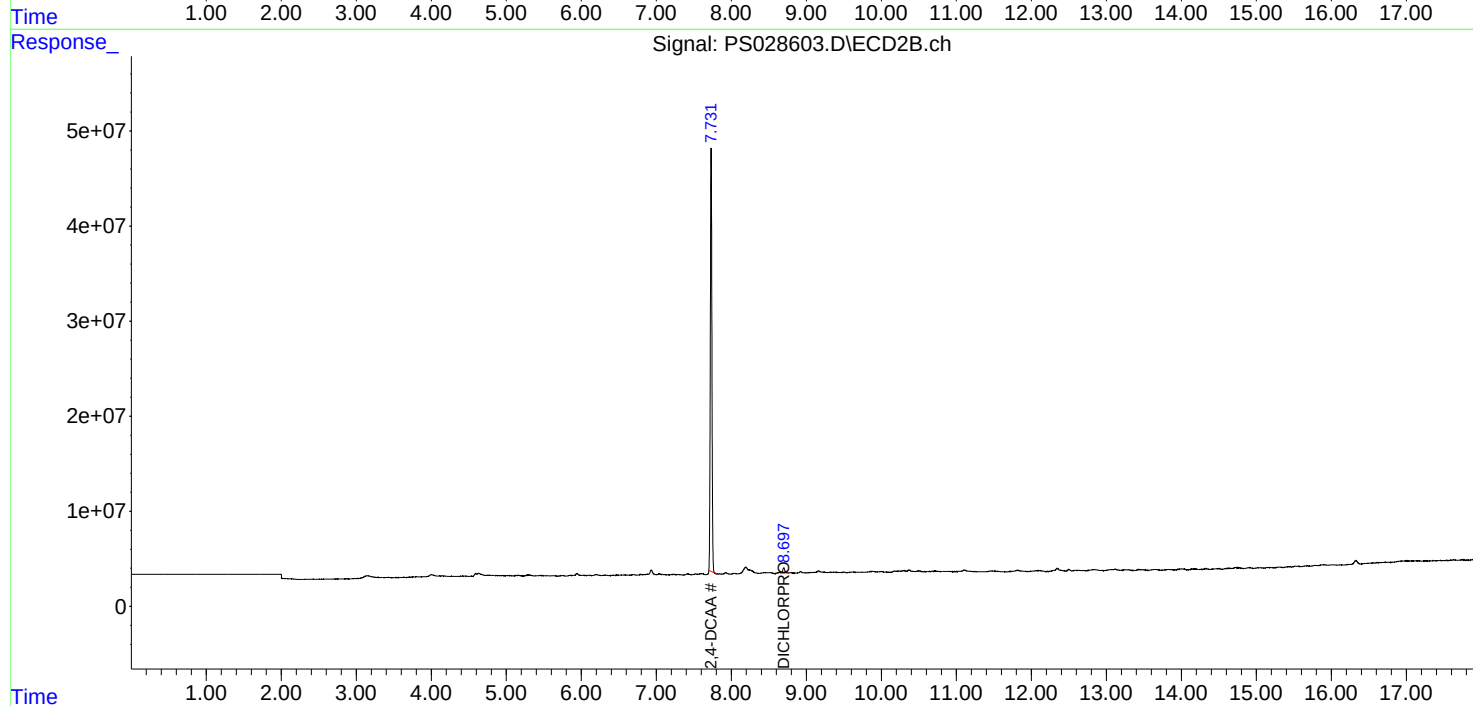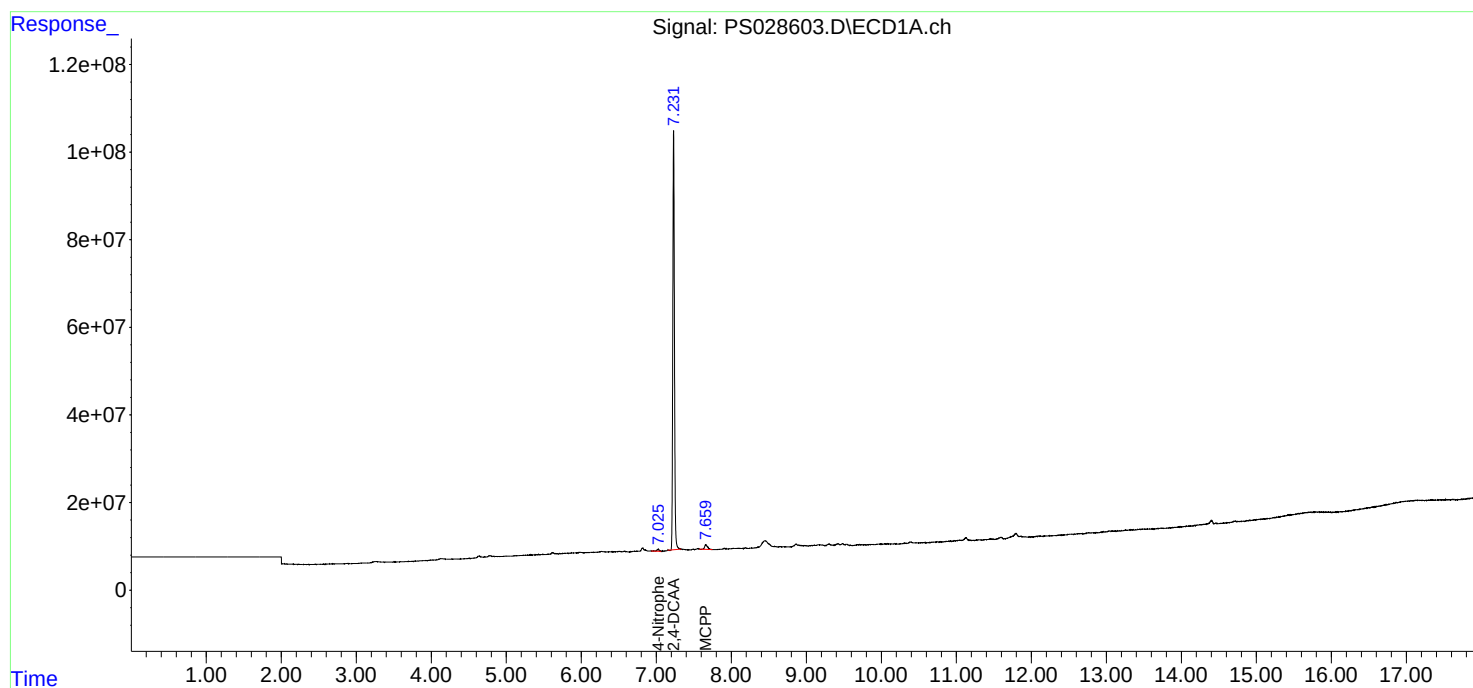


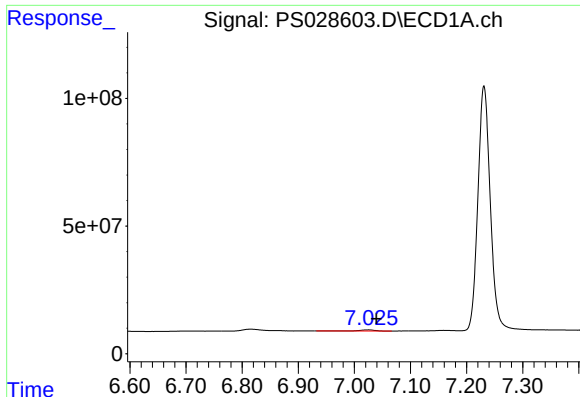

#3 4-Nitrophenol


R.T.: 7.024 min
Delta R.T.: -0.015 min
Response: 9289332
Conc: 5.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

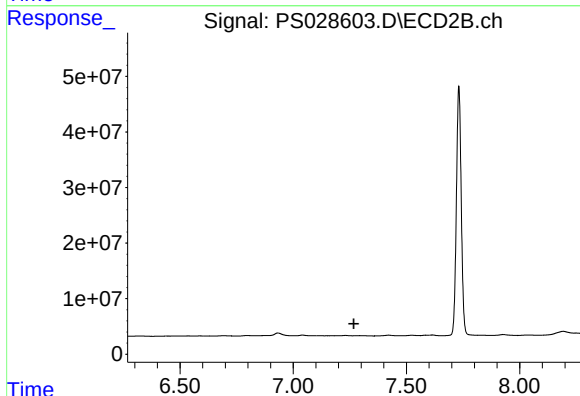


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

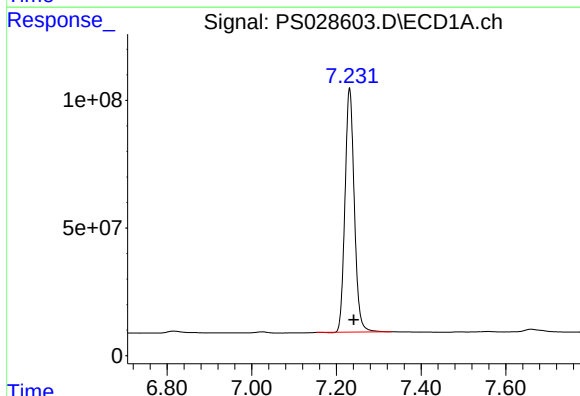


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.010 min
Response: 1461078709
Conc: 571.65 ng/ml

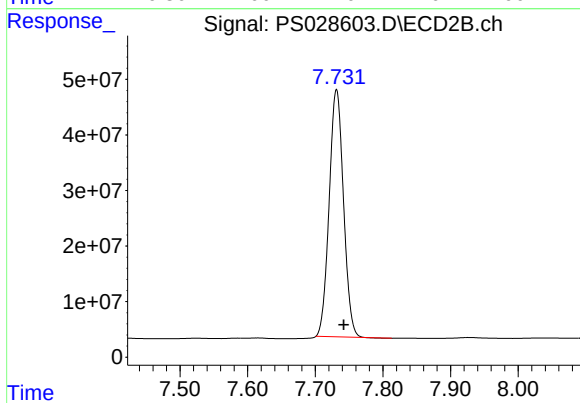

#4 2,4-DCAA


R.T.: 7.731 min
Delta R.T.: -0.011 min
Response: 654453166
Conc: 506.42 ng/ml

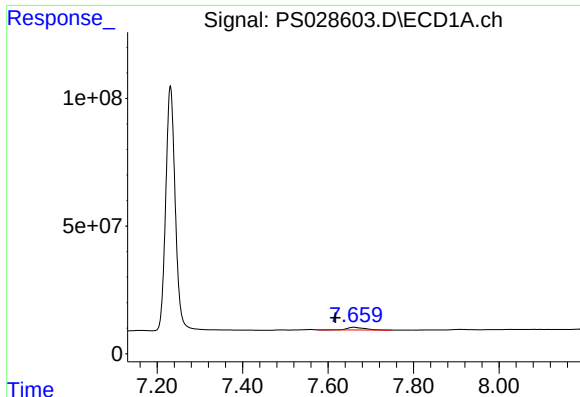

#6 MCP


R.T.: 7.660 min
Delta R.T.: 0.042 min
Response: 28502482
Conc: 4.05 ug/ml

Instrument :
ECD_S
ClientSampleId :

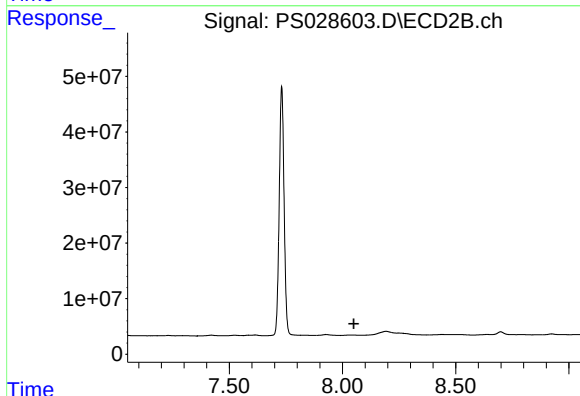


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

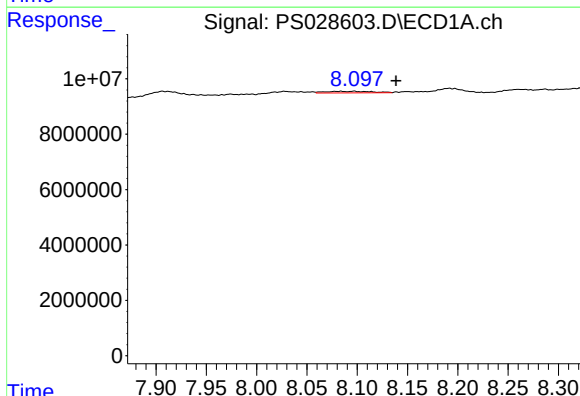

#8 DICHLORPROP

R.T.: 8.097 min
Delta R.T.: -0.042 min
Response: 1799476
Conc: N.D.

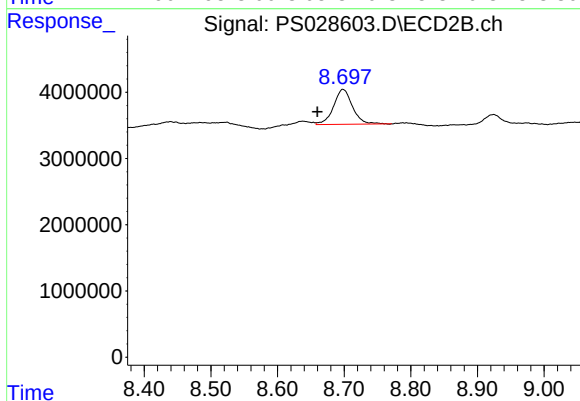

#8 DICHLORPROP

R.T.: 8.698 min
Delta R.T.: 0.039 min
Response: 10449032
Conc: 7.15 ng/ml