

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
 Data File : PS028610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2024 18:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 21:10:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	7.730	1483.3E6	667.0E6	580.355	516.096
Target Compounds							
1) T	Dalapon	2.673f	0.000	2405558	0	<MDL	N.D. #
3) T	4-Nitroph...	7.021	0.000	9952987	0	5.860	N.D. #
5) T	DICAMBA	0.000	7.925	0	4201739	N.D.	<MDL
6) T	MCP	7.659f	0.000	52373684	0	7.445	N.D. #
8) T	DICHLORPROP	8.097f	8.696f	2270945	23296760	<MDL	15.950 #
10) T	Pentachlo...	8.693	0.000	1448859	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.889	0	3589629	N.D.	<MDL
12) T	2,4,5-T	9.535	0.000	2276683	0	<MDL	N.D. #
14) T	DINOSEB	11.313	0.000	3282979	0	<MDL	N.D. #
15) T	Picloram	11.124	12.340	15613718	12097369	<MDL	1.069 #
16) T	DCPA	11.633	12.340f	186275	12097369	<MDL	1.247 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112224\
Data File : PS028610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2024 18:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 21:10:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

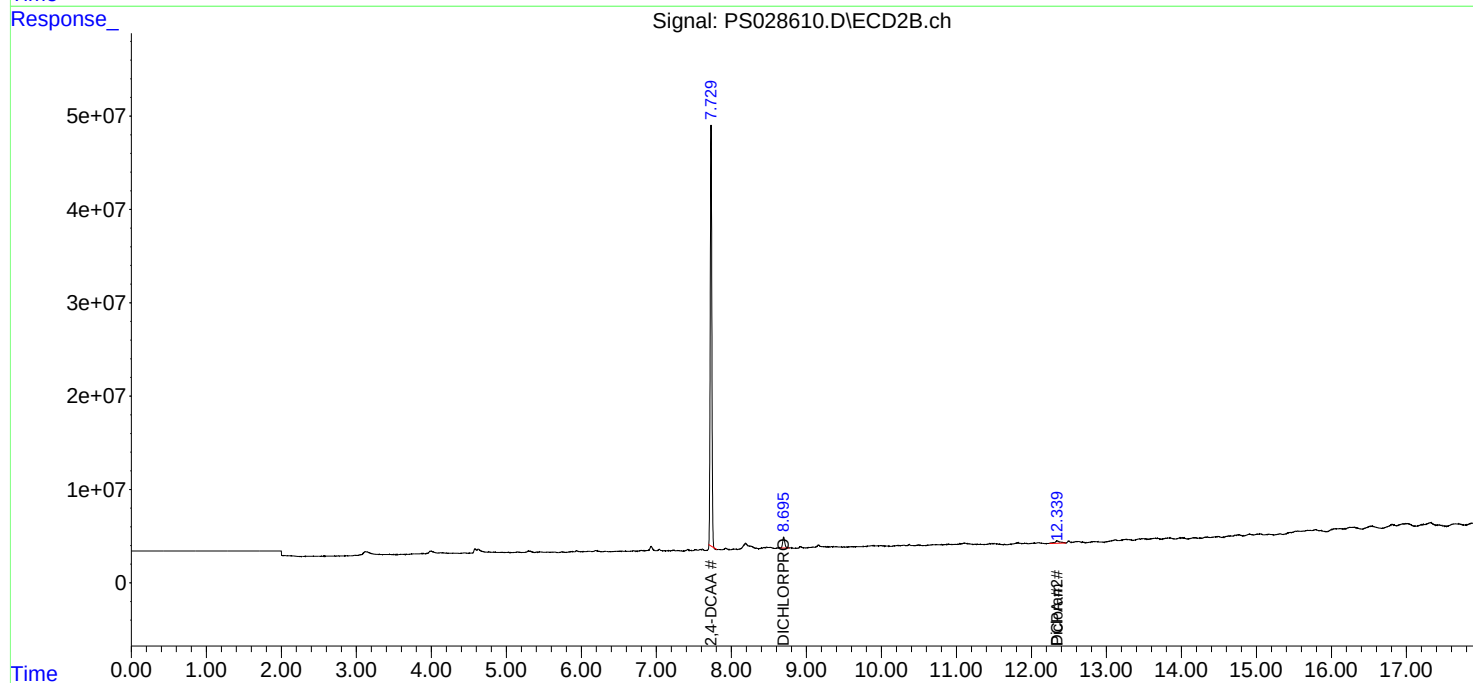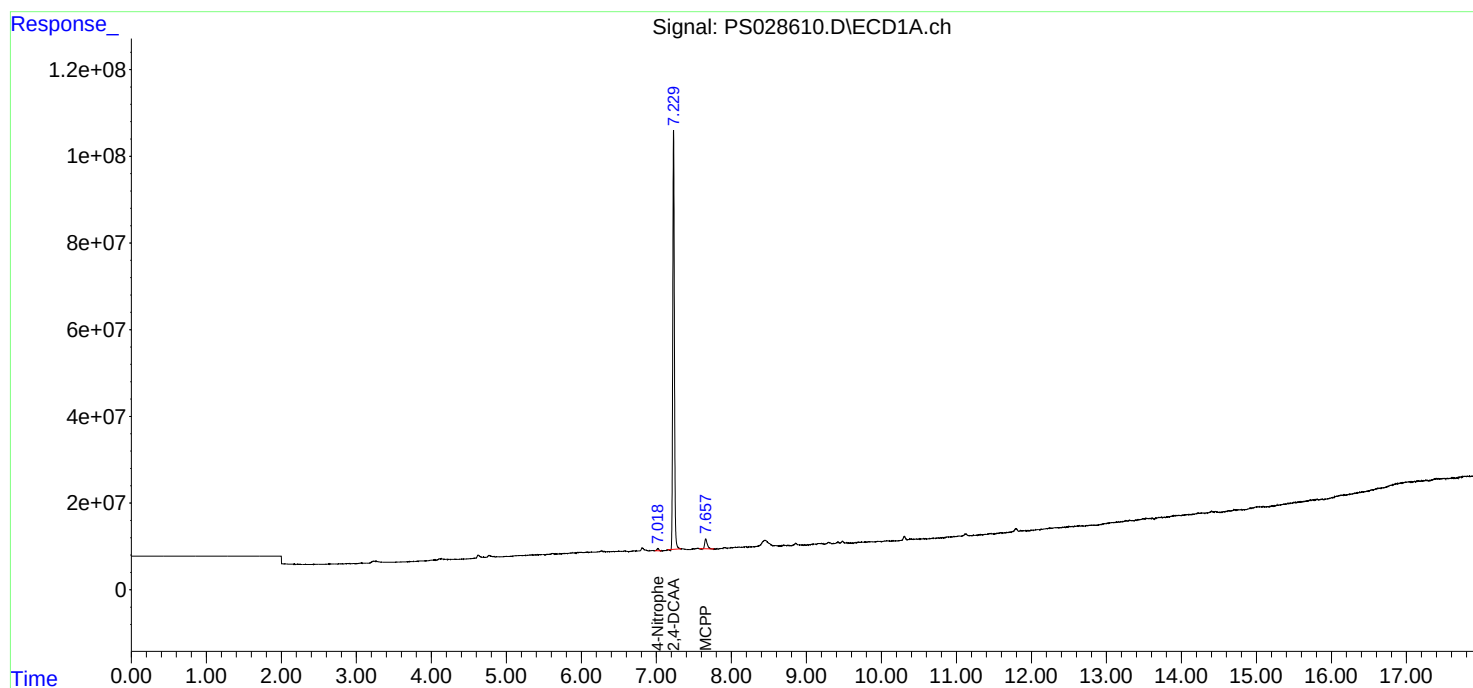


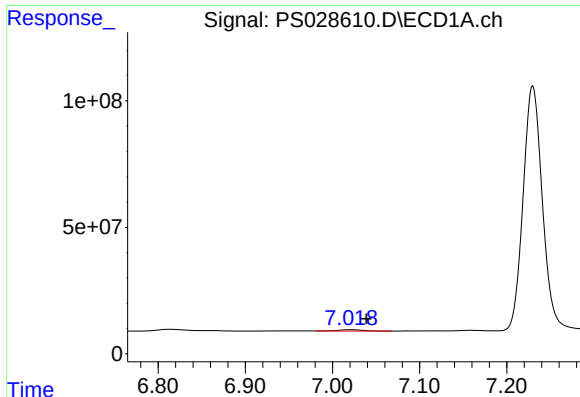

#3 4-Nitrophenol


R.T.: 7.021 min
Delta R.T.: -0.018 min
Response: 9952987
Conc: 5.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

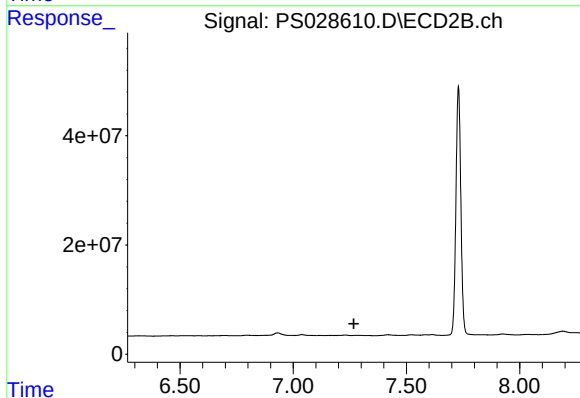


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

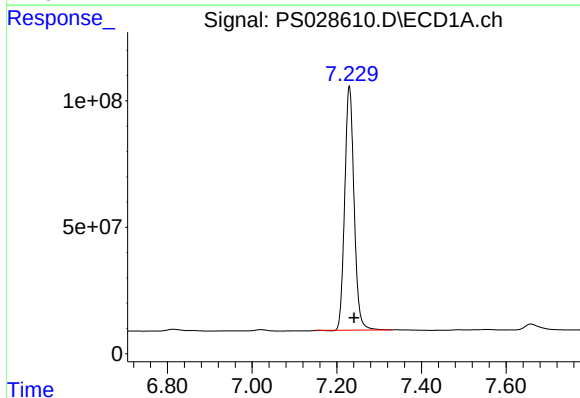


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: -0.011 min
Response: 1483319807
Conc: 580.36 ng/ml

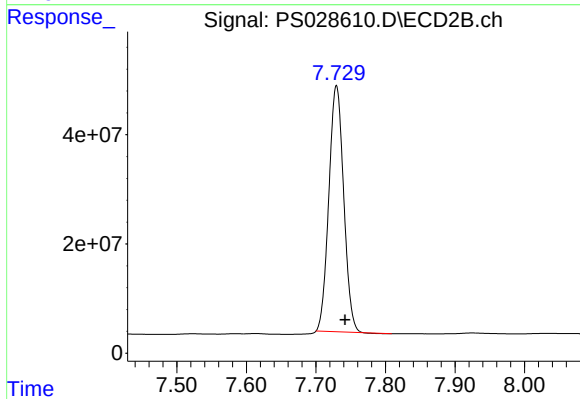

#4 2,4-DCAA


R.T.: 7.730 min
Delta R.T.: -0.012 min
Response: 666953364
Conc: 516.10 ng/ml

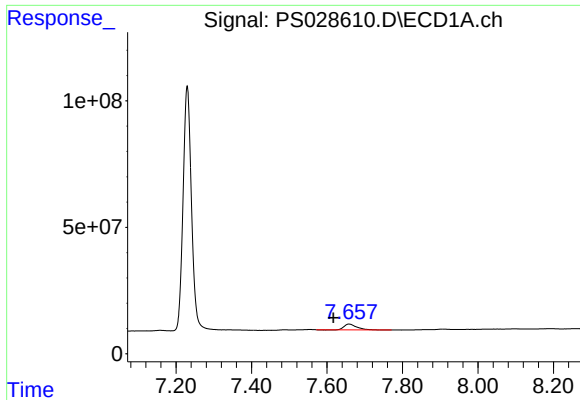

#6 MCP


R.T.: 7.659 min
Delta R.T.: 0.041 min
Response: 52373684
Conc: 7.45 ug/ml

Instrument :
ECD_S
ClientSampleId :

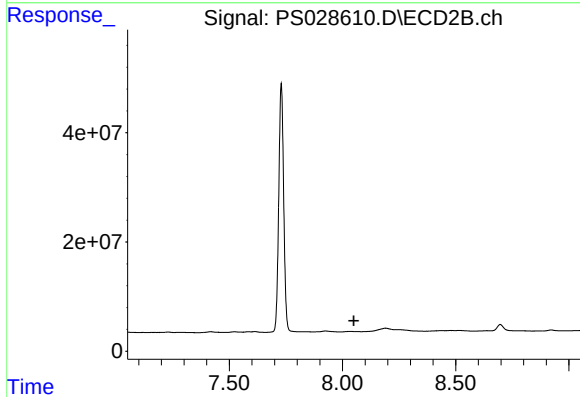


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

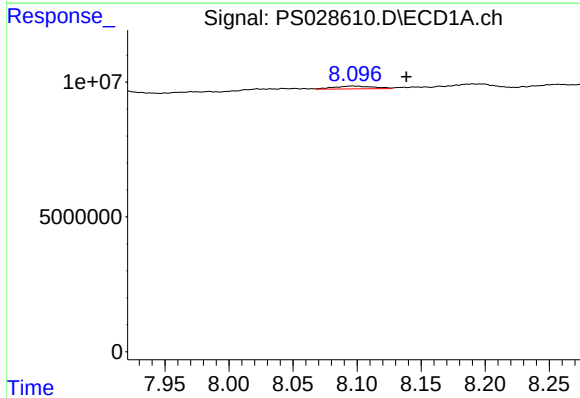


#8 DICHLORPROP

R.T.: 8.097 min
Delta R.T.: -0.041 min
Response: 2270945
Conc: N.D.

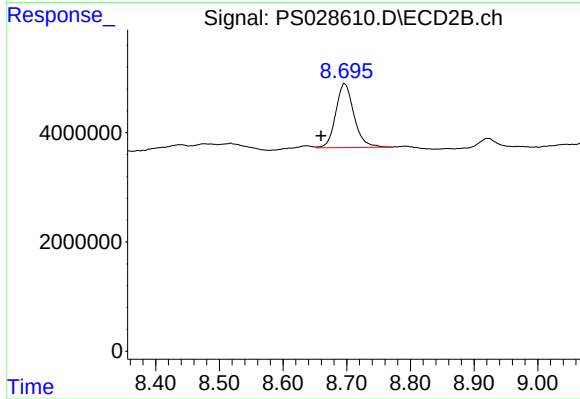

#8 DICHLORPROP


R.T.: 8.696 min
Delta R.T.: 0.037 min
Response: 23296760
Conc: 15.95 ng/ml

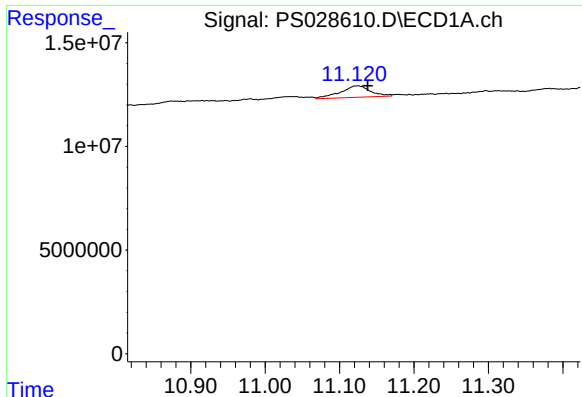

#15 Picloram


R.T.: 11.124 min
Delta R.T.: -0.014 min
Response: 15613718
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

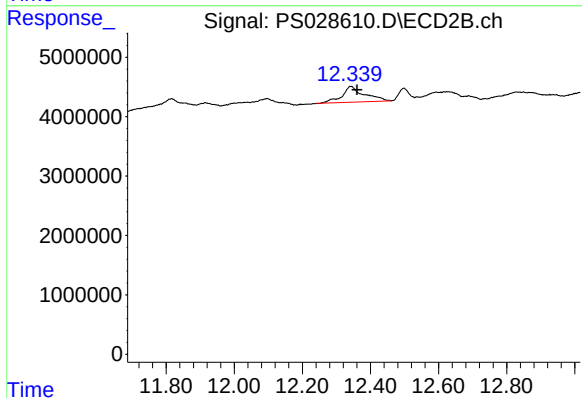


#15 Picloram

R.T.: 12.340 min
Delta R.T.: -0.020 min
Response: 12097369
Conc: 1.07 ng/ml

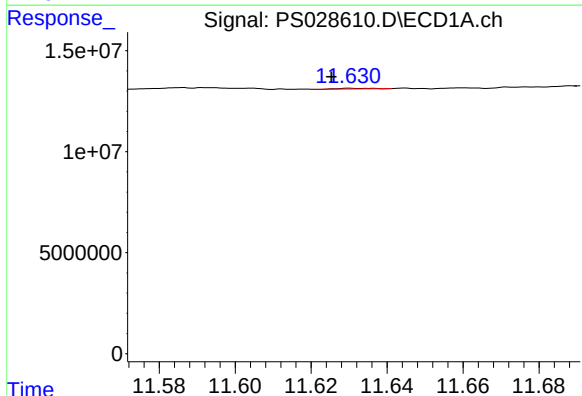

#16 DCPA

R.T.: 11.633 min
Delta R.T.: 0.007 min
Response: 186275
Conc: N.D.

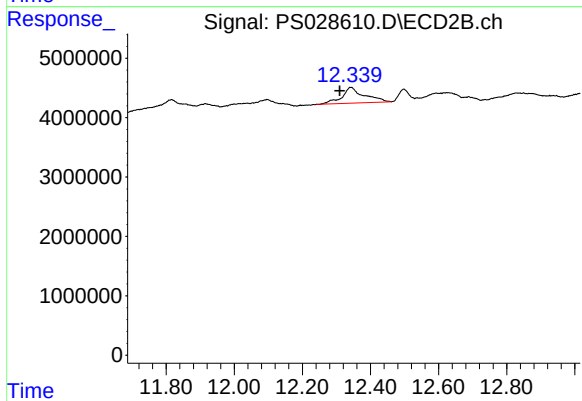

#16 DCPA

R.T.: 12.340 min
Delta R.T.: 0.031 min
Response: 12097369
Conc: 1.25 ng/ml