

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112421\
 Data File : PS017499.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2021 09:26
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 00:31:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.150	6.738	690.7E6	277.3E6	439.342	467.996
Target Compounds							
9) T	2,4-D	8.331f	0.000	28594809	0	15.303	N.D. #
12) T	2,4,5-T	9.355f	0.000	8672645	0	1.027	N.D. #
15) T	Picloram	10.975f	10.806	31140356	13215981	2.554	3.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112421\
Data File : PS017499.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2021 09:26
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 00:31:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

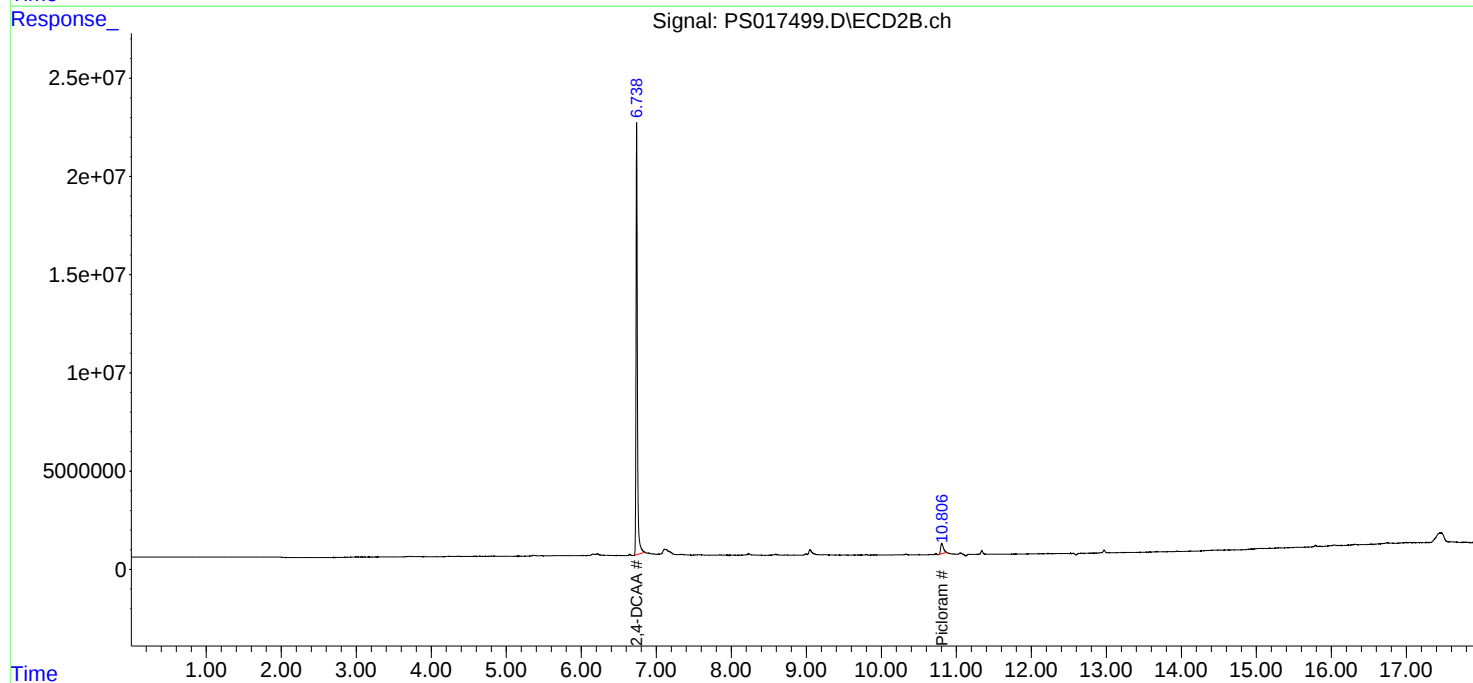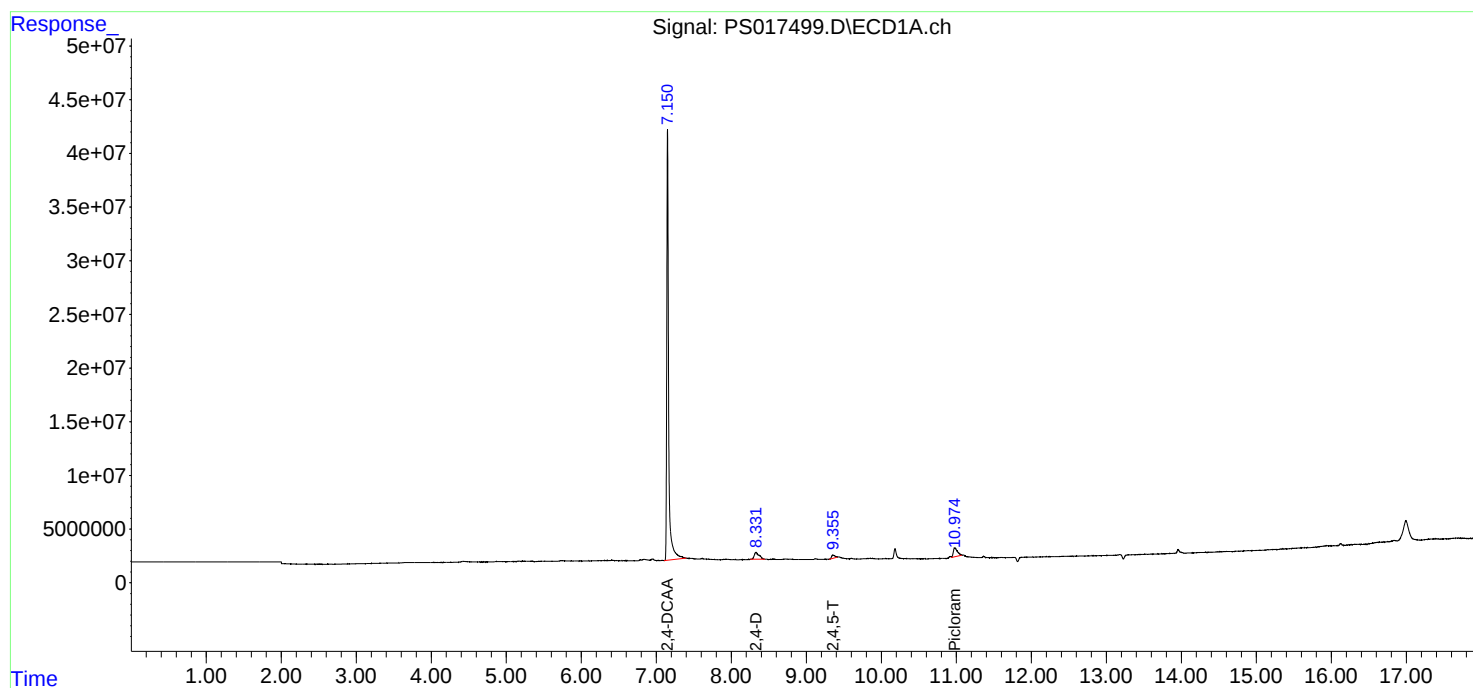


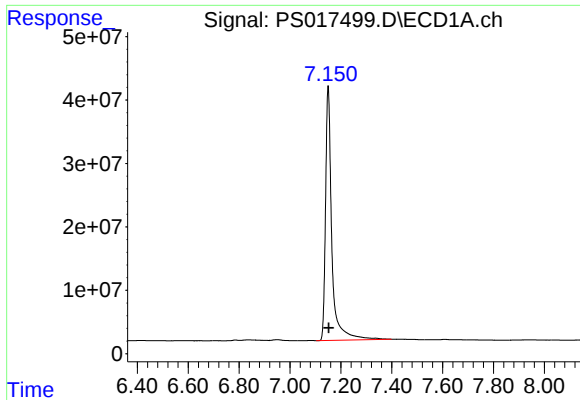

#4 2,4-DCAA


R.T.: 7.150 min
Delta R.T.: -0.003 min
Response: 690730870
Conc: 439.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

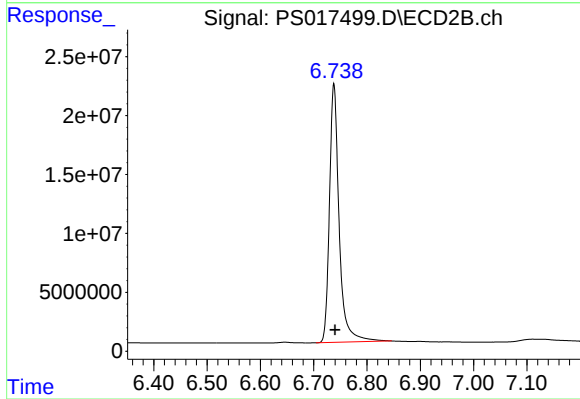


#4 2,4-DCAA

R.T.: 6.738 min
Delta R.T.: -0.002 min
Response: 277324152
Conc: 468.00 ng/ml

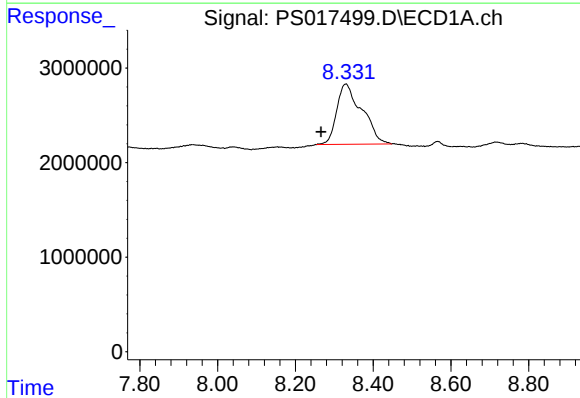


#9 2,4-D

R.T.: 8.331 min
Delta R.T.: 0.065 min
Response: 28594809
Conc: 15.30 ng/ml

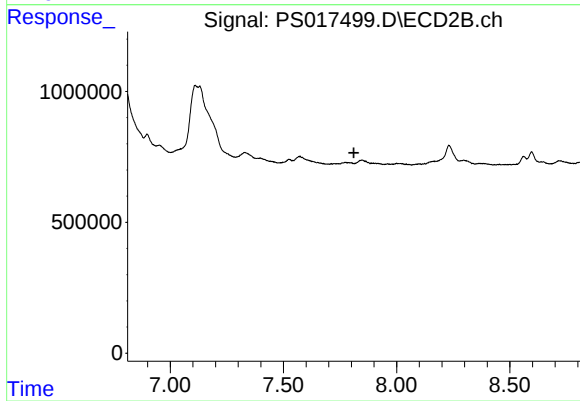

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.811 min
Response: 0
Conc: N.D.

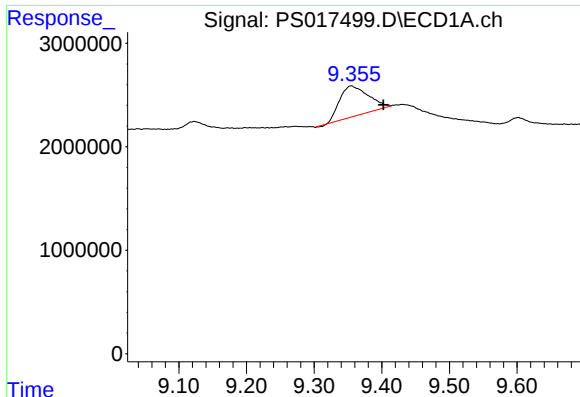

#12 2,4,5-T


R.T.: 9.355 min
Delta R.T.: -0.047 min
Response: 8672645
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

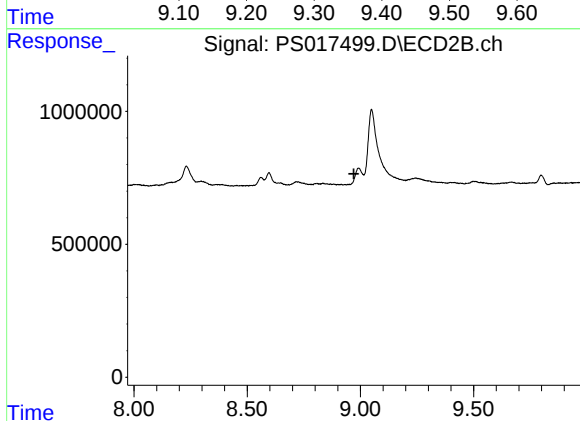


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.972 min
Response: 0
Conc: N.D.

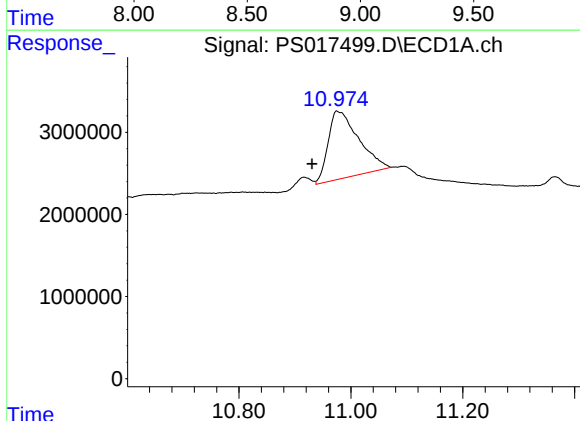

#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.044 min
Response: 31140356
Conc: 2.55 ng/ml

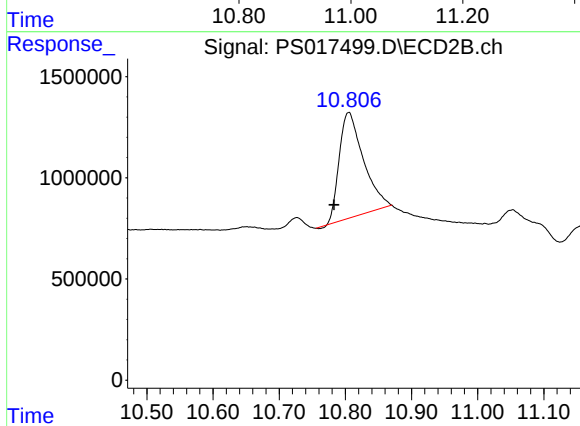

#15 Picloram

R.T.: 10.806 min
Delta R.T.: 0.023 min
Response: 13215981
Conc: 3.03 ng/ml