

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112421\
 Data File : PS017510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2021 15:02
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 00:37:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.148	6.737	704.7E6	285.0E6	448.225	480.882
Target Compounds							
5) T	DICAMBA	7.338	0.000	15906553	0	2.606	N.D. #
9) T	2,4-D	8.327f	0.000	48886971	0	26.162	N.D. #
10) T	Pentachlo...	8.564	0.000	12168134	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.121	0.000	12330948	0	1.480	N.D. #
12) T	2,4,5-T	9.426	9.040f	19618989	27181297	2.322	8.174 #
14) T	DINOSEB	11.095	0.000	23079868	0	3.706	N.D. #
15) T	Picloram	10.913	10.799	7446679	35628537	<MDL	8.165 #
16) T	DCPA	11.364	10.725	20618972	7986941	1.931	1.813



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112421\
Data File : PS017510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2021 15:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 00:37:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

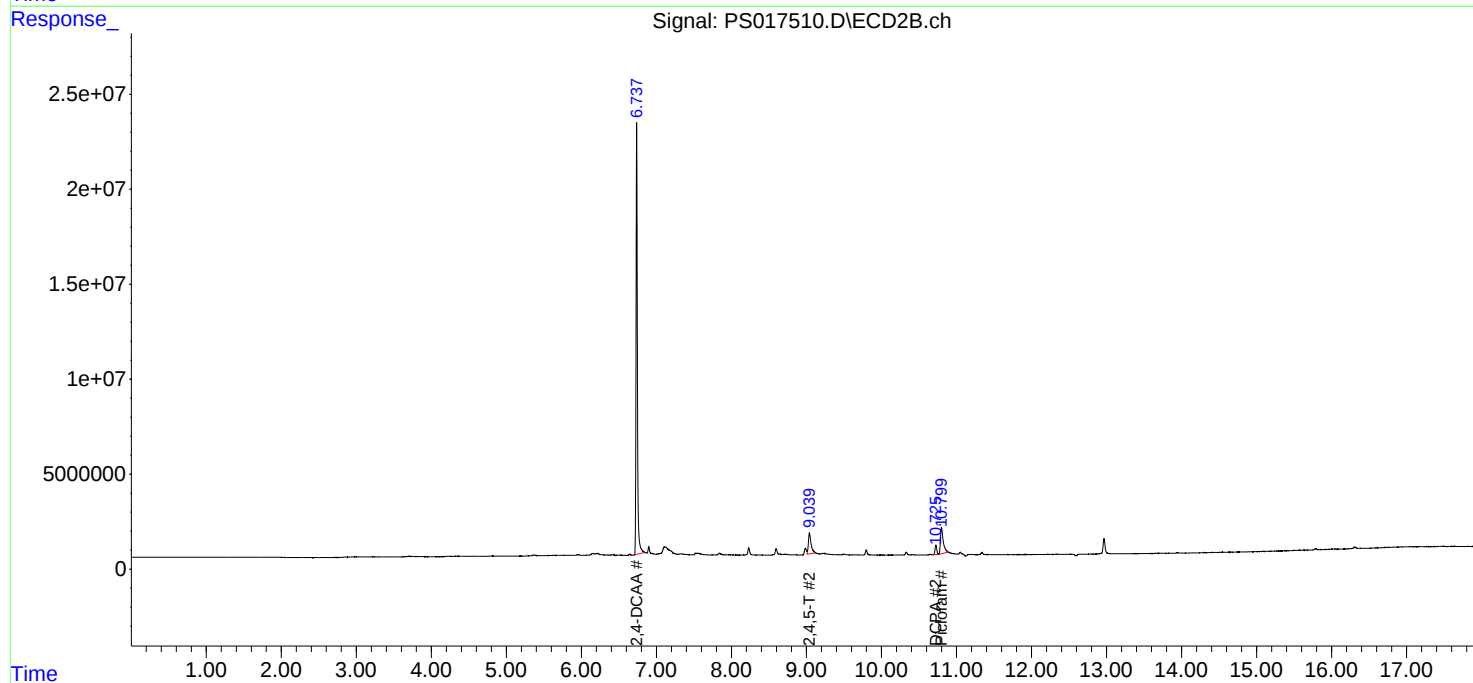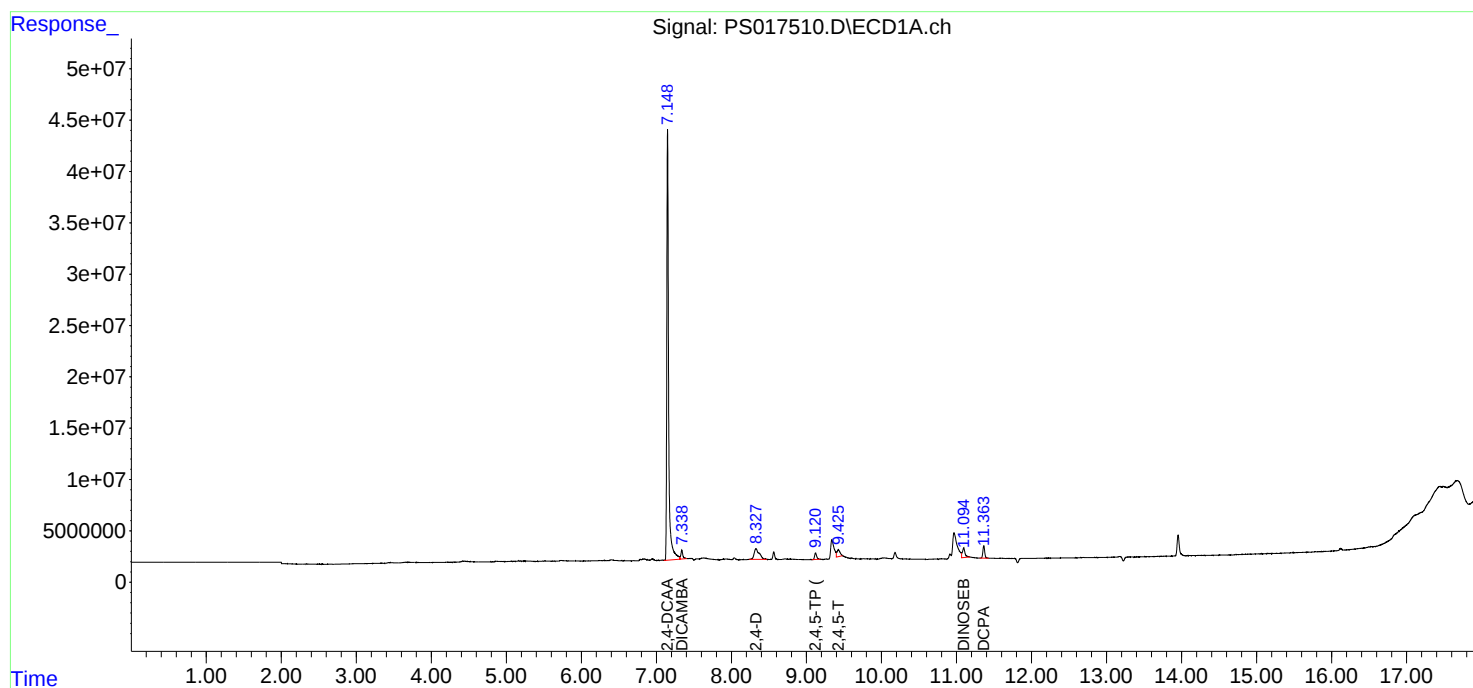


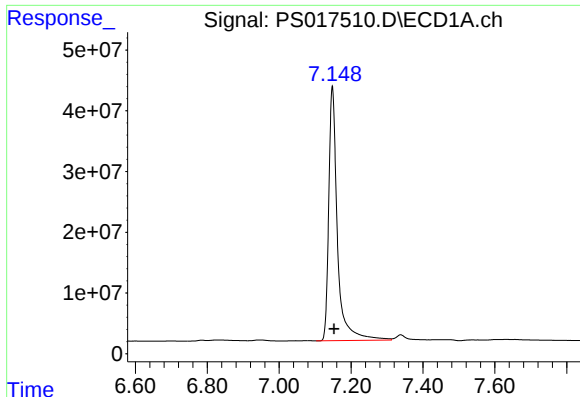

#4 2,4-DCAA


R.T.: 7.148 min
Delta R.T.: -0.005 min
Response: 704697433
Conc: 448.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

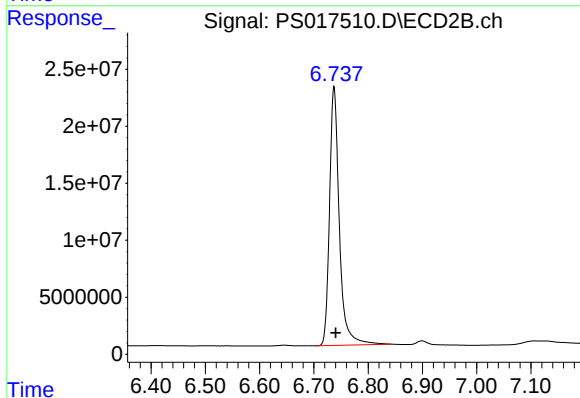


#4 2,4-DCAA

R.T.: 6.737 min
Delta R.T.: -0.003 min
Response: 284959807
Conc: 480.88 ng/ml

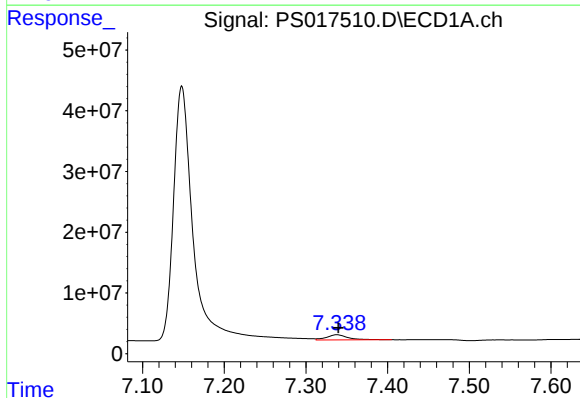


#5 DICAMBA

R.T.: 7.338 min
Delta R.T.: -0.002 min
Response: 15906553
Conc: 2.61 ng/ml

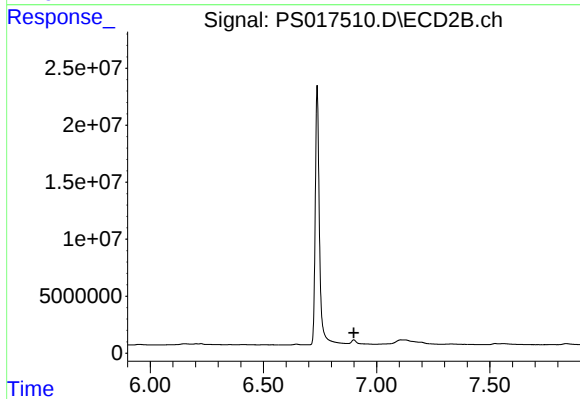

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

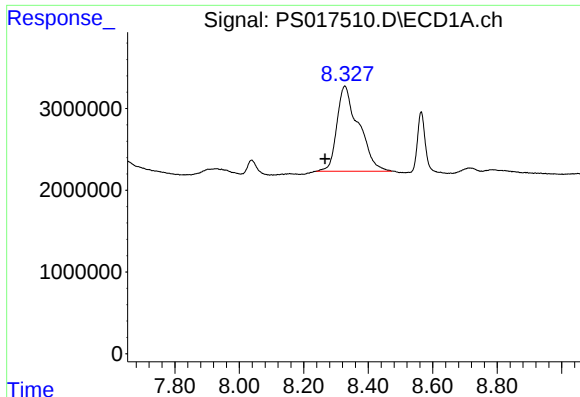

#9 2,4-D


R.T.: 8.327 min
Delta R.T.: 0.062 min
Response: 48886971
Conc: 26.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

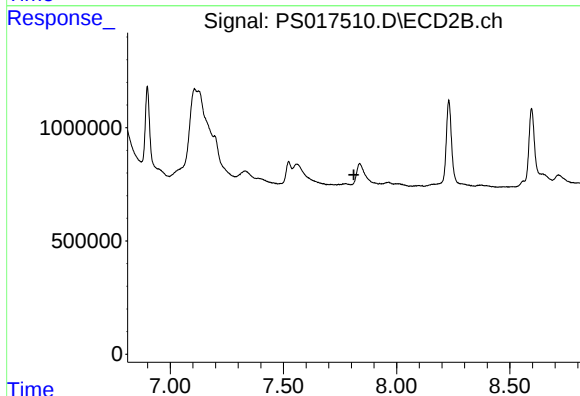


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.

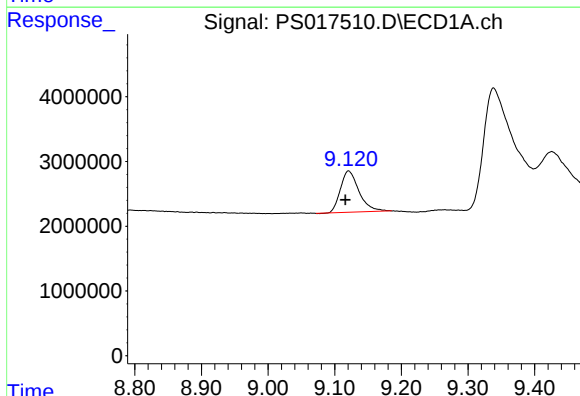


#11 2,4,5-TP (SILVEX)

R.T.: 9.121 min
Delta R.T.: 0.005 min
Response: 12330948
Conc: 1.48 ng/ml

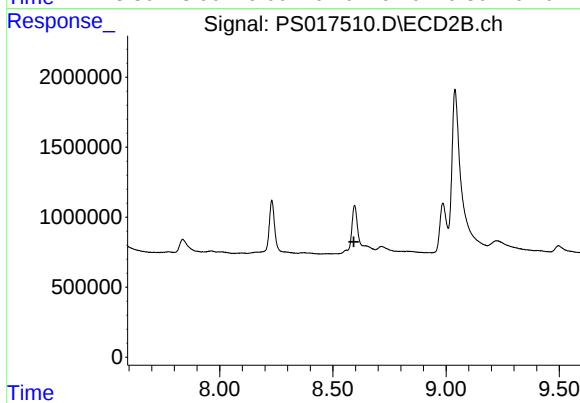

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.121 min
Response: 0
Conc: N.D.

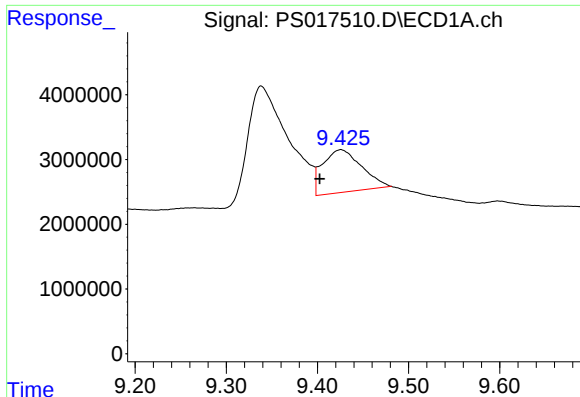

#12 2,4,5-T


R.T.: 9.426 min
Delta R.T.: 0.023 min
Response: 19618989
Conc: 2.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

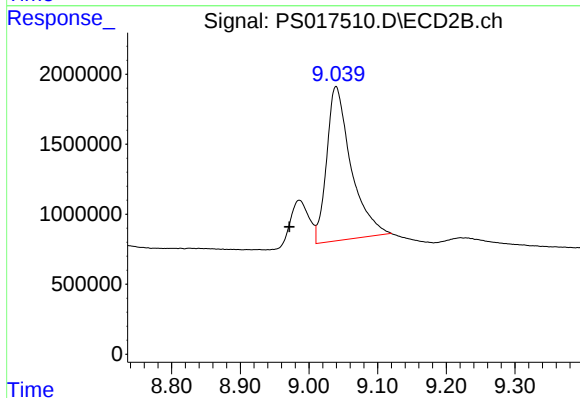


#12 2,4,5-T

R.T.: 9.040 min
Delta R.T.: 0.068 min
Response: 27181297
Conc: 8.17 ng/ml

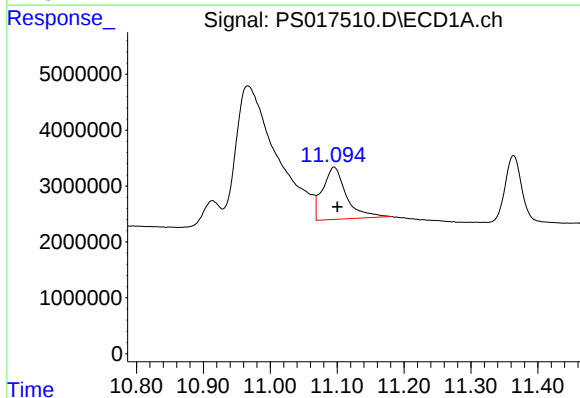


#14 DINOSEB

R.T.: 11.095 min
Delta R.T.: -0.005 min
Response: 23079868
Conc: 3.71 ng/ml

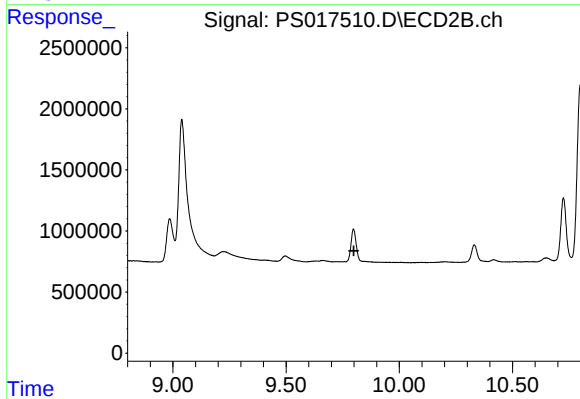

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.799 min
Response: 0
Conc: N.D.

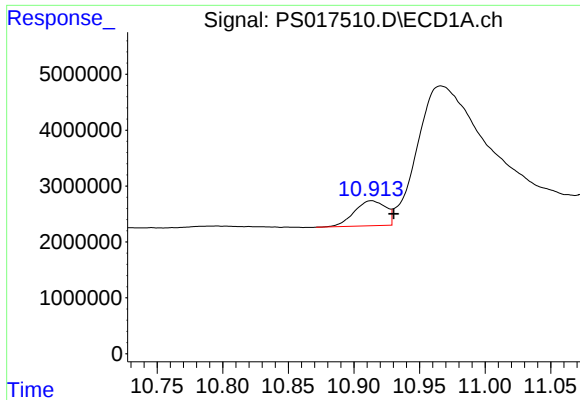

#15 Picloram


R.T.: 10.913 min
Delta R.T.: -0.017 min
Response: 7446679
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

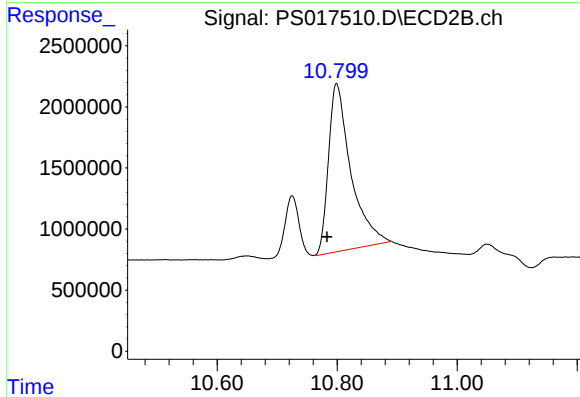


#15 Picloram

R.T.: 10.799 min
Delta R.T.: 0.016 min
Response: 35628537
Conc: 8.16 ng/ml

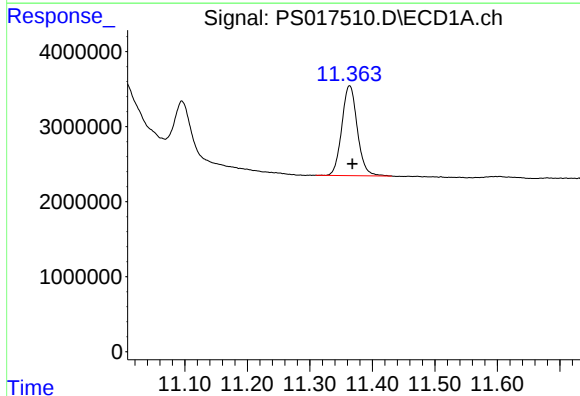

#16 DCPA

R.T.: 11.364 min
Delta R.T.: -0.005 min
Response: 20618972
Conc: 1.93 ng/ml

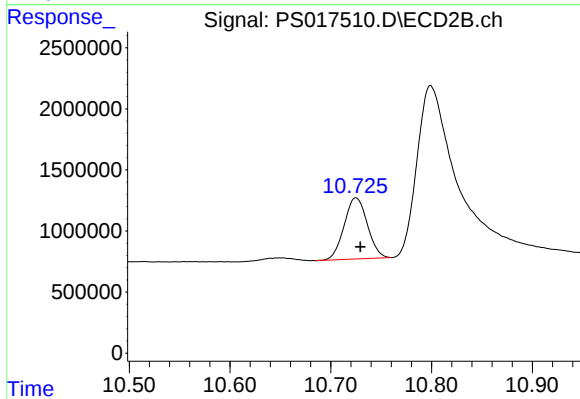

#16 DCPA

R.T.: 10.725 min
Delta R.T.: -0.004 min
Response: 7986941
Conc: 1.81 ng/ml