

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112421\  
 Data File : PS017524.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Nov 2021 01:28  
 Operator : AJ\MA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 25 02:43:43 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS111821.M  
 Quant Title : 8080.M  
 QLast Update : Fri Nov 19 21:46:29 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|-------|----------|---------|---------|---------|
| -----                       |              |        |       |          |         |         |         |
| System Monitoring Compounds |              |        |       |          |         |         |         |
| 4) S                        | 2,4-DCAA     | 7.148  | 6.737 | 711.7E6  | 290.5E6 | 452.654 | 490.282 |
| Target Compounds            |              |        |       |          |         |         |         |
| 5) T                        | DICAMBA      | 7.337  | 0.000 | 7367269  | 0       | 1.207   | N.D. #  |
| 9) T                        | 2,4-D        | 8.325f | 0.000 | 32551219 | 0       | 17.420  | N.D. #  |
| 10) T                       | Pentachlo... | 8.564  | 0.000 | 10393592 | 0       | <MDL    | N.D. #  |
| 11) T                       | 2,4,5-TP ... | 9.118  | 0.000 | 5709547  | 0       | <MDL    | N.D. #  |
| 12) T                       | 2,4,5-T      | 9.356f | 0.000 | 4600254  | 0       | <MDL    | N.D. #  |
| 14) T                       | DINSEB       | 11.094 | 0.000 | 8309114  | 0       | 1.334   | N.D. #  |
| 15) T                       | Picloram     | 10.911 | 0.000 | 7069280  | 0       | <MDL    | N.D. #  |
| 16) T                       | DCPA         | 11.363 | 0.000 | 8045729  | 0       | <MDL    | N.D. #  |
| -----                       |              |        |       |          |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112421\  
Data File : PS017524.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Nov 2021 01:28  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 25 02:43:43 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS111821.M  
Quant Title : 8080.M  
QLast Update : Fri Nov 19 21:46:29 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

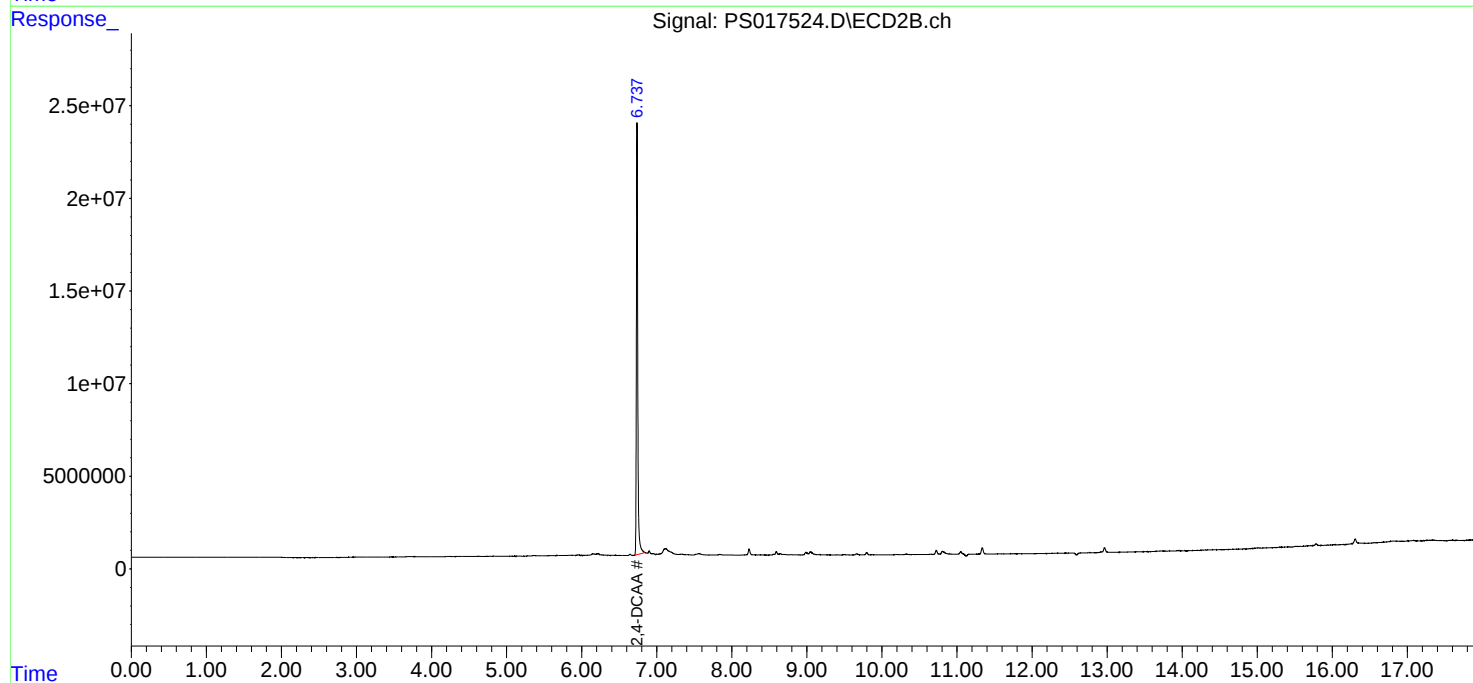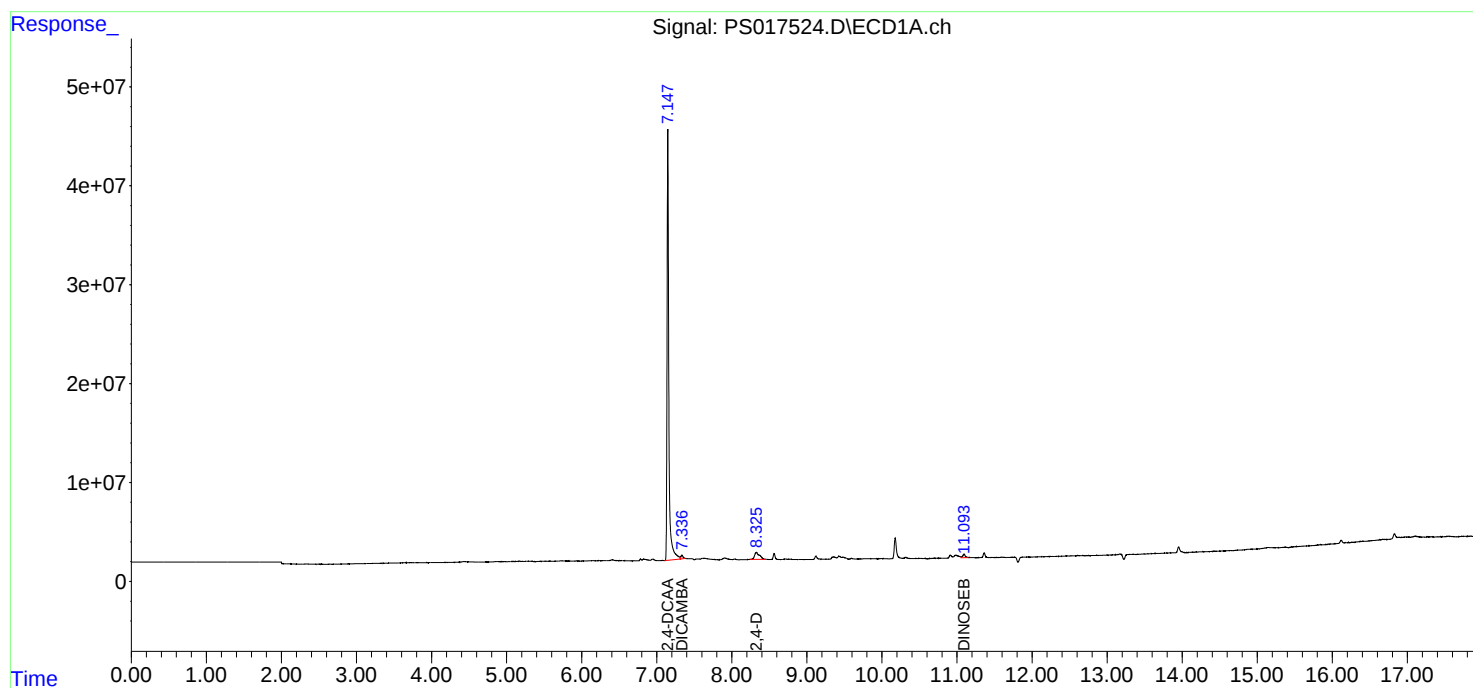


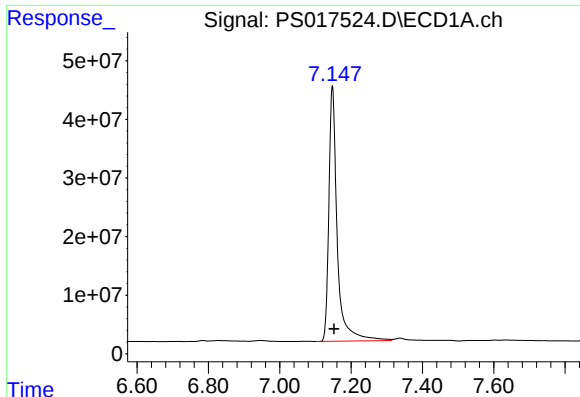

#4 2,4-DCAA


R.T.: 7.148 min  
Delta R.T.: -0.005 min  
Response: 711660475  
Conc: 452.65 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

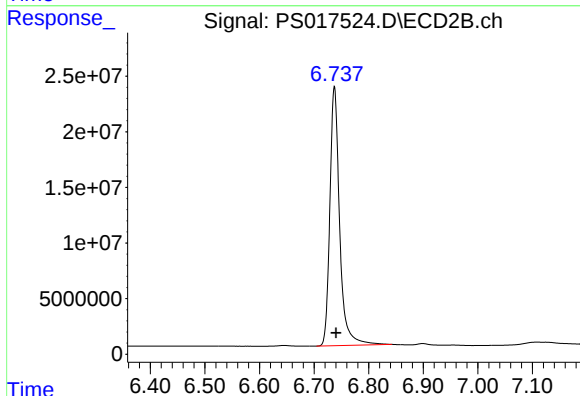


#4 2,4-DCAA

R.T.: 6.737 min  
Delta R.T.: -0.003 min  
Response: 290530497  
Conc: 490.28 ng/ml

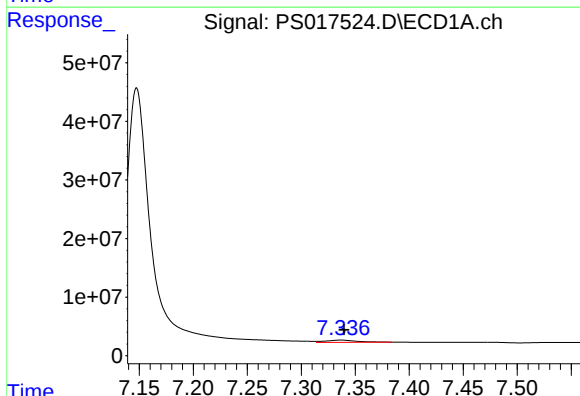


#5 DICAMBA

R.T.: 7.337 min  
Delta R.T.: -0.003 min  
Response: 7367269  
Conc: 1.21 ng/ml

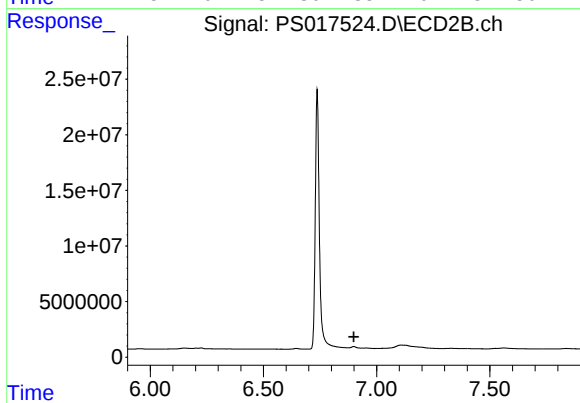

#5 DICAMBA


R.T.: 0.000 min  
Exp R.T. : 6.900 min  
Response: 0  
Conc: N.D.

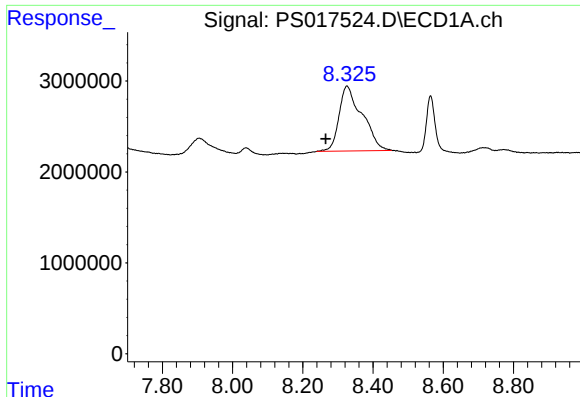

#9 2,4-D


R.T.: 8.325 min  
Delta R.T.: 0.060 min  
Response: 32551219  
Conc: 17.42 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

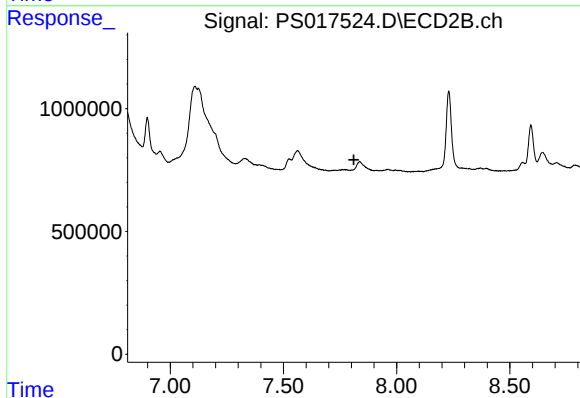


#9 2,4-D

R.T.: 0.000 min  
Exp R.T. : 7.811 min  
Response: 0  
Conc: N.D.

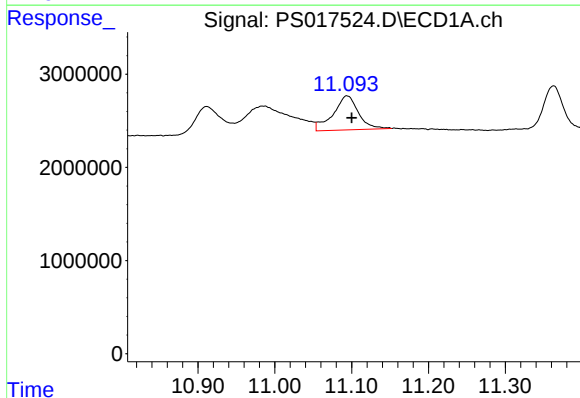

#14 DINOSEB

R.T.: 11.094 min  
Delta R.T.: -0.006 min  
Response: 8309114  
Conc: 1.33 ng/ml

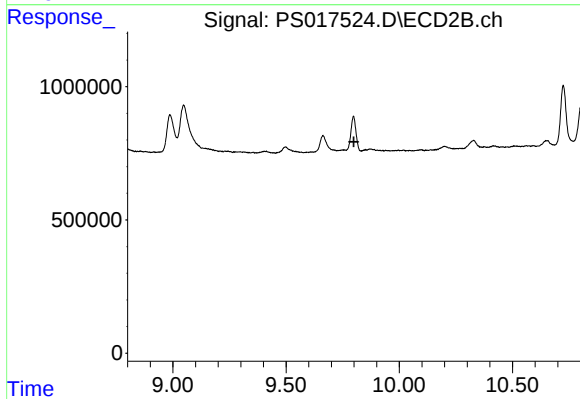

#14 DINOSEB

R.T.: 0.000 min  
Exp R.T. : 9.799 min  
Response: 0  
Conc: N.D.