

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112421\
 Data File : PS017504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2021 12:37
 Operator : AJ\MA
 Sample : M4801-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SITE-1-DRILL-CUTTINGS-20211119

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
 Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 00:34:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.146	6.736	609.1E6	242.6E6	387.434m	409.339

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112421\
Data File : PS017504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2021 12:37
Operator : AJ\MA
Sample : M4801-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SITE-1-DRILL-CUTTINGS-20211119


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 00:34:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

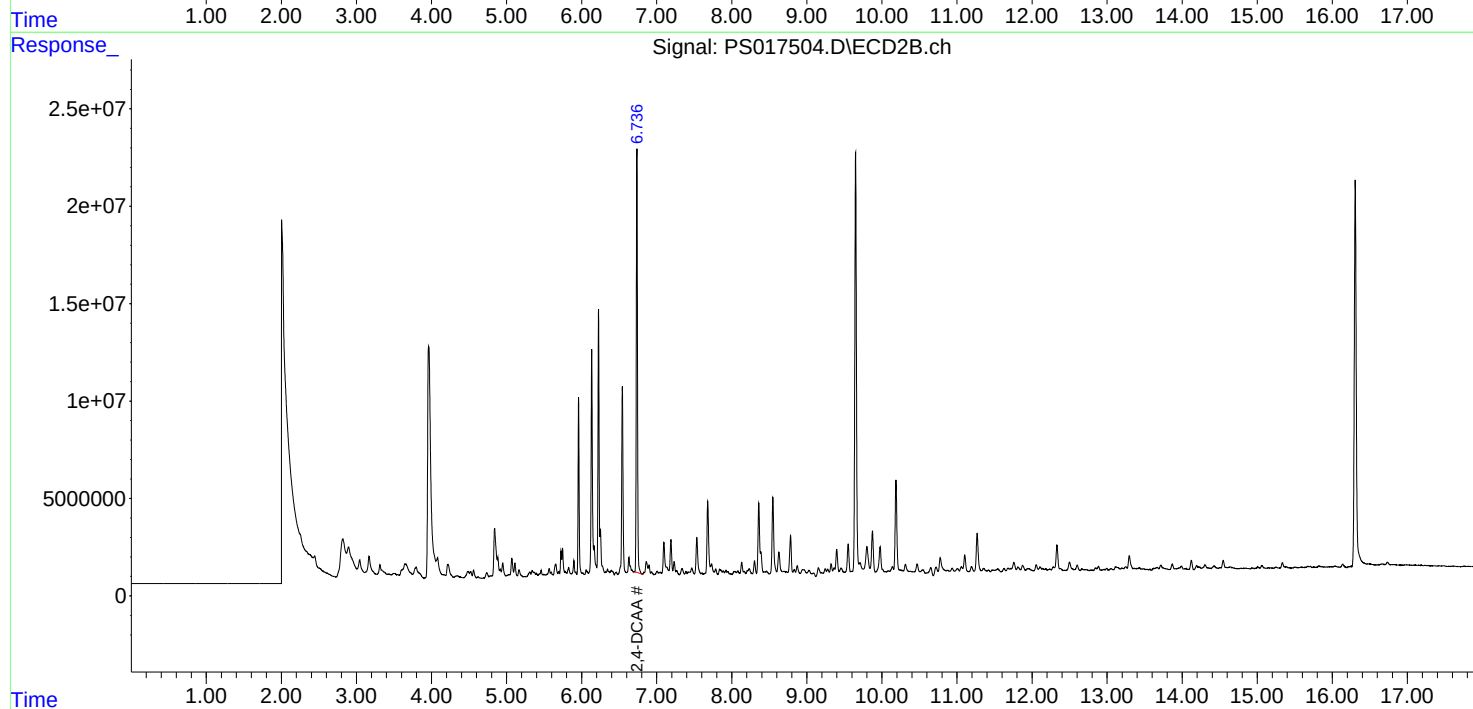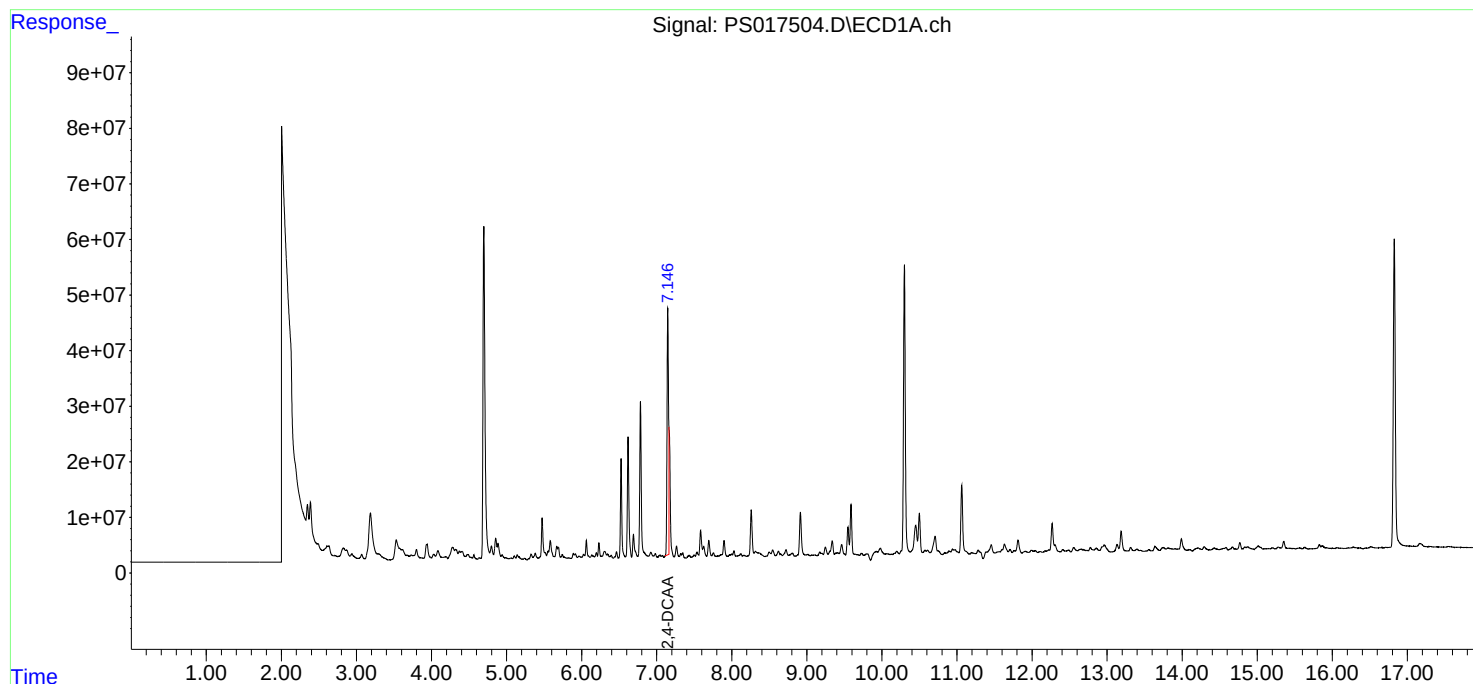

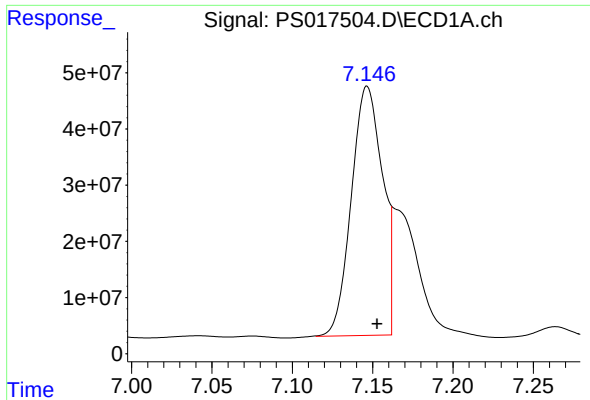


#4 2,4-DCAA

R.T.: 7.146 min
Delta R.T.: -0.007 min
Response: 609121019
Conc: 387.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
SITE-1-DRILL-CUTTINGS-20211119

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

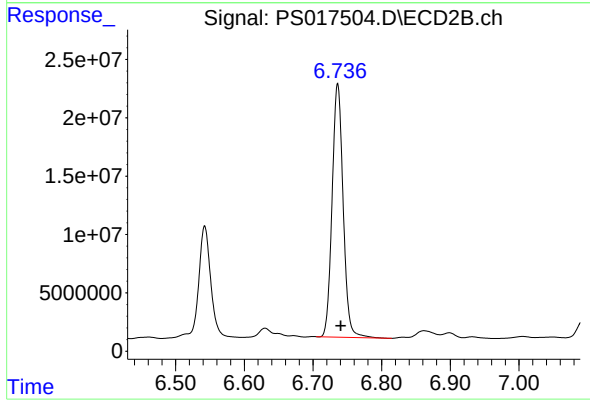

#4 2,4-DCAA

R.T.: 6.736 min
Delta R.T.: -0.004 min
Response: 242565083
Conc: 409.34 ng/ml