

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112425\
 Data File : PS032523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2025 19:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 14:18:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.279	7.621	1612.9E6	1738.0E6	355.952	476.744 #
Target Compounds							
2) T	3,5-DICHL...	6.444	6.612f	489967	7516987	<MDL	1.251 #
6) T	MCP	7.601f	0.000	753987	0	<MDL	N.D. #
7) T	MCPA	7.789	8.111f	6237524	1661220	<MDL	<MDL #
8) T	DICHLORPROP	8.171	0.000	271500	0	<MDL	N.D. #
9) T	2,4-D	0.000	8.837f	0	31935022	N.D.	6.088
10) T	Pentachlo...	8.704	9.325f	-349135	2737555	N.D.	<MDL
11) T	2,4,5-TP ...	9.292	0.000	135312	0	<MDL	N.D. #
12) T	2,4,5-T	9.541f	10.193	31158907	7235211	1.307	<MDL #
13) T	2,4-DB	10.163	10.747	1259401	3058094	<MDL	<MDL #
14) T	DINOSEB	11.353	11.107	1540590	3136777	<MDL	<MDL #
15) T	Picloram	11.185	0.000	1041152	0	<MDL	N.D. #
16) T	DCPA	11.646	0.000	810536	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112425\
Data File : PS032523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2025 19:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 14:18:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

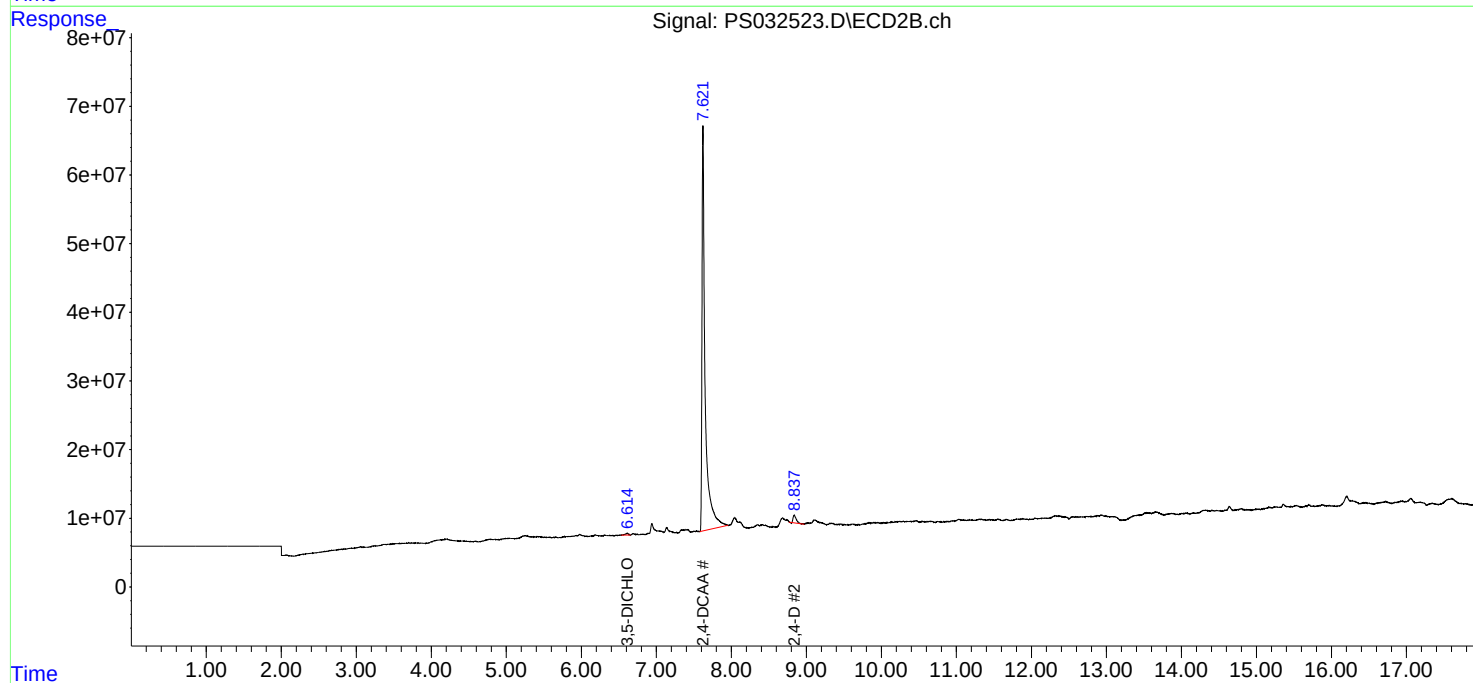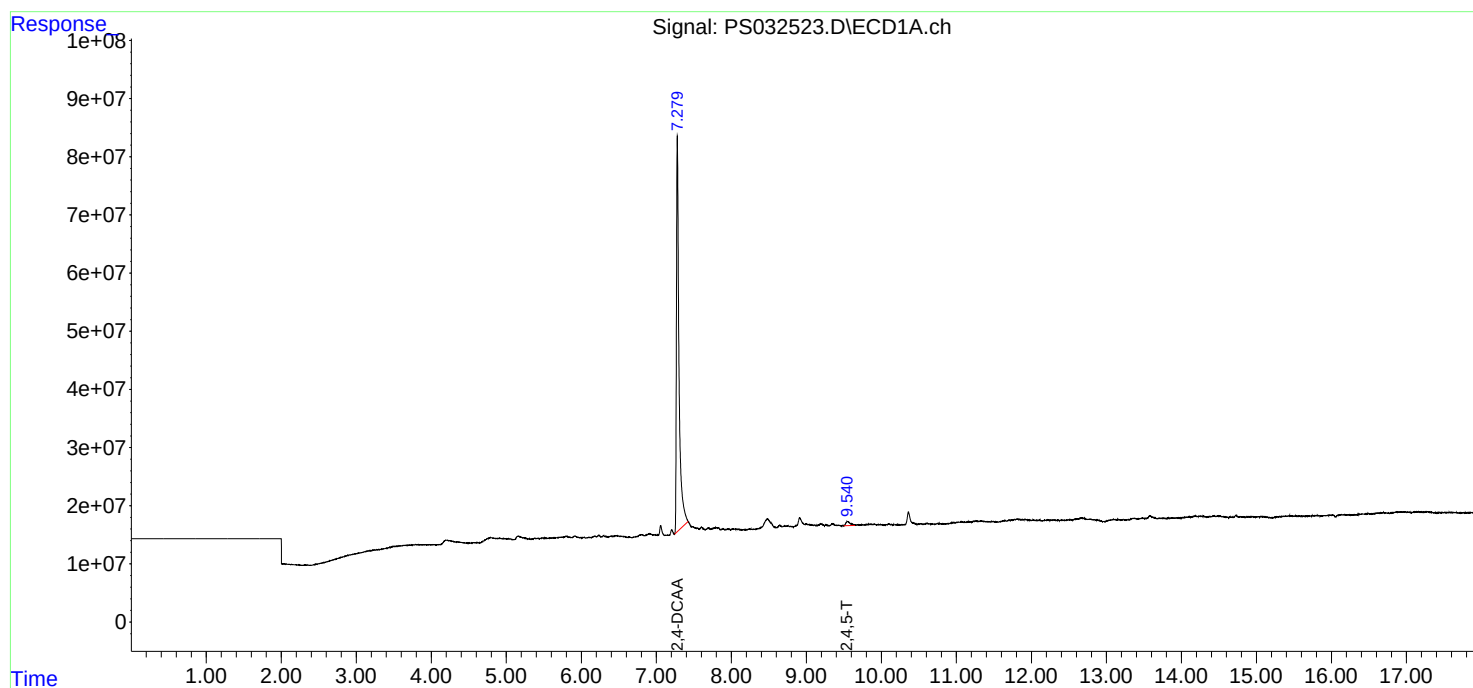


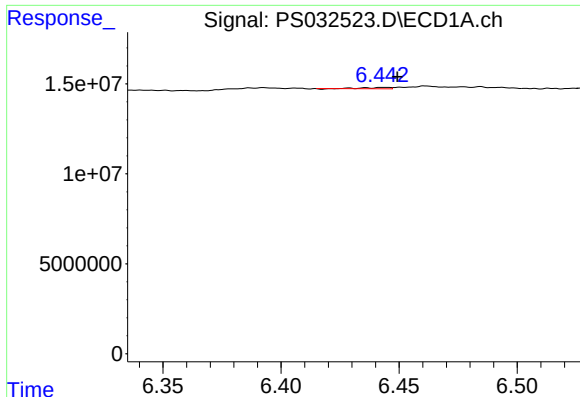

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.444 min
Delta R.T.: -0.006 min
Response: 489967
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

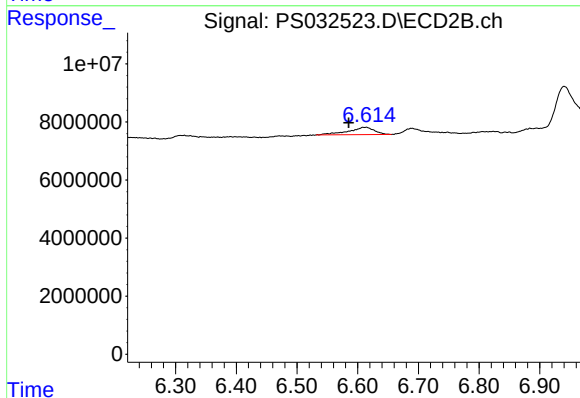


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.612 min
Delta R.T.: 0.027 min
Response: 7516987
Conc: 1.25 ng/ml

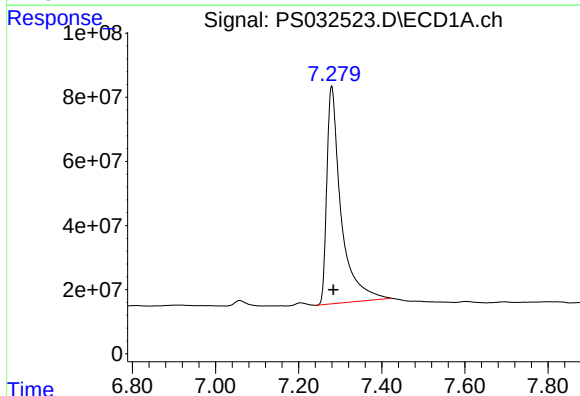


#4 2,4-DCAA

R.T.: 7.279 min
Delta R.T.: -0.004 min
Response: 1612914943
Conc: 355.95 ng/ml

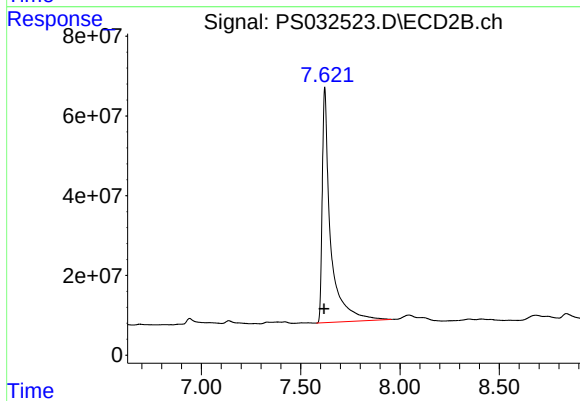

#4 2,4-DCAA


R.T.: 7.621 min
Delta R.T.: 0.004 min
Response: 1737968291
Conc: 476.74 ng/ml

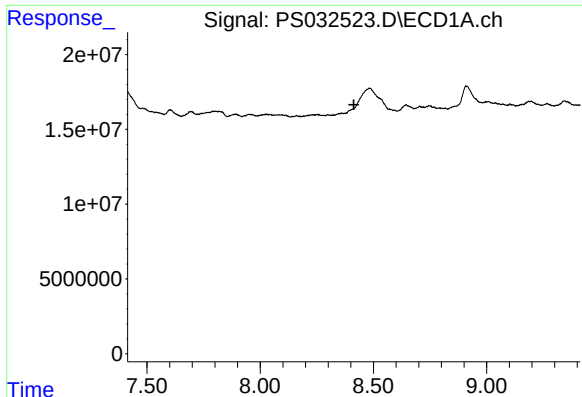

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

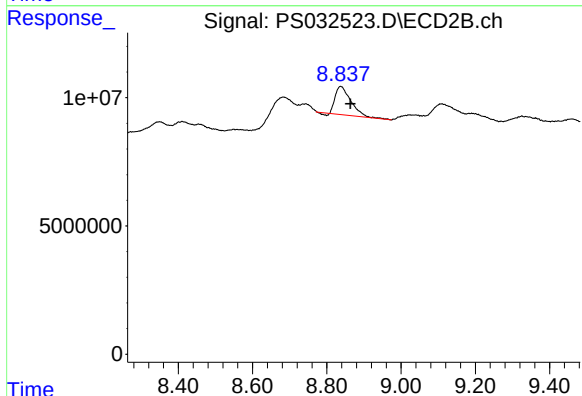


#9 2,4-D

R.T.: 8.837 min
Delta R.T.: -0.026 min
Response: 31935022
Conc: 6.09 ng/ml

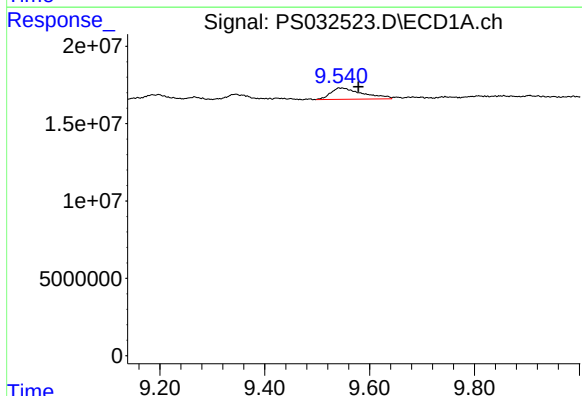

#12 2,4,5-T

R.T.: 9.541 min
Delta R.T.: -0.037 min
Response: 31158907
Conc: 1.31 ng/ml

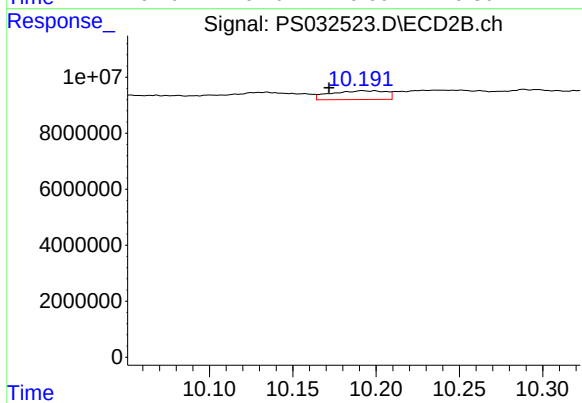

#12 2,4,5-T

R.T.: 10.193 min
Delta R.T.: 0.022 min
Response: 7235211
Conc: N.D.