

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112425\  
 Data File : PS032526.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 24 Nov 2025 21:25  
 Operator : AR\AJ  
 Sample : Q3710-03  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 COMPRESSOR-EXCAVATION

Manual Integrations  
 APPROVED

Reviewed By :Abdul Mirza 11/26/2025  
 Supervised By :mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 26 01:12:09 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110325.M  
 Quant Title : 8080.M  
 QLast Update : Tue Nov 04 04:59:50 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml | ng/ml  |
|-----------------------------|-------|-------|----------|----------|-------|--------|
| -----                       |       |       |          |          |       |        |
| System Monitoring Compounds |       |       |          |          |       |        |
| 4) S 2,4-DCAA               | 7.286 | 7.634 | 29713977 | 26364201 | 6.558 | 7.232m |

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112425\  
Data File : PS032526.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 24 Nov 2025 21:25  
Operator : AR\AJ  
Sample : Q3710-03  
Misc :  
ALS Vial : 15 Sample Multiplier: 1



Instrument :  
ECD\_S  
ClientSampleId :  
COMPRESSOR-EXCAVATION


Manual Integrations  
APPROVED

Reviewed By : Abdul Mirza 11/26/2025  
Supervised By : mohammad ahmed 11/27/2025

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 26 01:12:09 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110325.M  
Quant Title : 8080.M  
QLast Update : Tue Nov 04 04:59:50 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

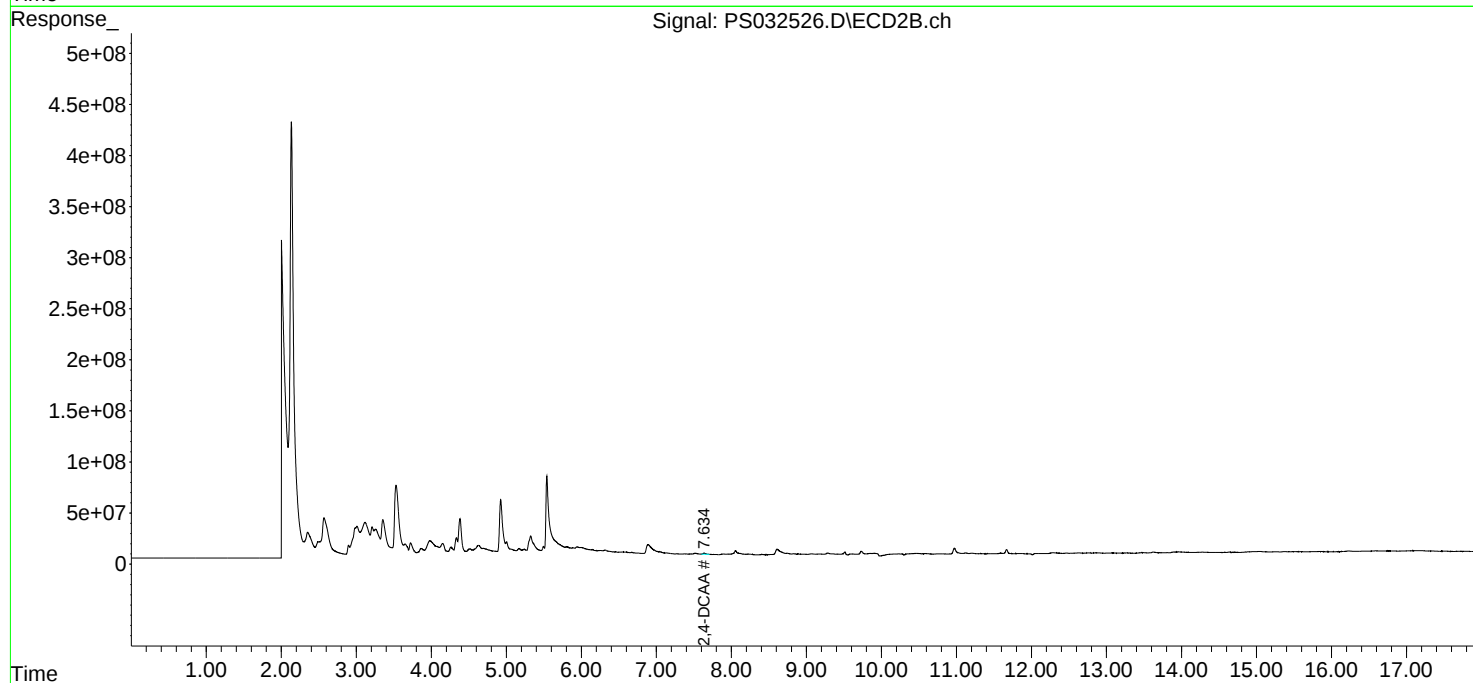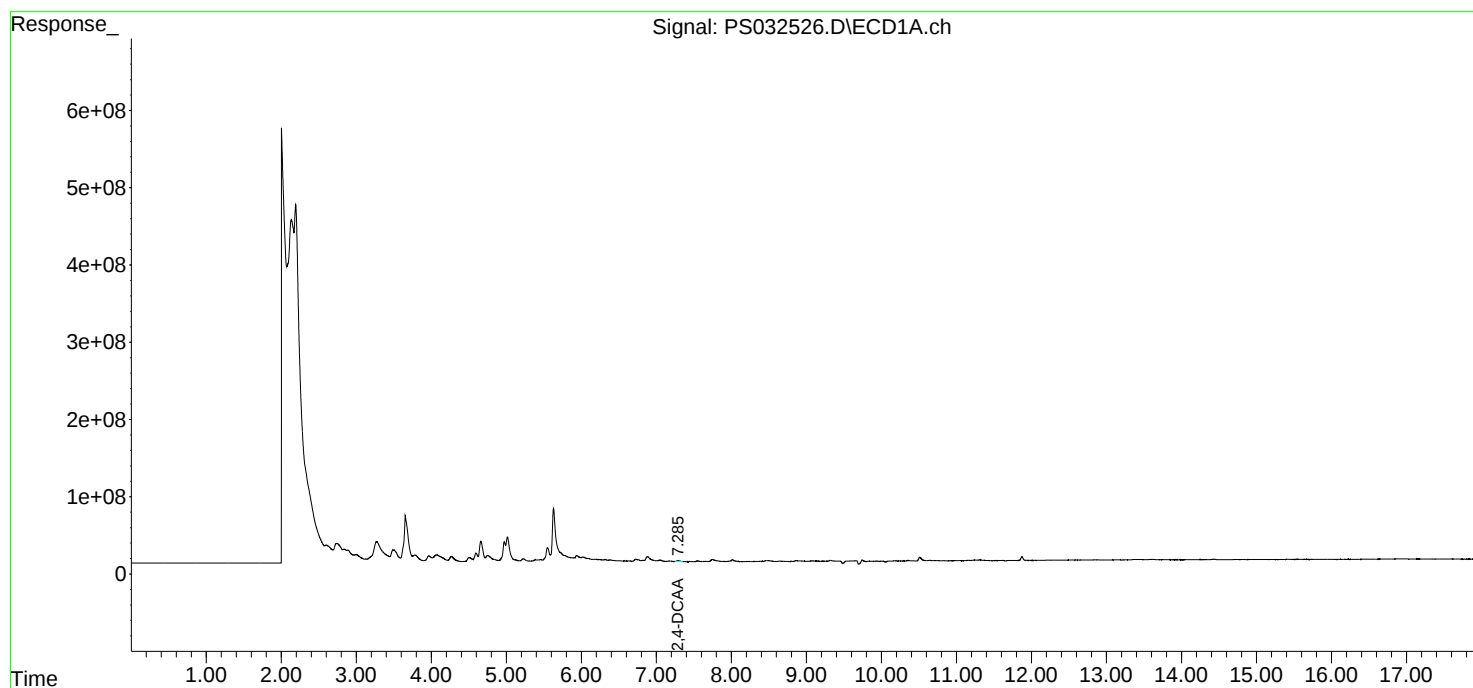

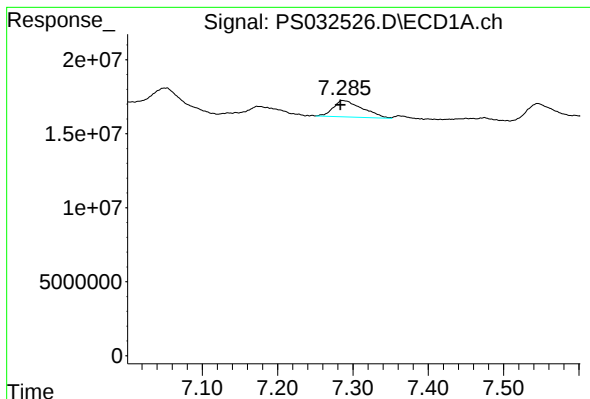


#4 2,4-DCAA

R.T.: 7.286 min  
Delta R.T.: 0.003 min  
Response: 29713977  
Conc: 6.56 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
COMPRESSOR-EXCAVATION

Manual Integrations  
APPROVED

Reviewed By :Abdul Mirza 11/26/2025  
Supervised By :mohammad ahmed 11/27/2025

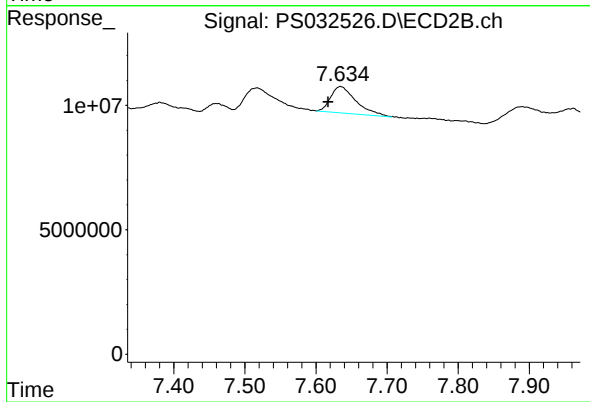

#4 2,4-DCAA

R.T.: 7.634 min  
Delta R.T.: 0.017 min  
Response: 26364201  
Conc: 7.23 ng/ml m