

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112519\
 Data File : PS007821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2019 10:27
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 10:46:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.434	5.157	634.2E6	335.9E6	460.485	478.100
Target Compounds							
7) T	MCPA	0.000	5.468	0	43348378	N.D.	14.422
9) T	2,4-D	6.482	0.000	68780493	0	49.040	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112519\
Data File : PS007821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2019 10:27
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 10:46:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

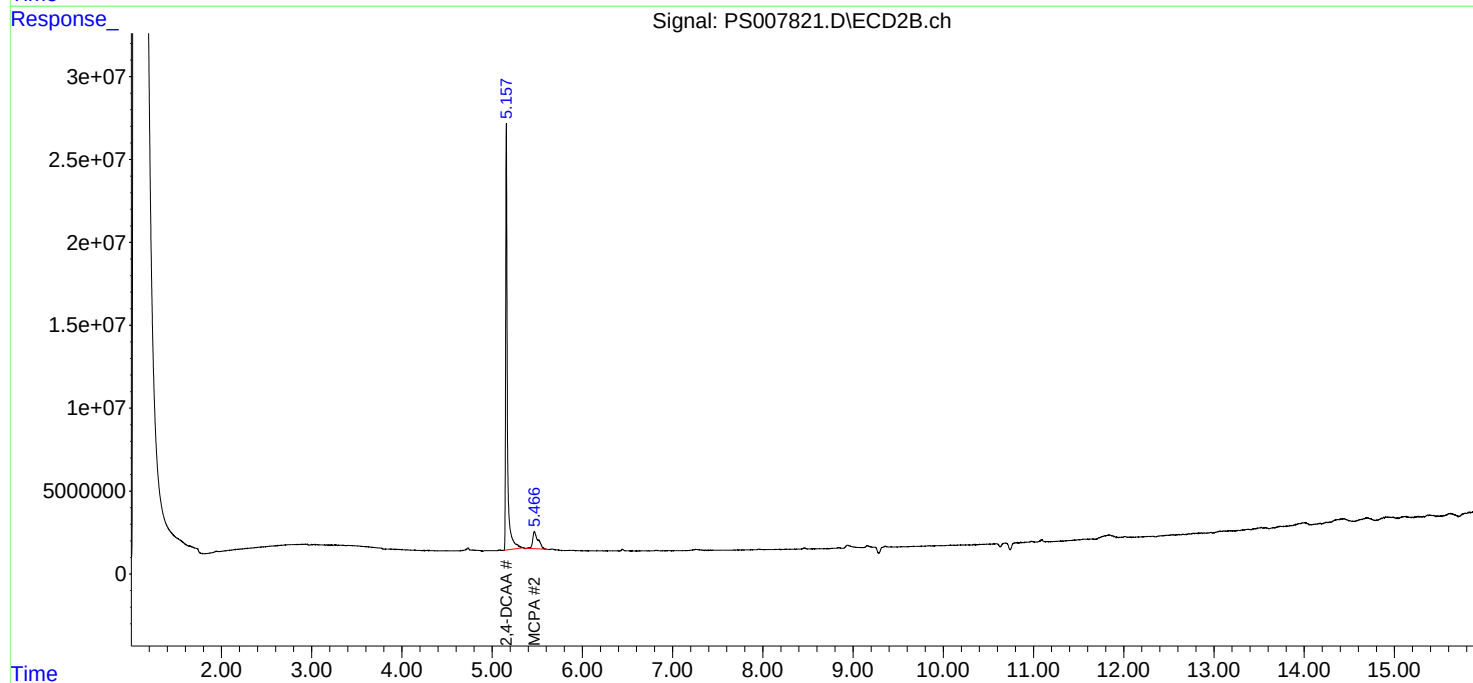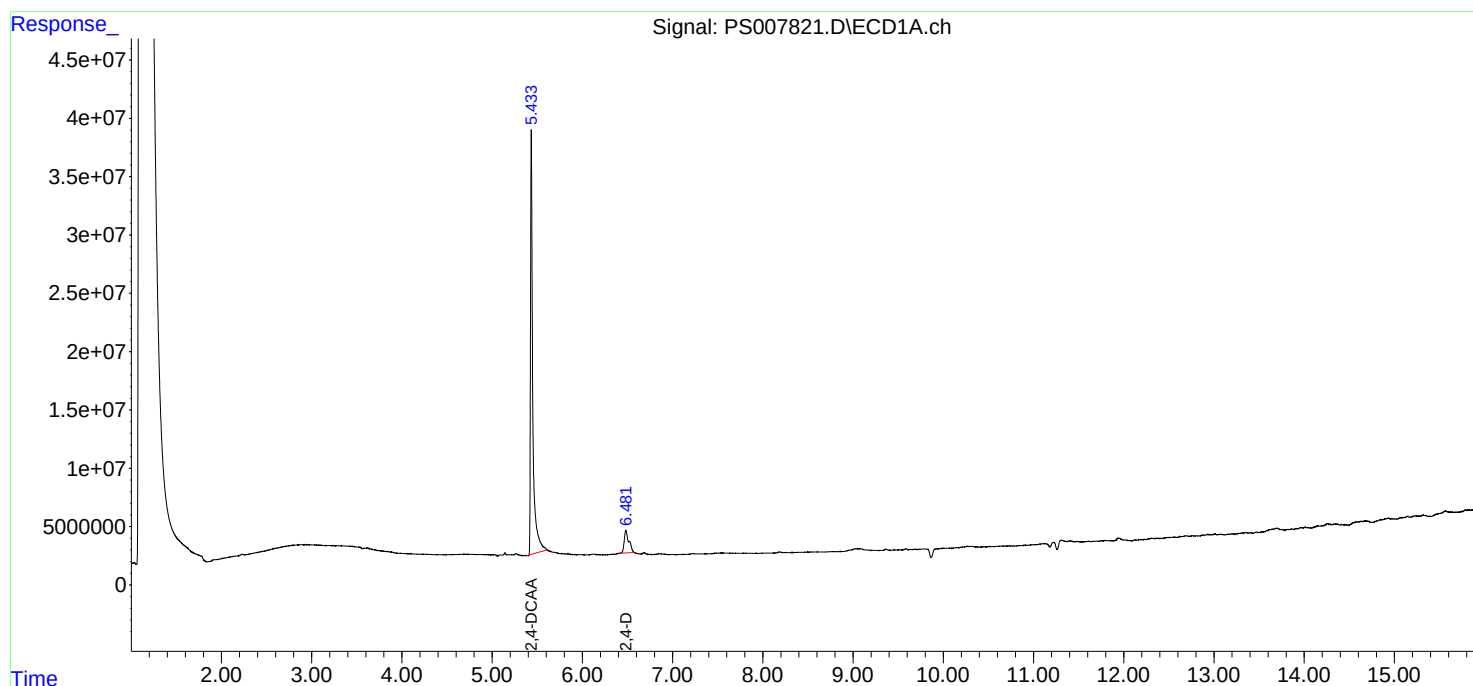


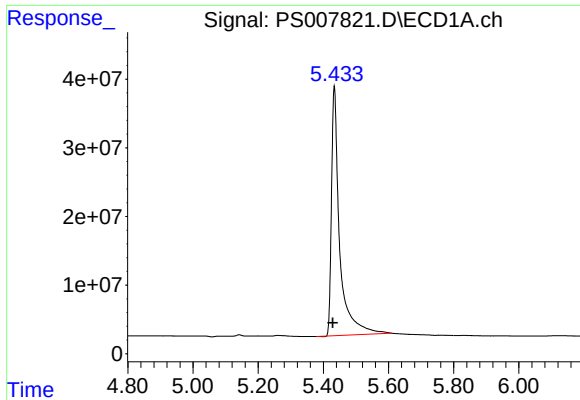

#4 2,4-DCAA


R.T.: 5.434 min
Delta R.T.: 0.005 min
Response: 634172847
Conc: 460.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

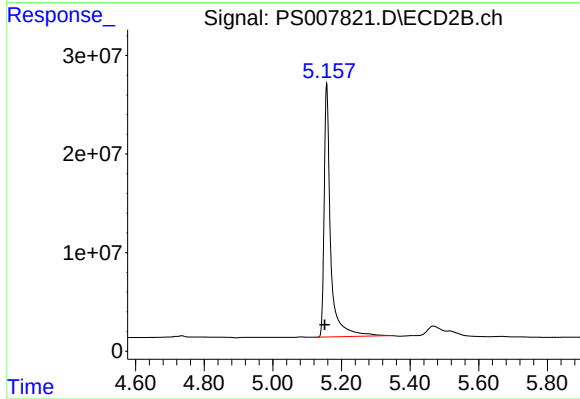


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: 0.006 min
Response: 335895622
Conc: 478.10 ng/ml

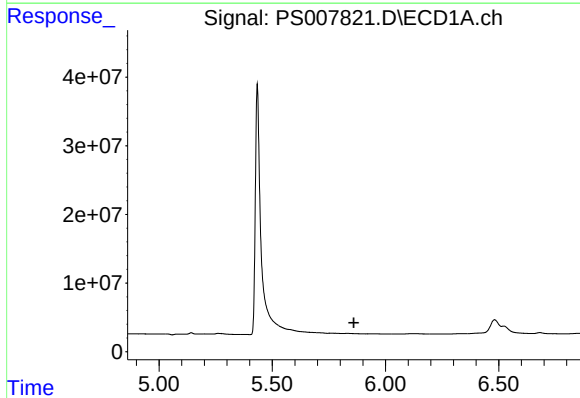


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

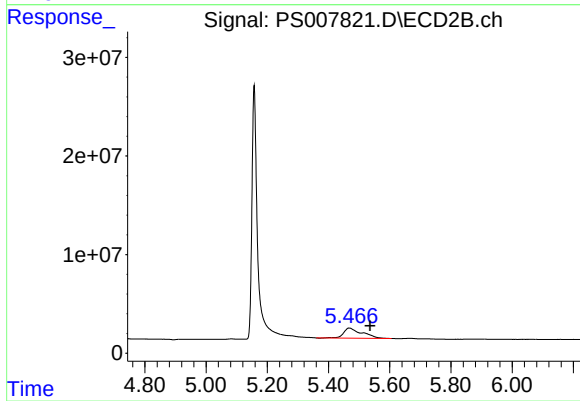

#7 MCPA


R.T.: 5.468 min
Delta R.T.: -0.068 min
Response: 43348378
Conc: 14.42 ug/ml

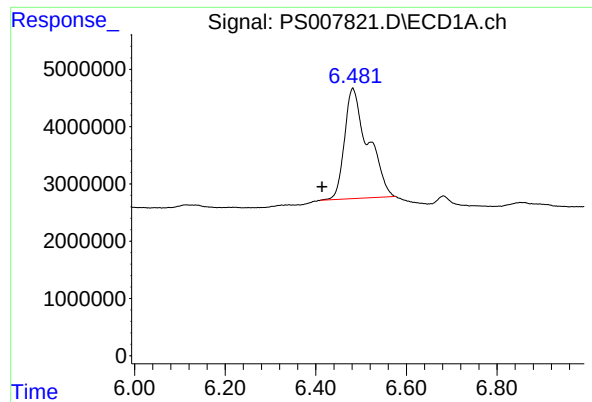

#9 2,4-D

R.T.: 6.482 min
Delta R.T.: 0.067 min
Response: 68780493
Conc: 49.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

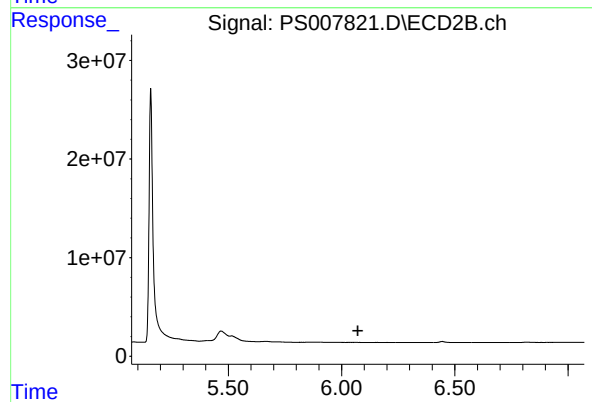

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.