

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112519\
 Data File : PS007820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2019 10:05
 Operator : SM\AJ
 Sample : K5973-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DUCT-BANK-2

Manual Integrations
 APPROVED

Ankita
 11/26/2019 1:19:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 10:29:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.433	5.154	90786197	41824122	65.922	59.531m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112519\
Data File : PS007820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2019 10:05
Operator : SM\AJ
Sample : K5973-04
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-2


Manual Integrations
APPROVED

Ankita
11/26/2019 1:19:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 10:29:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

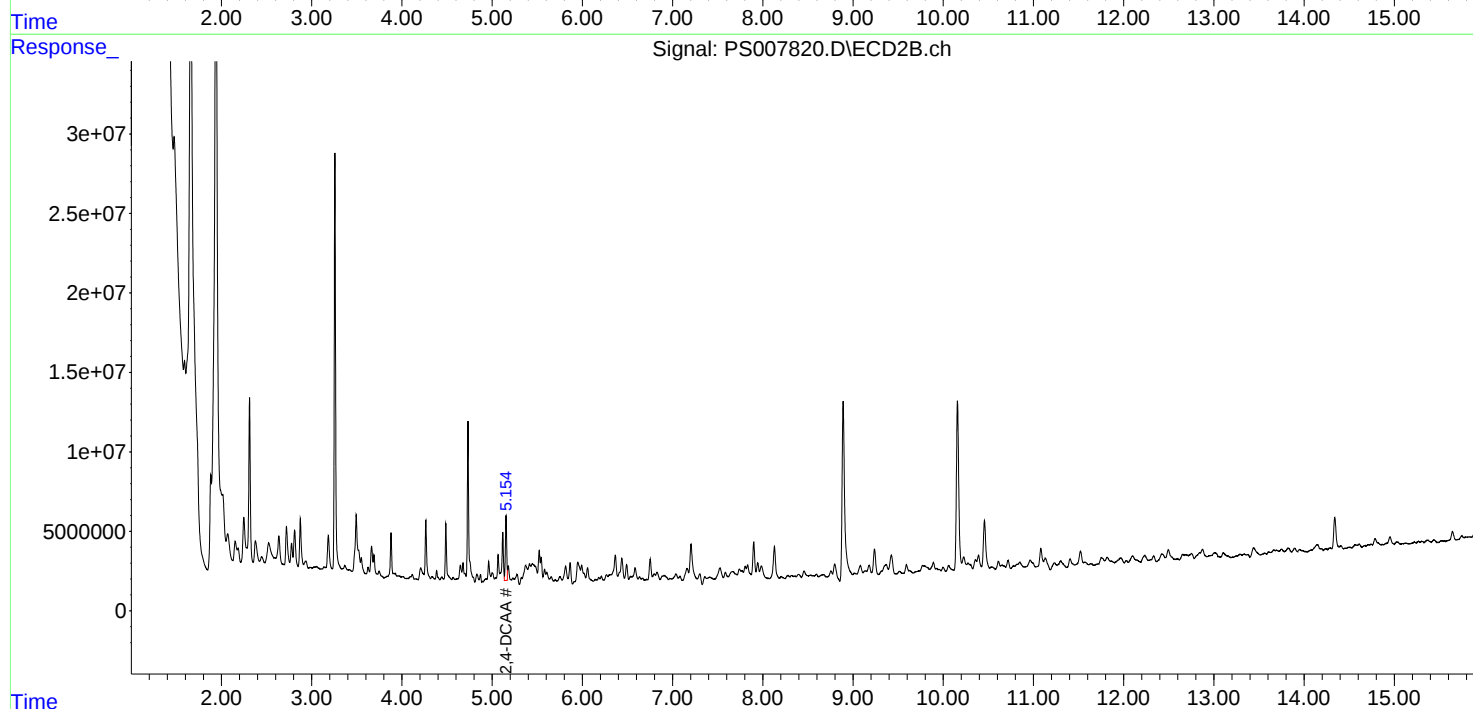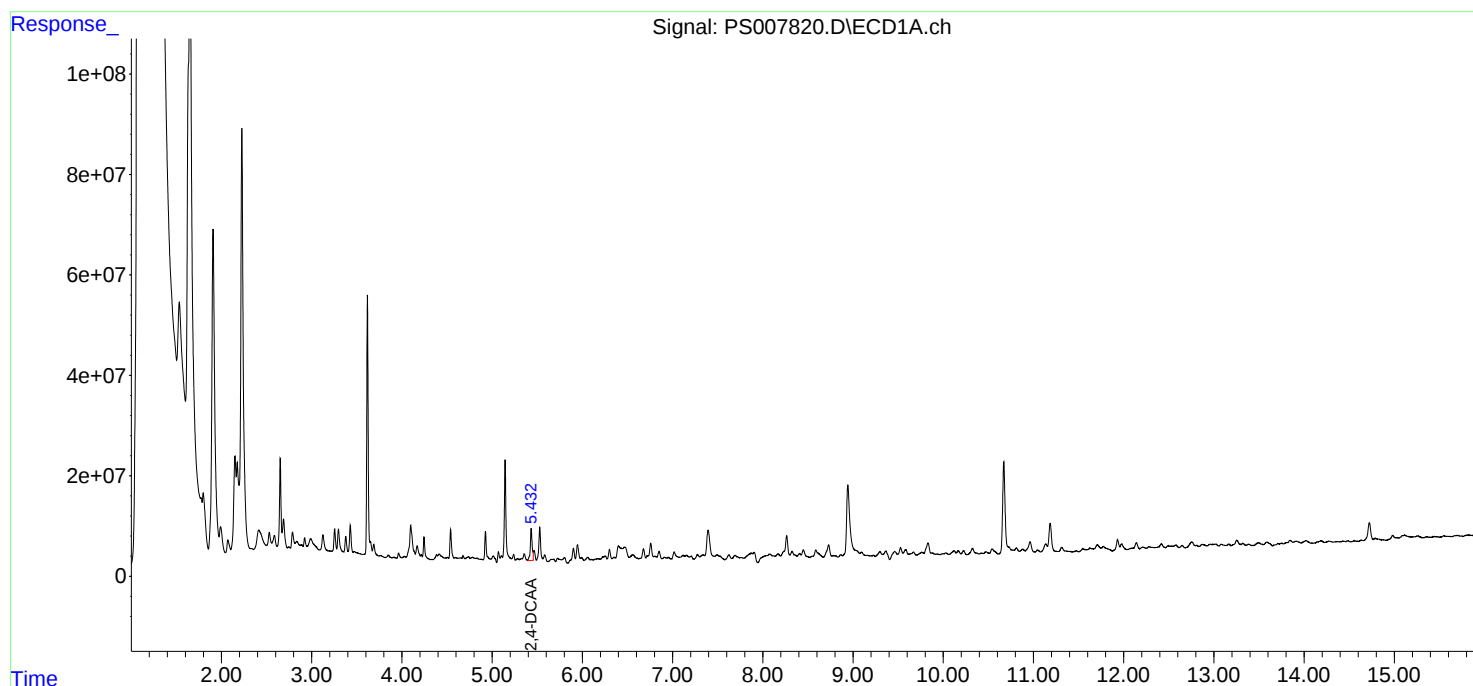

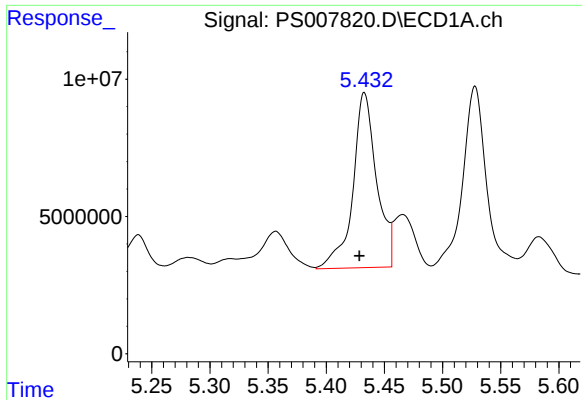


#4 2,4-DCAA

R.T.: 5.433 min
Delta R.T.: 0.004 min
Response: 90786197
Conc: 65.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUCT-BANK-2

Manual Integrations
APPROVED

Ankita
11/26/2019 1:19:40 PM

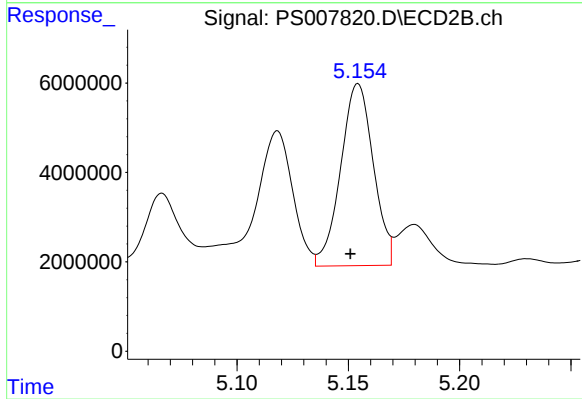

#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.003 min
Response: 41824122
Conc: 59.53 ng/ml m