

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112520\
 Data File : PS013323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 15:32
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 16:12:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.908	390.0E6	200.3E6	436.327	514.746
Target Compounds							
10) T	Pentachlo...	8.634	8.424	7190994	4257997	<MDL	<MDL #
12) T	2,4,5-T	9.397f	0.000	18794300	0	3.551	N.D. #
15) T	Picloram	11.028	11.015	64384460	44632374	9.791	12.365 #
16) T	DCPA	11.441	10.928	7174379	4255291	1.105	1.417 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112520\
Data File : PS013323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 15:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 16:12:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

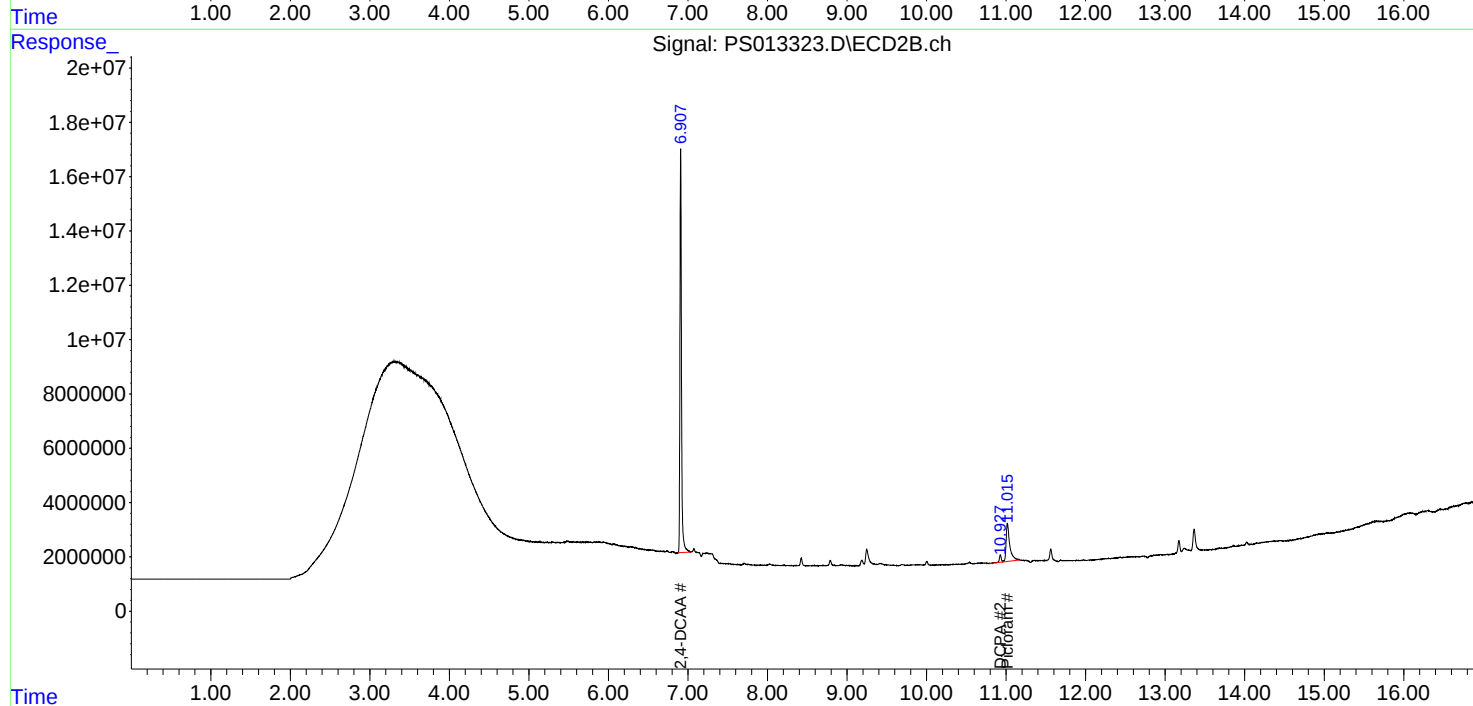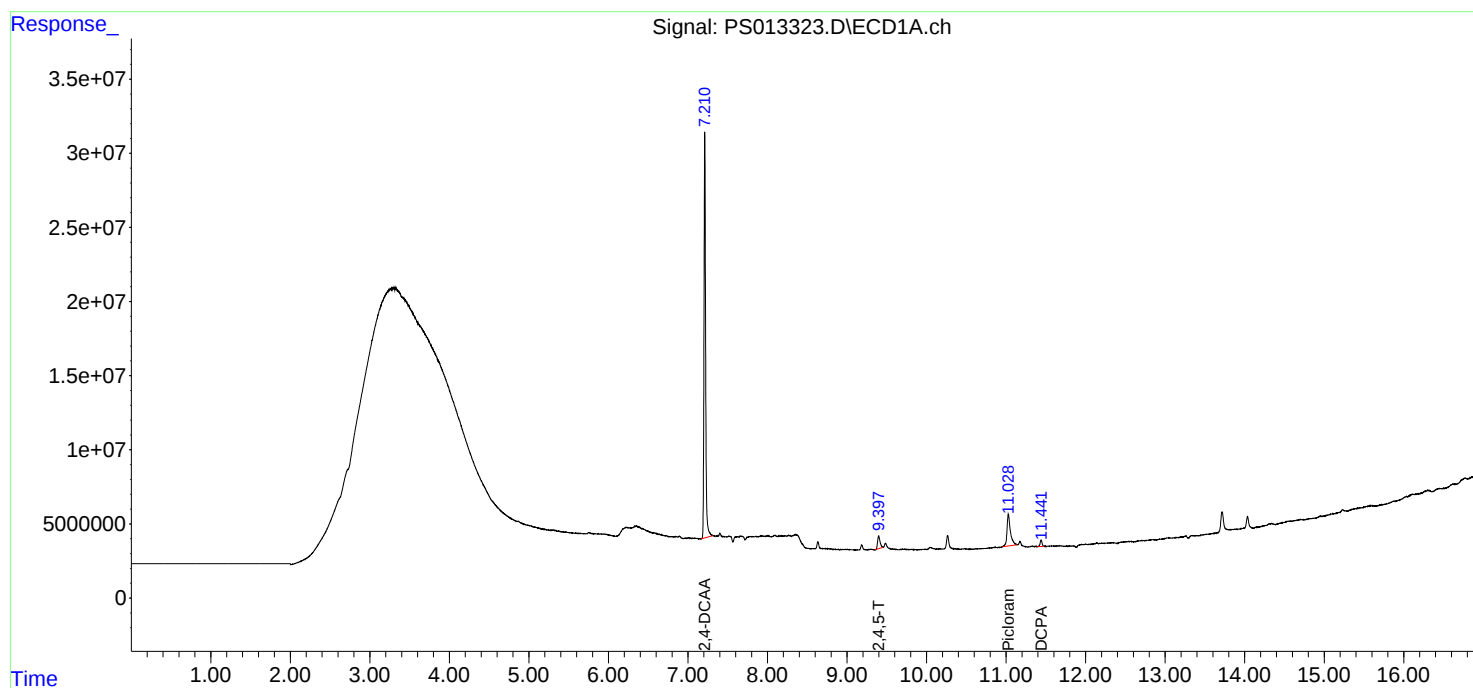


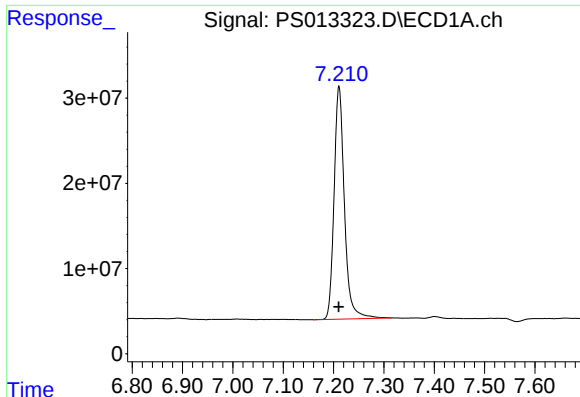

#4 2,4-DCAA


R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 390045459
Conc: 436.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

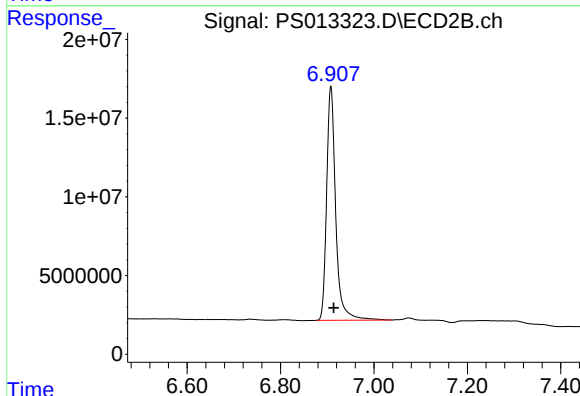


#4 2,4-DCAA

R.T.: 6.908 min
Delta R.T.: -0.006 min
Response: 200282088
Conc: 514.75 ng/ml

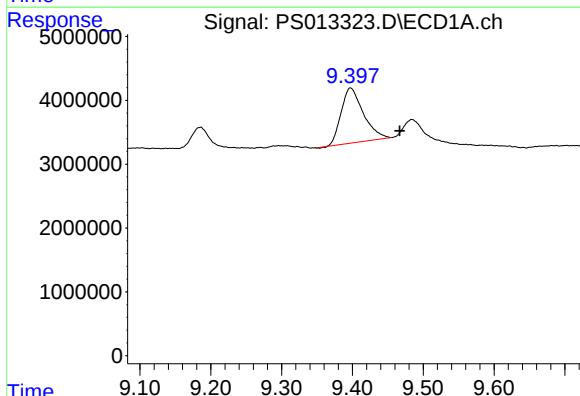


#12 2,4,5-T

R.T.: 9.397 min
Delta R.T.: -0.069 min
Response: 18794300
Conc: 3.55 ng/ml

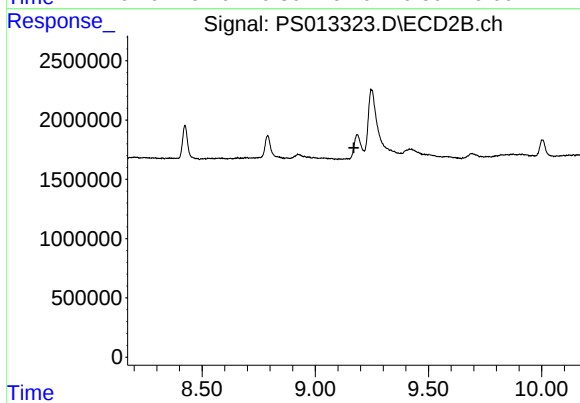

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.170 min
Response: 0
Conc: N.D.

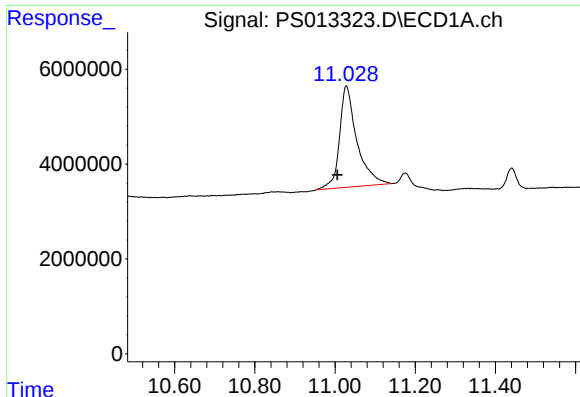

#15 Picloram


R.T.: 11.028 min
Delta R.T.: 0.022 min
Response: 64384460
Conc: 9.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

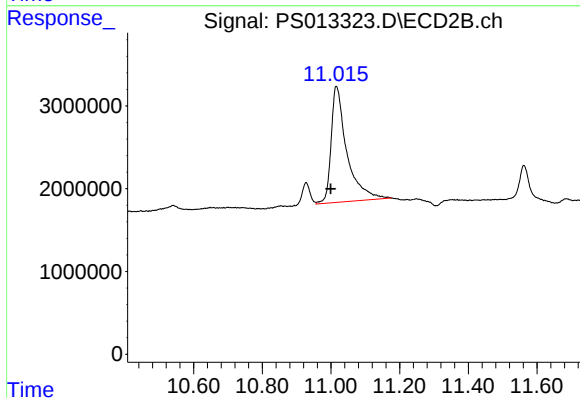


#15 Picloram

R.T.: 11.015 min
Delta R.T.: 0.016 min
Response: 44632374
Conc: 12.37 ng/ml

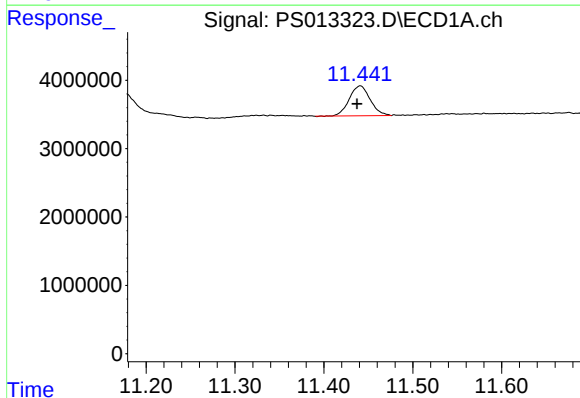

#16 DCPA

R.T.: 11.441 min
Delta R.T.: 0.003 min
Response: 7174379
Conc: 1.10 ng/ml

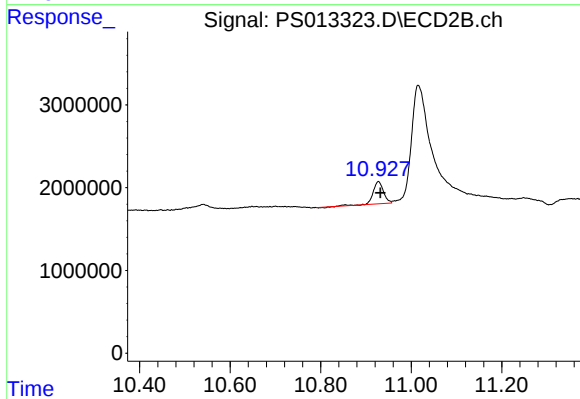

#16 DCPA

R.T.: 10.928 min
Delta R.T.: -0.004 min
Response: 4255291
Conc: 1.42 ng/ml