

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112524\
 Data File : PS028612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 09:26
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 23:46:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.668f	0.000	13107368	0	3.902	N.D.	#
2) T	3,5-DICHL...	6.421	0.000	388595	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.013f	0.000	4349552	0	2.561	N.D.	#
5) T	DICAMBA	0.000	7.923	0	3281287	N.D.	<MDL	
6) T	MCP	7.655f	0.000	8486259	0	1.206	N.D.	#
7) T	MCPA	7.765	8.251f	437028	9862501	<MDL	1.592	#
8) T	DICHLORPROP	0.000	8.694f	0	1160083	N.D.	<MDL	
11) T	2,4,5-TP ...	9.296f	9.894	3888171	17928191	<MDL	2.125	#
12) T	2,4,5-T	9.536	10.290f	1568870	8019978	<MDL	<MDL	#
13) T	2,4-DB	10.099	0.000	1147372	0	<MDL	N.D.	#
14) T	DINOSEB	11.309	0.000	1207297	0	<MDL	N.D.	#
15) T	Picloram	11.125	12.339	26367511	11627798	<MDL	1.027	#
16) T	DCPA	11.648	12.339f	793593	11627798	<MDL	1.199	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112524\
Data File : PS028612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 09:26
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 23:46:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

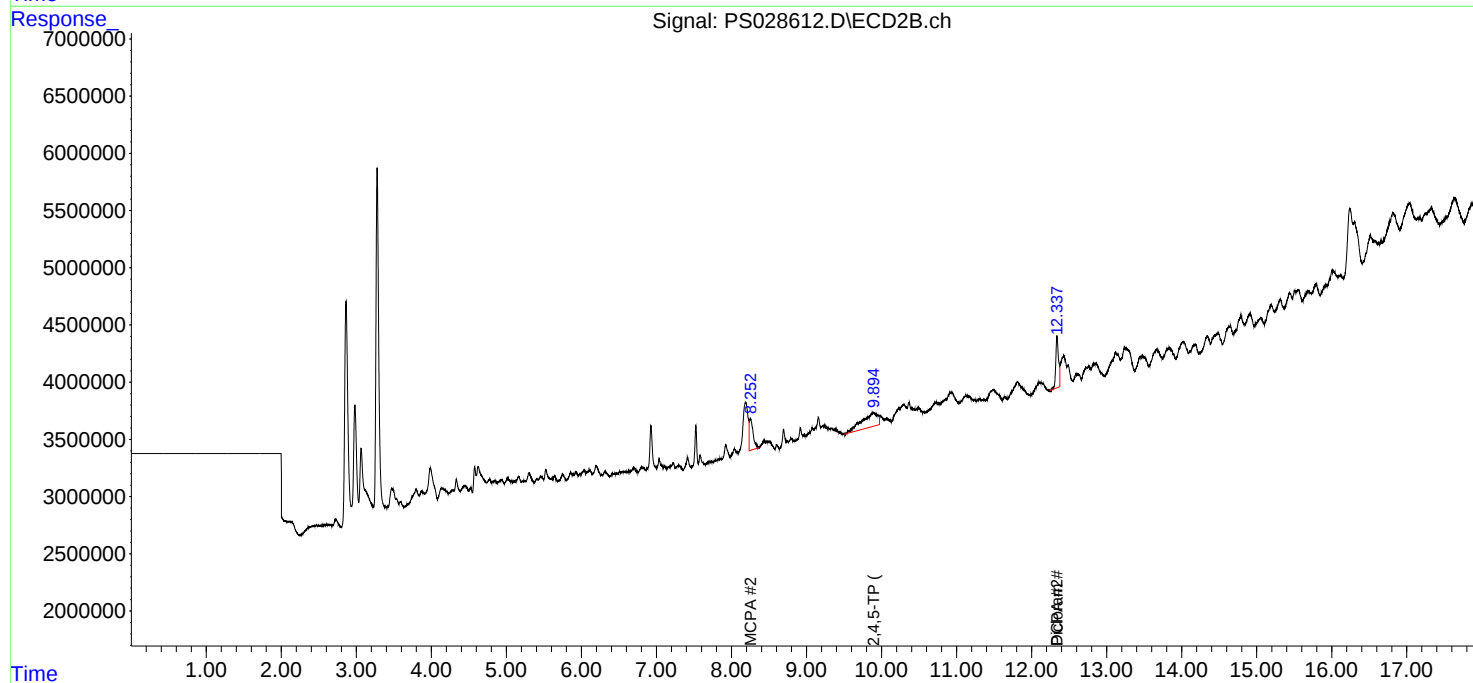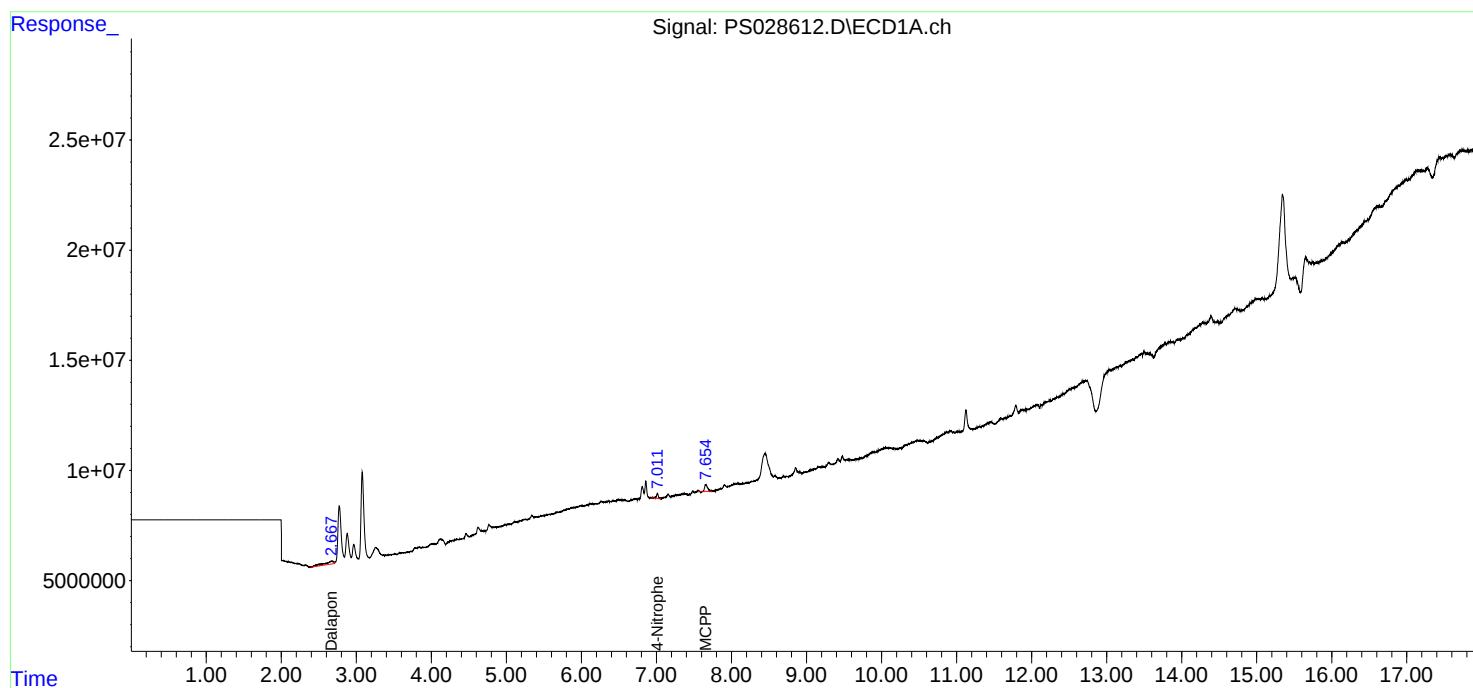


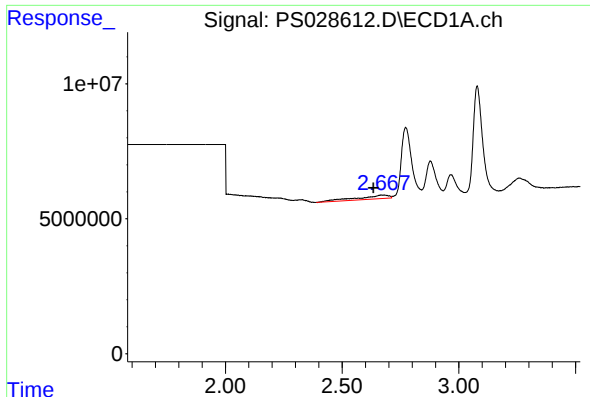

#1 Dalapon


R.T.: 2.668 min
Delta R.T.: 0.033 min
Response: 13107368
Conc: 3.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

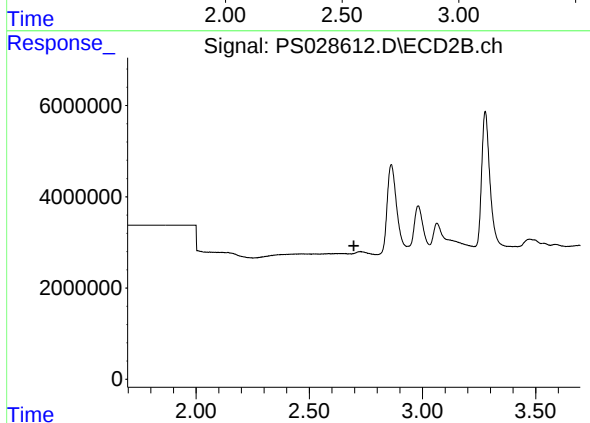


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.697 min
Response: 0
Conc: N.D.

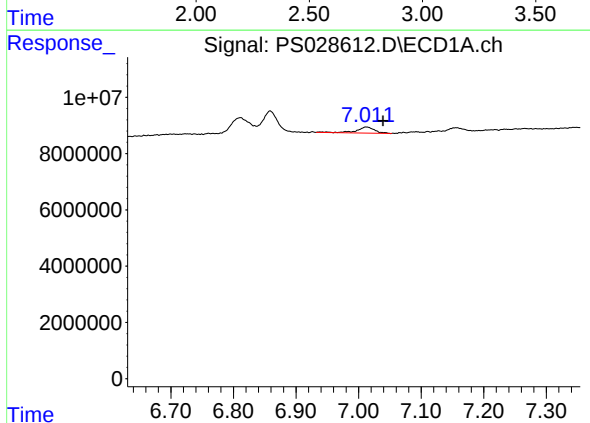


#3 4-Nitrophenol

R.T.: 7.013 min
Delta R.T.: -0.026 min
Response: 4349552
Conc: 2.56 ng/ml

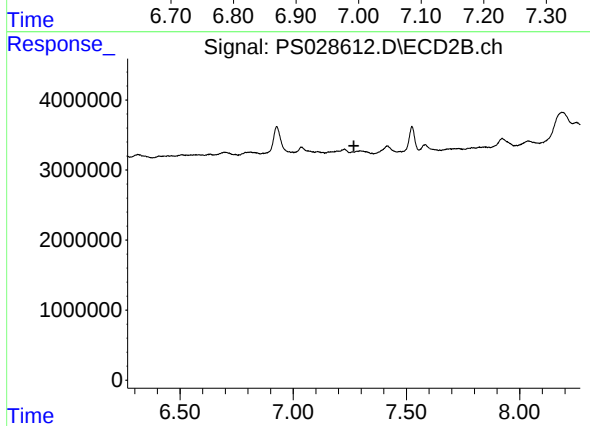

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

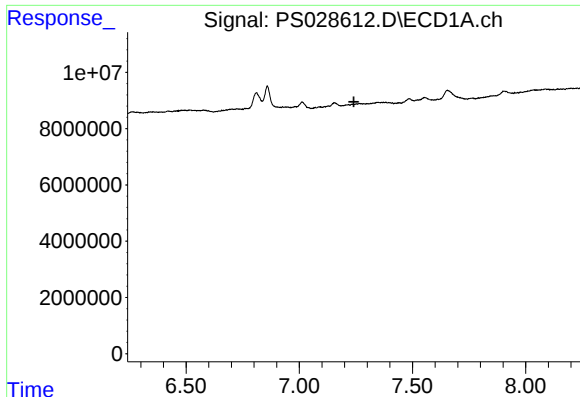

#4 2,4-DCAA


R.T.: 7.266 min
Delta R.T.: 0.025 min
Response: -2545726
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

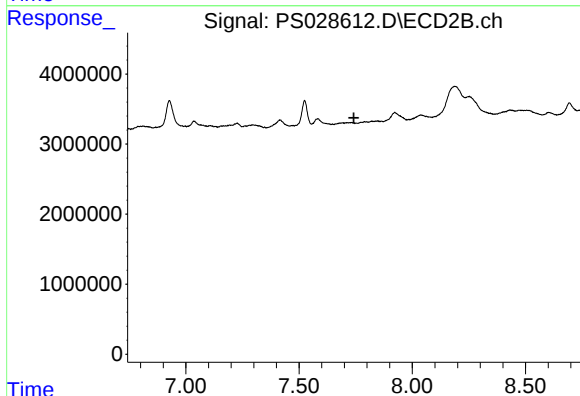


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.742 min
Response: 0
Conc: N.D.

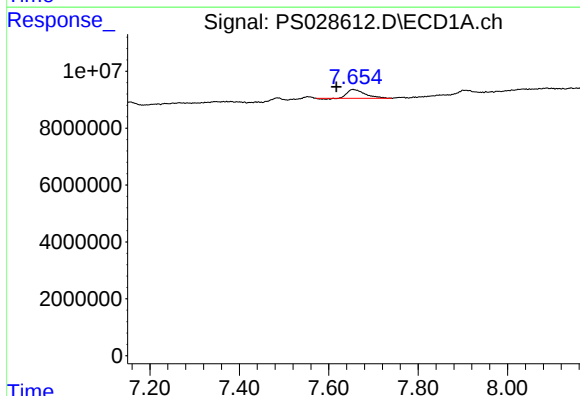


#6 MCPP

R.T.: 7.655 min
Delta R.T.: 0.037 min
Response: 8486259
Conc: 1.21 ug/ml

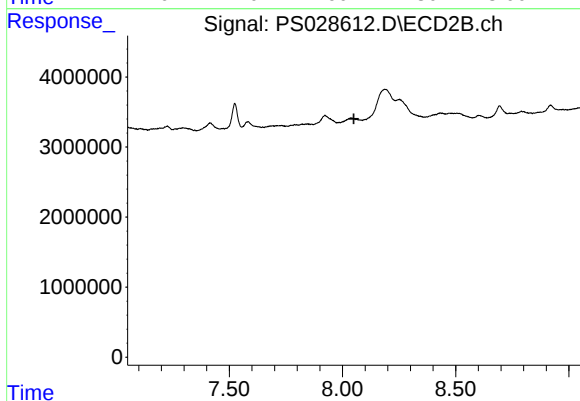

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

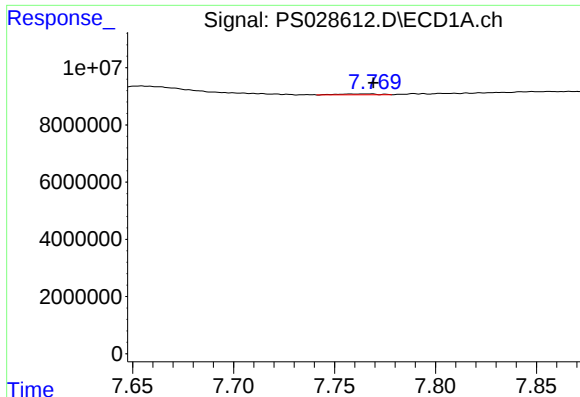

#7 MCPA


R.T.: 7.765 min
Delta R.T.: -0.004 min
Response: 437028
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

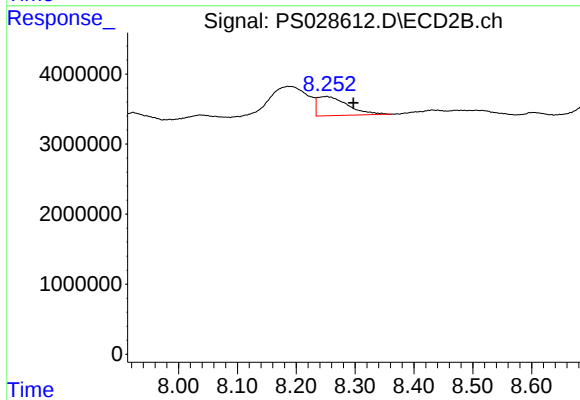


#7 MCPA

R.T.: 8.251 min
Delta R.T.: -0.047 min
Response: 9862501
Conc: 1.59 ug/ml

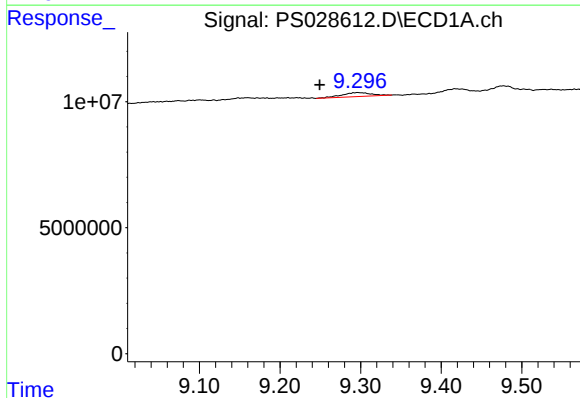


#11 2,4,5-TP (SILVEX)

R.T.: 9.296 min
Delta R.T.: 0.047 min
Response: 3888171
Conc: N.D.

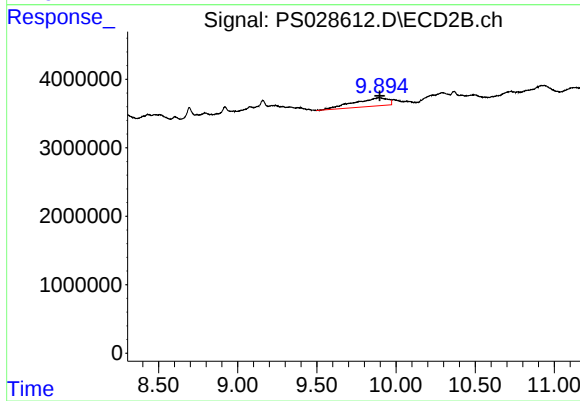

#11 2,4,5-TP (SILVEX)


R.T.: 9.894 min
Delta R.T.: -0.003 min
Response: 17928191
Conc: 2.12 ng/ml

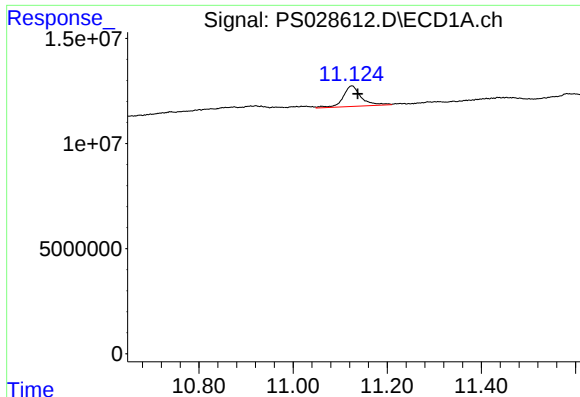

#15 Picloram


R.T.: 11.125 min
Delta R.T.: -0.013 min
Response: 26367511
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

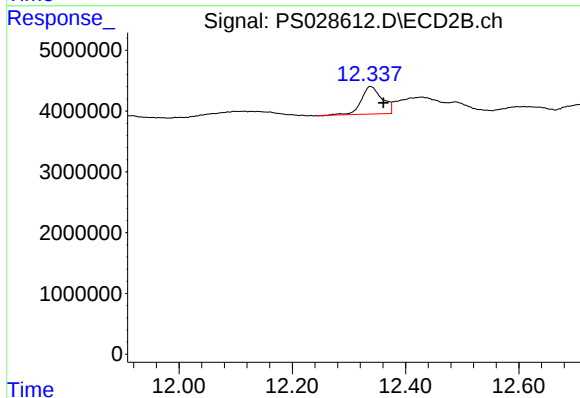


#15 Picloram

R.T.: 12.339 min
Delta R.T.: -0.022 min
Response: 11627798
Conc: 1.03 ng/ml

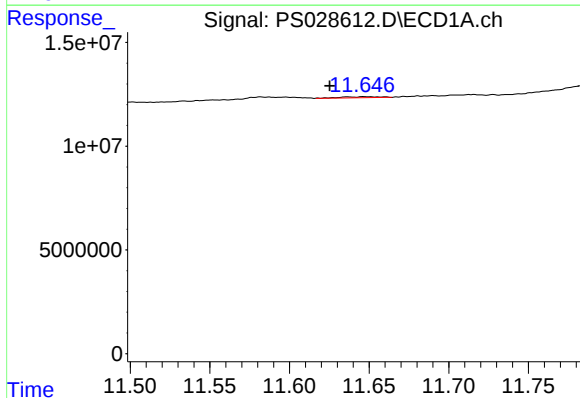

#16 DCPA

R.T.: 11.648 min
Delta R.T.: 0.023 min
Response: 793593
Conc: N.D.

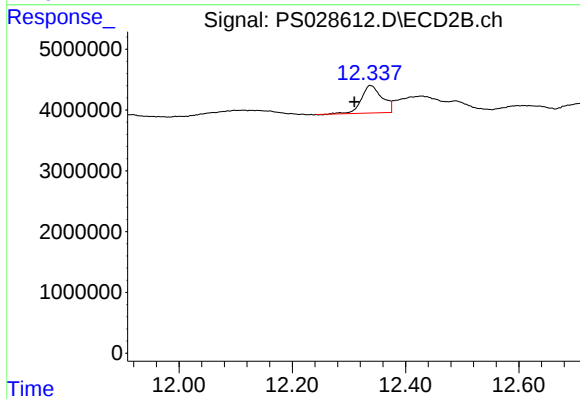

#16 DCPA

R.T.: 12.339 min
Delta R.T.: 0.029 min
Response: 11627798
Conc: 1.20 ng/ml