

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112524\
 Data File : PS028628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 20:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 23:59:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	7.726	1430.2E6	609.3E6	559.569	471.469
Target Compounds							
1) T	Dalapon	2.665f	0.000	1052555	0	<MDL	N.D. #
3) T	4-Nitroph...	7.021	0.000	6594531	0	3.883	N.D. #
5) T	DICAMBA	0.000	7.920	0	3302355	N.D.	<MDL
6) T	MCP	7.654f	0.000	21959120	0	3.122	N.D. #
8) T	DICHLORPROP	8.093f	8.692f	493355	8186656	<MDL	5.605 #
11) T	2,4,5-TP ...	9.294f	0.000	10877207	0	<MDL	N.D. #
12) T	2,4,5-T	9.528	0.000	722329	0	<MDL	N.D. #
15) T	Picloram	11.120	12.338	12448552	3564347	<MDL	<MDL #
16) T	DCPA	11.594f	12.338f	1987899	3564347	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112524\
Data File : PS028628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 20:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 23:59:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

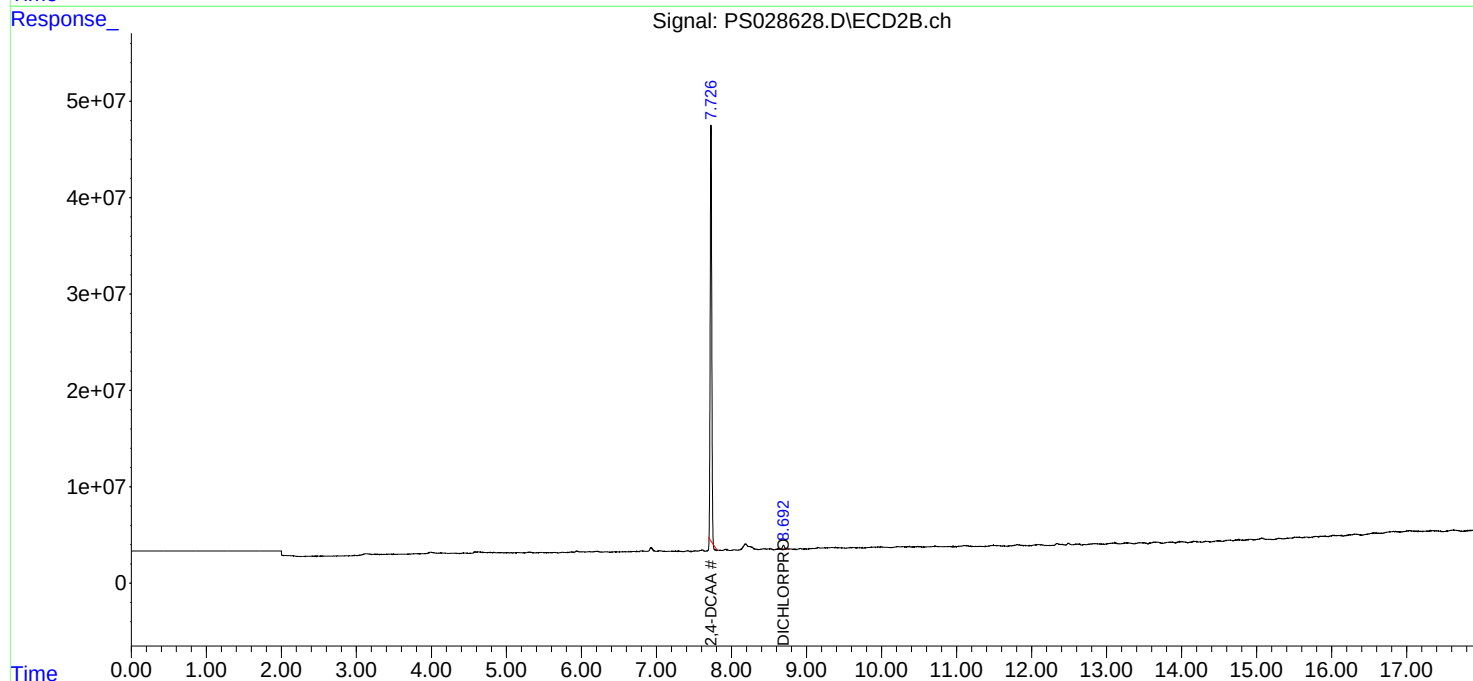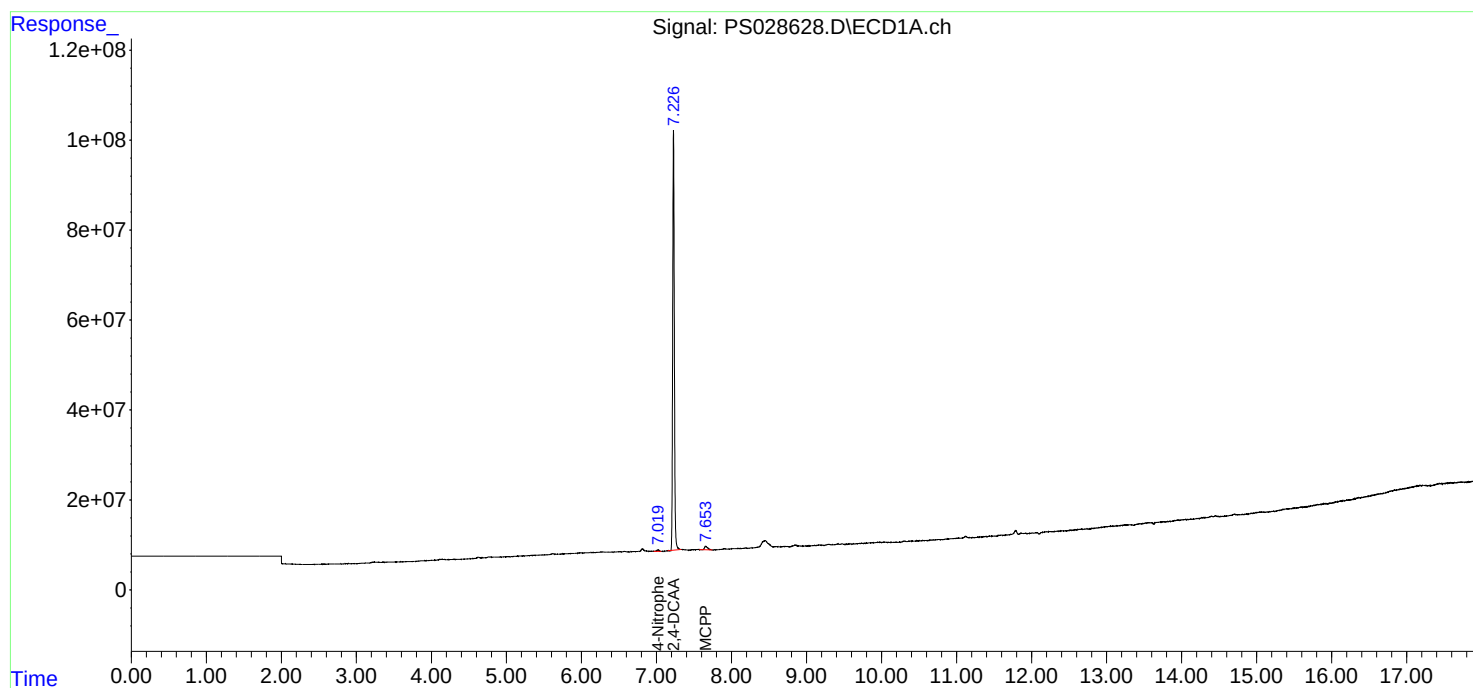


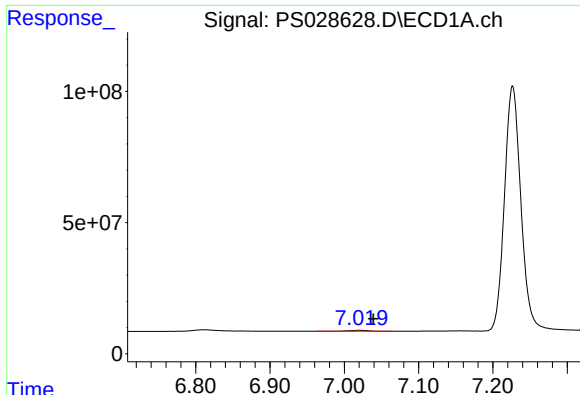

#3 4-Nitrophenol


R.T.: 7.021 min
Delta R.T.: -0.018 min
Response: 6594531
Conc: 3.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

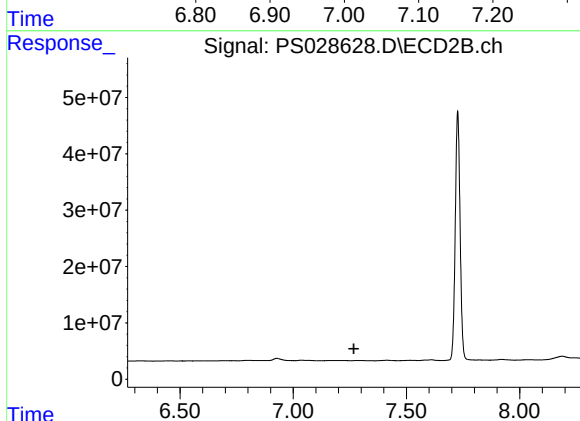


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

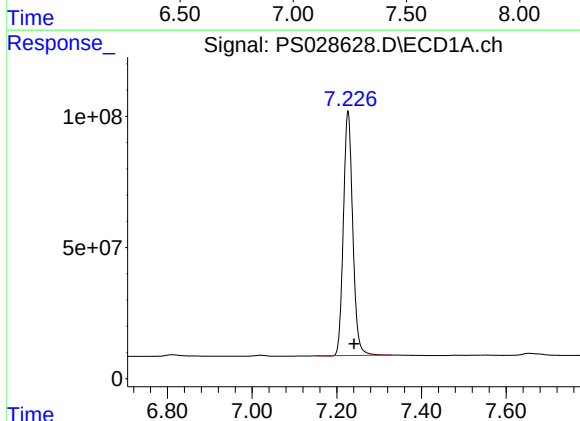


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: -0.014 min
Response: 1430191903
Conc: 559.57 ng/ml

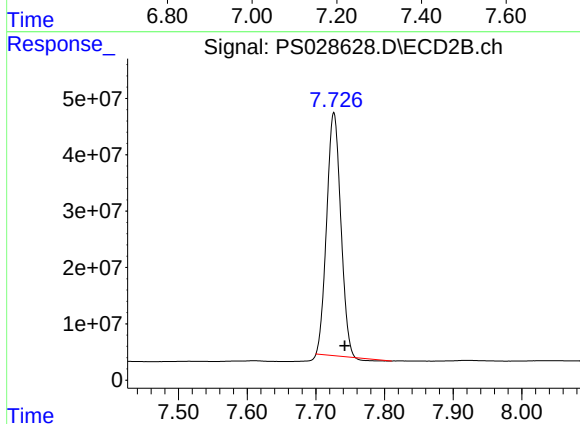

#4 2,4-DCAA


R.T.: 7.726 min
Delta R.T.: -0.016 min
Response: 609281566
Conc: 471.47 ng/ml

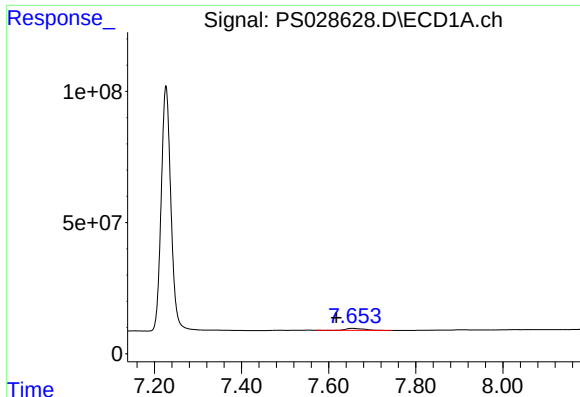

#6 MCP


R.T.: 7.654 min
Delta R.T.: 0.037 min
Response: 21959120
Conc: 3.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

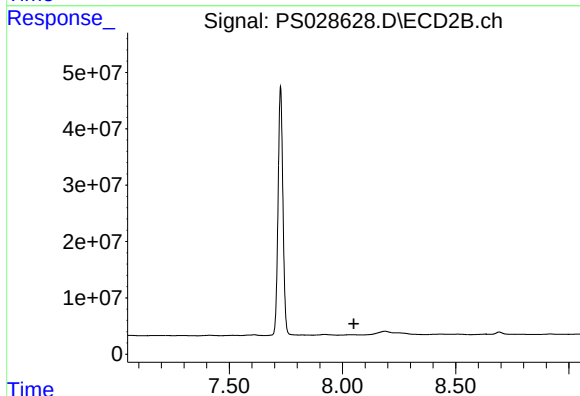


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

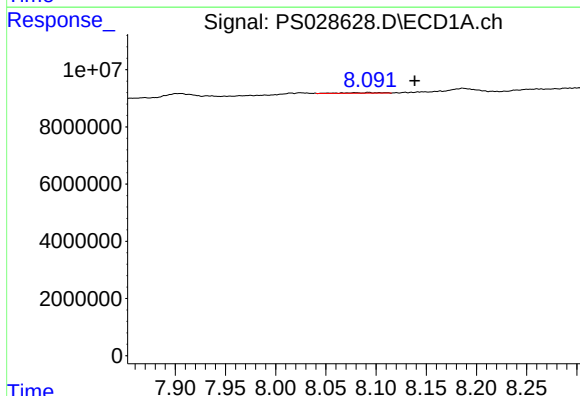

#8 DICHLORPROP

R.T.: 8.093 min
Delta R.T.: -0.046 min
Response: 493355
Conc: N.D.

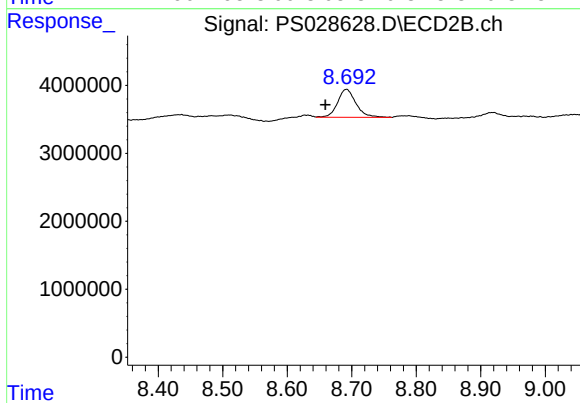

#8 DICHLORPROP

R.T.: 8.692 min
Delta R.T.: 0.032 min
Response: 8186656
Conc: 5.61 ng/ml