

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112425\
 Data File : PS032526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2025 21:25
 Operator : AR\AJ
 Sample : Q3710-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMPRESSOR-EXCAVATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 14:19:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.635	29713977	27095961	6.558	7.433
Target Compounds							
1) T	Dalapon	0.000	2.570f	0	2738.0E6	N.D.	393.727
2) T	3,5-DICHL...	0.000	6.552f	0	4863173	N.D.	<MDL
5) T	DICAMBA	7.475	0.000	2106445	0	<MDL	N.D. #
6) T	MCP	7.659	7.889	8927024	16864374	<MDL	1.268 #
7) T	MCPA	7.745f	0.000	125.3E6	0	9.331	N.D. #
8) T	DICHLORPROP	8.178	8.531	1423223	2186757	<MDL	<MDL #
9) T	2,4-D	8.422	8.830f	310286	2099220	<MDL	<MDL #
10) T	Pentachlo...	8.694	9.353	717041	16920934	<MDL	<MDL #
11) T	2,4,5-TP ...	9.320f	9.732	29821665	154.0E6	1.146	5.733 #
12) T	2,4,5-T	9.599	10.172	107.5E6	144.6E6	4.511	6.098 #
13) T	2,4-DB	10.173	10.759	57996997	36786699	22.009	9.754 #
14) T	DINOSEB	11.311f	11.123	56646303	19550971	2.722	1.105 #
15) T	Picloram	11.153f	0.000	14989373	0	<MDL	N.D. #
16) T	DCPA	11.621	0.000	9215541	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112425\
Data File : PS032526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2025 21:25
Operator : AR\AJ
Sample : Q3710-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 14:19:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

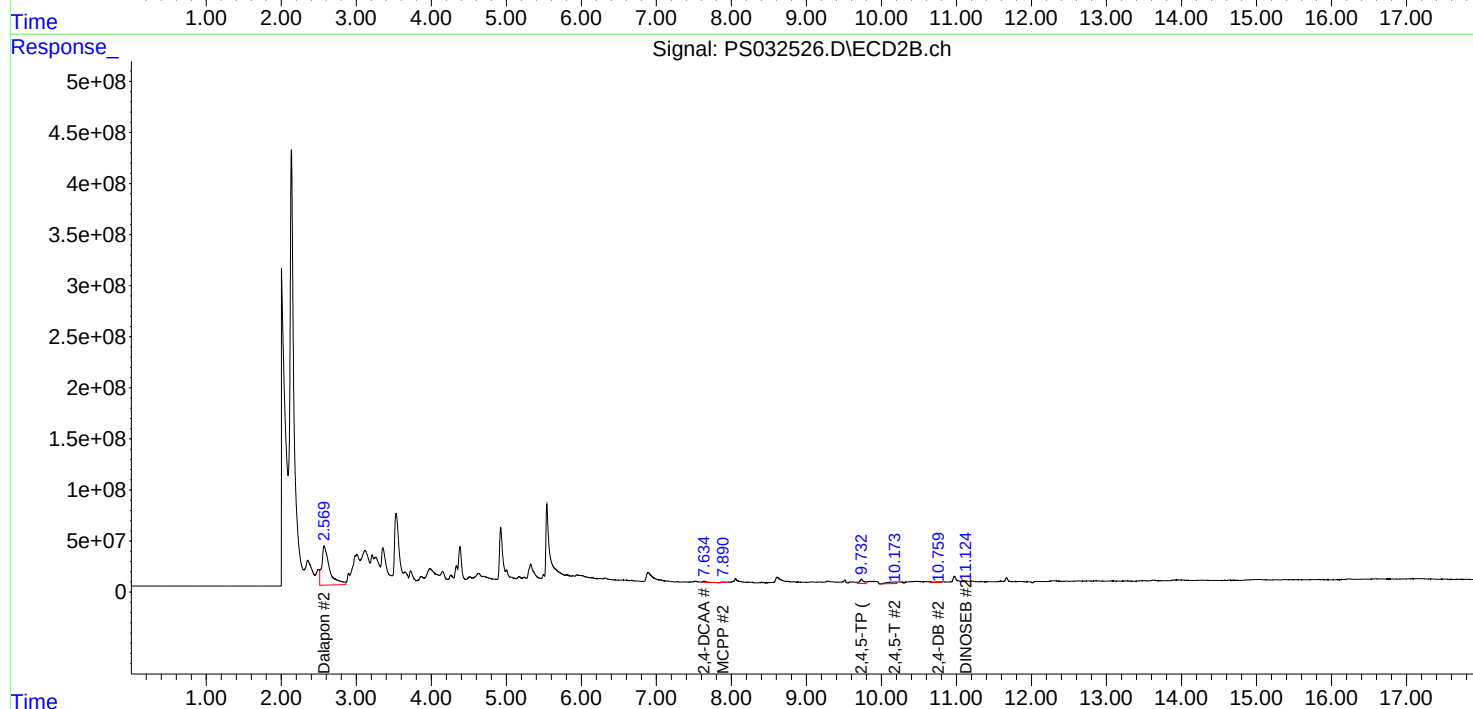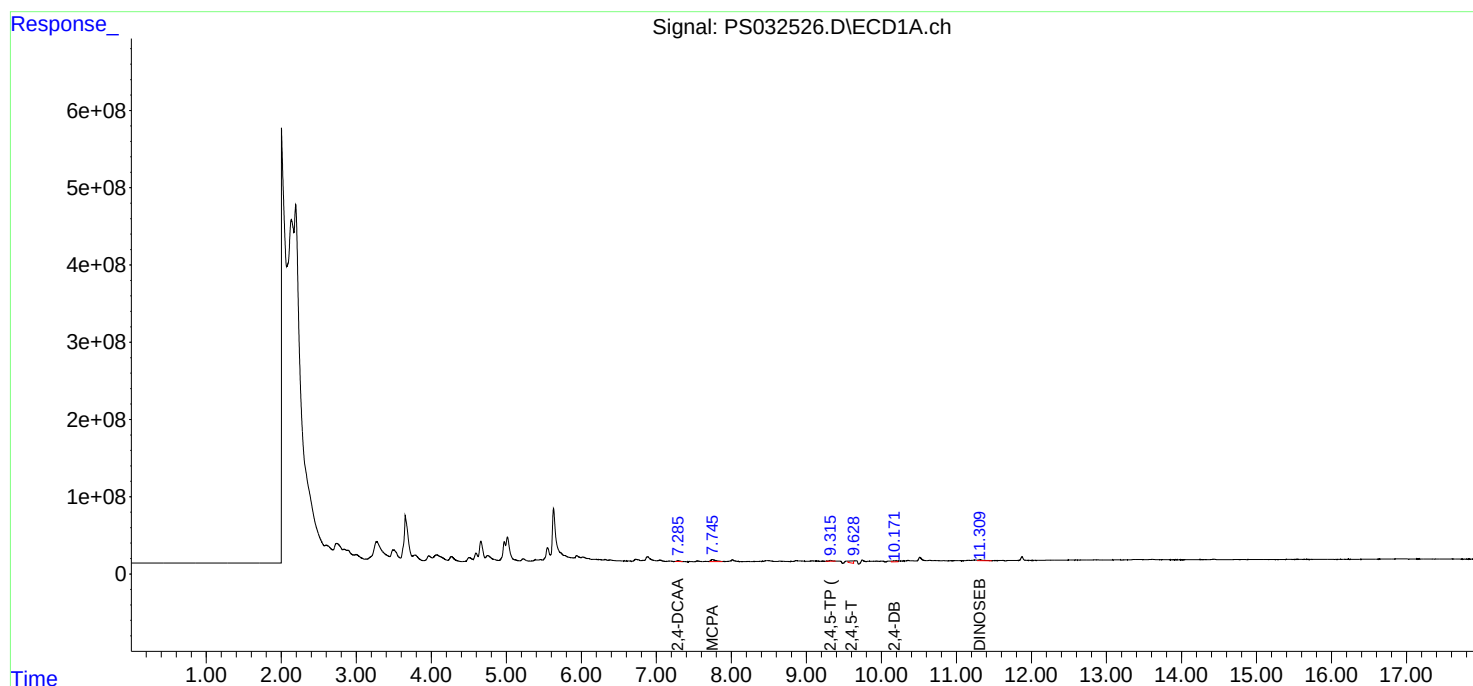


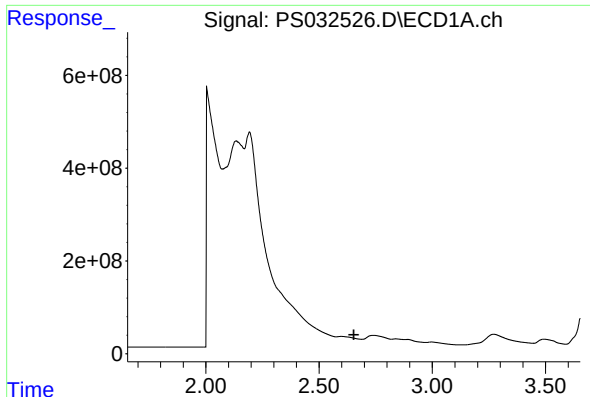

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

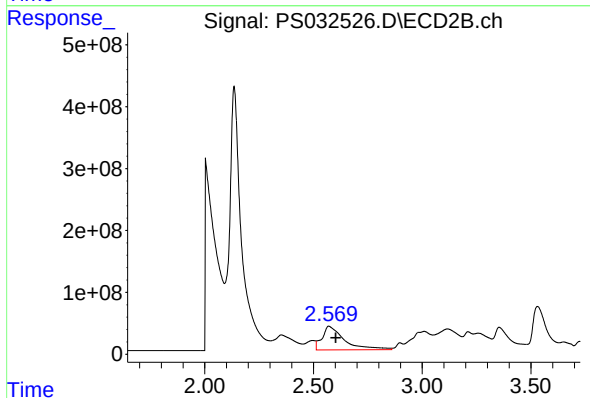


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: -0.033 min
Response: 2737973780
Conc: 393.73 ng/ml

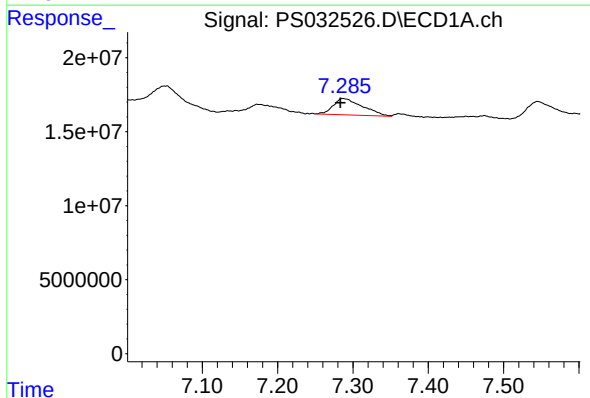


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.003 min
Response: 29713977
Conc: 6.56 ng/ml

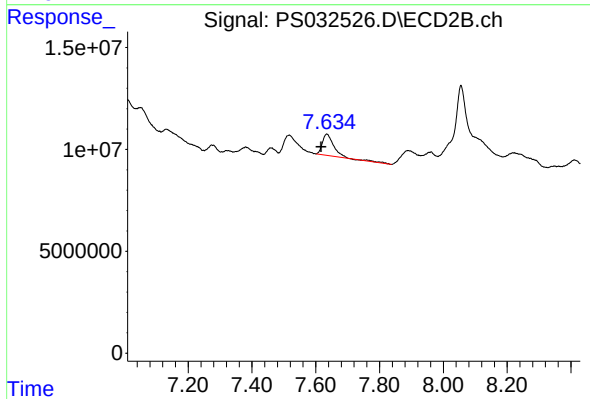

#4 2,4-DCAA


R.T.: 7.635 min
Delta R.T.: 0.017 min
Response: 27095961
Conc: 7.43 ng/ml

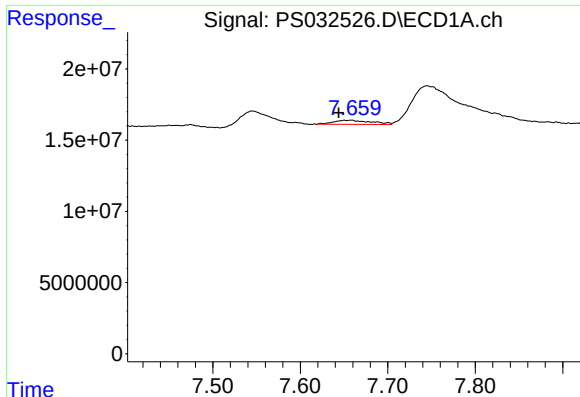

#6 MCPP


R.T.: 7.659 min
Delta R.T.: 0.015 min
Response: 8927024
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

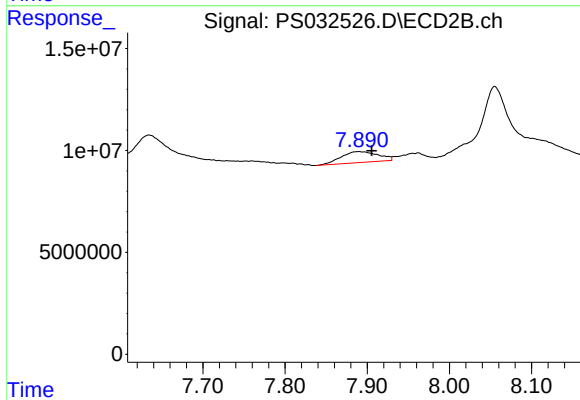


#6 MCPP

R.T.: 7.889 min
Delta R.T.: -0.016 min
Response: 16864374
Conc: 1.27 ug/ml

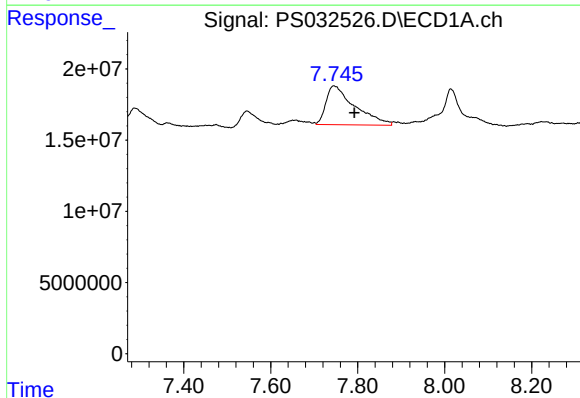


#7 MCPA

R.T.: 7.745 min
Delta R.T.: -0.048 min
Response: 125271418
Conc: 9.33 ug/ml

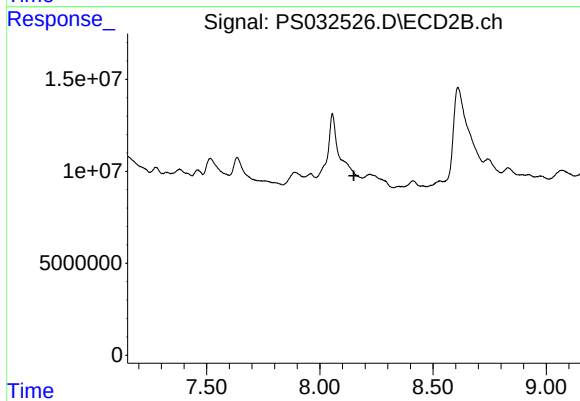

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

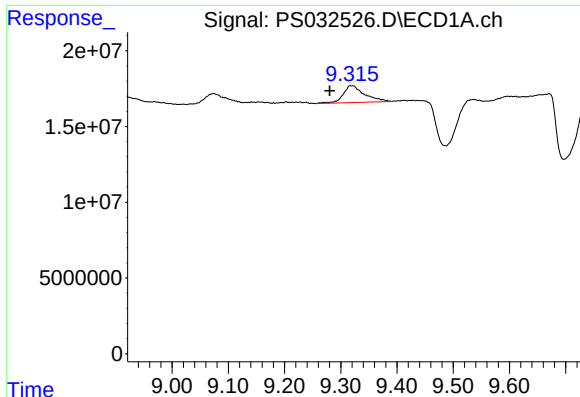

#11 2,4,5-TP (SILVEX)


R.T.: 9.320 min
Delta R.T.: 0.039 min
Response: 29821665
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

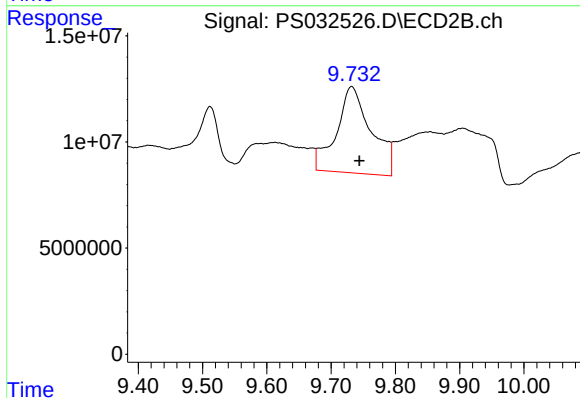


#11 2,4,5-TP (SILVEX)

R.T.: 9.732 min
Delta R.T.: -0.012 min
Response: 153950820
Conc: 5.73 ng/ml

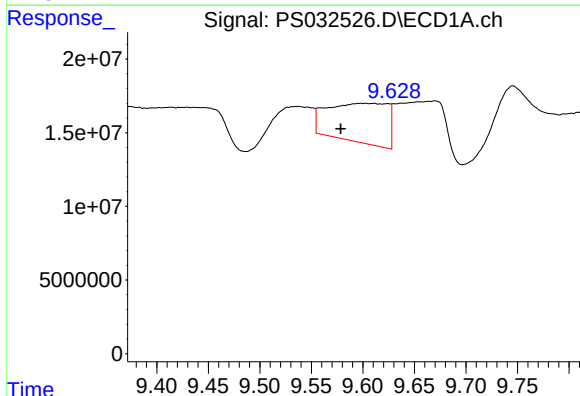


#12 2,4,5-T

R.T.: 9.599 min
Delta R.T.: 0.021 min
Response: 107533577
Conc: 4.51 ng/ml

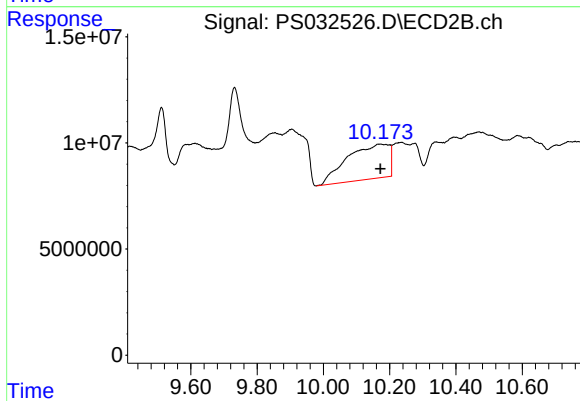

#12 2,4,5-T


R.T.: 10.172 min
Delta R.T.: 0.000 min
Response: 144625899
Conc: 6.10 ng/ml

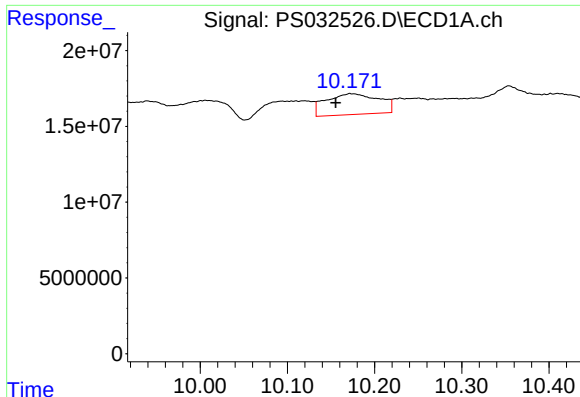

#13 2,4-DB


R.T.: 10.173 min
Delta R.T.: 0.018 min
Response: 57996997
Conc: 22.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMPRESSOR-EXCAVATION

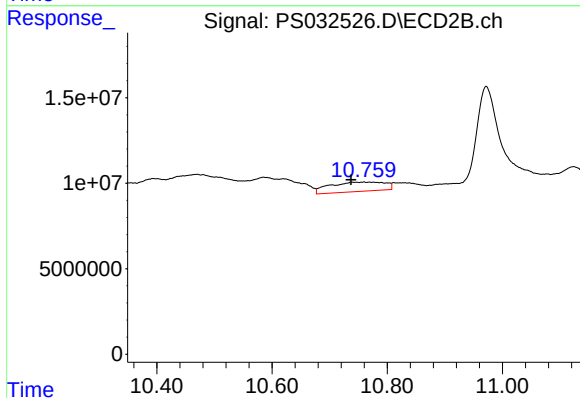


#13 2,4-DB

R.T.: 10.759 min
Delta R.T.: 0.022 min
Response: 36786699
Conc: 9.75 ng/ml

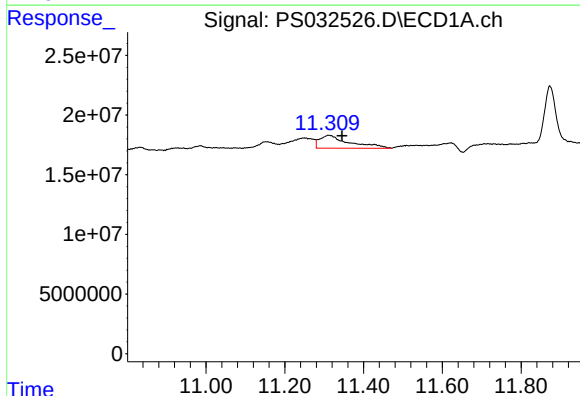

#14 DINOSEB

R.T.: 11.311 min
Delta R.T.: -0.034 min
Response: 56646303
Conc: 2.72 ng/ml

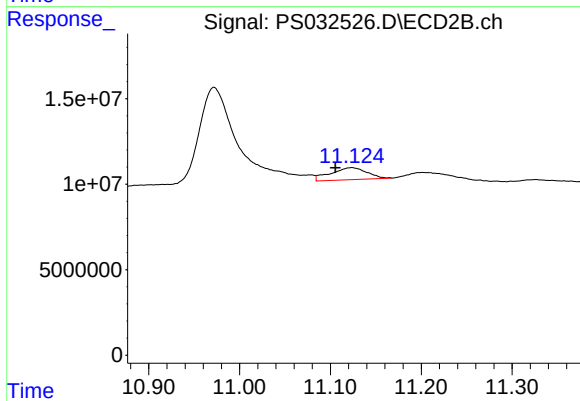

#14 DINOSEB

R.T.: 11.123 min
Delta R.T.: 0.018 min
Response: 19550971
Conc: 1.11 ng/ml