

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112425\
 Data File : PS032531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2025 23:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 14:21:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.279	7.623	1622.5E6	1763.8E6	358.077	483.842 #
Target Compounds							
2) T	3,5-DICHL...	6.438	0.000	2507206	0	<MDL	N.D. #
7) T	MCPA	7.808	0.000	17442118	0	1.299	N.D. #
8) T	DICHLORPROP	8.171	0.000	567238	0	<MDL	N.D. #
9) T	2,4-D	8.380f	0.000	174467	0	<MDL	N.D. #
10) T	Pentachlo...	8.716	0.000	2129285	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.274	0.000	2908071	0	<MDL	N.D. #
12) T	2,4,5-T	9.571	10.140f	2955609	32473746	<MDL	1.369 #
13) T	2,4-DB	10.165	0.000	866238	0	<MDL	N.D. #
14) T	DINOSEB	11.340	0.000	2018061	0	<MDL	N.D. #
15) T	Picloram	11.191	0.000	1719888	0	<MDL	N.D. #
16) T	DCPA	11.640	0.000	2092787	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112425\
Data File : PS032531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2025 23:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 14:21:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

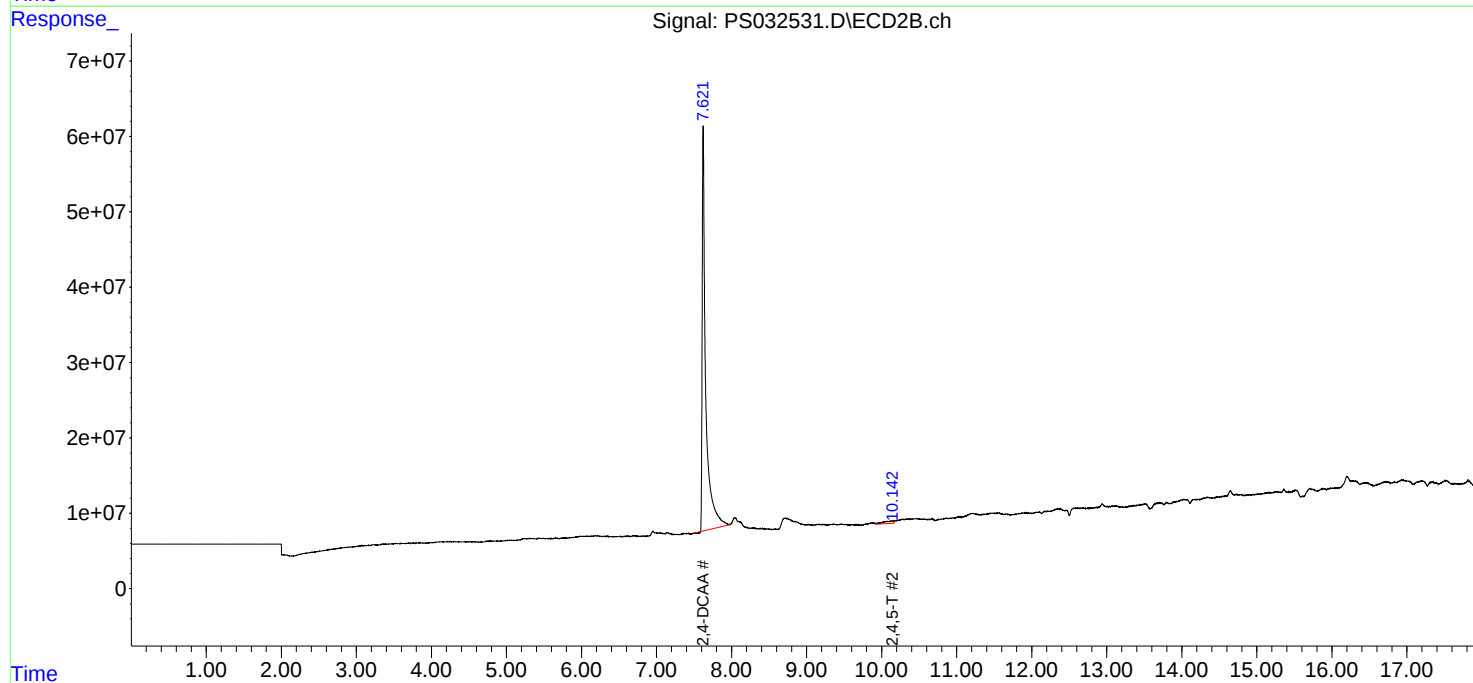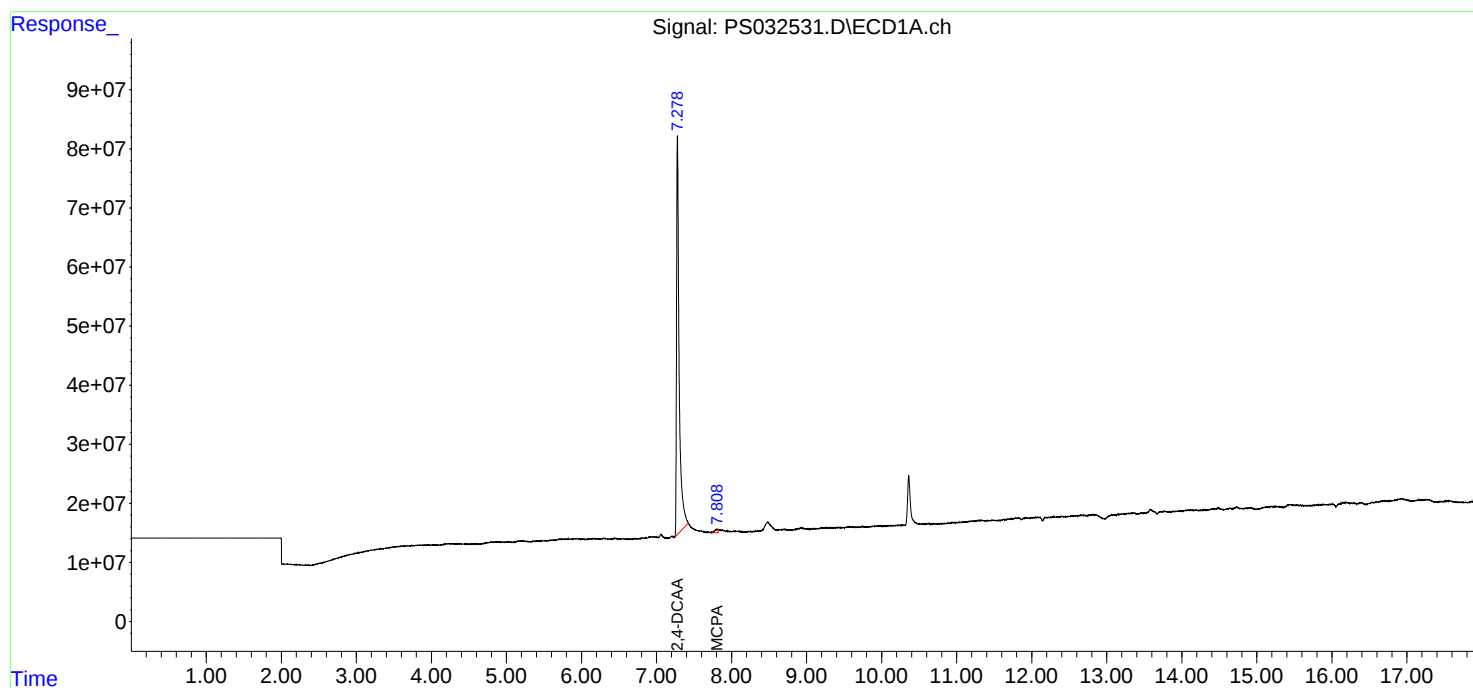


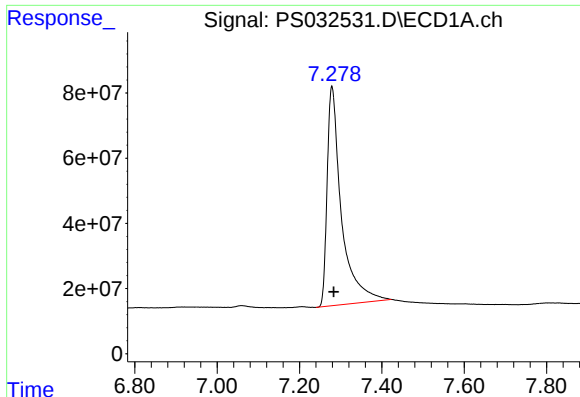

#4 2,4-DCAA


R.T.: 7.279 min
Delta R.T.: -0.005 min
Response: 1622545178
Conc: 358.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

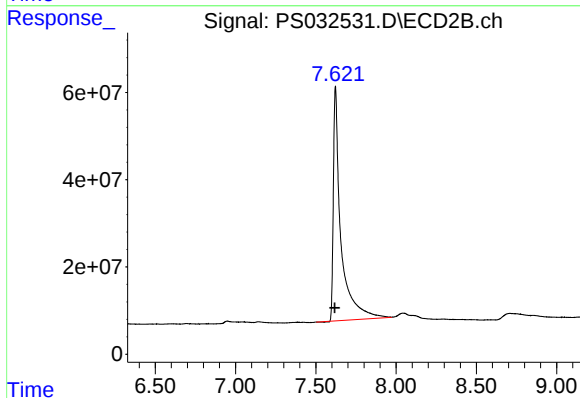


#4 2,4-DCAA

R.T.: 7.623 min
Delta R.T.: 0.005 min
Response: 1763843537
Conc: 483.84 ng/ml

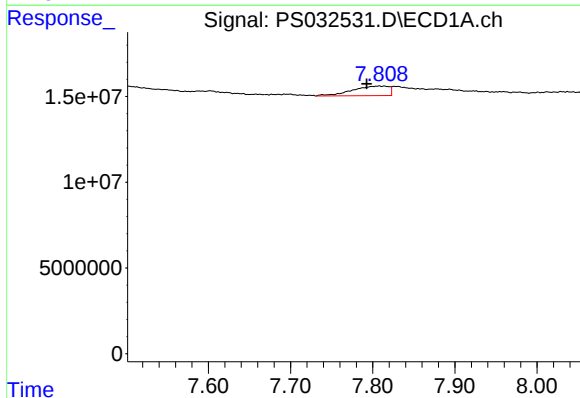


#7 MCPA

R.T.: 7.808 min
Delta R.T.: 0.015 min
Response: 17442118
Conc: 1.30 ug/ml

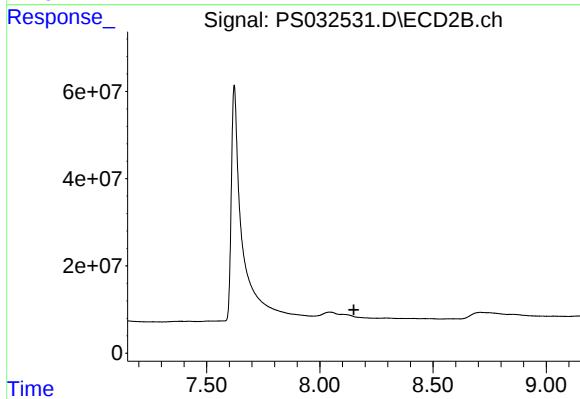

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

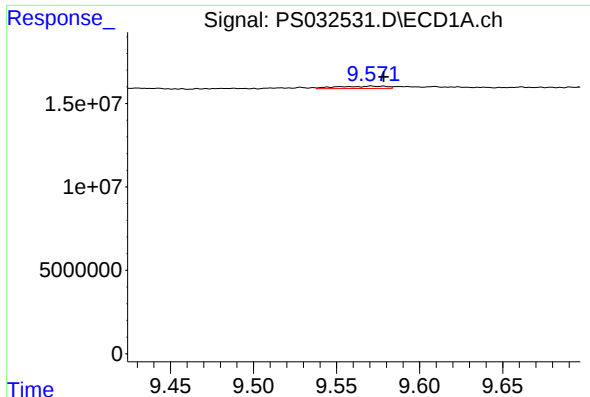

#12 2,4,5-T

R.T.: 9.571 min
Delta R.T.: -0.007 min
Response: 2955609
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

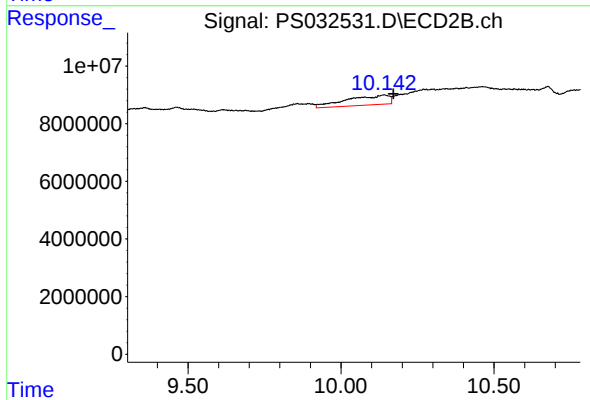

#12 2,4,5-T

R.T.: 10.140 min
Delta R.T.: -0.031 min
Response: 32473746
Conc: 1.37 ng/ml