

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112525\  
 Data File : PS032533.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Nov 2025 09:27  
 Operator : AR\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 25 13:41:51 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110325.M  
 Quant Title : 8080.M  
 QLast Update : Tue Nov 04 04:59:50 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2    | Resp#1   | Resp#2   | ng/ml | ng/ml   |
|-----------------------------|--------------|--------|---------|----------|----------|-------|---------|
| -----                       |              |        |         |          |          |       |         |
| System Monitoring Compounds |              |        |         |          |          |       |         |
| 4) S                        | 2,4-DCAA     | 7.266  | 0.000   | 7149315  | 0        | 1.578 | N.D. #  |
| Target Compounds            |              |        |         |          |          |       |         |
| 2) T                        | 3,5-DICHL... | 6.437  | 0.000   | 18818800 | 0        | 2.910 | N.D. #  |
| 5) T                        | DICAMBA      | 7.512f | 0.000   | 1555245  | 0        | <MDL  | N.D. #  |
| 6) T                        | MCP          | 7.679f | 7.907   | 3081170  | 48649098 | <MDL  | 3.658 # |
| 7) T                        | MCPA         | 7.798  | 0.000   | 3062827  | 0        | <MDL  | N.D. #  |
| 8) T                        | DICHLORPROP  | 8.185  | 8.555f  | 568606   | 2374586  | <MDL  | <MDL #  |
| 9) T                        | 2,4-D        | 8.441f | 8.841   | 31198424 | 5865125  | 6.915 | 1.118 # |
| 10) T                       | Pentachlo... | 8.699  | 9.352   | 4030065  | 5729696  | <MDL  | <MDL #  |
| 11) T                       | 2,4,5-TP ... | 9.285  | 9.784f  | 1140391  | 2916140  | <MDL  | <MDL #  |
| 12) T                       | 2,4,5-T      | 9.570  | 10.187  | 8172158  | 14845800 | <MDL  | <MDL #  |
| 13) T                       | 2,4-DB       | 10.149 | 0.000   | 819950   | 0        | <MDL  | N.D. #  |
| 14) T                       | DINOSEB      | 0.000  | 11.101  | 0        | 5038608  | N.D.  | <MDL    |
| 15) T                       | Picloram     | 11.178 | 12.192f | 73349295 | 119.1E6  | 3.456 | 3.203   |
| 16) T                       | DCPA         | 11.633 | 0.000   | 7544813  | 0        | <MDL  | N.D. #  |
| -----                       |              |        |         |          |          |       |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS112525\  
Data File : PS032533.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Nov 2025 09:27  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 25 13:41:51 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110325.M  
Quant Title : 8080.M  
QLast Update : Tue Nov 04 04:59:50 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

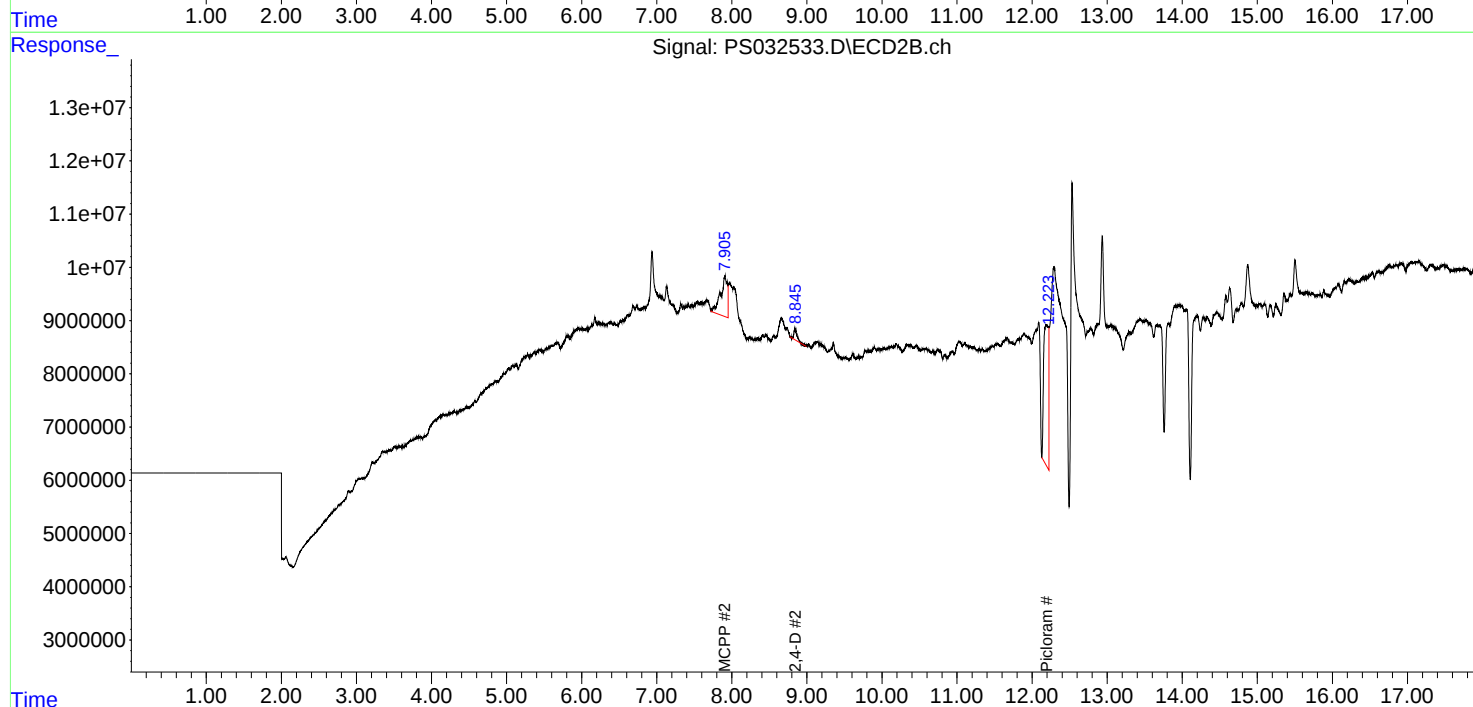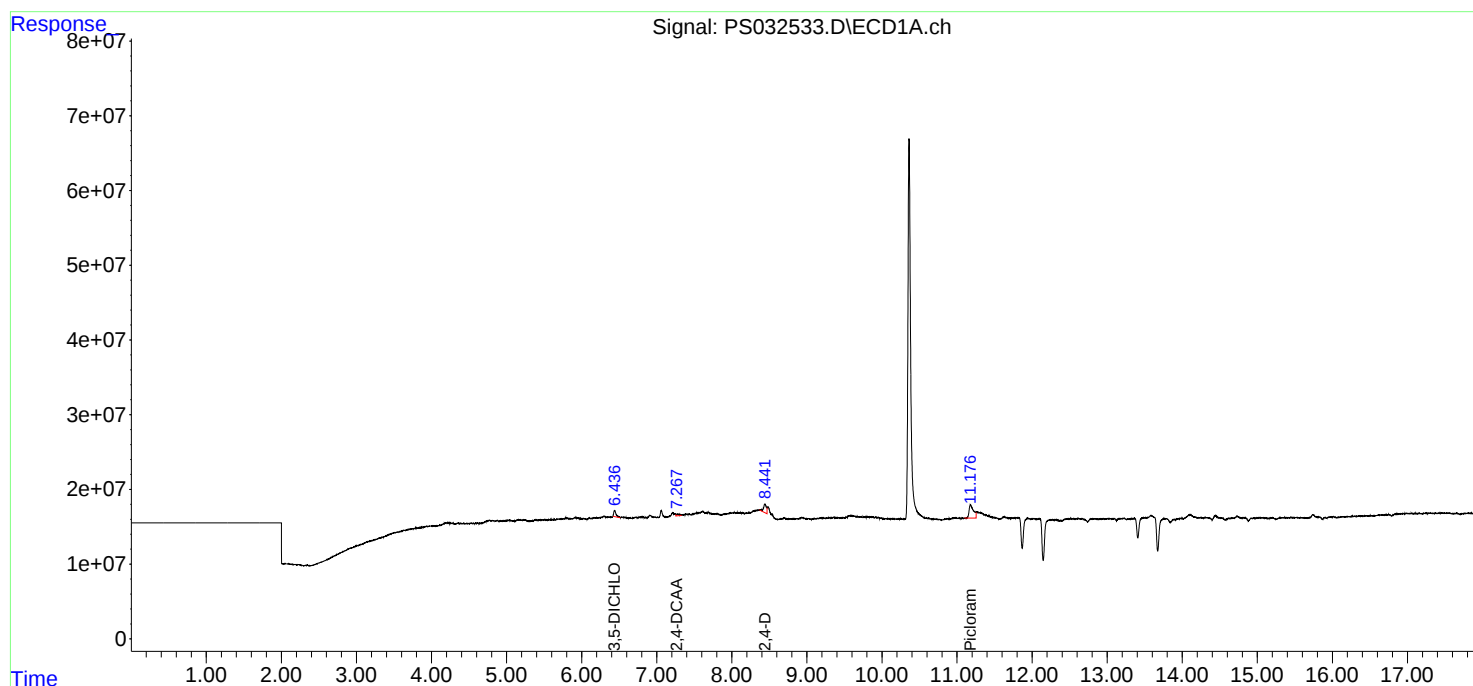


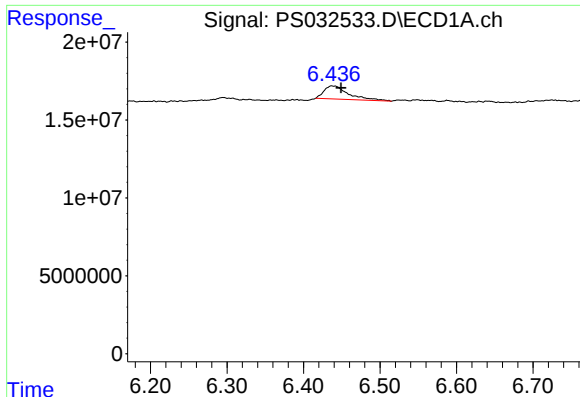

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.437 min  
Delta R.T.: -0.012 min  
Response: 18818800  
Conc: 2.91 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

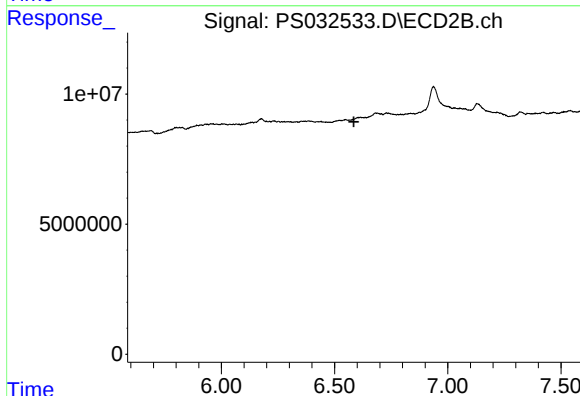


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min  
Exp R.T. : 6.585 min  
Response: 0  
Conc: N.D.

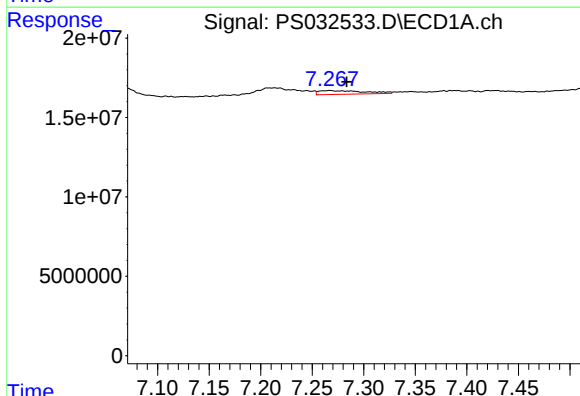


#4 2,4-DCAA

R.T.: 7.266 min  
Delta R.T.: -0.017 min  
Response: 7149315  
Conc: 1.58 ng/ml

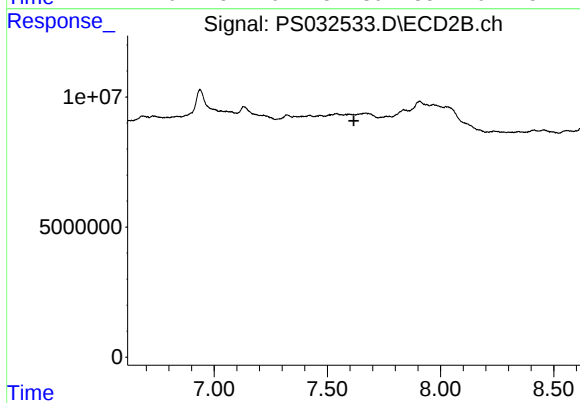

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T. : 7.617 min  
Response: 0  
Conc: N.D.

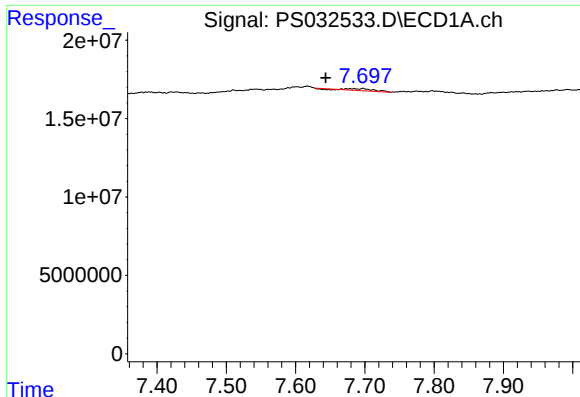

#6 MCPP


R.T.: 7.679 min  
Delta R.T.: 0.036 min  
Response: 3081170  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

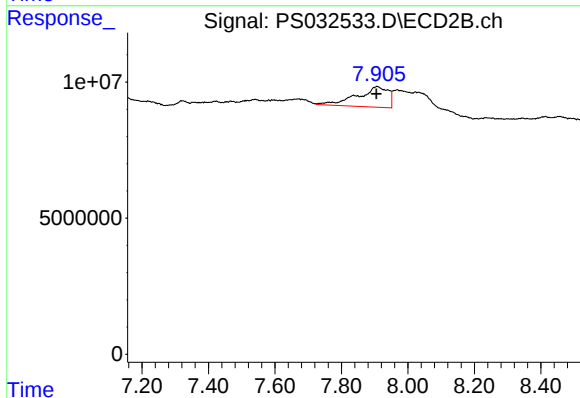


#6 MCPP

R.T.: 7.907 min  
Delta R.T.: 0.002 min  
Response: 48649098  
Conc: 3.66 ug/ml

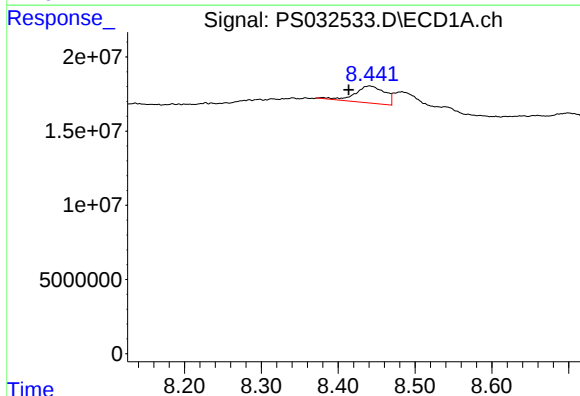


#9 2,4-D

R.T.: 8.441 min  
Delta R.T.: 0.027 min  
Response: 31198424  
Conc: 6.91 ng/ml

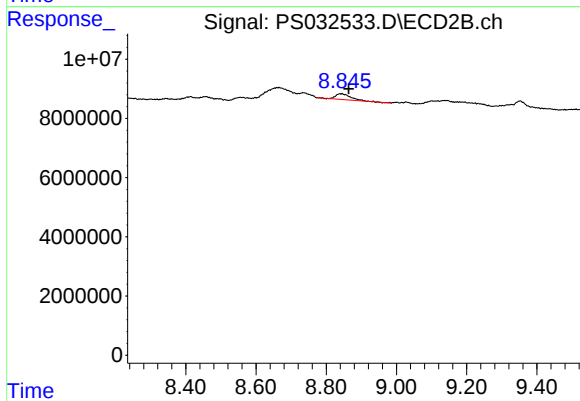

#9 2,4-D


R.T.: 8.841 min  
Delta R.T.: -0.022 min  
Response: 5865125  
Conc: 1.12 ng/ml

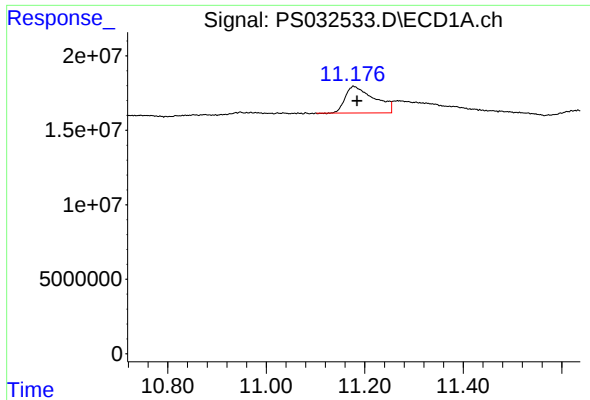

#15 Picloram

R.T.: 11.178 min  
Delta R.T.: -0.006 min  
Response: 73349295  
Conc: 3.46 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

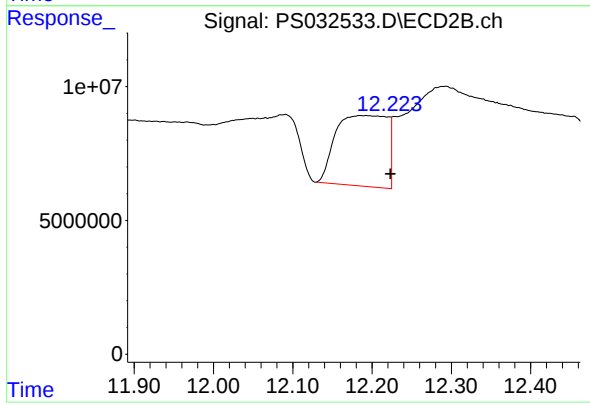

#15 Picloram

R.T.: 12.192 min  
Delta R.T.: -0.031 min  
Response: 119098504  
Conc: 3.20 ng/ml