

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112525\
 Data File : PS032536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 11:08
 Operator : AR\AJ
 Sample : Q3699-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-112025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:43:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.623	482.2E6	521.1E6	106.427	142.955 #
Target Compounds							
1) T	Dalapon	2.636	2.638f	1506.8E6	968.8E6	209.899	139.322 #
2) T	3,5-DICHL...	6.494f	6.601	7009899	6420502	1.084	1.068
3) T	4-Nitroph...	7.083	7.229f	9195190	31906996	6.850	14.056 #
5) T	DICAMBA	7.480	7.830	2329750	14174665	<MDL	<MDL #
6) T	MCPD	7.687f	7.883	59592738	31119955	5.472	2.340 #
7) T	MCPA	7.760f	0.000	42861169	0	3.192	N.D. #
8) T	DICHLORPROP	0.000	8.539	0	13587464	N.D.	2.849
9) T	2,4-D	8.404	8.828f	29922322	24844028	6.632	4.736 #
10) T	Pentachlo...	8.695	0.000	3169836	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.283	9.732	9997155	179.7E6	<MDL	6.692 #
12) T	2,4,5-T	9.608f	0.000	208.9E6	0	8.765	N.D. #
13) T	2,4-DB	10.181f	10.742	50716049	22135040	19.246	5.869 #
14) T	DINOSEB	0.000	11.117	0	27133980	N.D.	1.534
15) T	Picloram	11.161	12.272f	17828358	541.2E6	<MDL	14.555 #
16) T	DCPA	11.636	12.135	11217830	-1650541	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112525\
Data File : PS032536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 11:08
Operator : AR\AJ
Sample : Q3699-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:43:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

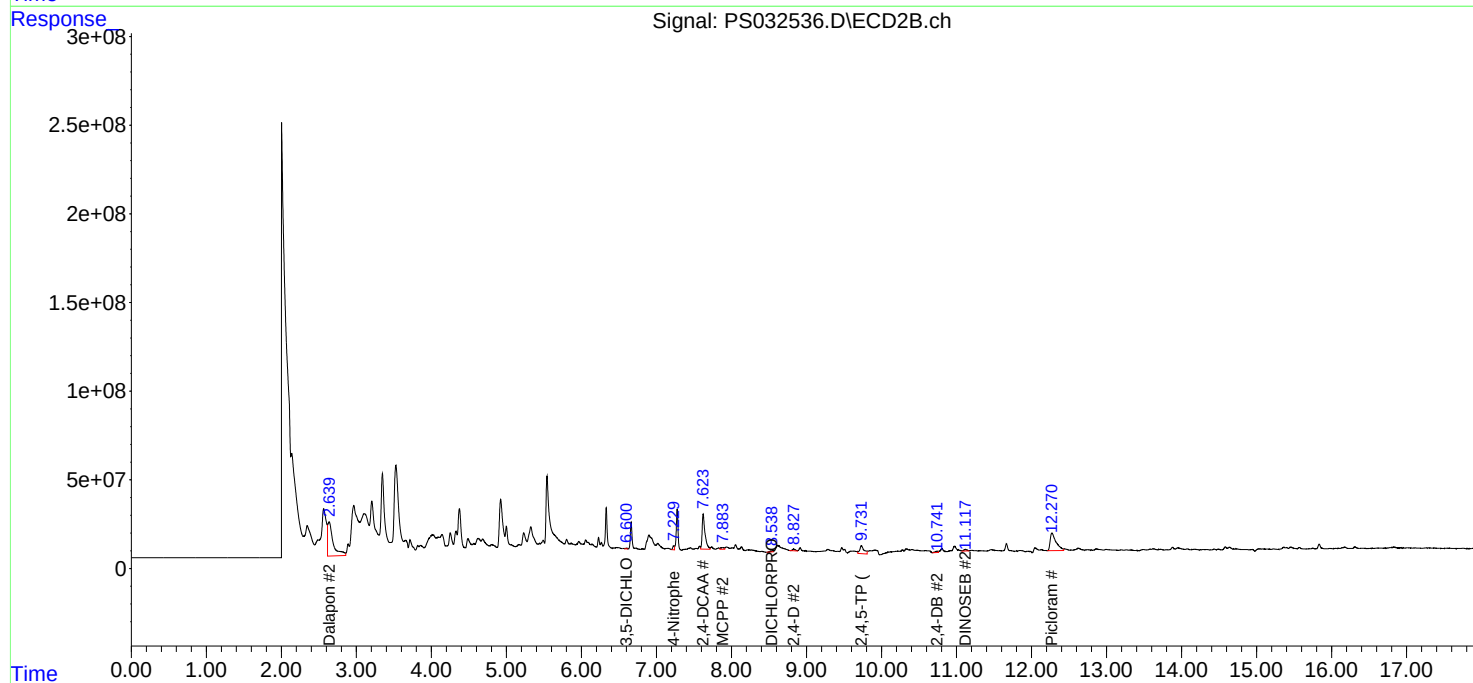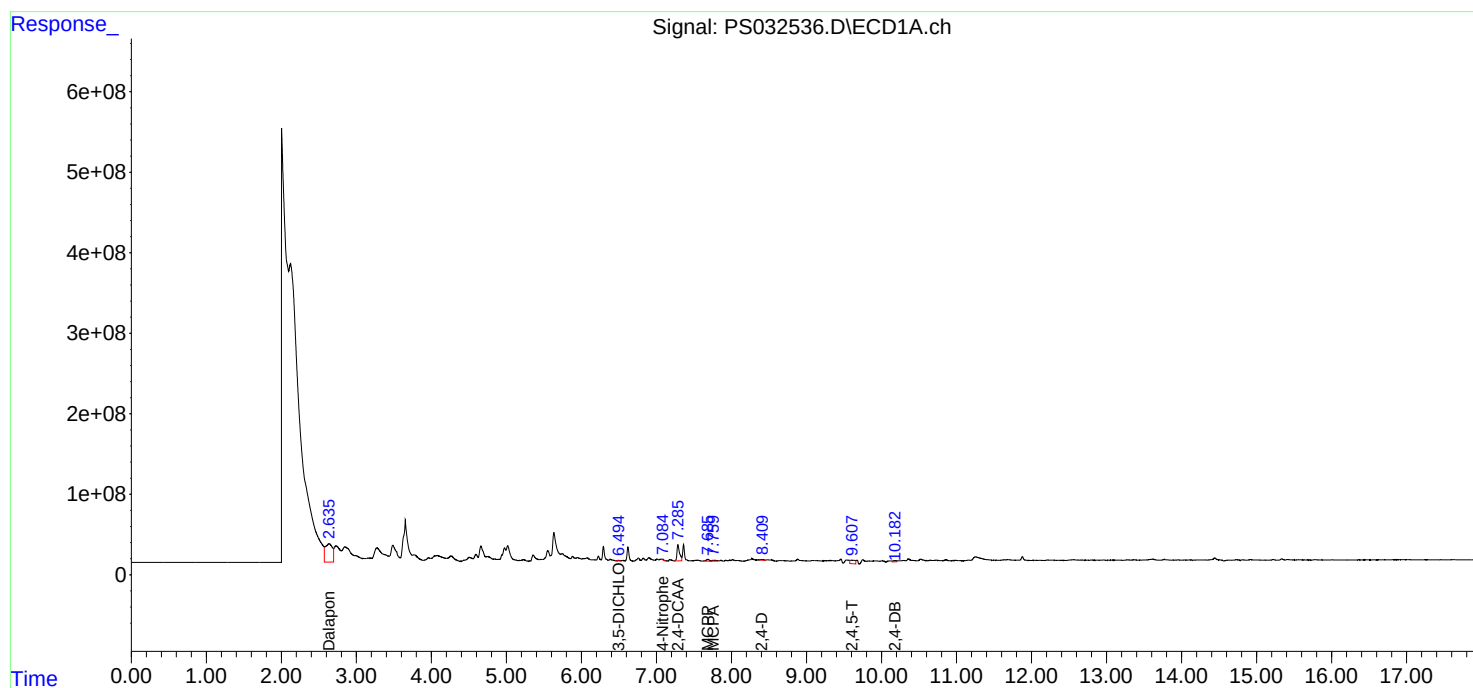


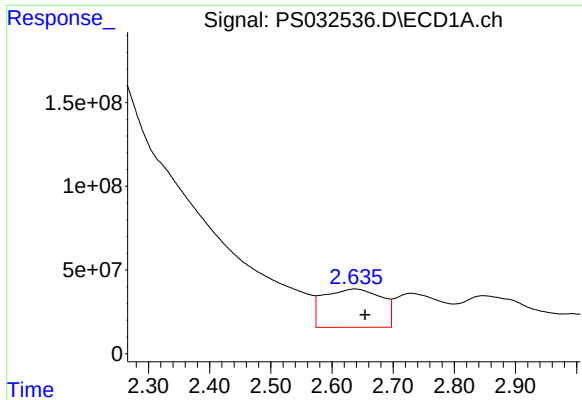

#1 Dalapon


R.T.: 2.636 min
Delta R.T.: -0.018 min
Response: 1506814078
Conc: 209.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

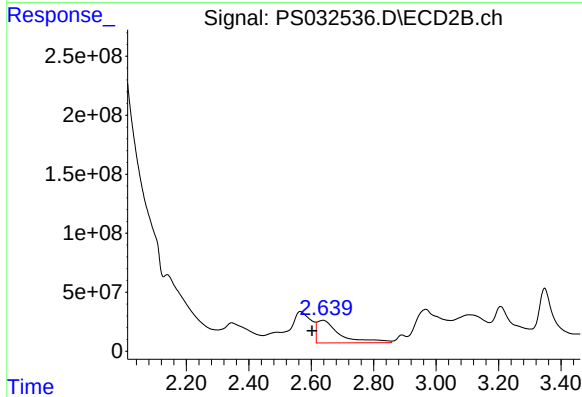


#1 Dalapon

R.T.: 2.638 min
Delta R.T.: 0.036 min
Response: 968843151
Conc: 139.32 ng/ml

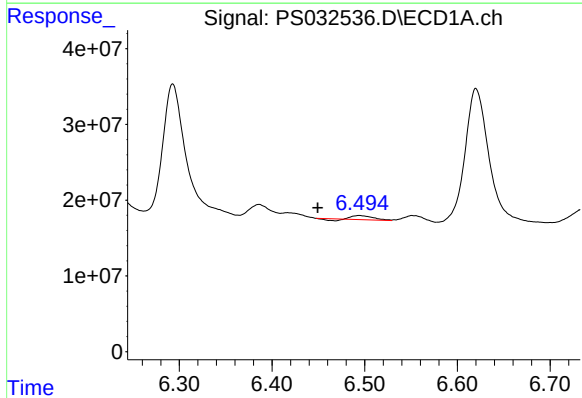


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.494 min
Delta R.T.: 0.045 min
Response: 7009899
Conc: 1.08 ng/ml

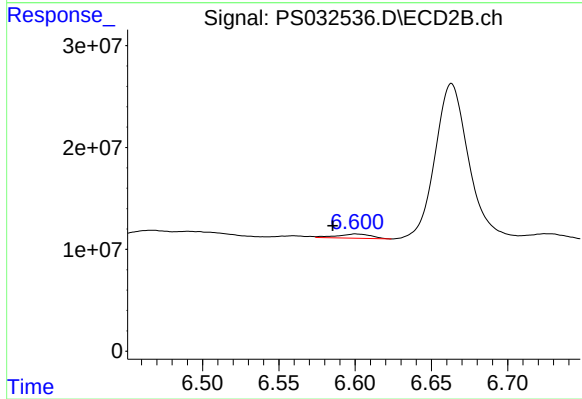

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.601 min
Delta R.T.: 0.016 min
Response: 6420502
Conc: 1.07 ng/ml

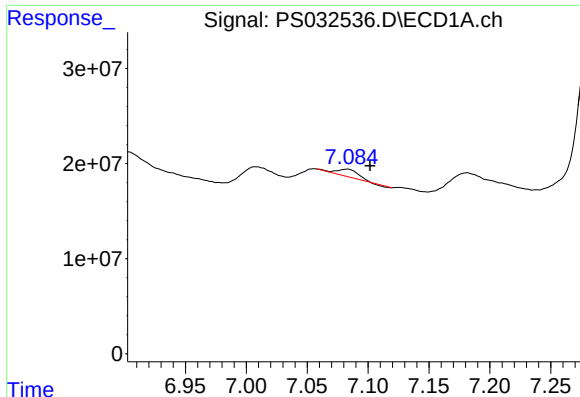

#3 4-Nitrophenol


R.T.: 7.083 min
Delta R.T.: -0.019 min
Response: 9195190
Conc: 6.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

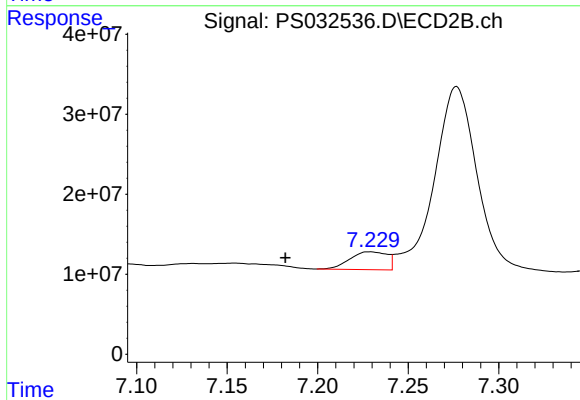


#3 4-Nitrophenol

R.T.: 7.229 min
Delta R.T.: 0.047 min
Response: 31906996
Conc: 14.06 ng/ml

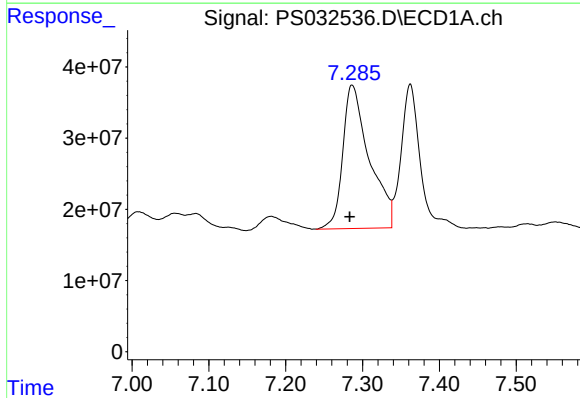


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.003 min
Response: 482249175
Conc: 106.43 ng/ml

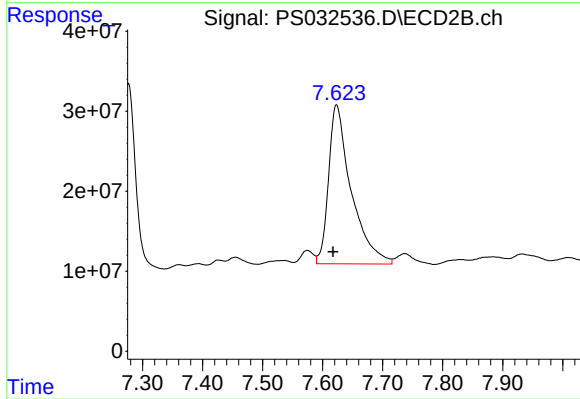

#4 2,4-DCAA


R.T.: 7.623 min
Delta R.T.: 0.006 min
Response: 521141169
Conc: 142.95 ng/ml

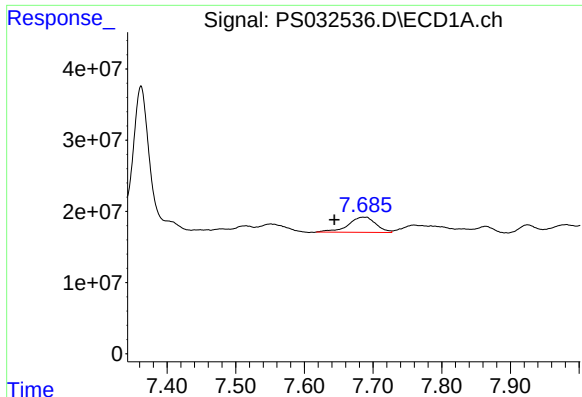

#6 MCP


R.T.: 7.687 min
Delta R.T.: 0.043 min
Response: 59592738
Conc: 5.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

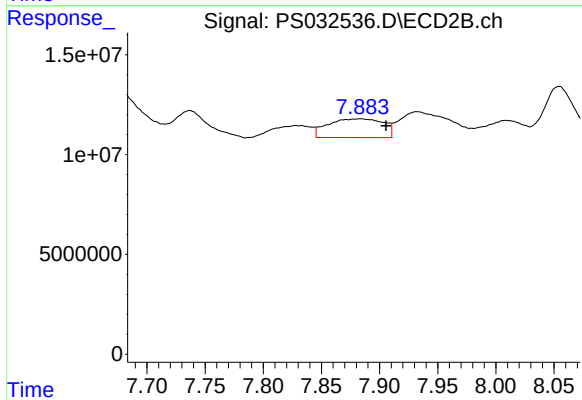


#6 MCP

R.T.: 7.883 min
Delta R.T.: -0.022 min
Response: 31119955
Conc: 2.34 ug/ml

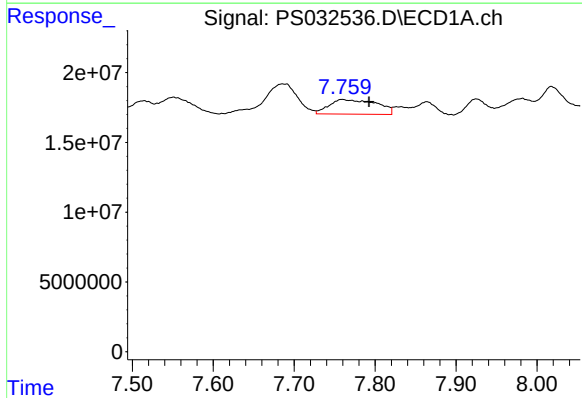


#7 MCP

R.T.: 7.760 min
Delta R.T.: -0.033 min
Response: 42861169
Conc: 3.19 ug/ml

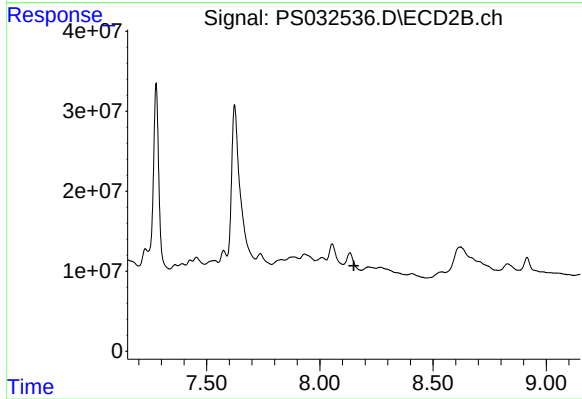

#7 MCP


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

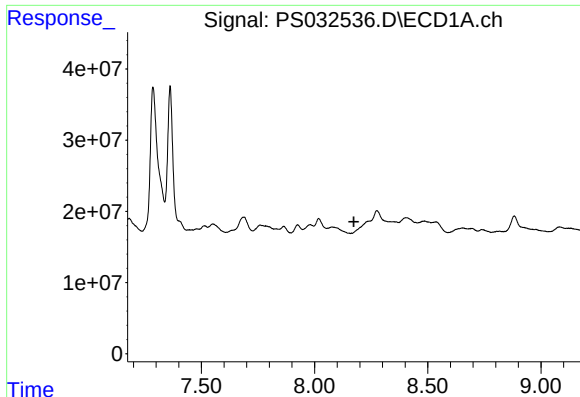

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

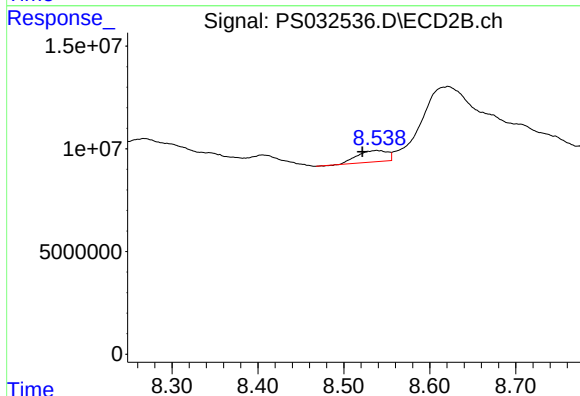


#8 DICHLORPROP

R.T.: 8.539 min
Delta R.T.: 0.017 min
Response: 13587464
Conc: 2.85 ng/ml

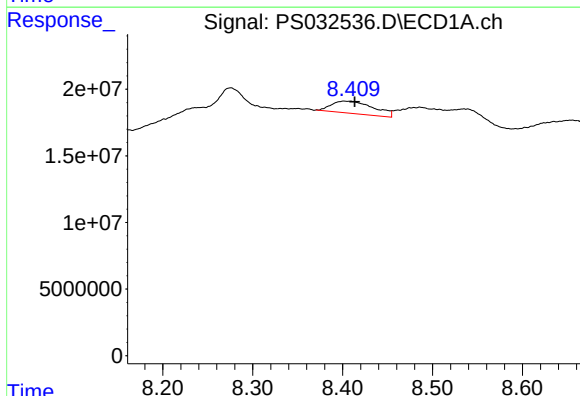


#9 2,4-D

R.T.: 8.404 min
Delta R.T.: -0.010 min
Response: 29922322
Conc: 6.63 ng/ml

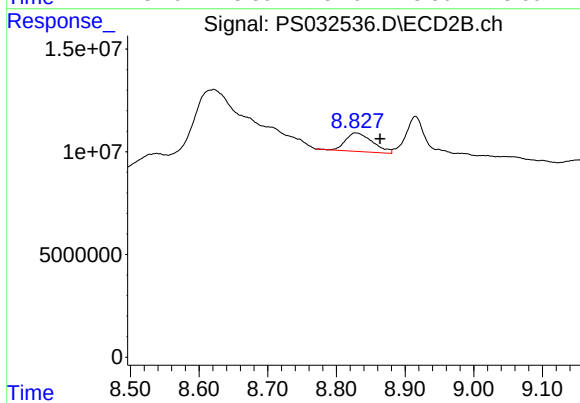

#9 2,4-D


R.T.: 8.828 min
Delta R.T.: -0.035 min
Response: 24844028
Conc: 4.74 ng/ml

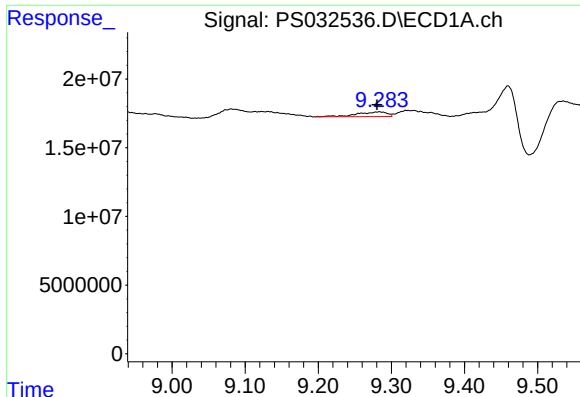

#11 2,4,5-TP (SILVEX)


R.T.: 9.283 min
Delta R.T.: 0.003 min
Response: 9997155
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

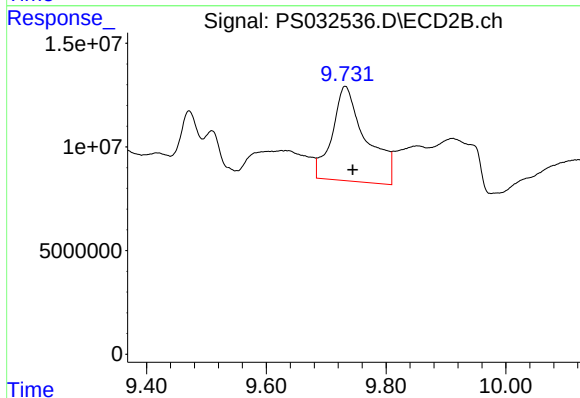


#11 2,4,5-TP (SILVEX)

R.T.: 9.732 min
Delta R.T.: -0.012 min
Response: 179699591
Conc: 6.69 ng/ml

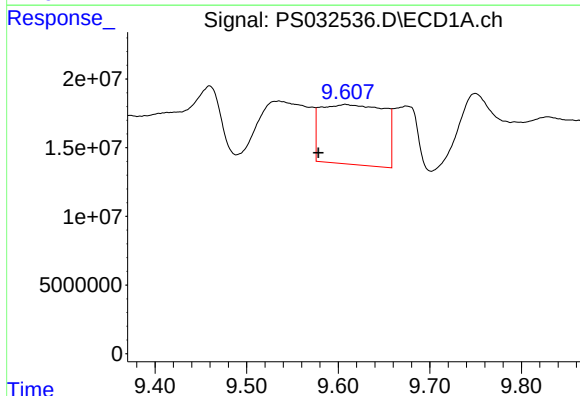


#12 2,4,5-T

R.T.: 9.608 min
Delta R.T.: 0.029 min
Response: 208931124
Conc: 8.76 ng/ml

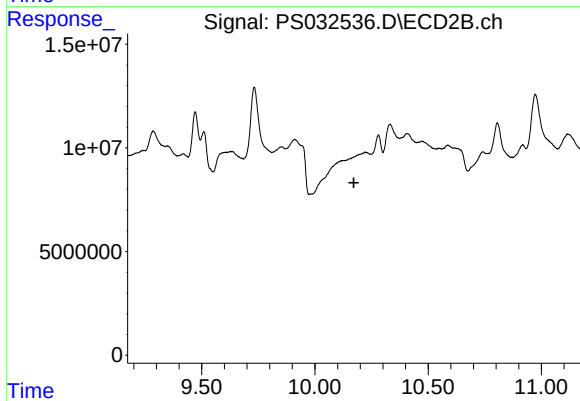

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 10.172 min
Response: 0
Conc: N.D.

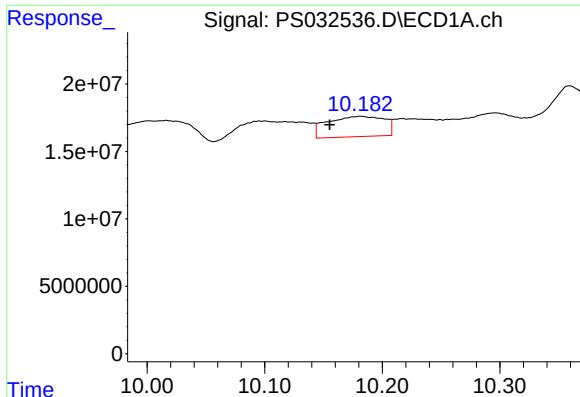

#13 2,4-DB


R.T.: 10.181 min
Delta R.T.: 0.026 min
Response: 50716049
Conc: 19.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

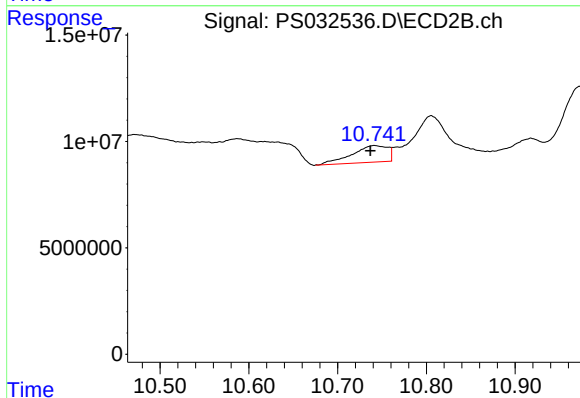


#13 2,4-DB

R.T.: 10.742 min
Delta R.T.: 0.005 min
Response: 22135040
Conc: 5.87 ng/ml

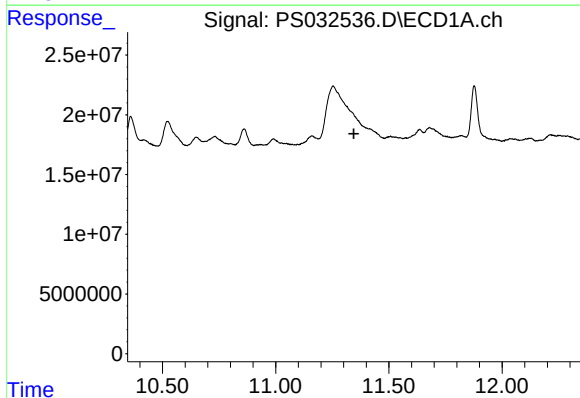


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.345 min
Response: 0
Conc: N.D.

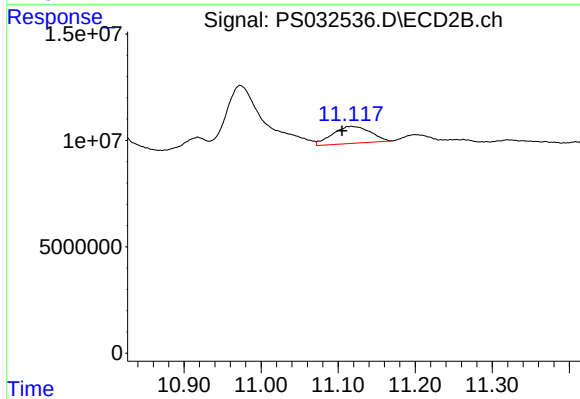

#14 DINOSEB


R.T.: 11.117 min
Delta R.T.: 0.012 min
Response: 27133980
Conc: 1.53 ng/ml

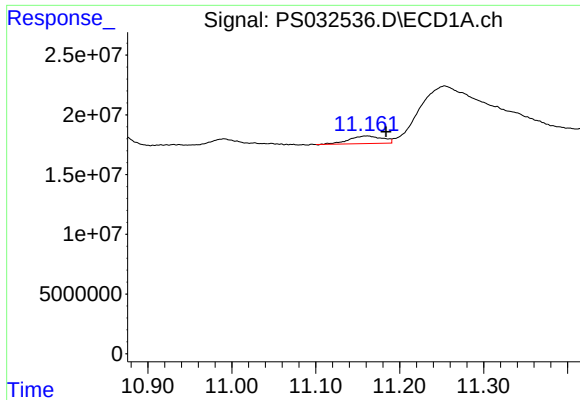

#15 Picloram

R.T.: 11.161 min
Delta R.T.: -0.023 min
Response: 17828358
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-112025

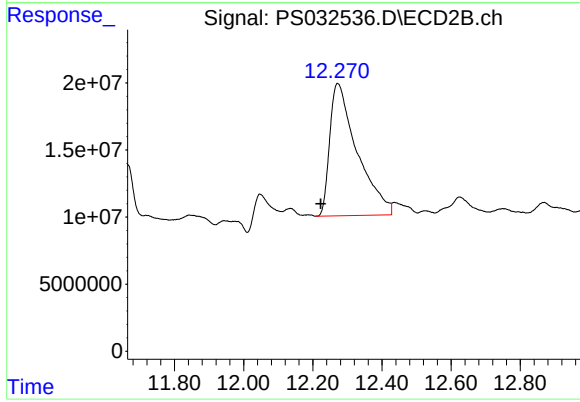

#15 Picloram

R.T.: 12.272 min
Delta R.T.: 0.049 min
Response: 541200931
Conc: 14.56 ng/ml