

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112525\
 Data File : PS032537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 11:32
 Operator : AR\AJ
 Sample : Q3699-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-06-112025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:43:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.627	420.4E6	502.6E6	92.784	137.857 #
Target Compounds							
1) T	Dalapon	2.637	2.570f	1534.4E6	1297.0E6	213.746	186.514
2) T	3,5-DICHL...	6.493f	6.607	7576506	7738480	1.172	1.288
3) T	4-Nitroph...	7.082	7.232f	28671921	60190441	21.358	26.517
5) T	DICAMBA	7.463	7.814	73060	12219096	<MDL	<MDL #
6) T	MCP	7.679f	7.898	114.8E6	11306670	10.538	<MDL #
7) T	MCPA	7.785	8.135	22589845	28027996	1.683	1.719
8) T	DICHLORPROP	0.000	8.548f	0	19102740	N.D.	4.005
9) T	2,4-D	8.397	8.834f	28932218	28578219	6.413	5.448
10) T	Pentachlo...	8.684	0.000	4225018	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.279	9.733	8505434	207.2E6	<MDL	7.715 #
12) T	2,4,5-T	9.615f	10.155	118.3E6	144.1E6	4.963	6.074
13) T	2,4-DB	10.175	0.000	43730240	0	16.595	N.D. #
14) T	DINOSEB	0.000	11.126	0	20473050	N.D.	1.157
15) T	Picloram	11.179	12.193f	2374555	3946396	<MDL	<MDL #
16) T	DCPA	11.629	0.000	4235082	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS112525\
Data File : PS032537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 11:32
Operator : AR\AJ
Sample : Q3699-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:43:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

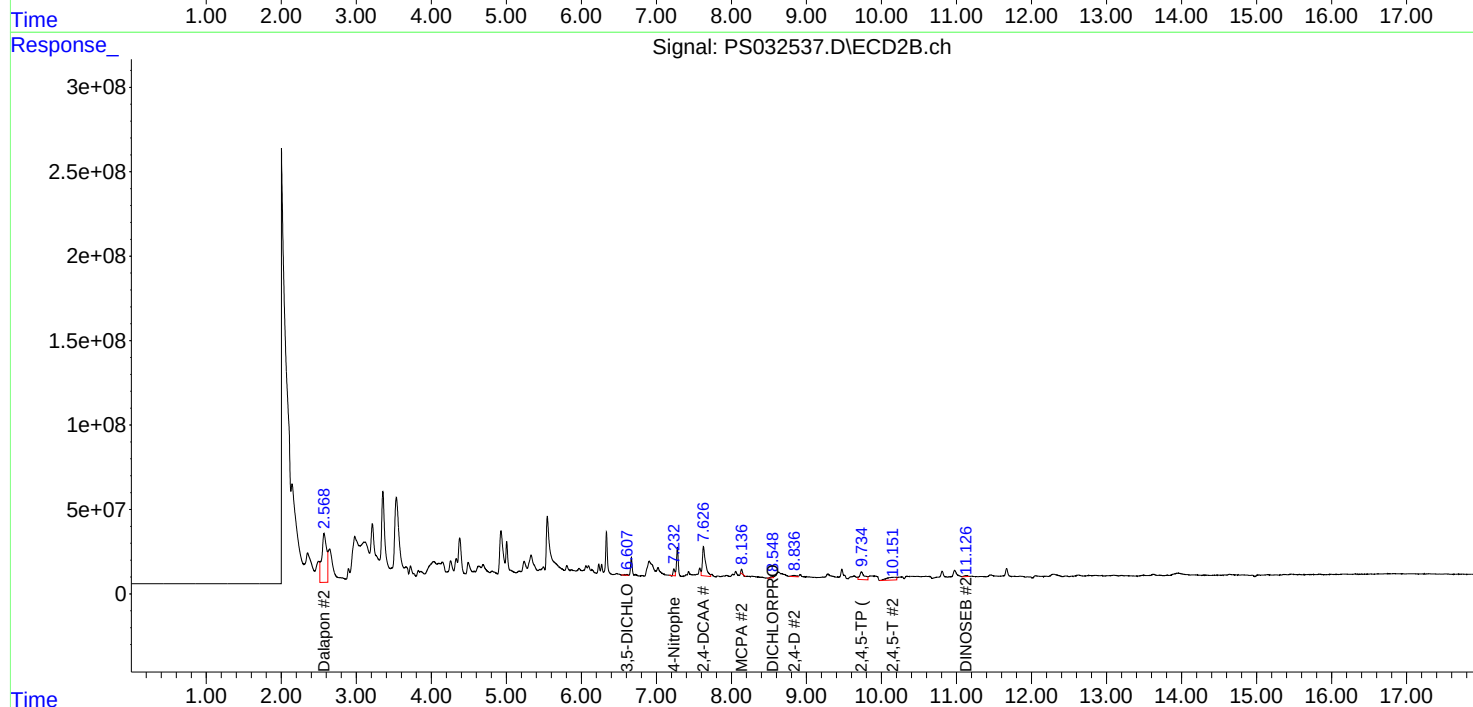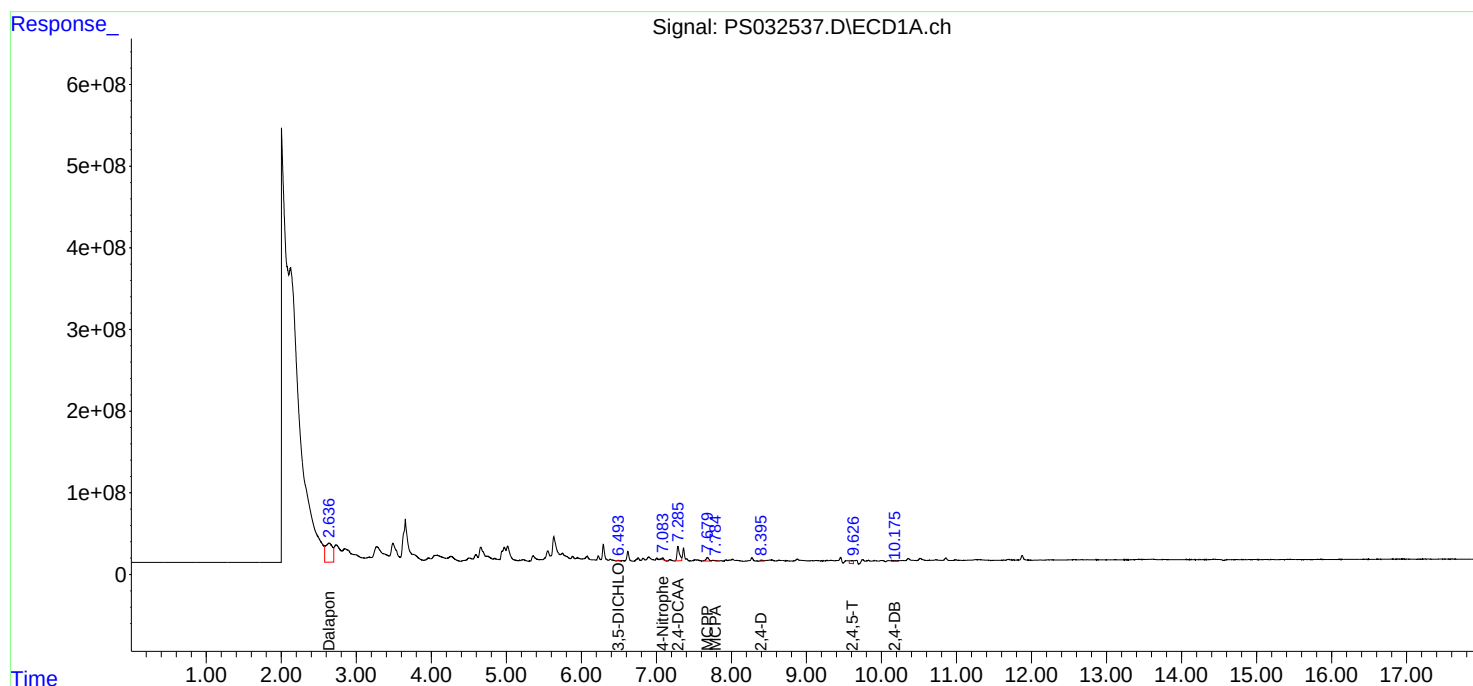


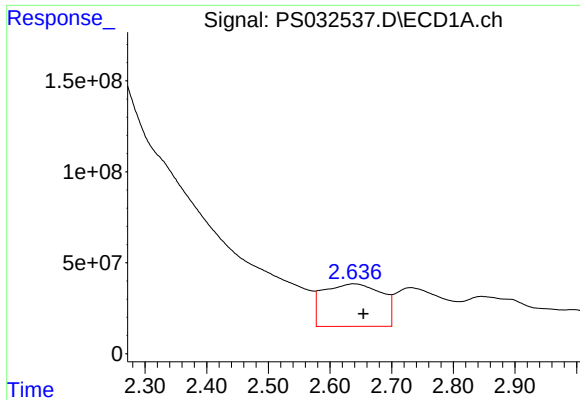

#1 Dalapon


R.T.: 2.637 min
Delta R.T.: -0.017 min
Response: 1534431256
Conc: 213.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

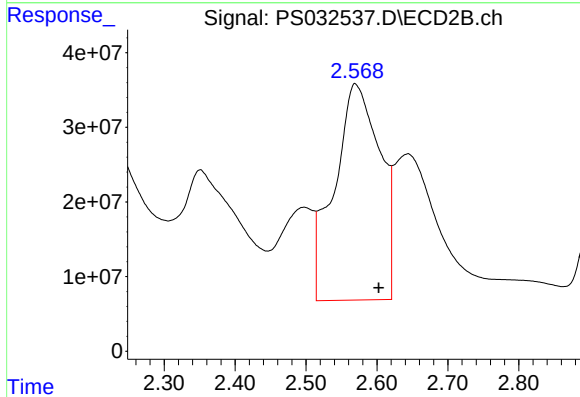


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: -0.033 min
Response: 1297014543
Conc: 186.51 ng/ml

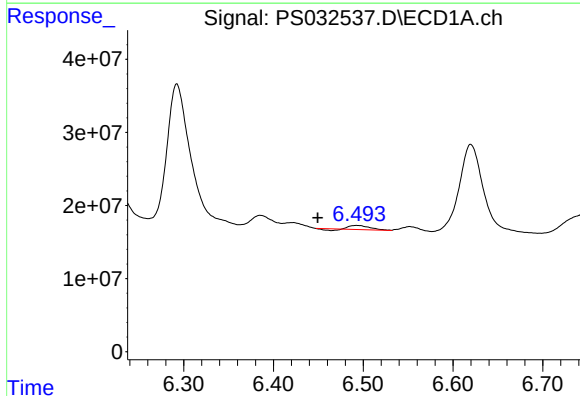


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.493 min
Delta R.T.: 0.043 min
Response: 7576506
Conc: 1.17 ng/ml

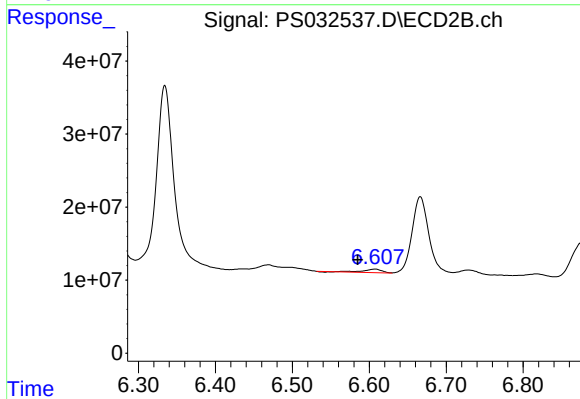

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.607 min
Delta R.T.: 0.022 min
Response: 7738480
Conc: 1.29 ng/ml

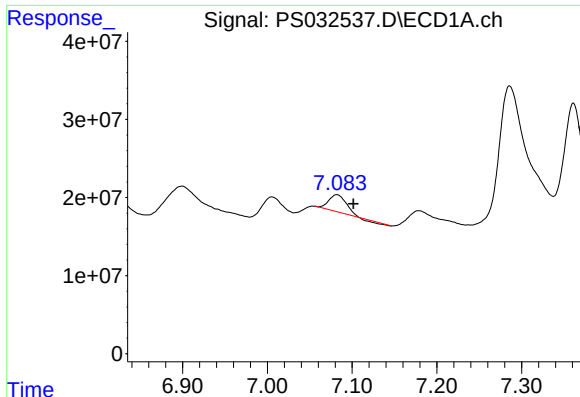

#3 4-Nitrophenol


R.T.: 7.082 min
Delta R.T.: -0.020 min
Response: 28671921
Conc: 21.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

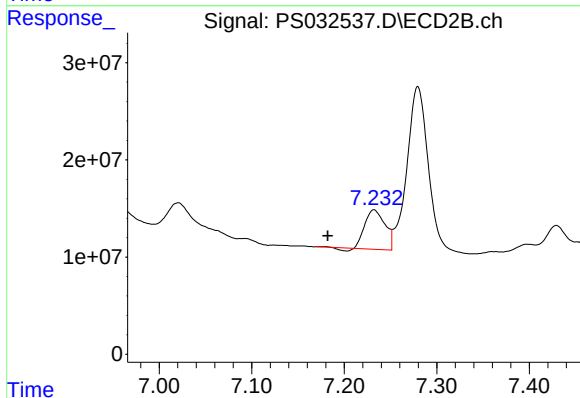


#3 4-Nitrophenol

R.T.: 7.232 min
Delta R.T.: 0.050 min
Response: 60190441
Conc: 26.52 ng/ml

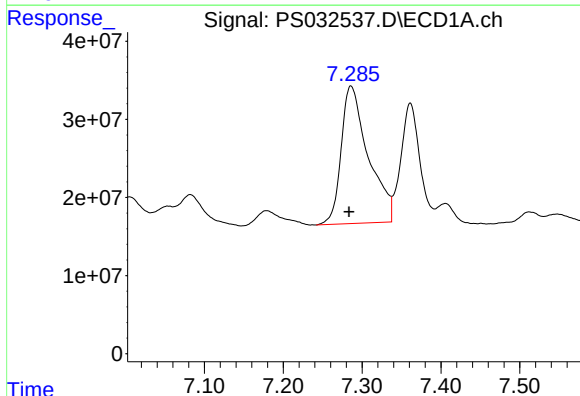


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.002 min
Response: 420430313
Conc: 92.78 ng/ml

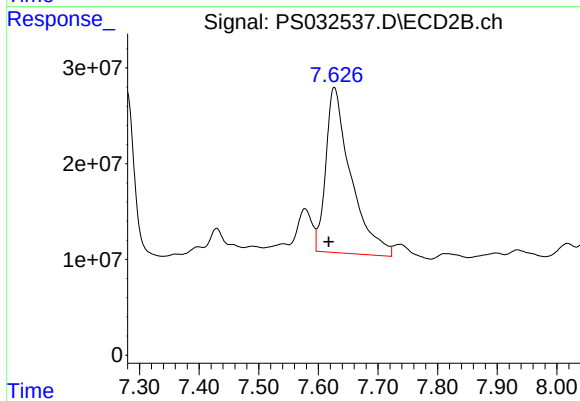

#4 2,4-DCAA


R.T.: 7.627 min
Delta R.T.: 0.010 min
Response: 502557757
Conc: 137.86 ng/ml

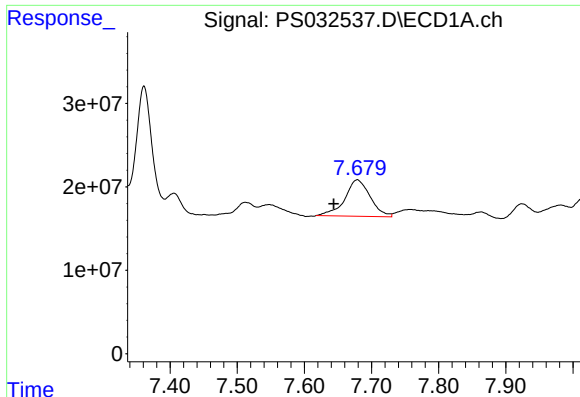

#6 MCPP


R.T.: 7.679 min
Delta R.T.: 0.035 min
Response: 114760424
Conc: 10.54 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

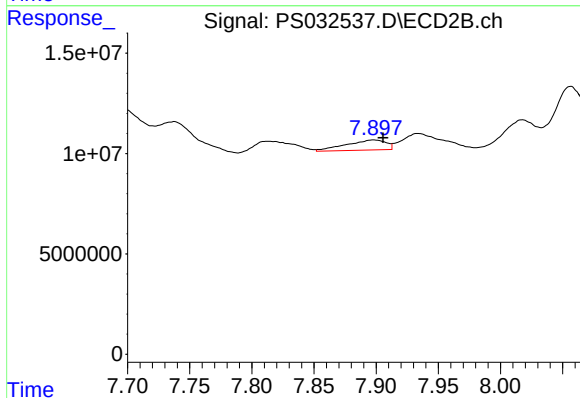


#6 MCPP

R.T.: 7.898 min
Delta R.T.: -0.008 min
Response: 11306670
Conc: N.D.

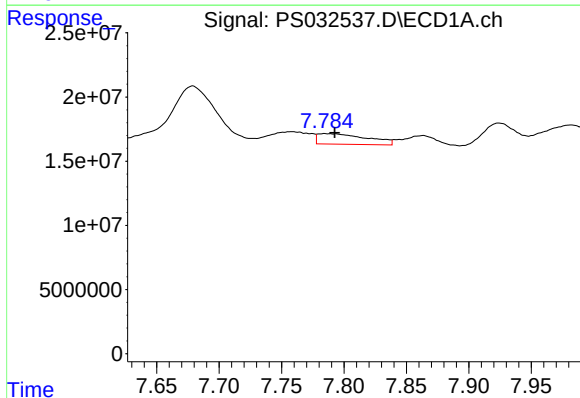


#7 MCPA

R.T.: 7.785 min
Delta R.T.: -0.008 min
Response: 22589845
Conc: 1.68 ug/ml

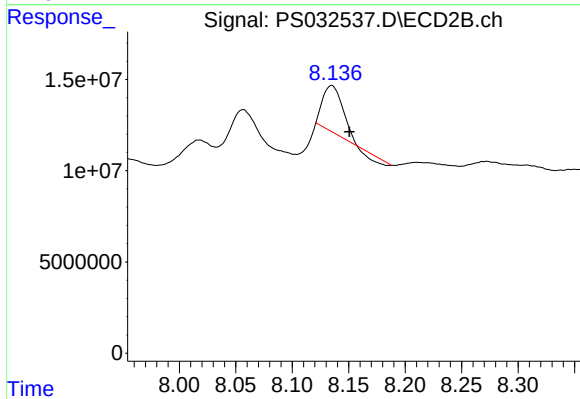

#7 MCPA


R.T.: 8.135 min
Delta R.T.: -0.016 min
Response: 28027996
Conc: 1.72 ug/ml

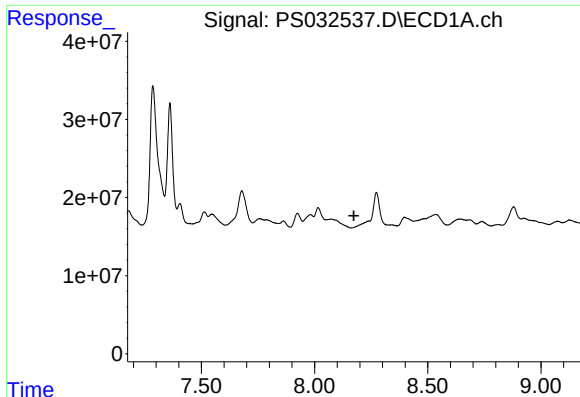

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

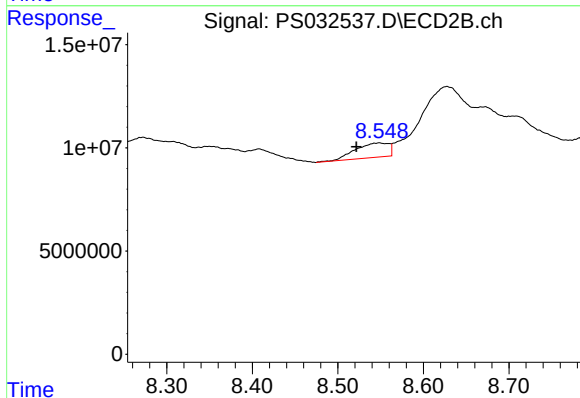


#8 DICHLORPROP

R.T.: 8.548 min
Delta R.T.: 0.026 min
Response: 19102740
Conc: 4.01 ng/ml

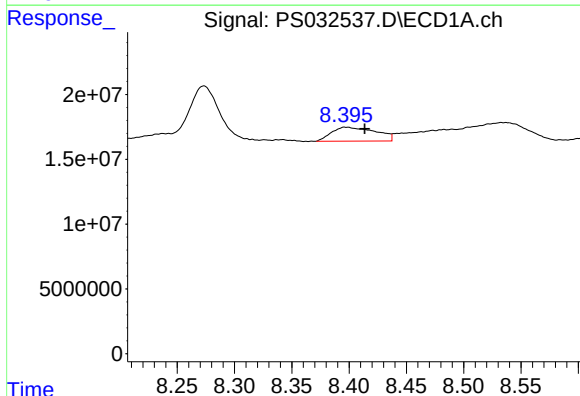


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: -0.017 min
Response: 28932218
Conc: 6.41 ng/ml

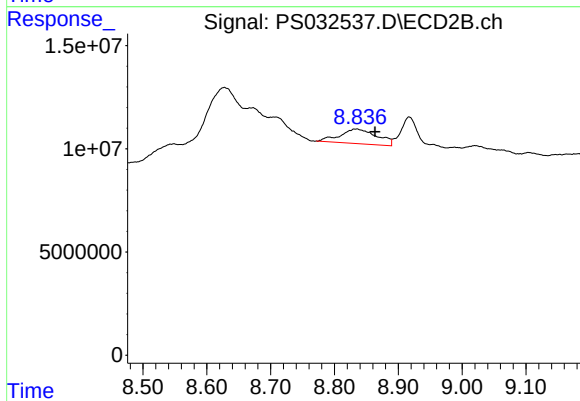

#9 2,4-D


R.T.: 8.834 min
Delta R.T.: -0.030 min
Response: 28578219
Conc: 5.45 ng/ml

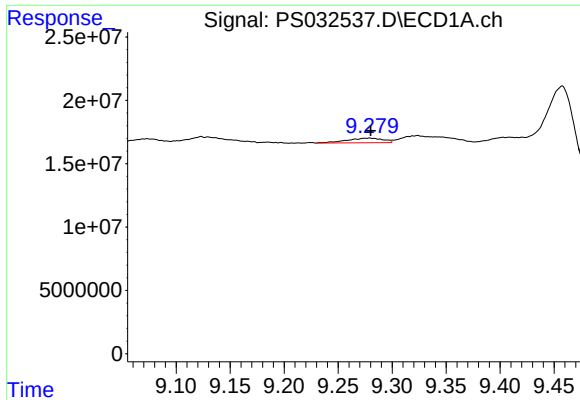

#11 2,4,5-TP (SILVEX)


R.T.: 9.279 min
Delta R.T.: -0.001 min
Response: 8505434
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

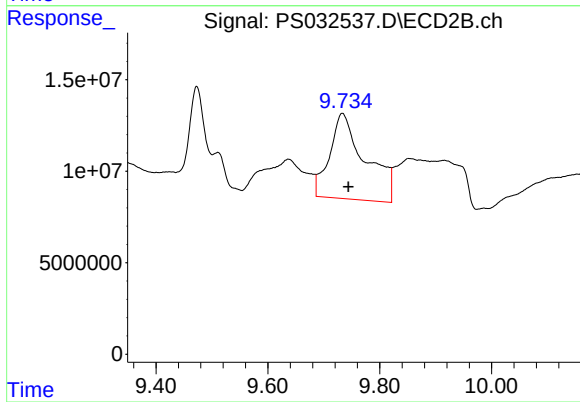


#11 2,4,5-TP (SILVEX)

R.T.: 9.733 min
Delta R.T.: -0.011 min
Response: 207186498
Conc: 7.72 ng/ml

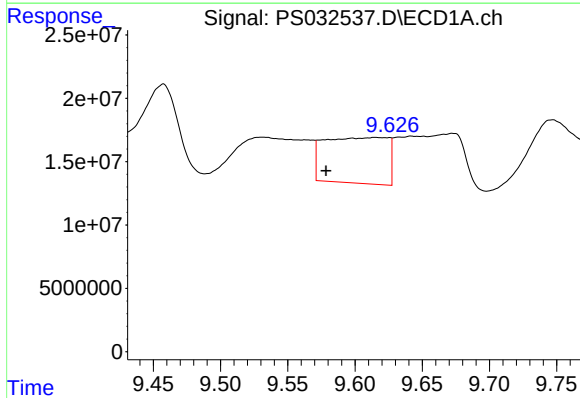


#12 2,4,5-T

R.T.: 9.615 min
Delta R.T.: 0.037 min
Response: 118304924
Conc: 4.96 ng/ml

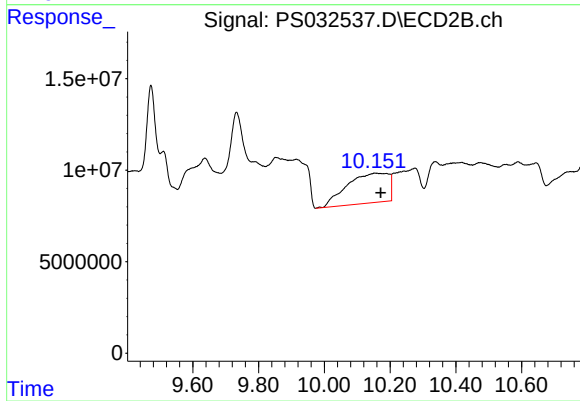

#12 2,4,5-T


R.T.: 10.155 min
Delta R.T.: -0.017 min
Response: 144060853
Conc: 6.07 ng/ml

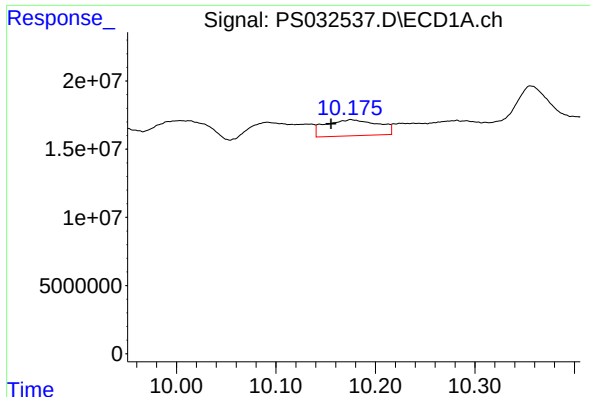

#13 2,4-DB


R.T.: 10.175 min
Delta R.T.: 0.020 min
Response: 43730240
Conc: 16.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-06-112025

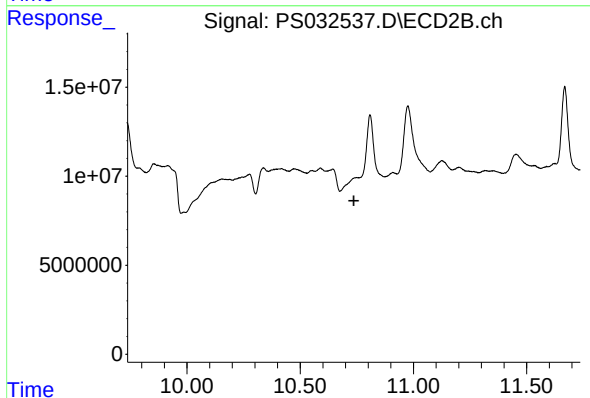


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

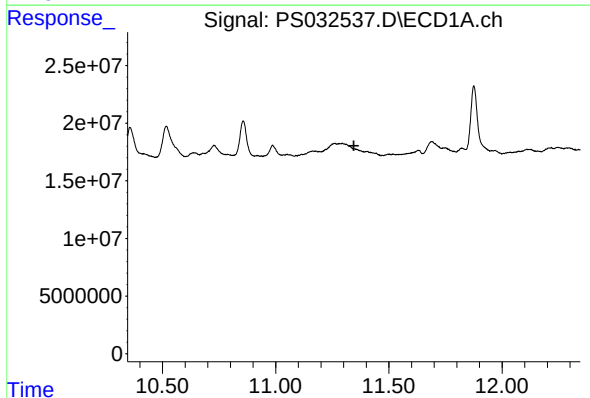

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.345 min
Response: 0
Conc: N.D.

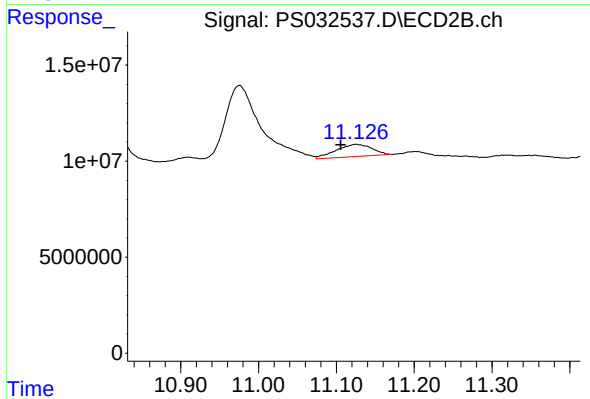

#14 DINOSEB

R.T.: 11.126 min
Delta R.T.: 0.020 min
Response: 20473050
Conc: 1.16 ng/ml